

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
 Data File : PL067816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2021 20:10
 Operator : AR\AJ
 Sample : M2842-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BIN-2-72-11966-RB-21140

Manual Integrations
 APPROVED

Ankita
 6/28/2021 9:29:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 06:29:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.475	5.526	6030155	10813735	10.968m	11.471
28) SA Decachlor...	10.214	11.419	7490246	12935417	10.569	12.987

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
Data File : PL067816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2021 20:10
Operator : AR\AJ
Sample : M2842-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BIN-2-72-11966-RB-21140


Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 06:29:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

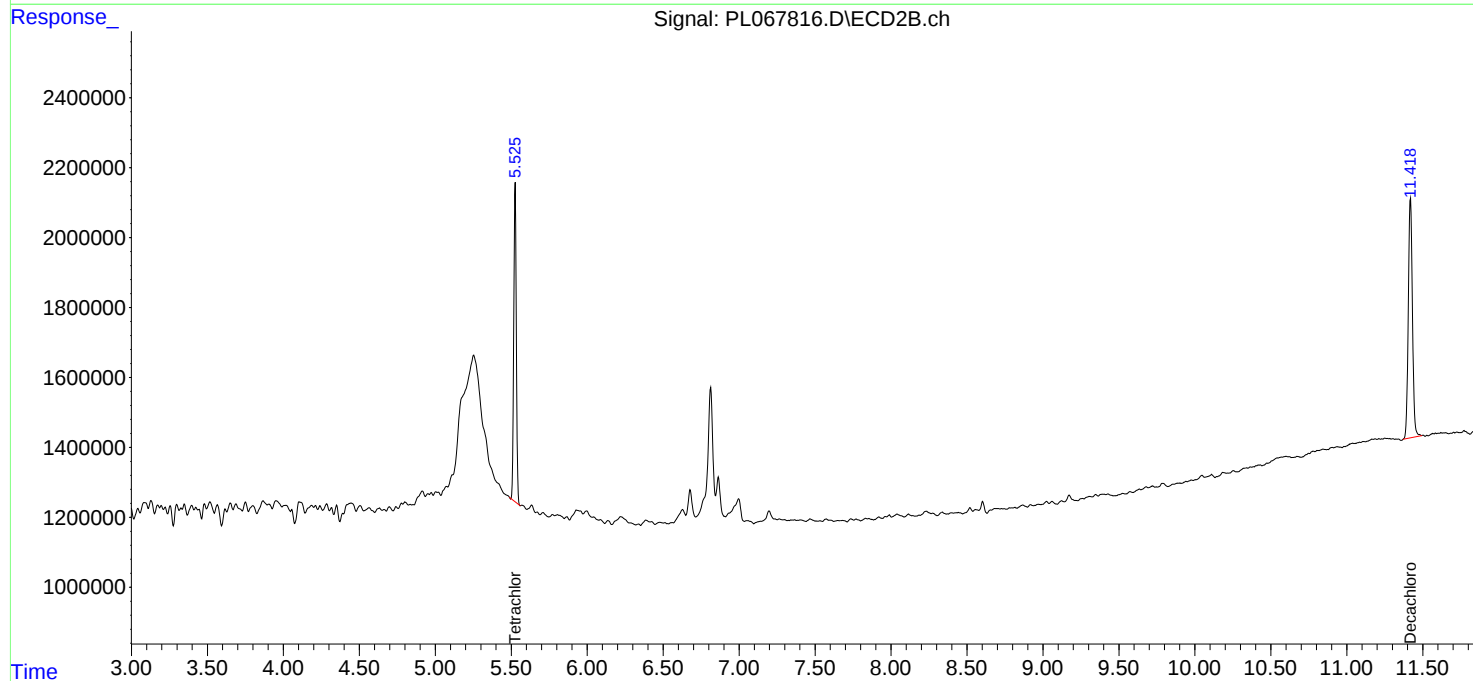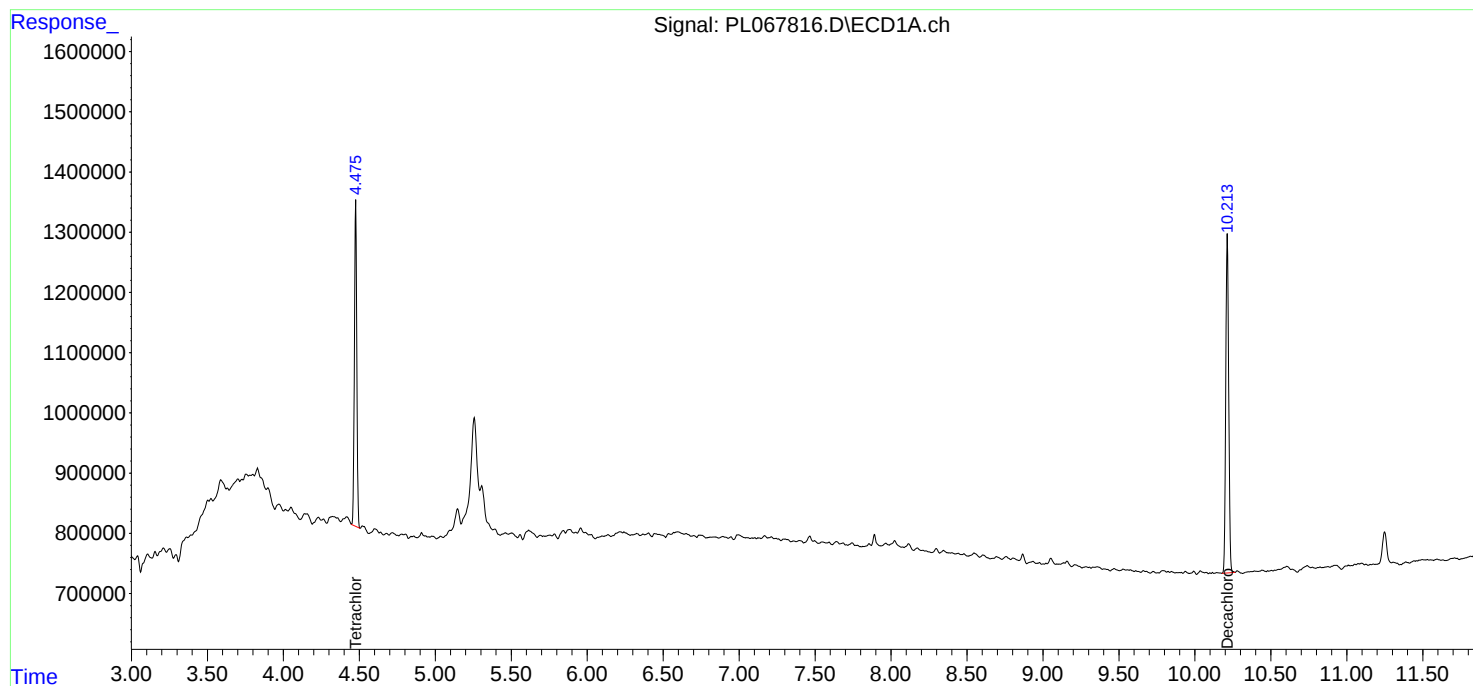

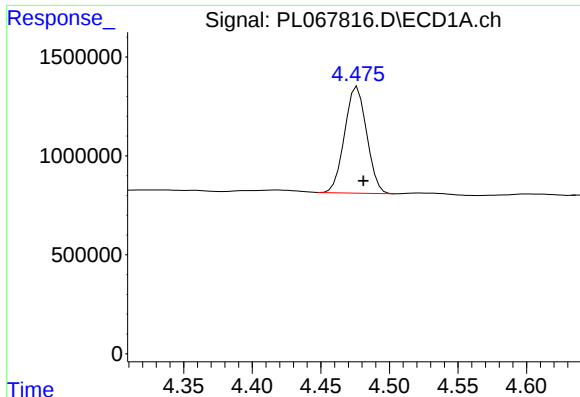


#1 Tetrachloro-m-xylene

R.T.: 4.475 min
Delta R.T.: -0.006 min
Response: 6030155
Conc: 10.97 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BIN-2-72-11966-RB-21140


Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:18 AM

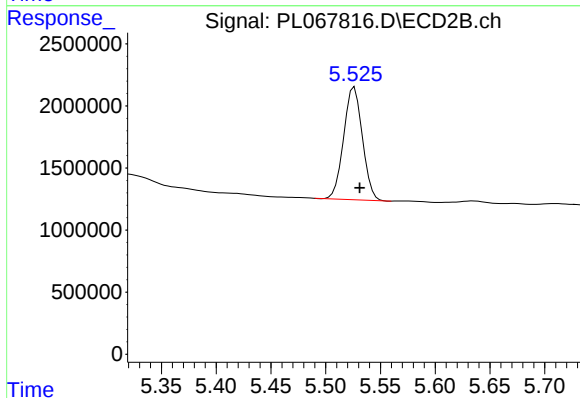


#1 Tetrachloro-m-xylene

R.T.: 5.526 min
Delta R.T.: -0.005 min
Response: 10813735
Conc: 11.47 ng/ml

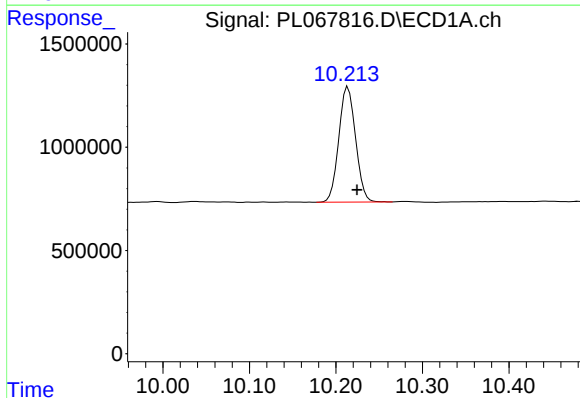

#28 Decachlorobiphenyl

R.T.: 10.214 min
Delta R.T.: -0.010 min
Response: 7490246
Conc: 10.57 ng/ml

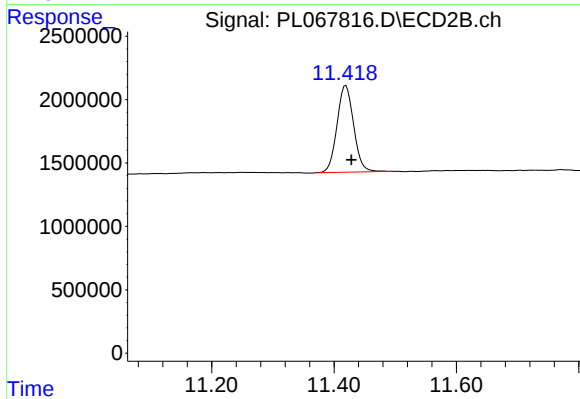

#28 Decachlorobiphenyl

R.T.: 11.419 min
Delta R.T.: -0.009 min
Response: 12935417
Conc: 12.99 ng/ml