

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
 Data File : PL067817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2021 20:26
 Operator : AR\AJ
 Sample : M2843-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-062421

Manual Integrations
 APPROVED

Ankita
 6/28/2021 9:29:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 06:31:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.476	5.526	5515962	9853158	10.033	10.452
28)	SA Decachlor...	10.215	11.419	7345061	11712567	10.364	11.759
Target Compounds							
10)	B gamma-Chl...	7.177	8.251	313793	629374	0.433	0.623m#
11)	B alpha-Chl...	7.245	8.336	463612	1321815	0.633	1.309 #
12)	B 4,4'-DDE	7.464	8.523	358384	424919	0.539	0.469

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
Data File : PL067817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2021 20:26
Operator : AR\AJ
Sample : M2843-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-02-062421


Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 06:31:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

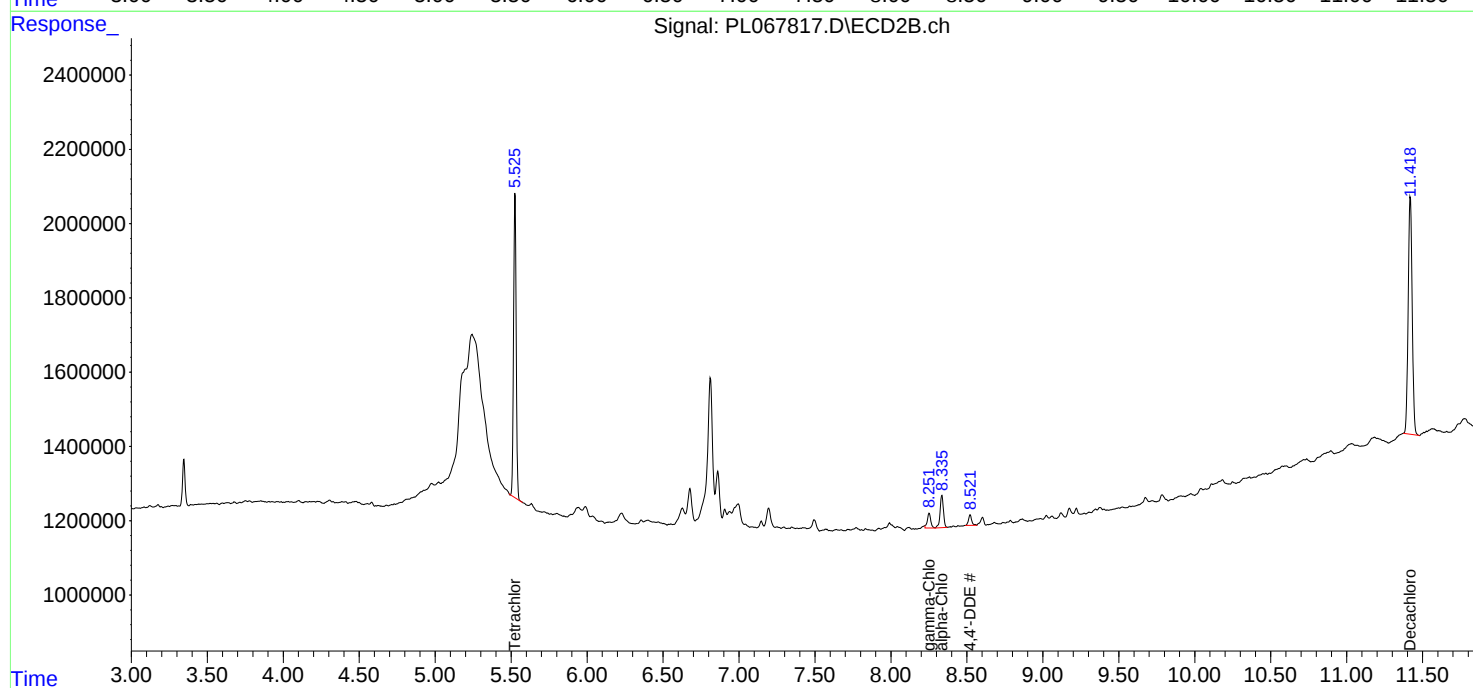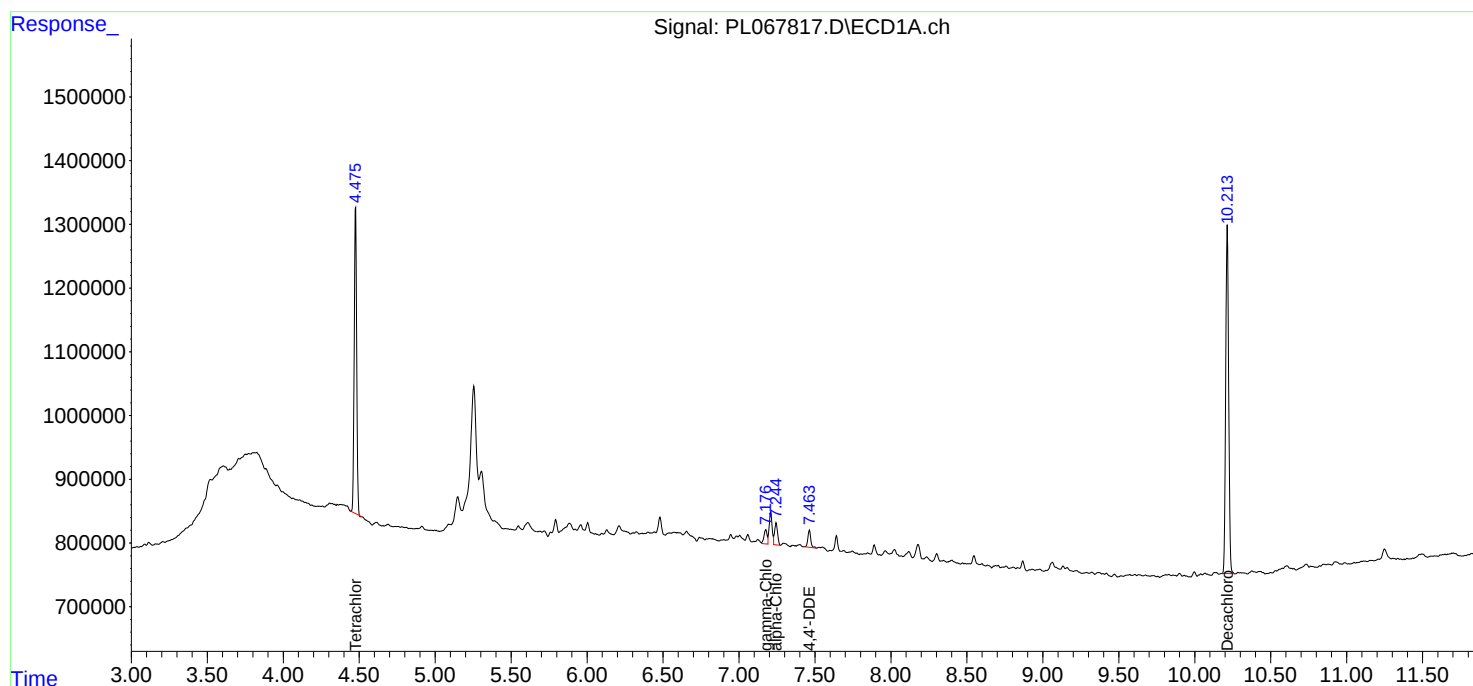

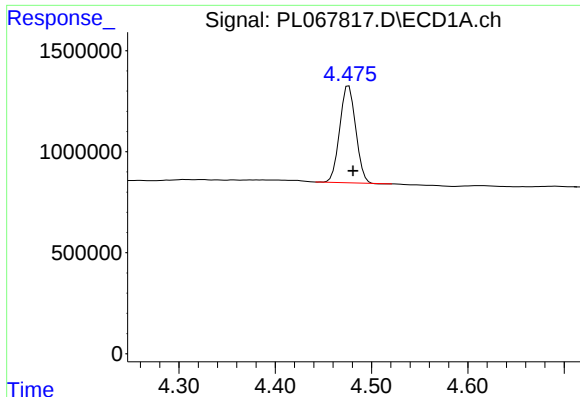


#1 Tetrachloro-m-xylene

R.T.: 4.476 min
Delta R.T.: -0.005 min
Response: 5515962
Conc: 10.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-062421


Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:20 AM

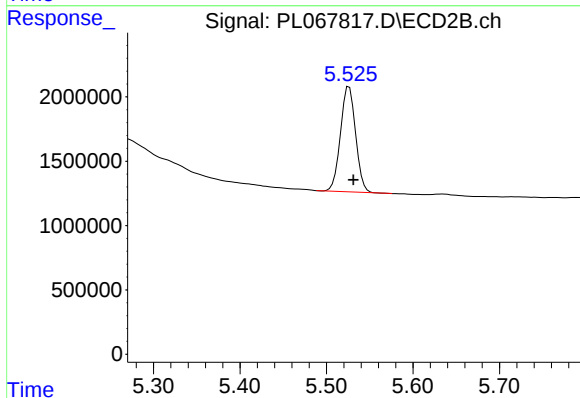


#1 Tetrachloro-m-xylene

R.T.: 5.526 min
Delta R.T.: -0.005 min
Response: 9853158
Conc: 10.45 ng/ml

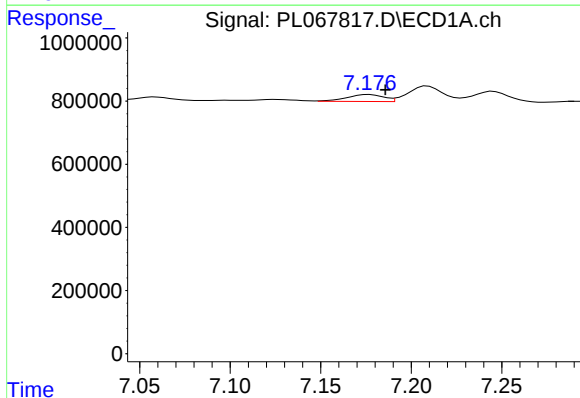


#10 gamma-Chlordane

R.T.: 7.177 min
Delta R.T.: -0.009 min
Response: 313793
Conc: 0.43 ng/ml

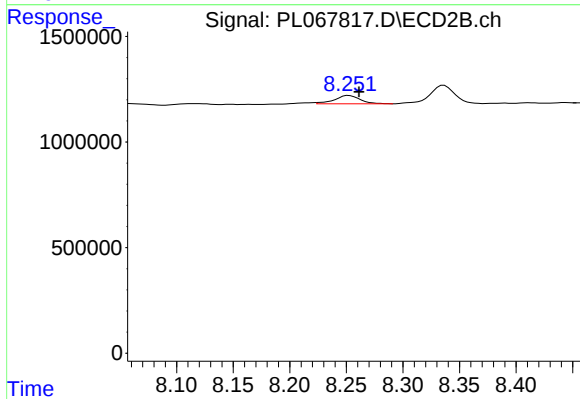

#10 gamma-Chlordane

R.T.: 8.251 min
Delta R.T.: -0.010 min
Response: 629374
Conc: 0.62 ng/ml m

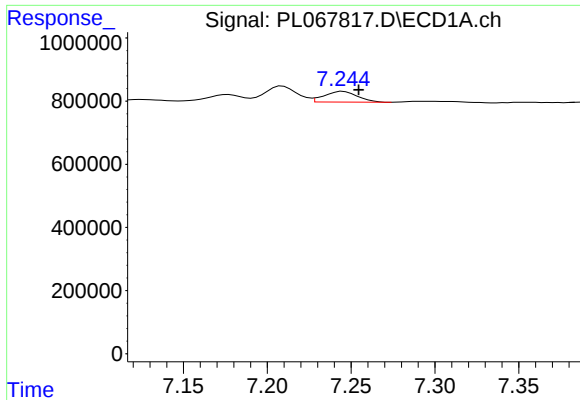


#11 alpha-Chlordane

R.T.: 7.245 min
Delta R.T.: -0.009 min
Response: 463612
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-062421


Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:20 AM

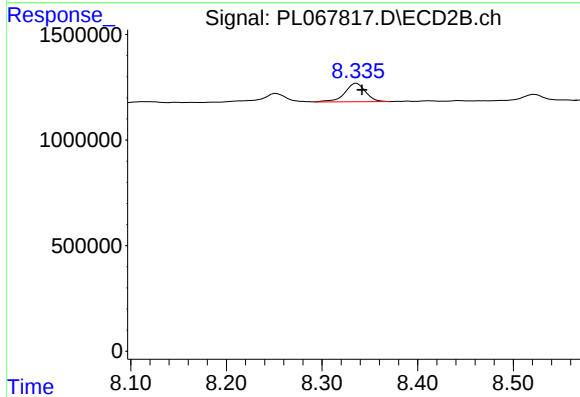


#11 alpha-Chlordane

R.T.: 8.336 min
Delta R.T.: -0.006 min
Response: 1321815
Conc: 1.31 ng/ml

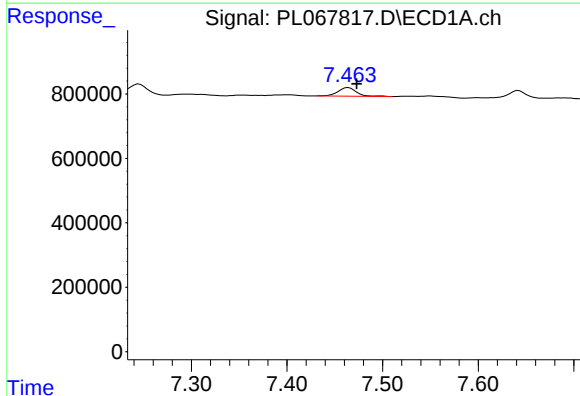


#12 4,4'-DDE

R.T.: 7.464 min
Delta R.T.: -0.009 min
Response: 358384
Conc: 0.54 ng/ml

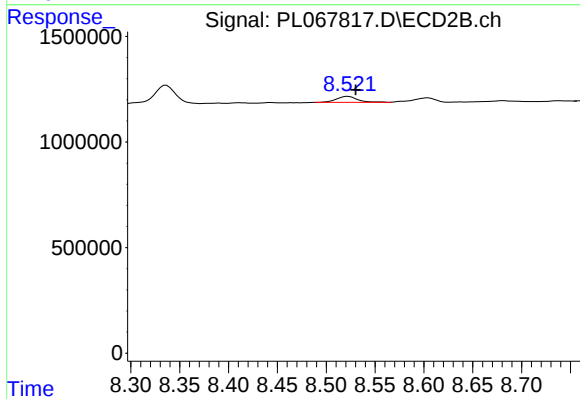

#12 4,4'-DDE

R.T.: 8.523 min
Delta R.T.: -0.008 min
Response: 424919
Conc: 0.47 ng/ml

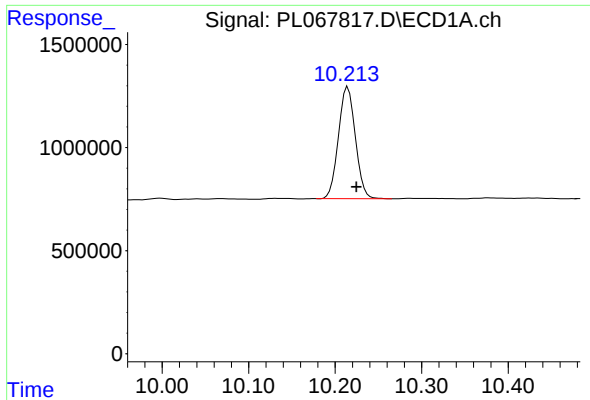


#28 Decachlorobiphenyl

R.T.: 10.215 min
Delta R.T.: -0.010 min
Response: 7345061
Conc: 10.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-062421

Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:20 AM

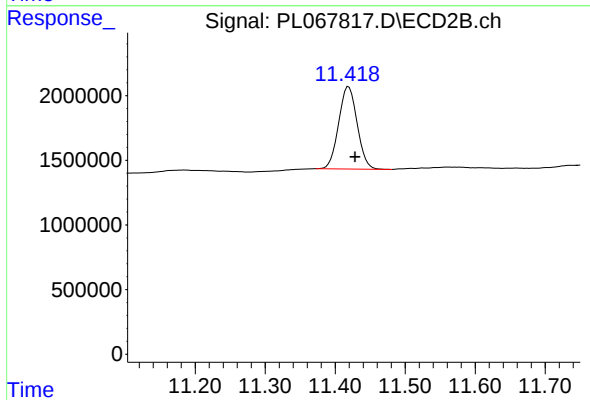

#28 Decachlorobiphenyl

R.T.: 11.419 min
Delta R.T.: -0.009 min
Response: 11712567
Conc: 11.76 ng/ml