

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
 Data File : PL067821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2021 21:33
 Operator : AR\AJ
 Sample : M2829-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 15B-STOCKPILE-3A

Manual Integrations
 APPROVED

Ankita
 6/28/2021 9:29:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 06:45:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.476	5.526	4205622	7417620	7.650	7.868
28)	SA Decachlor...	10.215	11.419	6739058	9652377	9.509	9.691
Target Compounds							
10)	B gamma-Chl...	7.177	8.254	4322099	9713815	5.961	9.621 #
11)	B alpha-Chl...	7.245	8.337	8888300	22764342	12.141	22.548 #
12)	B 4,4'-DDE	7.464	8.522	2757320	3307820	4.144	3.651
16)	A 4,4'-DDD	8.045	9.063	496557	1740519	0.854	2.447 #
17)	MA 4,4'-DDT	8.304	9.377	3951670	3866588	6.791	5.274m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062521\
Data File : PL067821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2021 21:33
Operator : AR\AJ
Sample : M2829-04
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
15B-STOCKPILE-3A


Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 06:45:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

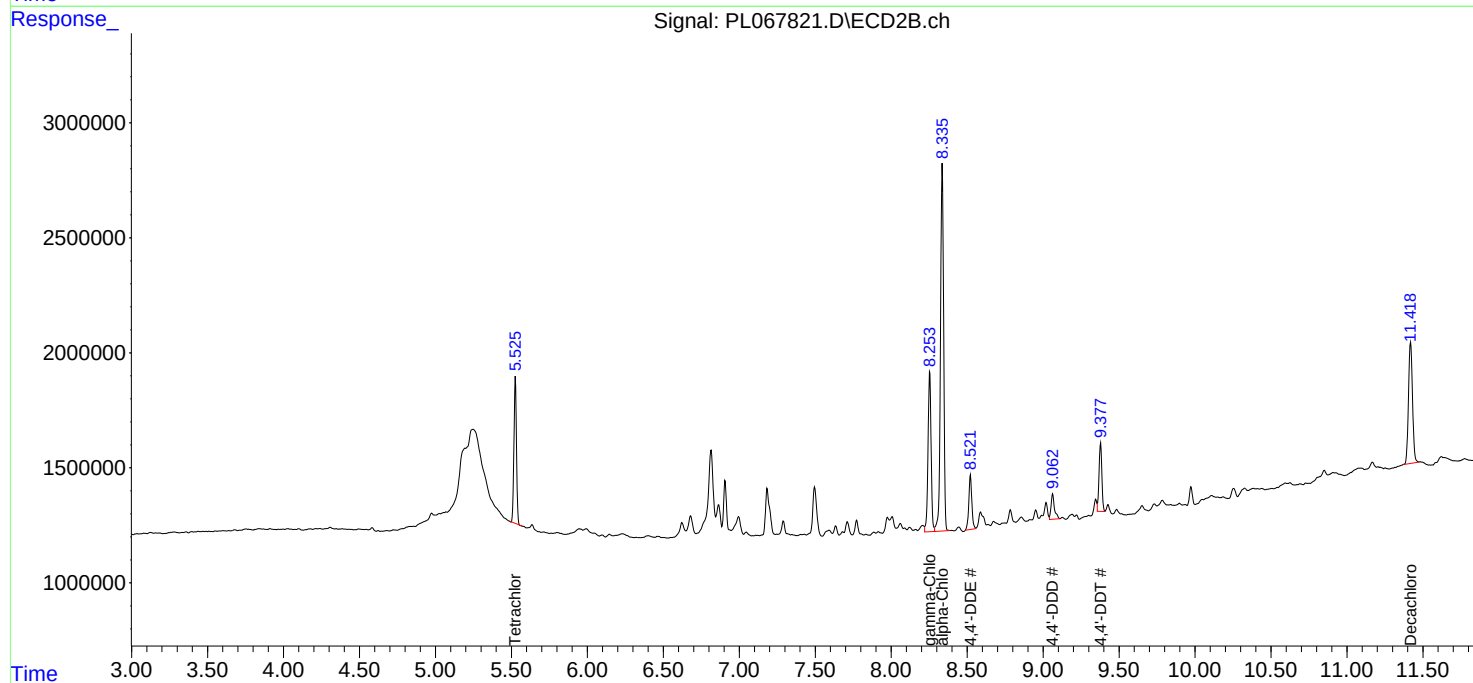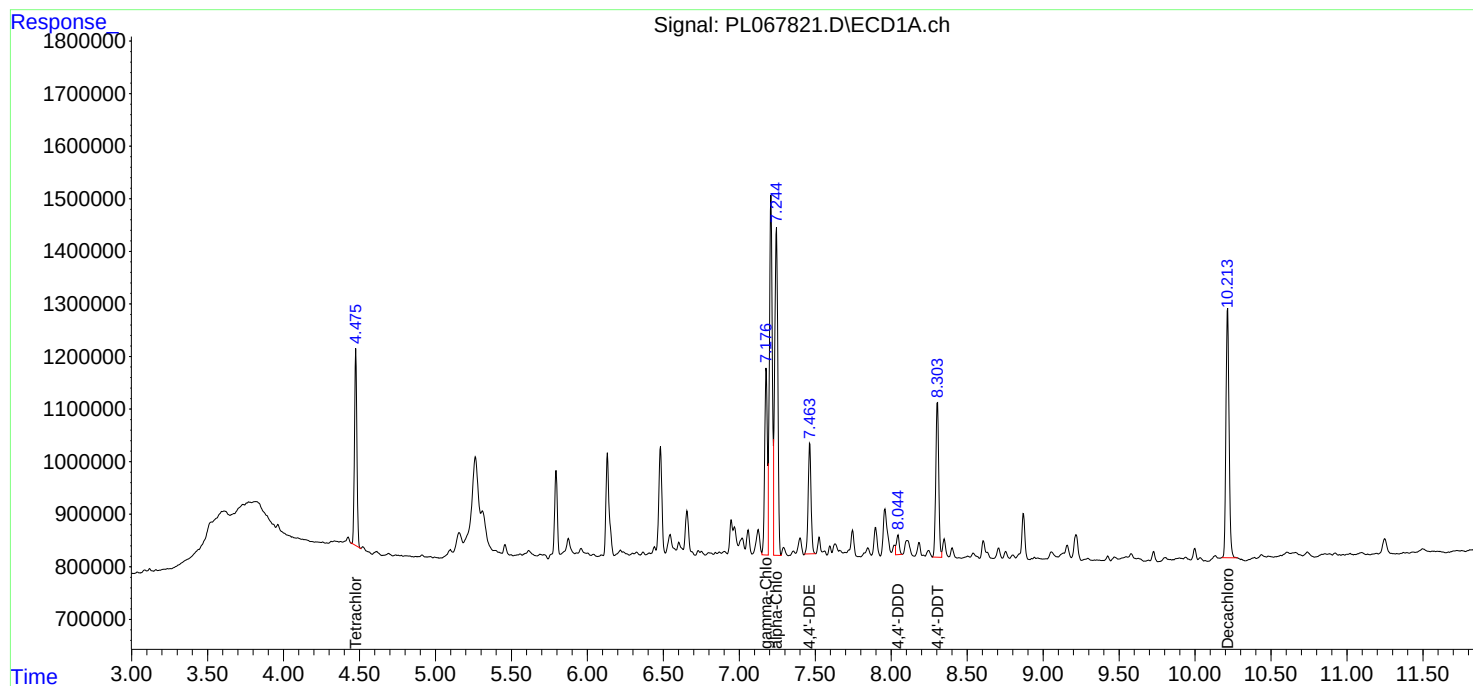

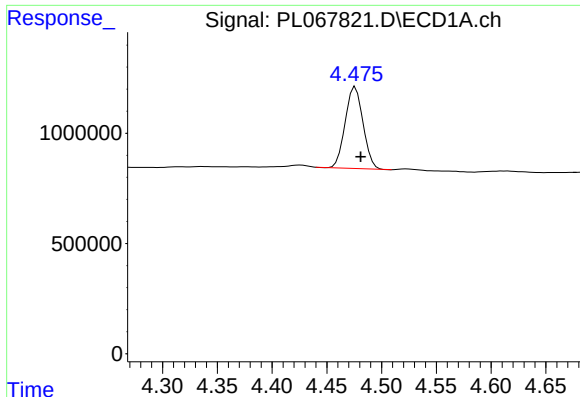


#1 Tetrachloro-m-xylene

R.T.: 4.476 min
Delta R.T.: -0.005 min
Response: 4205622
Conc: 7.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
15B-STOCKPILE-3A


Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:27 AM

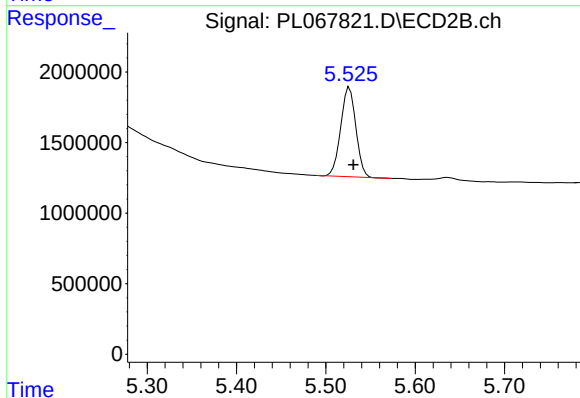


#1 Tetrachloro-m-xylene

R.T.: 5.526 min
Delta R.T.: -0.005 min
Response: 7417620
Conc: 7.87 ng/ml

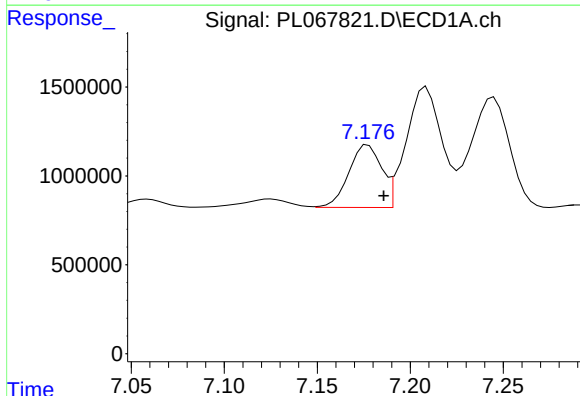


#10 gamma-Chlordane

R.T.: 7.177 min
Delta R.T.: -0.008 min
Response: 4322099
Conc: 5.96 ng/ml

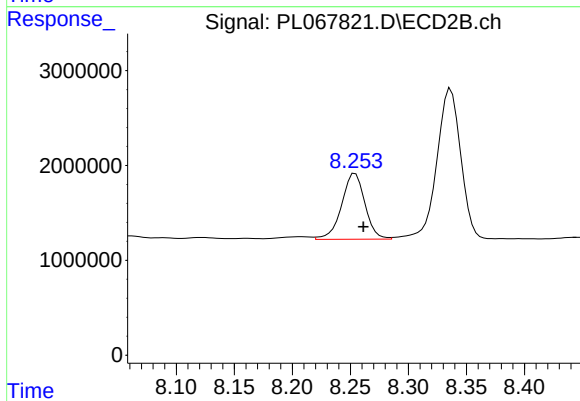

#10 gamma-Chlordane

R.T.: 8.254 min
Delta R.T.: -0.007 min
Response: 9713815
Conc: 9.62 ng/ml

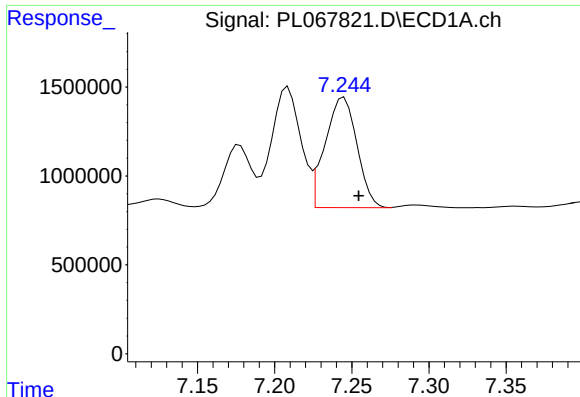


#11 alpha-Chlordane

R.T.: 7.245 min
Delta R.T.: -0.010 min
Response: 8888300
Conc: 12.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
15B-STOCKPILE-3A


Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:27 AM

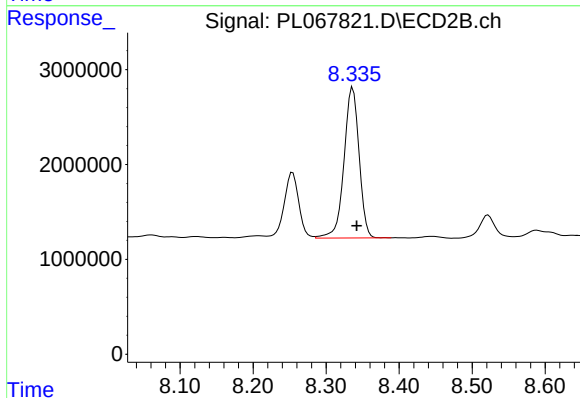


#11 alpha-Chlordane

R.T.: 8.337 min
Delta R.T.: -0.006 min
Response: 22764342
Conc: 22.55 ng/ml

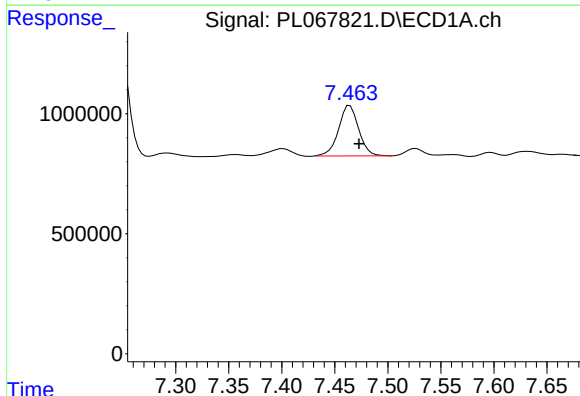


#12 4,4'-DDE

R.T.: 7.464 min
Delta R.T.: -0.009 min
Response: 2757320
Conc: 4.14 ng/ml

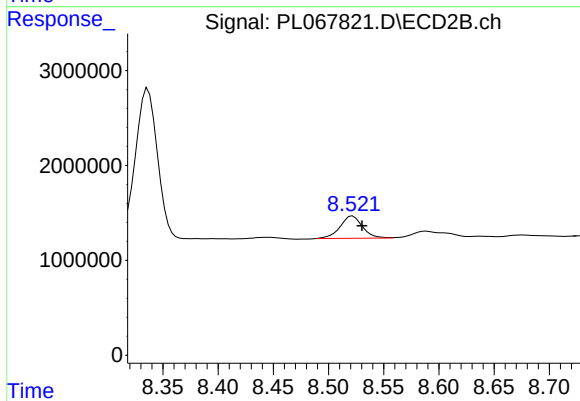

#12 4,4'-DDE

R.T.: 8.522 min
Delta R.T.: -0.008 min
Response: 3307820
Conc: 3.65 ng/ml

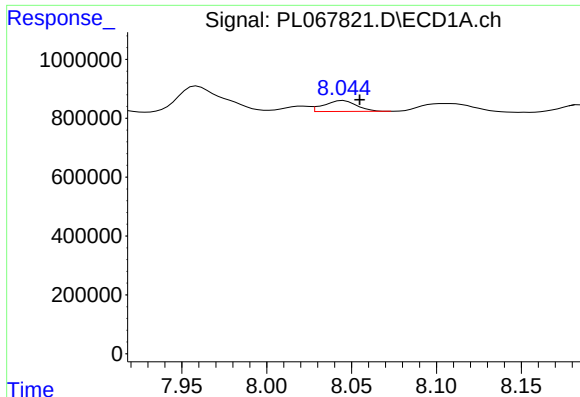


#16 4,4'-DDD

R.T.: 8.045 min
Delta R.T.: -0.009 min
Response: 496557
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
15B-STOCKPILE-3A


Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:27 AM

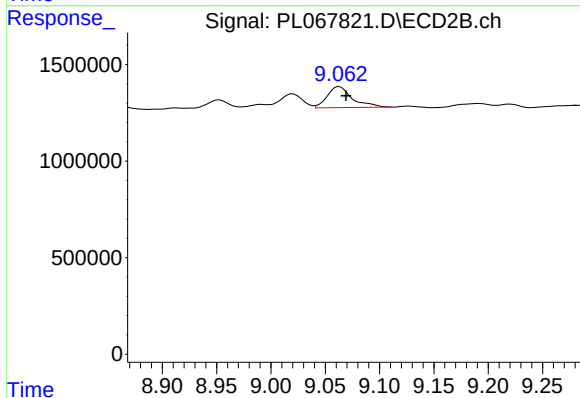


#16 4,4'-DDD

R.T.: 9.063 min
Delta R.T.: -0.006 min
Response: 1740519
Conc: 2.45 ng/ml

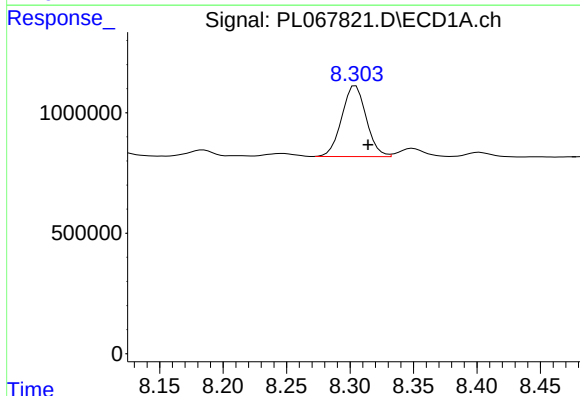


#17 4,4'-DDT

R.T.: 8.304 min
Delta R.T.: -0.010 min
Response: 3951670
Conc: 6.79 ng/ml

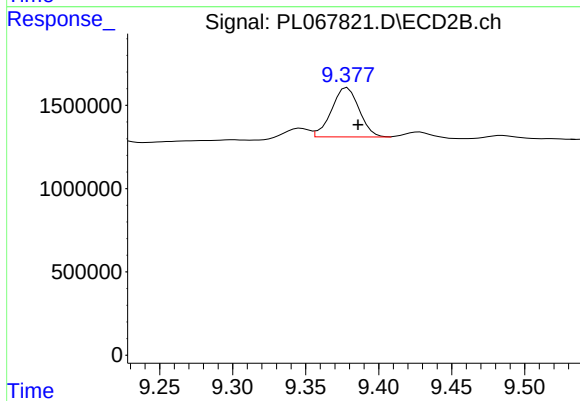

#17 4,4'-DDT

R.T.: 9.377 min
Delta R.T.: -0.009 min
Response: 3866588
Conc: 5.27 ng/ml m

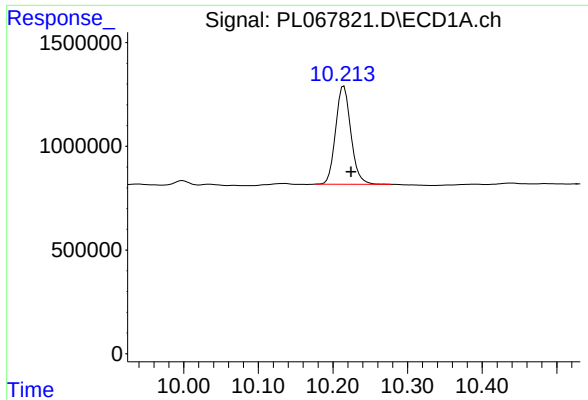


#28 Decachlorobiphenyl

R.T.: 10.215 min
Delta R.T.: -0.010 min
Response: 6739058
Conc: 9.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
15B-STOCKPILE-3A

Manual Integrations
APPROVED

Ankita
6/28/2021 9:29:27 AM

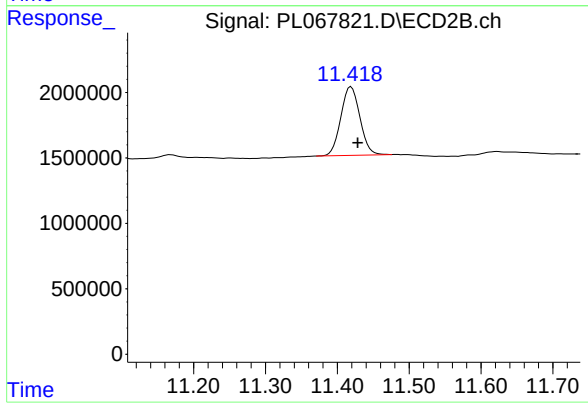

#28 Decachlorobiphenyl

R.T.: 11.419 min
Delta R.T.: -0.009 min
Response: 9652377
Conc: 9.69 ng/ml