

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062523\
 Data File : PL083683.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2023 23:28
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 02:14:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 26 02:14:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	2.692	231.1E6	354.1E6	97.710	100.400
28)	SA Decachlor...	8.973	7.882	152.7E6	229.7E6	93.682	98.150
Target Compounds							
23)	Chlordane-1	4.597	3.697	107.1E6	102.9E6	968.350	1000.423
24)	Chlordane-2	5.130	4.278	111.4E6	112.3E6	937.240	968.090
25)	Chlordane-3	5.843	4.913	500.4E6	359.2E6	997.309	1032.901
26)	Chlordane-4	5.927	4.976	587.8E6	376.3E6	983.018	1035.924
27)	Chlordane-5	6.777	5.875	92176988	103.4E6	989.583	1013.922



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062523\
Data File : PL083683.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2023 23:28
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 02:14:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
Quant Title : GC Extractables
QLast Update : Mon Jun 26 02:14:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

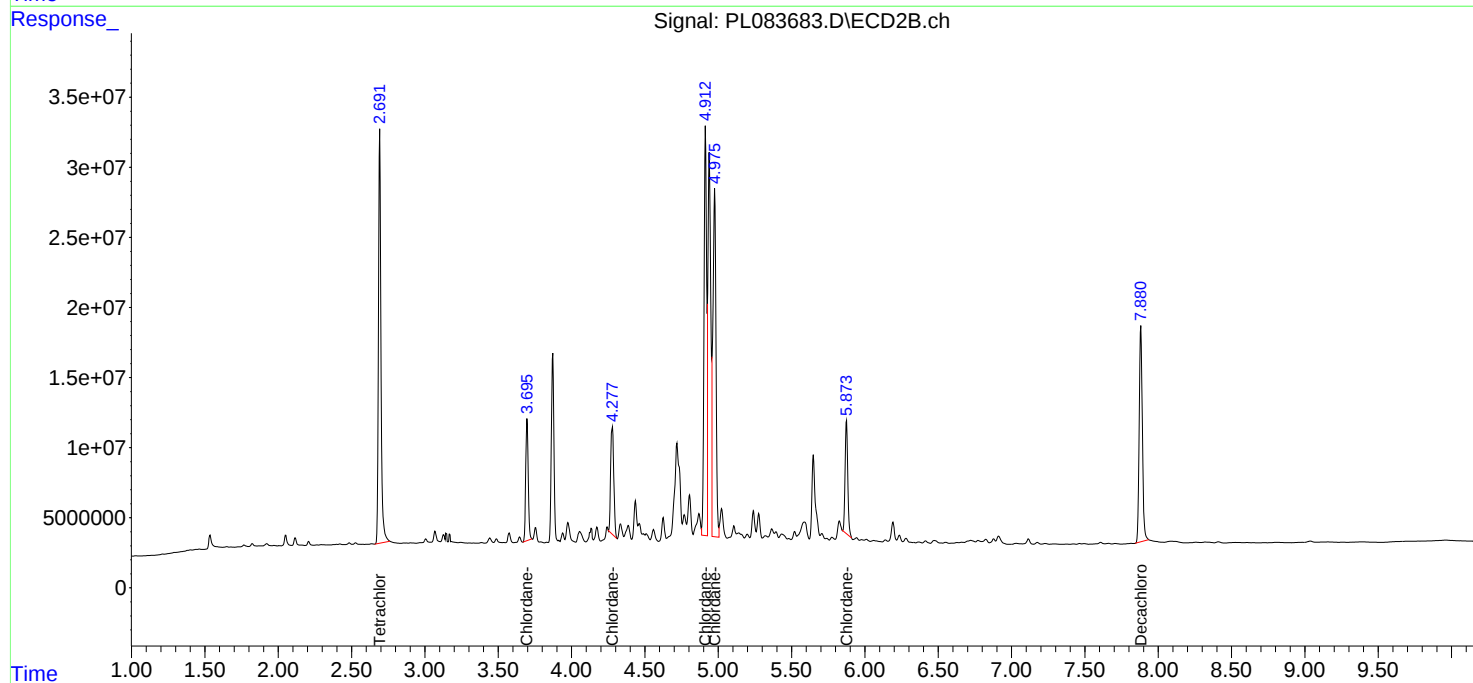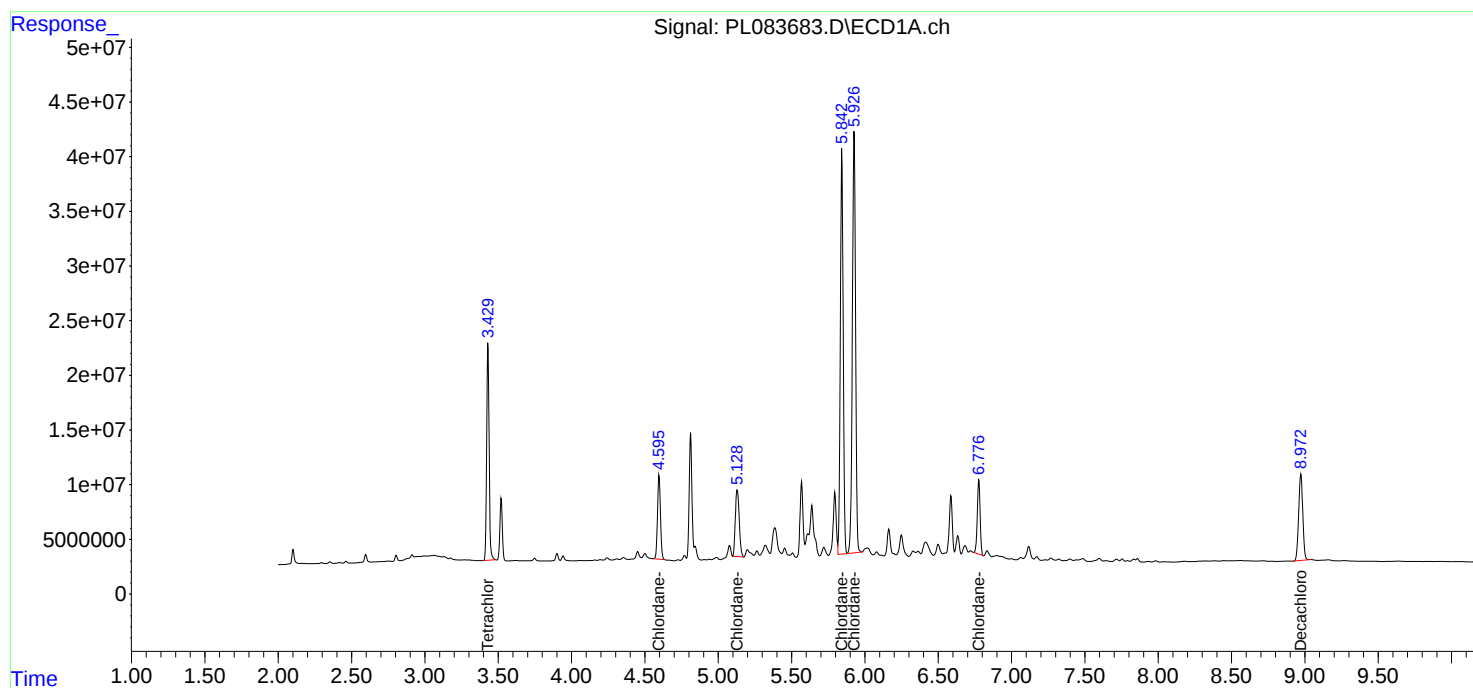


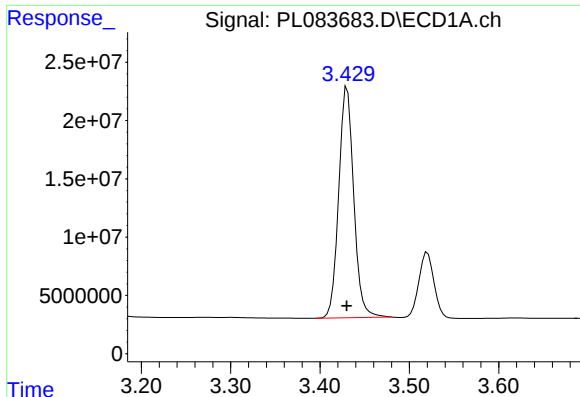

#1 Tetrachloro-m-xylene


R.T.: 3.430 min
Delta R.T.: 0.000 min
Response: 231137387
Conc: 97.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

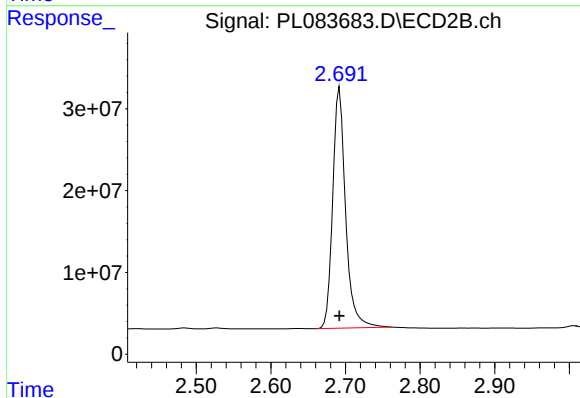


#1 Tetrachloro-m-xylene

R.T.: 2.692 min
Delta R.T.: 0.000 min
Response: 354119626
Conc: 100.40 ng/ml

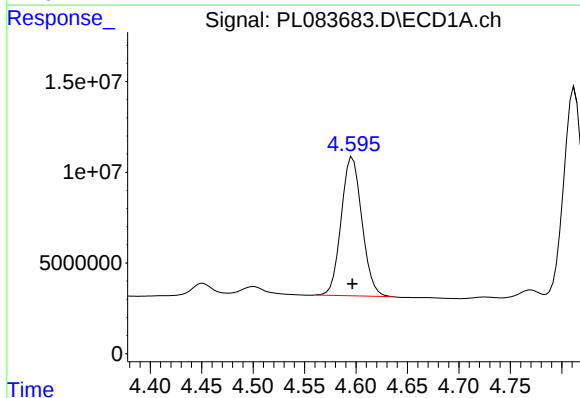


#23 Chlordane-1

R.T.: 4.597 min
Delta R.T.: 0.000 min
Response: 107113964
Conc: 968.35 ng/ml

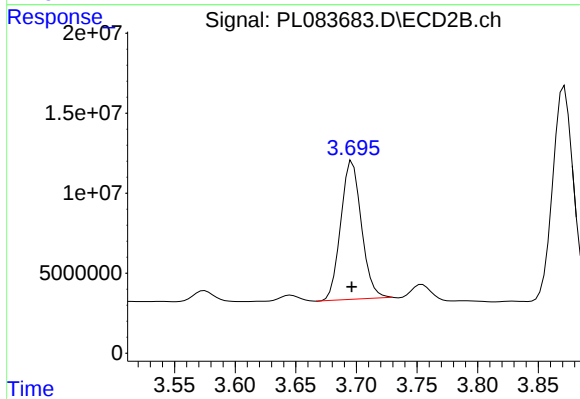

#23 Chlordane-1


R.T.: 3.697 min
Delta R.T.: 0.000 min
Response: 102888714
Conc: 1000.42 ng/ml

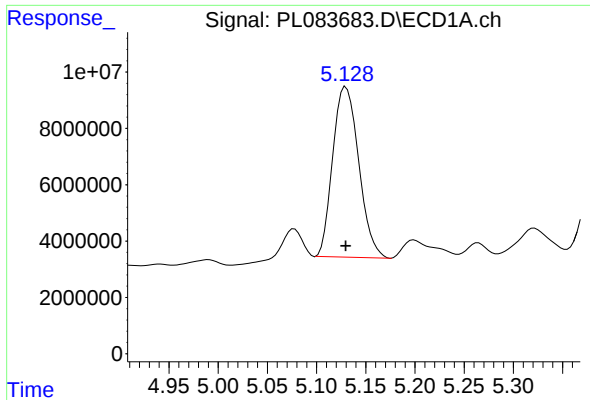

#24 Chlordane-2


R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 111386860
Conc: 937.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

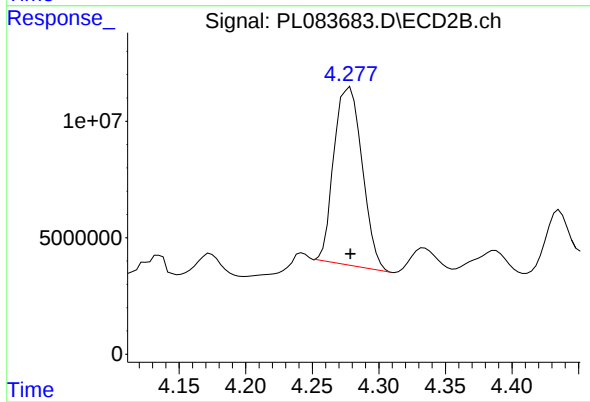


#24 Chlordane-2

R.T.: 4.278 min
Delta R.T.: 0.000 min
Response: 112284944
Conc: 968.09 ng/ml

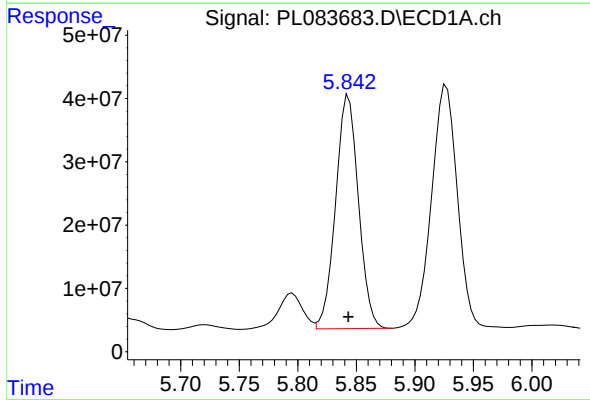


#25 Chlordane-3

R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 500427491
Conc: 997.31 ng/ml

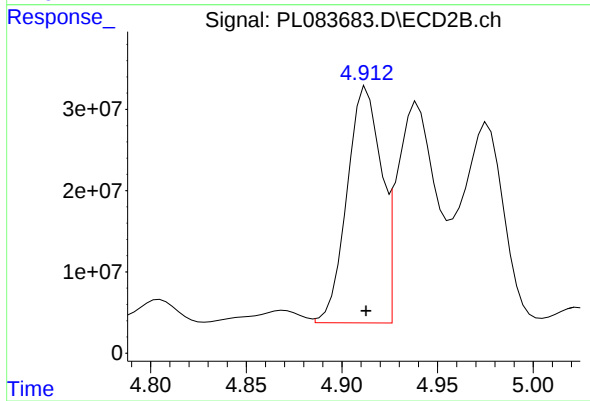

#25 Chlordane-3


R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 359177136
Conc: 1032.90 ng/ml

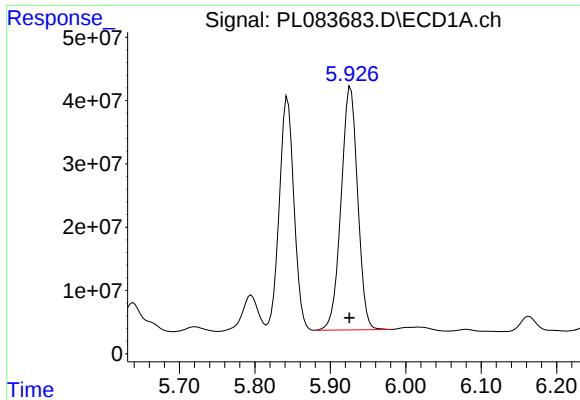

#26 Chlordane-4


R.T.: 5.927 min
Delta R.T.: 0.001 min
Response: 587808639
Conc: 983.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

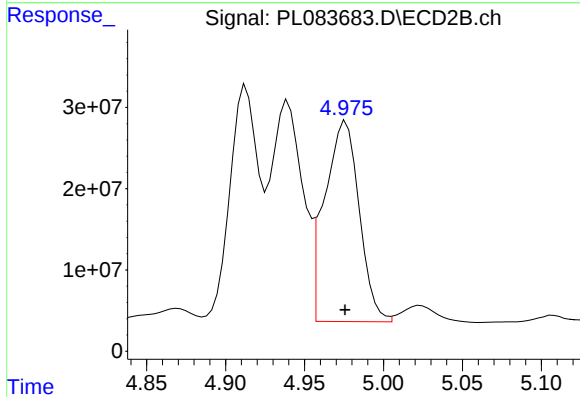


#26 Chlordane-4

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 376339863
Conc: 1035.92 ng/ml

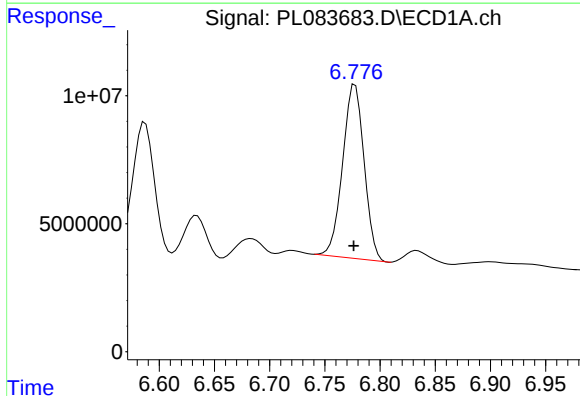


#27 Chlordane-5

R.T.: 6.777 min
Delta R.T.: 0.001 min
Response: 92176988
Conc: 989.58 ng/ml

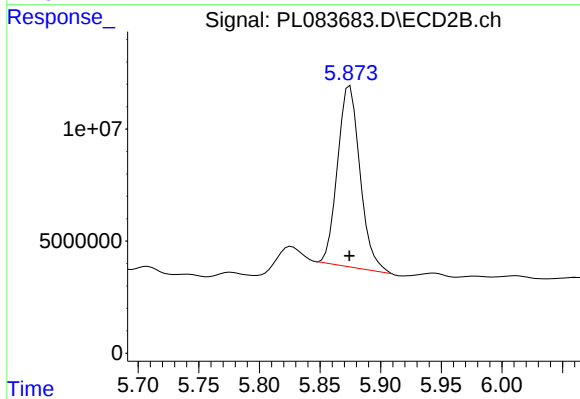

#27 Chlordane-5


R.T.: 5.875 min
Delta R.T.: 0.000 min
Response: 103442118
Conc: 1013.92 ng/ml

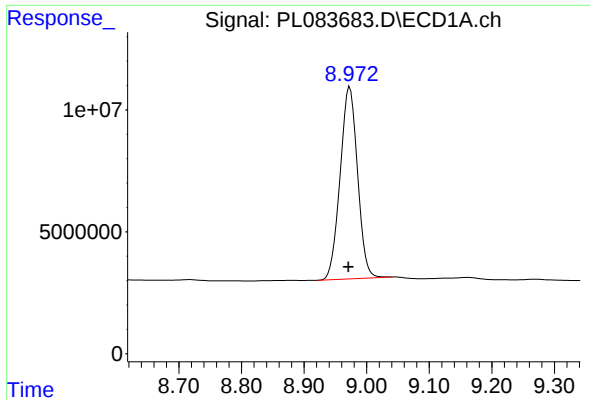

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: 0.002 min
Response: 152723361
Conc: 93.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

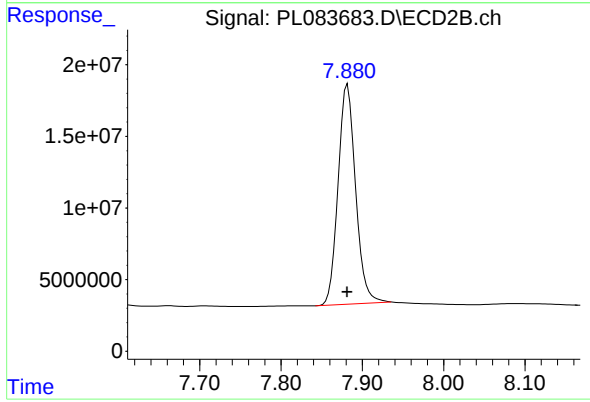

#28 Decachlorobiphenyl

R.T.: 7.882 min
Delta R.T.: 0.000 min
Response: 229665732
Conc: 98.15 ng/ml