

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062523\
 Data File : PL083684.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2023 23:42
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 02:14:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 26 02:14:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	2.692	168.1E6	256.7E6	71.043	72.789
28)	SA Decachlor...	8.972	7.882	113.9E6	166.4E6	69.875	71.102
Target Compounds							
23)	Chlordane-1	4.597	3.697	78018392	74233278	705.316	721.796
24)	Chlordane-2	5.130	4.279	82327506	81383941	692.727	701.670
25)	Chlordane-3	5.843	4.913	360.0E6	258.0E6	717.369	742.014
26)	Chlordane-4	5.927	4.976	426.2E6	266.0E6	712.709	732.230
27)	Chlordane-5	6.777	5.874	65351249	74824107	701.591	733.413



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062523\
Data File : PL083684.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2023 23:42
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 02:14:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
Quant Title : GC Extractables
QLast Update : Mon Jun 26 02:14:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

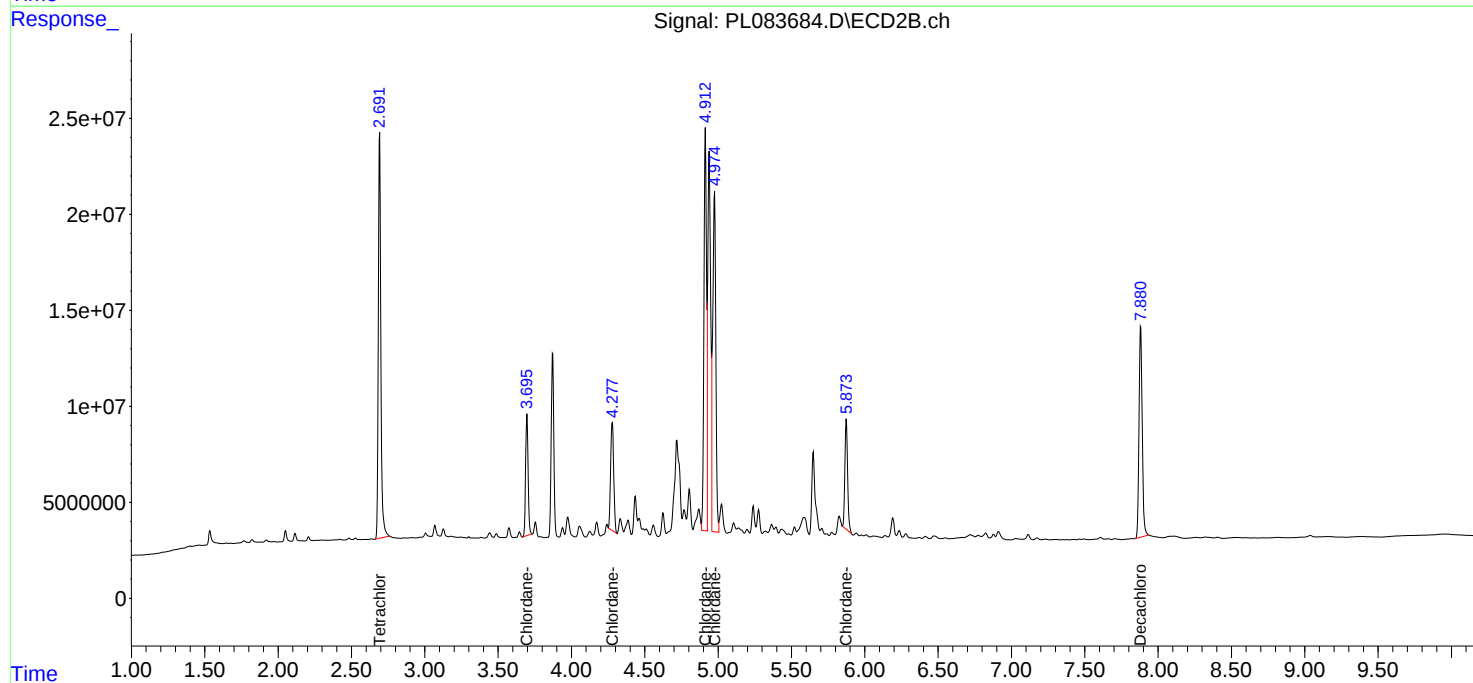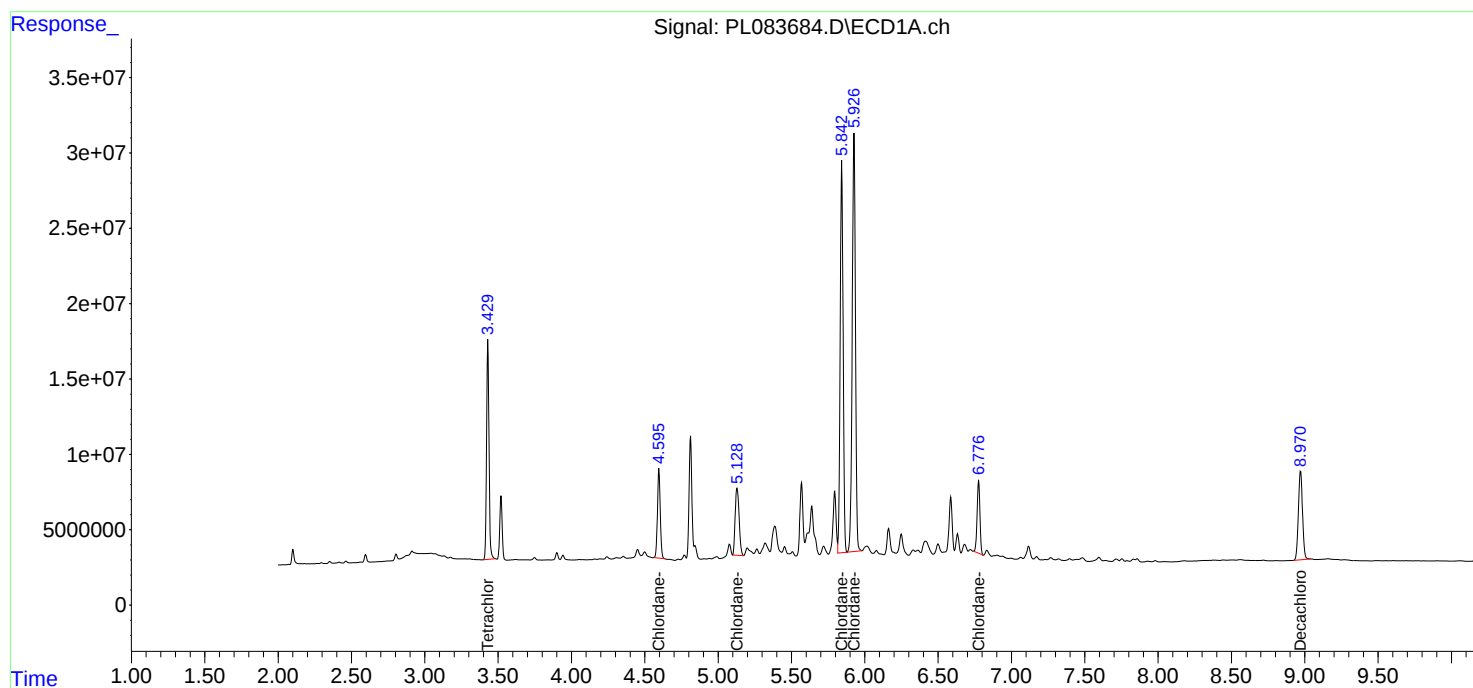


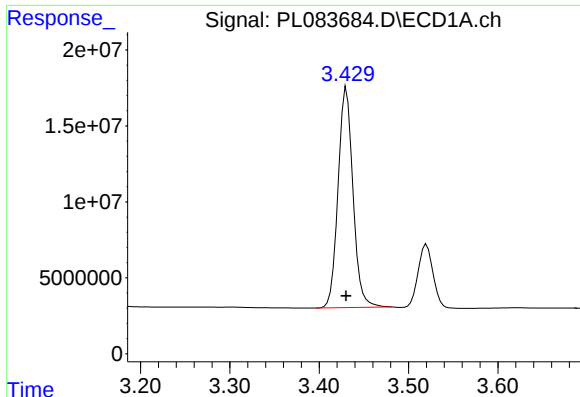

#1 Tetrachloro-m-xylene


R.T.: 3.431 min
Delta R.T.: 0.000 min
Response: 168055829
Conc: 71.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

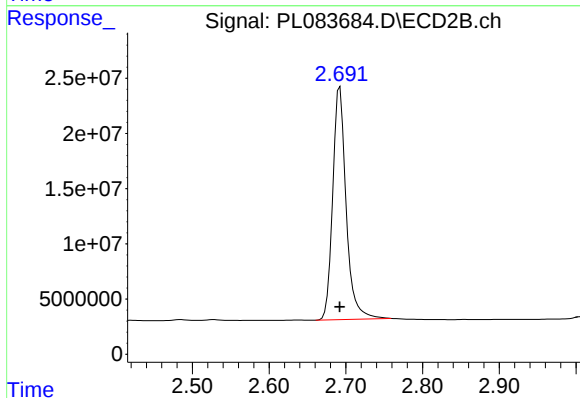


#1 Tetrachloro-m-xylene

R.T.: 2.692 min
Delta R.T.: 0.000 min
Response: 256734234
Conc: 72.79 ng/ml

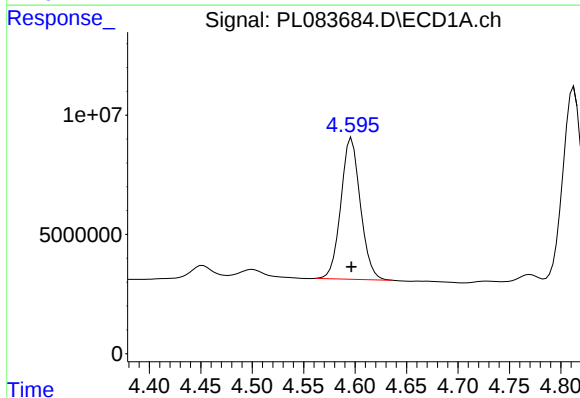


#23 Chlordane-1

R.T.: 4.597 min
Delta R.T.: 0.000 min
Response: 78018392
Conc: 705.32 ng/ml

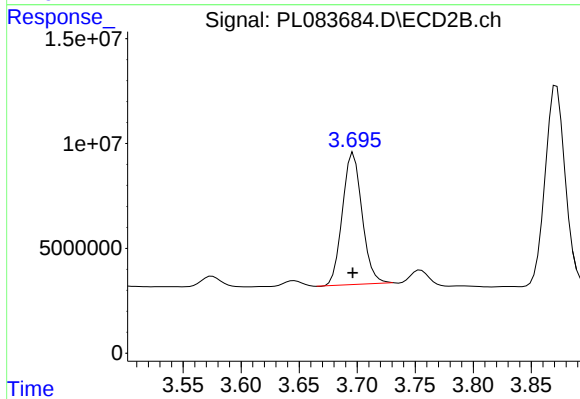

#23 Chlordane-1


R.T.: 3.697 min
Delta R.T.: 0.000 min
Response: 74233278
Conc: 721.80 ng/ml

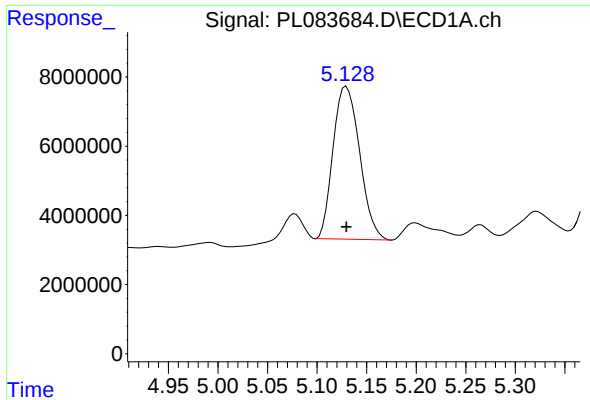

#24 Chlordane-2


R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 82327506
Conc: 692.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

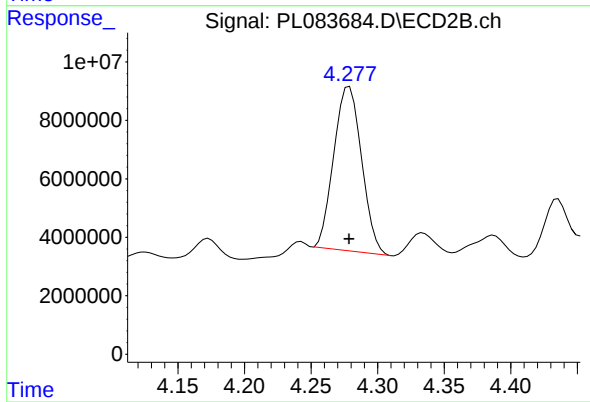


#24 Chlordane-2

R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 81383941
Conc: 701.67 ng/ml

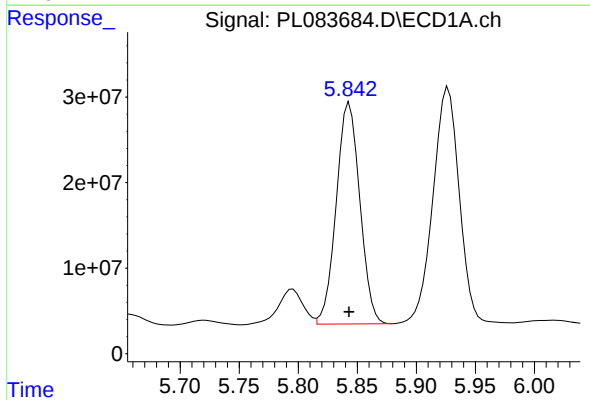


#25 Chlordane-3

R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 359959709
Conc: 717.37 ng/ml

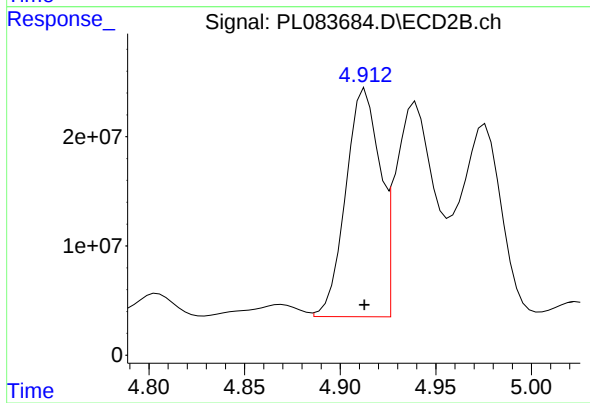

#25 Chlordane-3


R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 258025046
Conc: 742.01 ng/ml

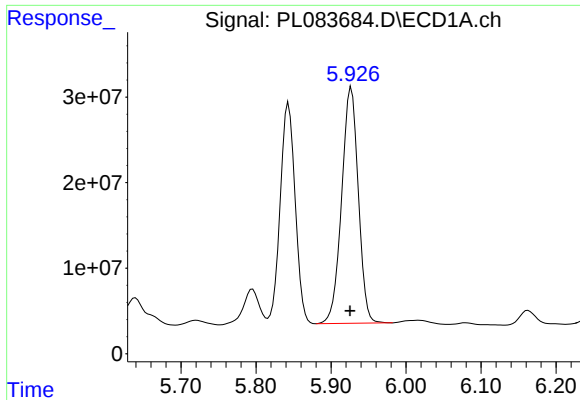

#26 Chlordane-4


R.T.: 5.927 min
Delta R.T.: 0.002 min
Response: 426173756
Conc: 712.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

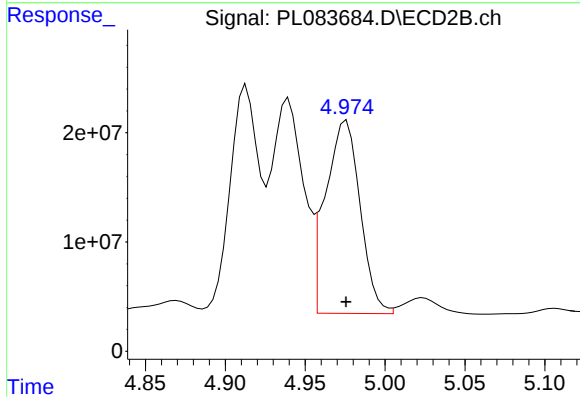


#26 Chlordane-4

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 266011266
Conc: 732.23 ng/ml

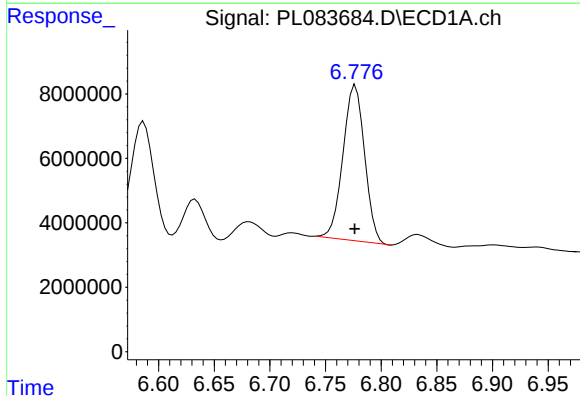


#27 Chlordane-5

R.T.: 6.777 min
Delta R.T.: 0.000 min
Response: 65351249
Conc: 701.59 ng/ml

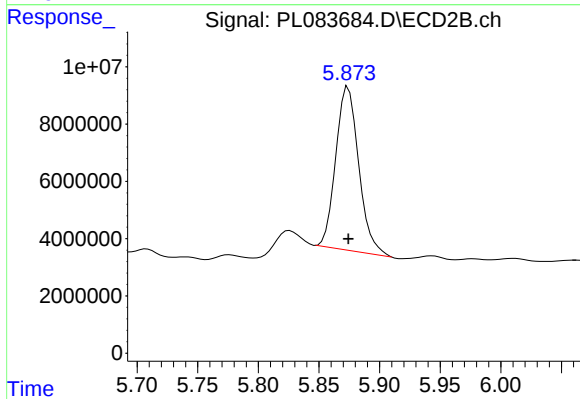

#27 Chlordane-5


R.T.: 5.874 min
Delta R.T.: 0.000 min
Response: 74824107
Conc: 733.41 ng/ml

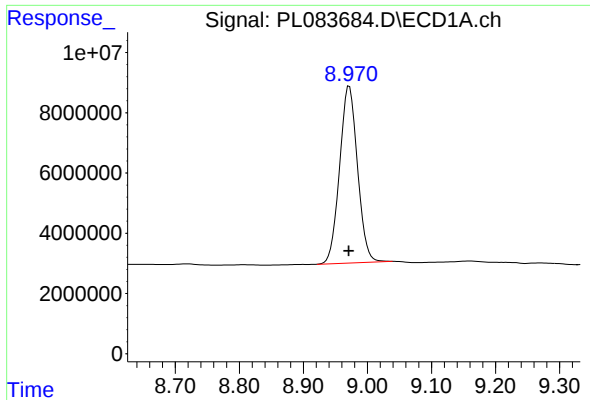

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: 0.001 min
Response: 113913487
Conc: 69.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

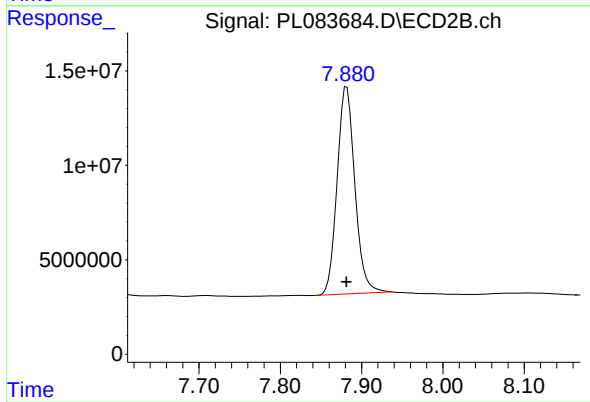

#28 Decachlorobiphenyl

R.T.: 7.882 min
Delta R.T.: 0.000 min
Response: 166373920
Conc: 71.10 ng/ml