

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062523\
 Data File : PL083685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2023 23:56
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 02:15:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 26 02:14:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	2.692	118.3E6	176.4E6	50.000	50.000
28)	SA Decachlor...	8.971	7.881	81511938	117.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.596	3.696	55307435	51422598	500.000	500.000
24)	Chlordane-2	5.130	4.279	59422794	57993042	500.000	500.000
25)	Chlordane-3	5.843	4.913	250.9E6	173.9E6	500.000	500.000
26)	Chlordane-4	5.925	4.976	299.0E6	181.6E6	500.000	500.000
27)	Chlordane-5	6.776	5.874	46573629	51010881	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062523\
Data File : PL083685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2023 23:56
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 02:15:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
Quant Title : GC Extractables
QLast Update : Mon Jun 26 02:14:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

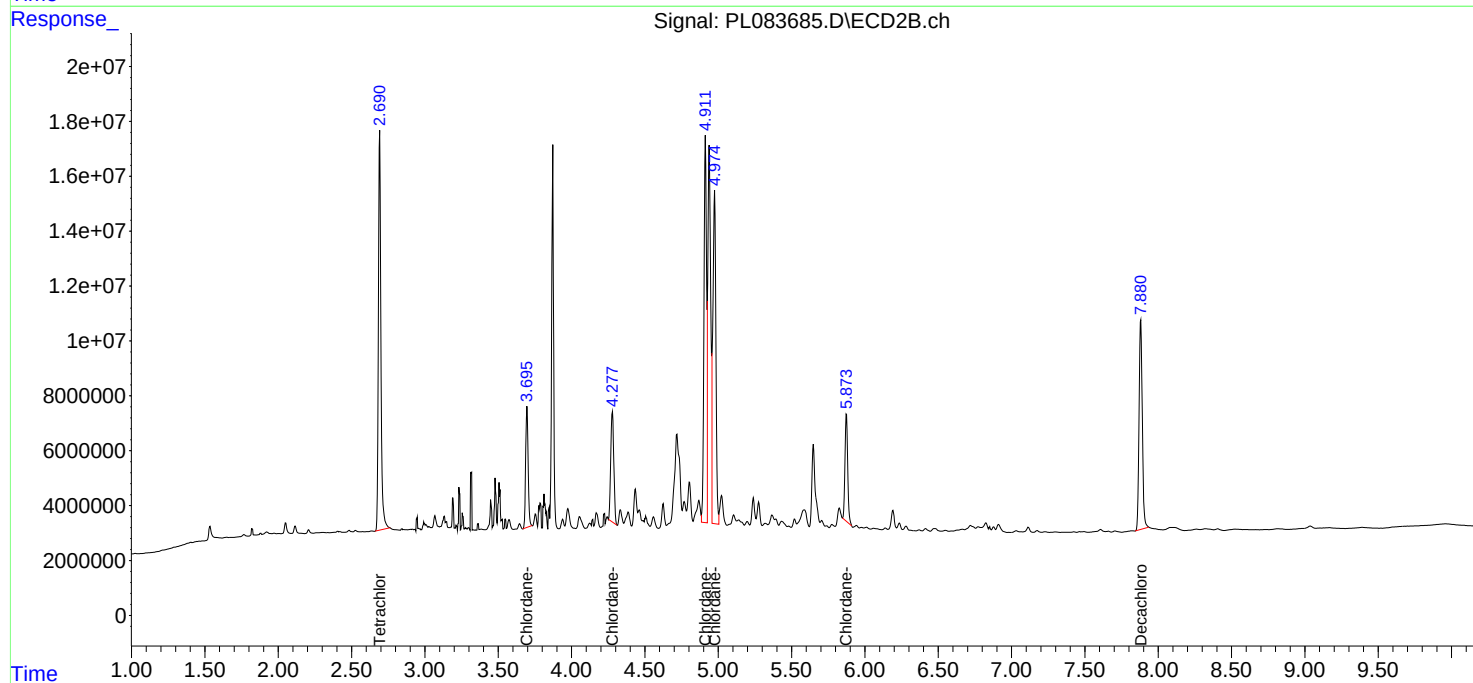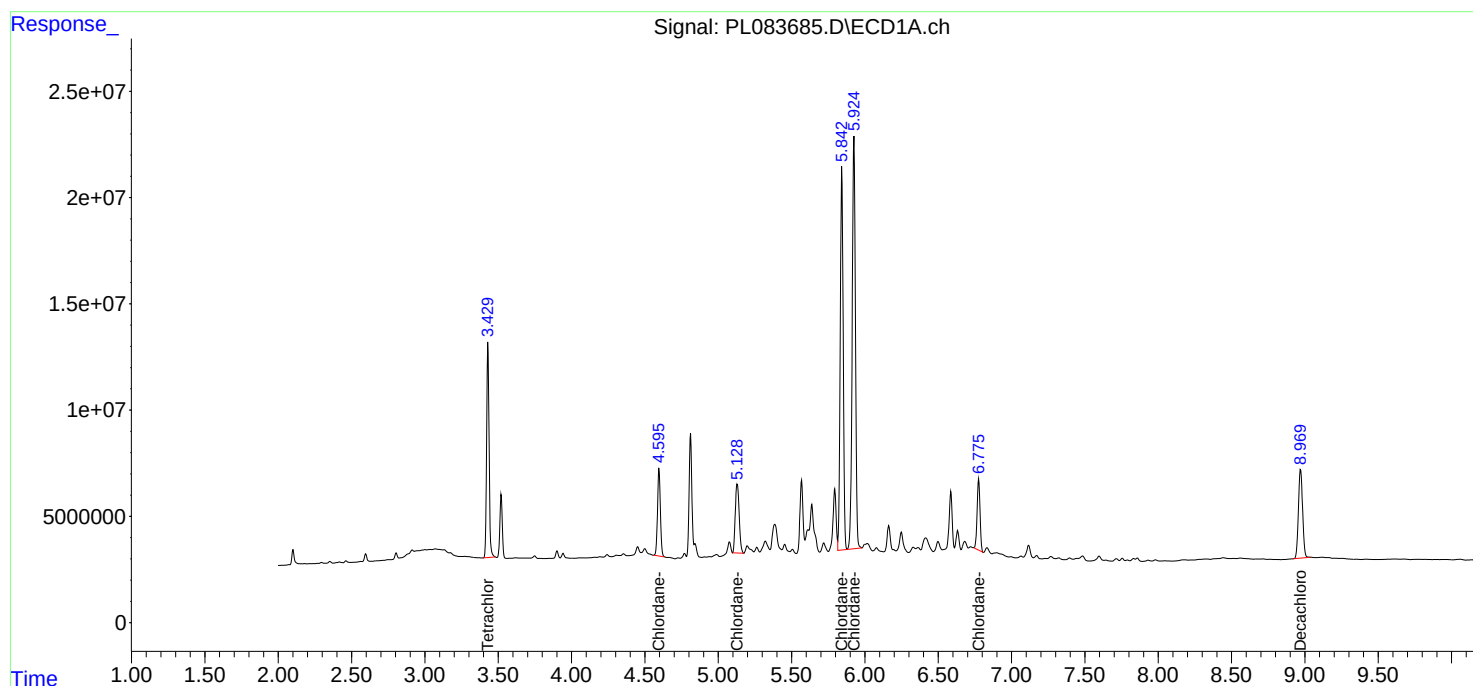


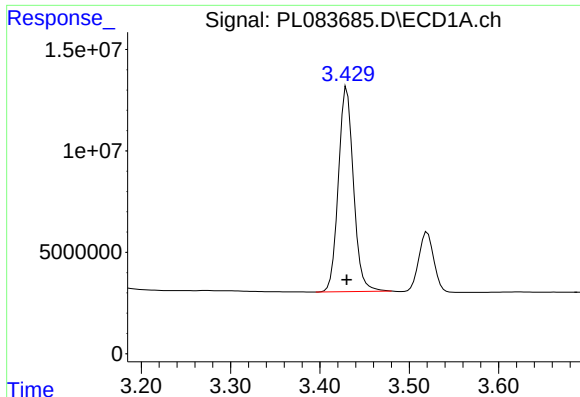

#1 Tetrachloro-m-xylene


R.T.: 3.430 min
Delta R.T.: 0.000 min
Response: 118277128
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

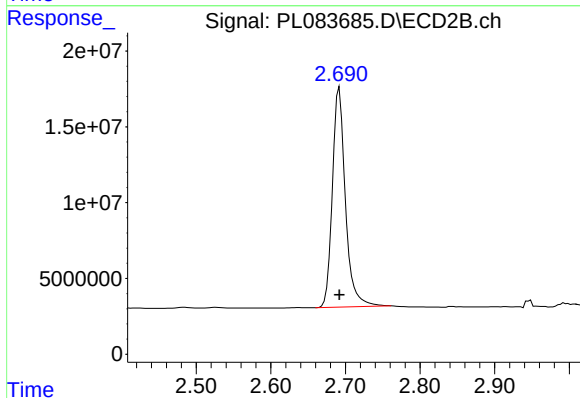


#1 Tetrachloro-m-xylene

R.T.: 2.692 min
Delta R.T.: 0.000 min
Response: 176354380
Conc: 50.00 ng/ml

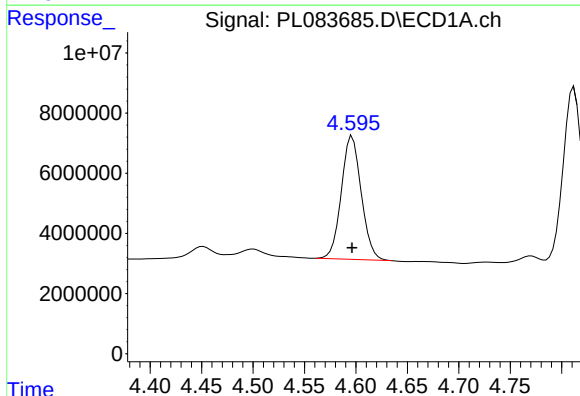


#23 Chlordane-1

R.T.: 4.596 min
Delta R.T.: 0.000 min
Response: 55307435
Conc: 500.00 ng/ml

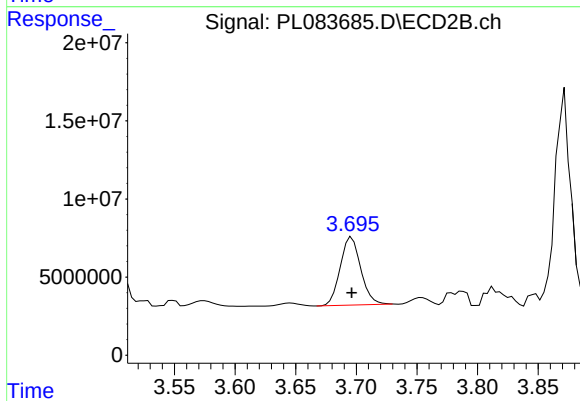

#23 Chlordane-1


R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 51422598
Conc: 500.00 ng/ml

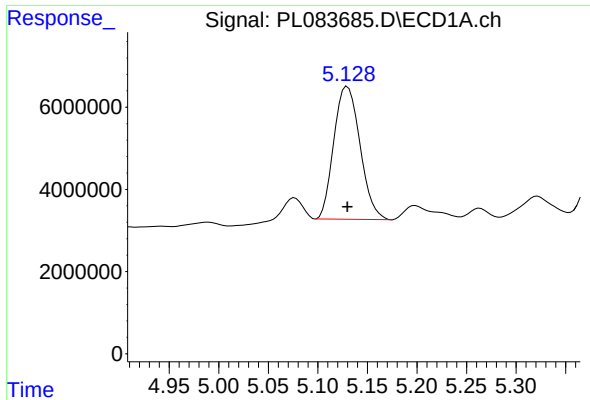

#24 Chlordane-2


R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 59422794
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

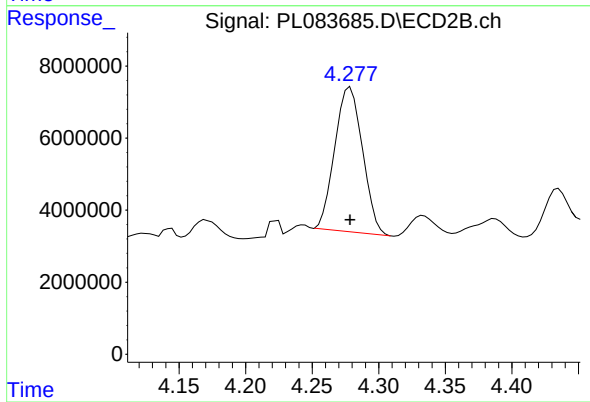


#24 Chlordane-2

R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 57993042
Conc: 500.00 ng/ml

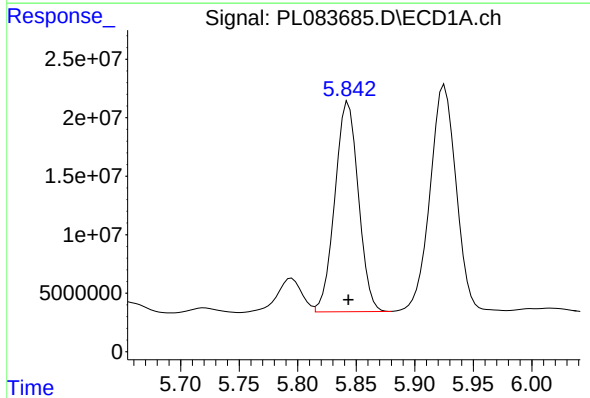


#25 Chlordane-3

R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 250888844
Conc: 500.00 ng/ml

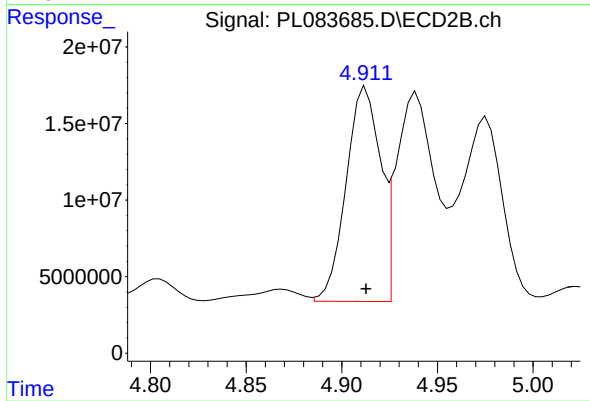

#25 Chlordane-3


R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 173868152
Conc: 500.00 ng/ml

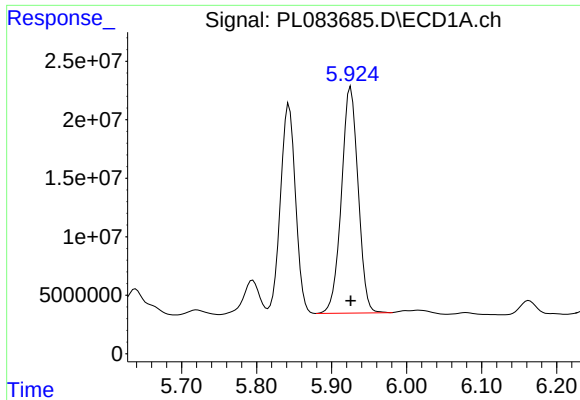

#26 Chlordane-4


R.T.: 5.925 min
Delta R.T.: 0.000 min
Response: 298981712
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

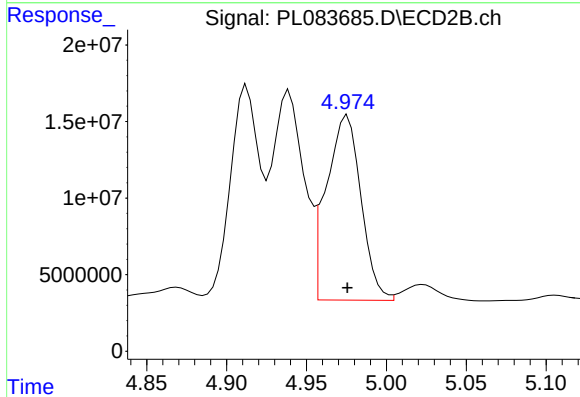


#26 Chlordane-4

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 181644495
Conc: 500.00 ng/ml

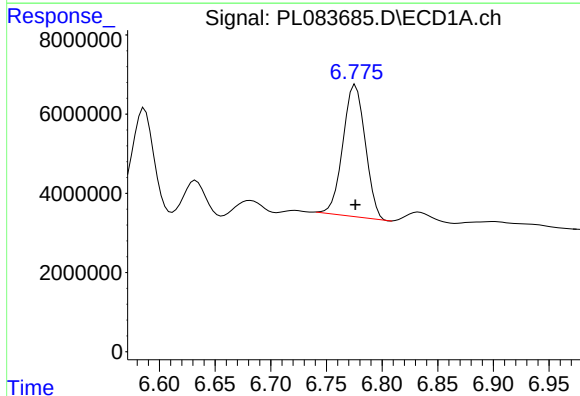


#27 Chlordane-5

R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 46573629
Conc: 500.00 ng/ml

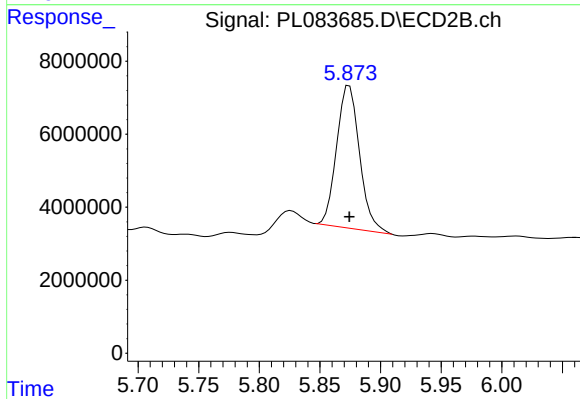

#27 Chlordane-5


R.T.: 5.874 min
Delta R.T.: 0.000 min
Response: 51010881
Conc: 500.00 ng/ml

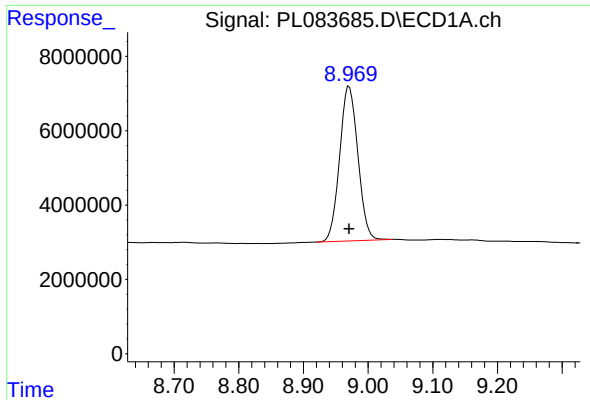

#28 Decachlorobiphenyl

R.T.: 8.971 min
Delta R.T.: 0.000 min
Response: 81511938
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

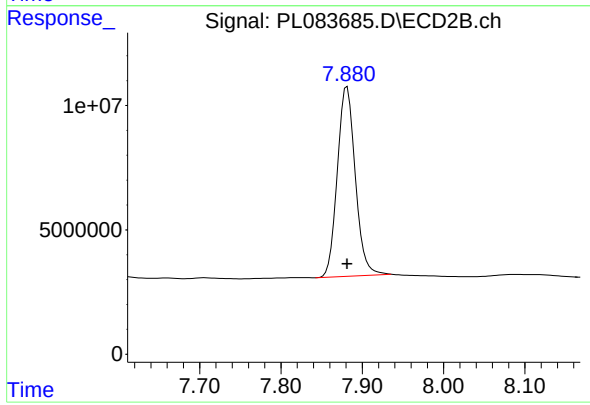

#28 Decachlorobiphenyl

R.T.: 7.881 min
Delta R.T.: 0.000 min
Response: 116996776
Conc: 50.00 ng/ml