

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062523\
 Data File : PL083686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2023 00:09
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 02:15:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 26 02:14:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	2.692	55515699	83345658	23.468	23.630
28)	SA Decachlor...	8.971	7.881	40709056	56022725	24.971	23.942
Target Compounds							
23)	Chlordane-1	4.595	3.696	25872979	24406750	233.901	237.315
24)	Chlordane-2	5.129	4.278	29373204	34612430	247.154	298.419
25)	Chlordane-3	5.842	4.913	116.9E6	80591928	233.028	231.762
26)	Chlordane-4	5.925	4.976	143.2E6	83048095	239.437	228.601
27)	Chlordane-5	6.775	5.874	21901543	23902139	235.128	234.285



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062523\
Data File : PL083686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2023 00:09
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 02:15:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
Quant Title : GC Extractables
QLast Update : Mon Jun 26 02:14:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

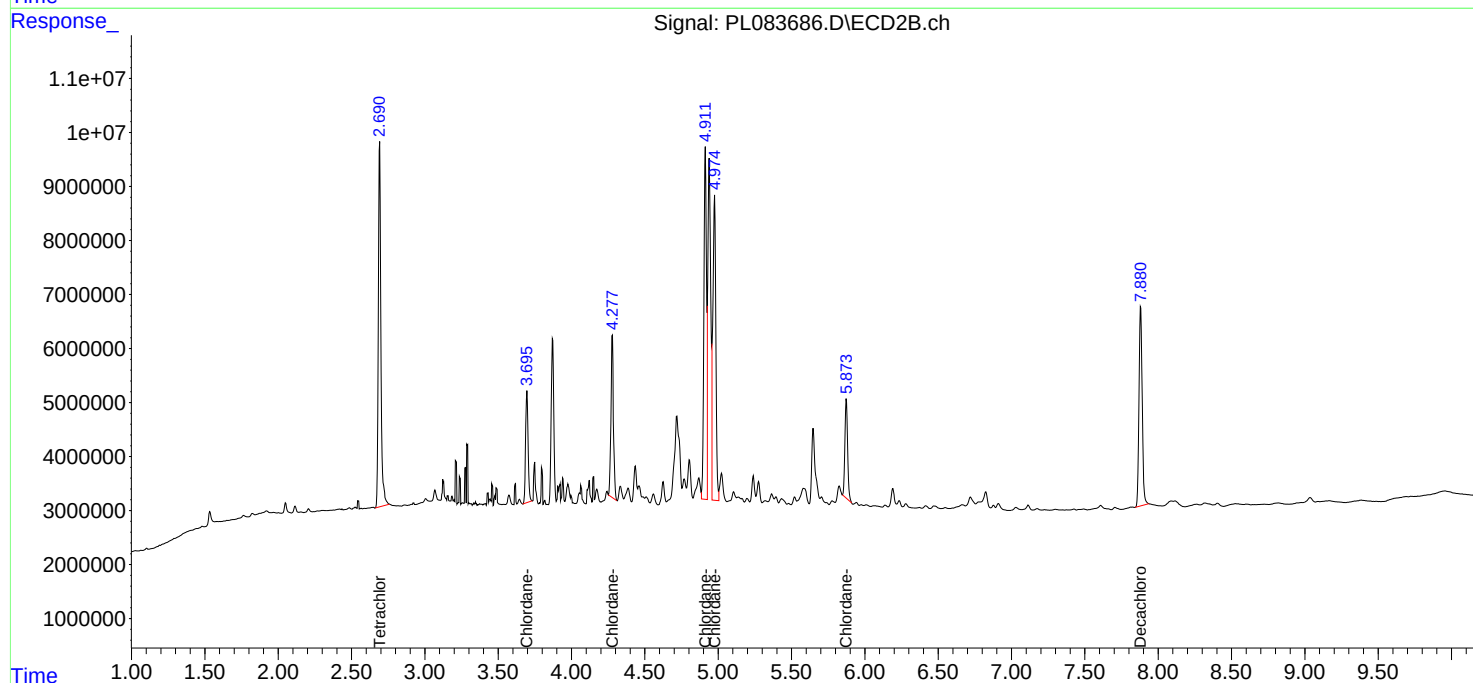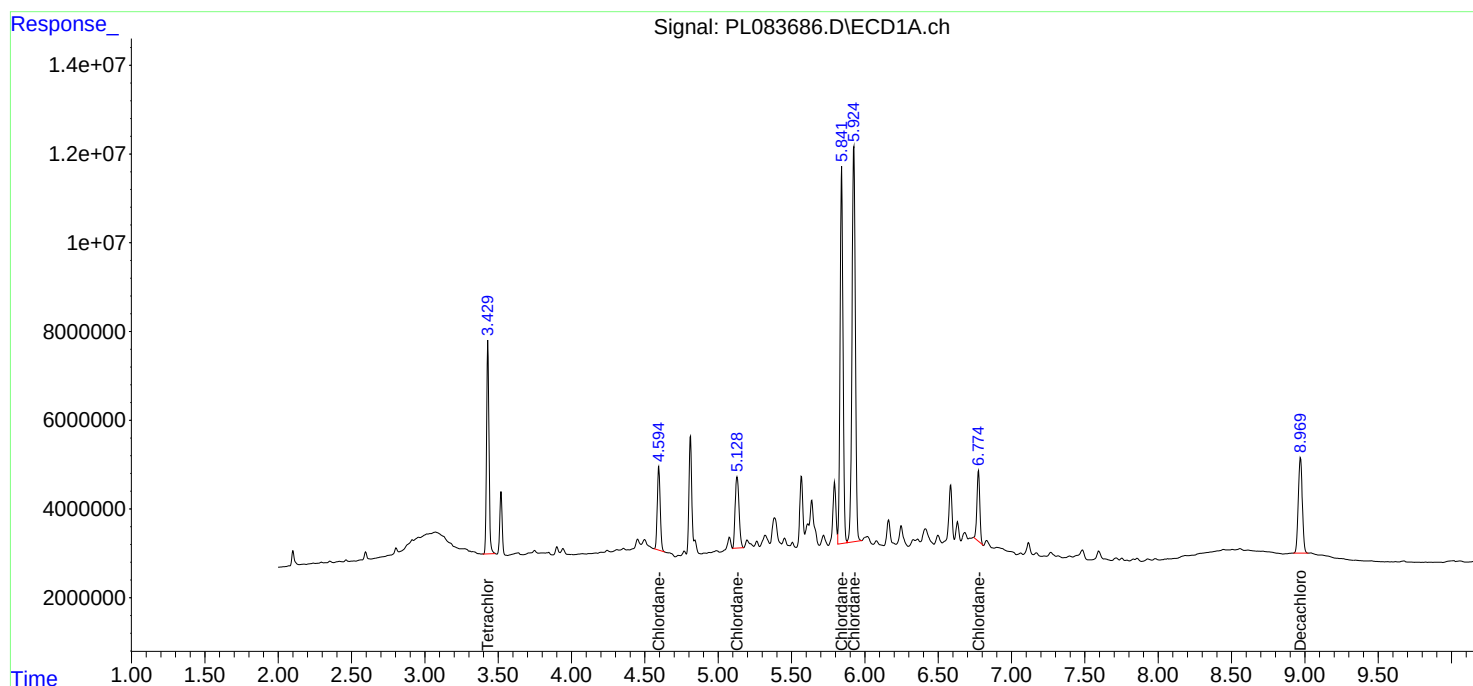


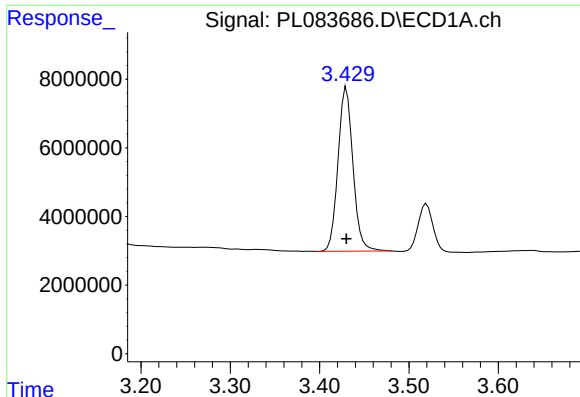

#1 Tetrachloro-m-xylene


R.T.: 3.430 min
Delta R.T.: 0.000 min
Response: 55515699
Conc: 23.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

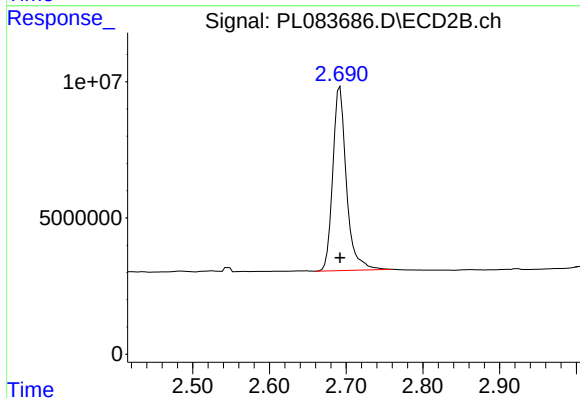


#1 Tetrachloro-m-xylene

R.T.: 2.692 min
Delta R.T.: 0.000 min
Response: 83345658
Conc: 23.63 ng/ml

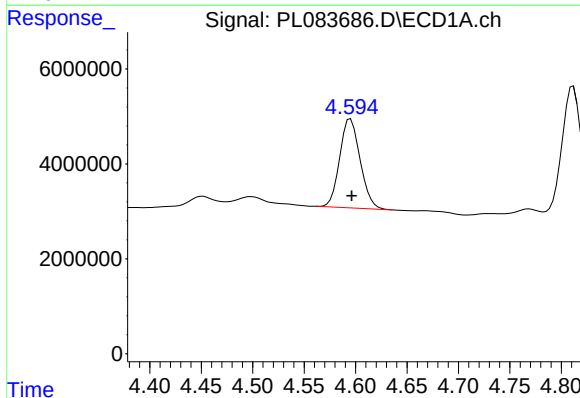


#23 Chlordane-1

R.T.: 4.595 min
Delta R.T.: -0.001 min
Response: 25872979
Conc: 233.90 ng/ml

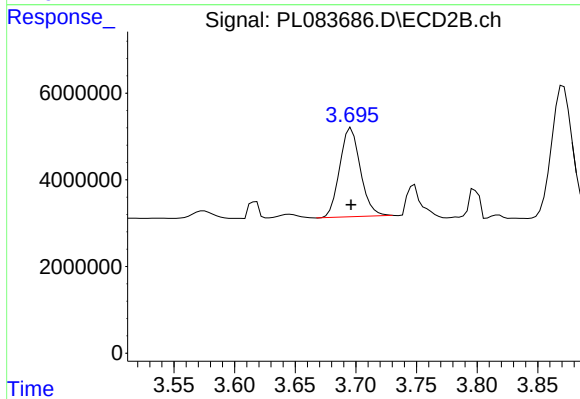

#23 Chlordane-1


R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 24406750
Conc: 237.32 ng/ml

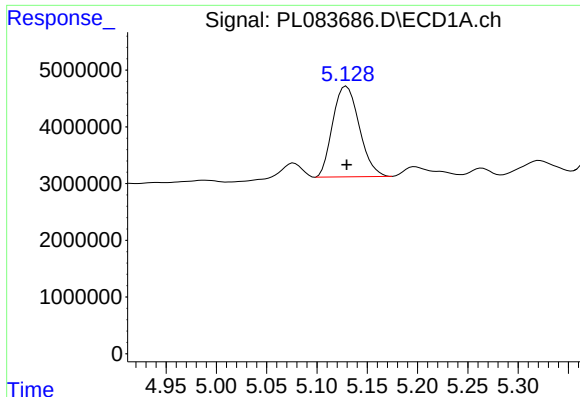

#24 Chlordane-2


R.T.: 5.129 min
Delta R.T.: 0.000 min
Response: 29373204
Conc: 247.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

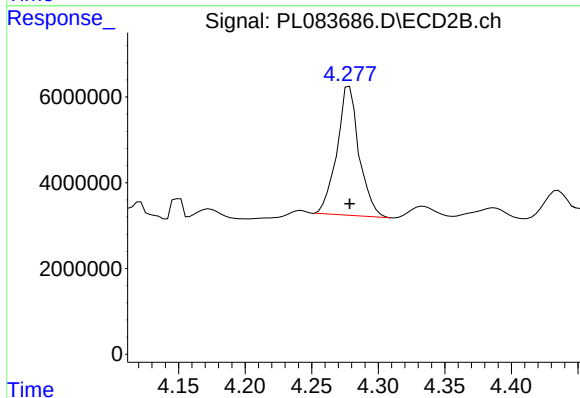


#24 Chlordane-2

R.T.: 4.278 min
Delta R.T.: 0.000 min
Response: 34612430
Conc: 298.42 ng/ml

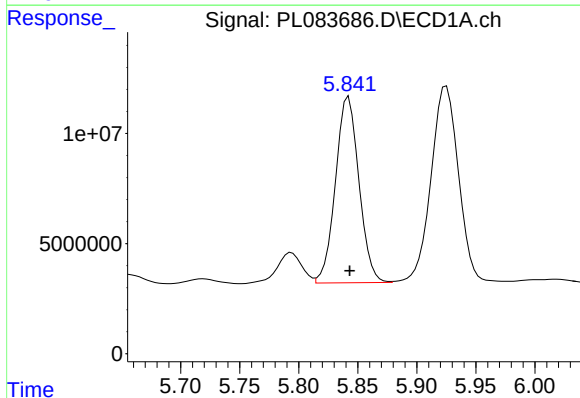


#25 Chlordane-3

R.T.: 5.842 min
Delta R.T.: 0.000 min
Response: 116928142
Conc: 233.03 ng/ml

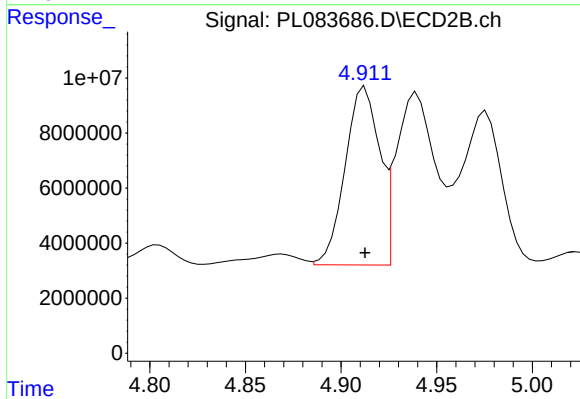

#25 Chlordane-3


R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 80591928
Conc: 231.76 ng/ml

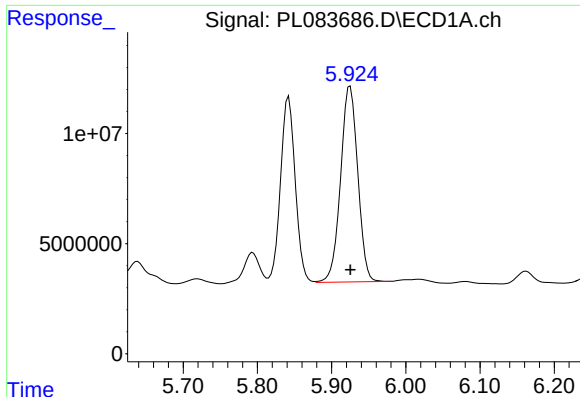

#26 Chlordane-4


R.T.: 5.925 min
Delta R.T.: 0.000 min
Response: 143174753
Conc: 239.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

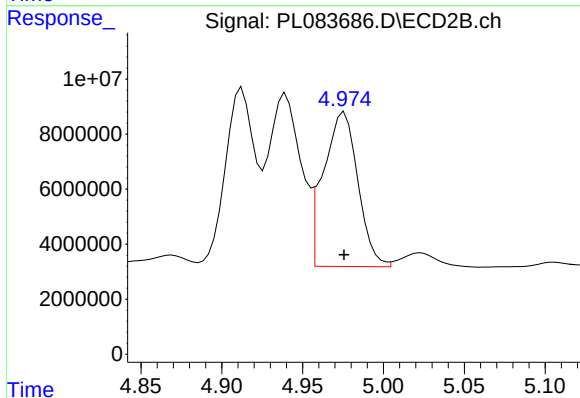


#26 Chlordane-4

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 83048095
Conc: 228.60 ng/ml

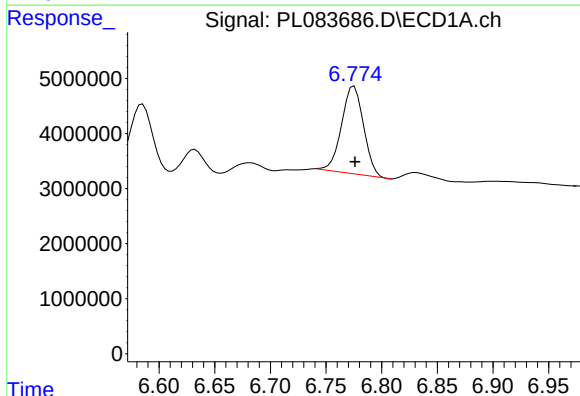


#27 Chlordane-5

R.T.: 6.775 min
Delta R.T.: 0.000 min
Response: 21901543
Conc: 235.13 ng/ml

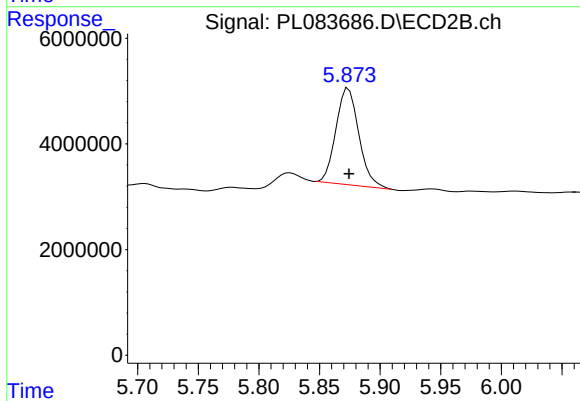

#27 Chlordane-5


R.T.: 5.874 min
Delta R.T.: 0.000 min
Response: 23902139
Conc: 234.28 ng/ml

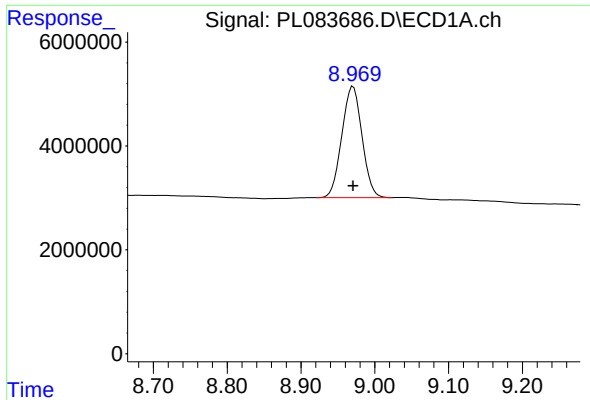

#28 Decachlorobiphenyl

R.T.: 8.971 min
Delta R.T.: 0.000 min
Response: 40709056
Conc: 24.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

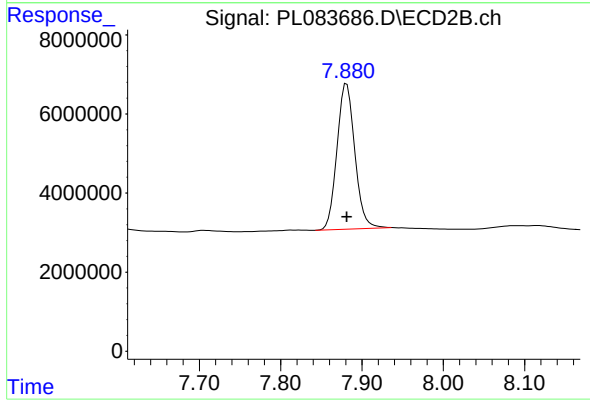

#28 Decachlorobiphenyl

R.T.: 7.881 min
Delta R.T.: 0.000 min
Response: 56022725
Conc: 23.94 ng/ml