

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
 Data File : PL037421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 13:51
 Operator : UA\AJ
 Sample : J3251-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 05:11:52 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.936	90032220	30972910	11.382	11.195
28)	SA Decachlor...	8.014	8.946	72655528	23224506	12.041	11.706
Target Compounds							
6)	B beta-BHC	4.253f	0.000	9049974	0	1.984	N.D. #
10)	B gamma-Chl...	5.248	0.000	15879588	0	1.695	N.D. #
11)	B alpha-Chl...	5.248f	0.000	15879588	0	1.749	N.D. #
12)	B 4,4'-DDE	5.454	6.249	35175336	9227093	3.982	3.626
17)	MA 4,4'-DDT	6.199	0.000	7736857	0	1.198	N.D. #
23)	Chlordane-1	4.116	0.000	15027292	0	48.941	N.D. #
25)	Chlordane-3	5.248	0.000	15879588	0	14.940	N.D. #
26)	Chlordane-4	5.248	0.000	15879588	0	16.481	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
Data File : PL037421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 13:51
Operator : UA\AJ
Sample : J3251-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 05:11:52 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

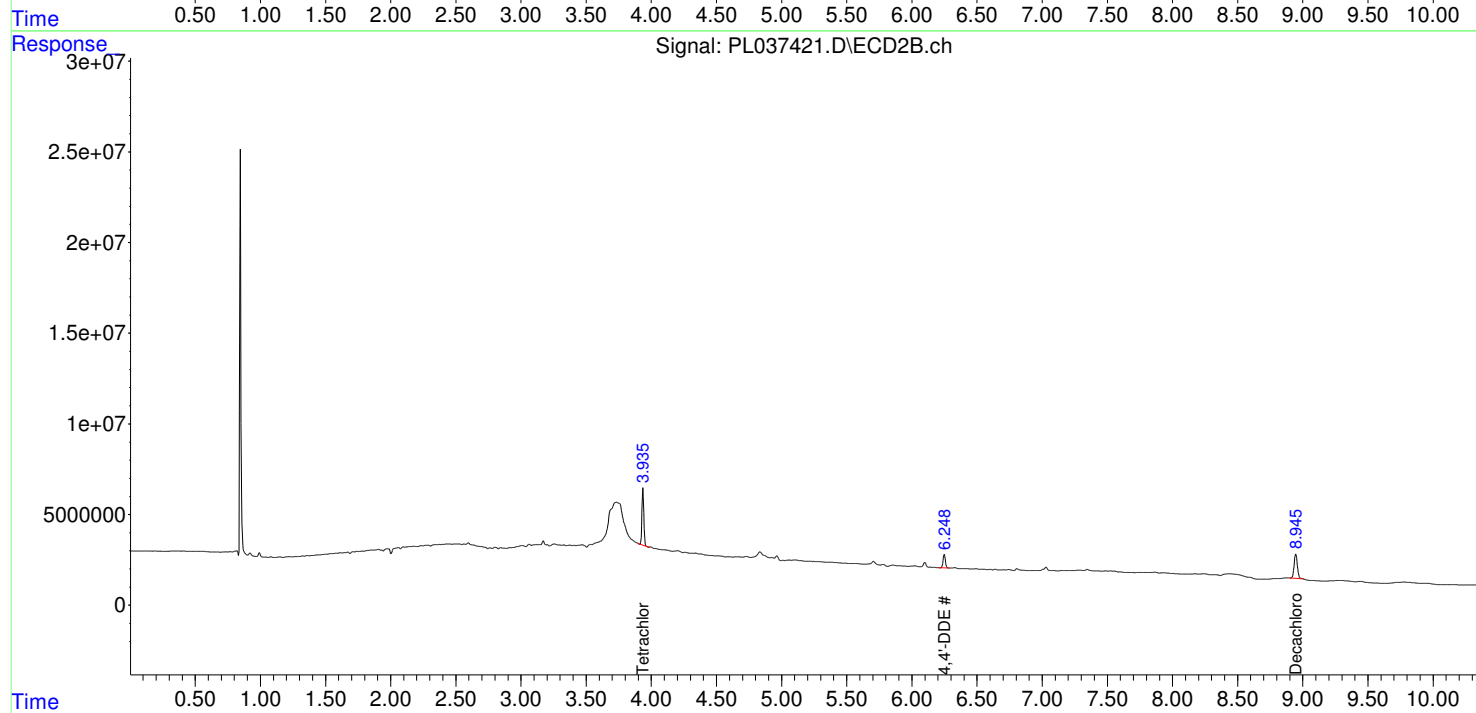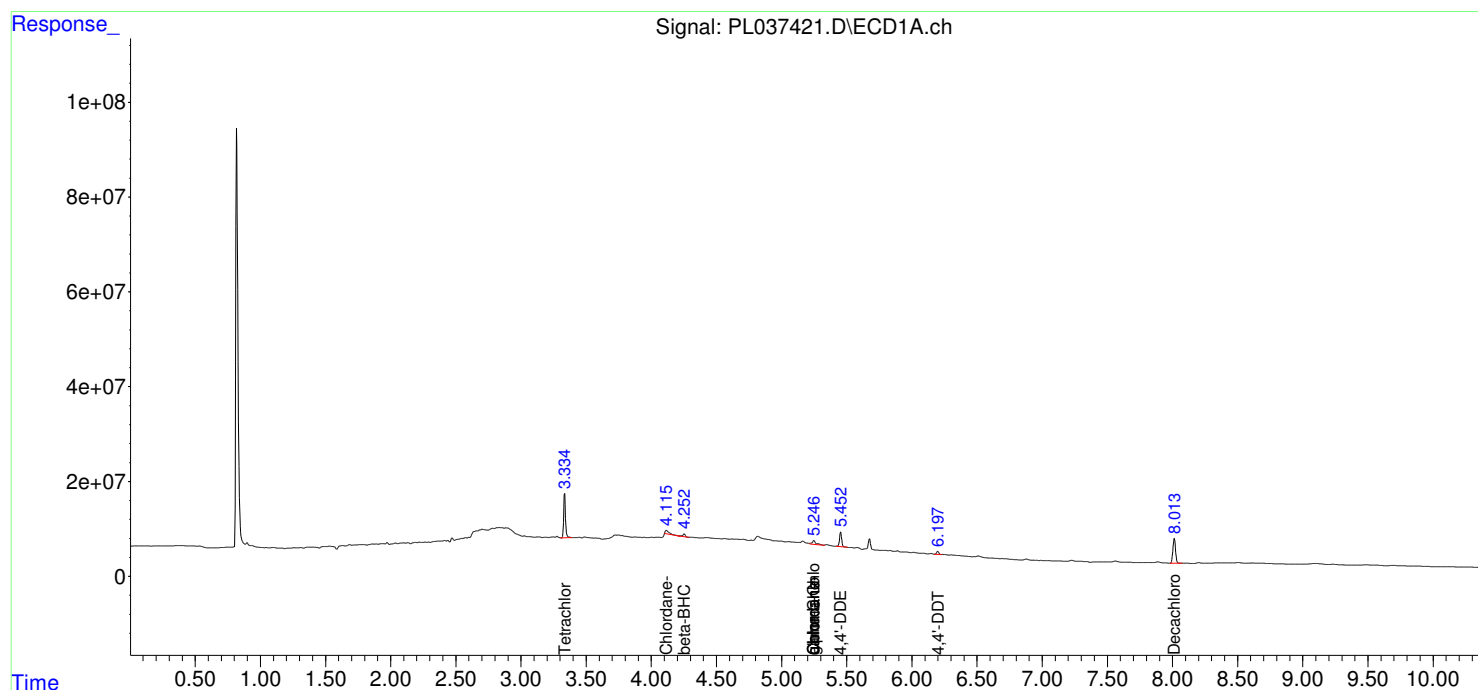


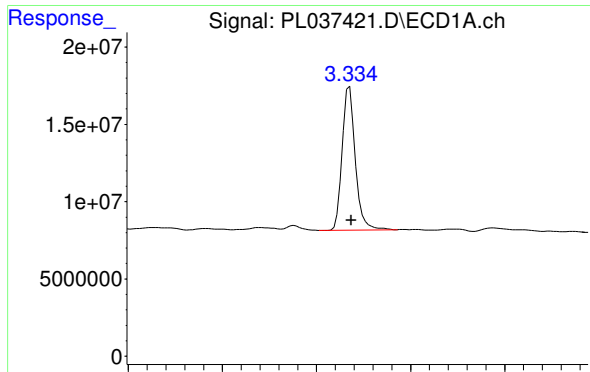

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 90032220
Conc: 11.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

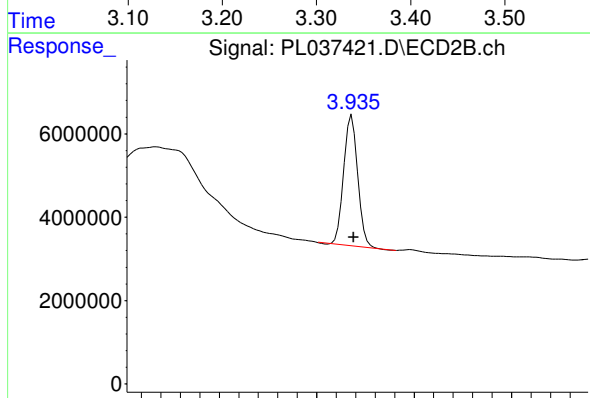


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 30972910
Conc: 11.19 ng/ml

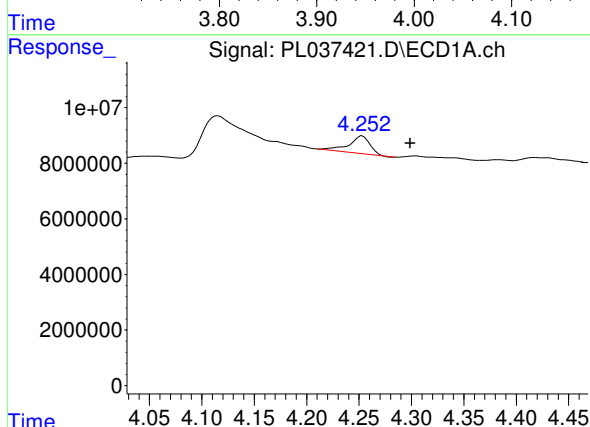


#6 beta-BHC

R.T.: 4.253 min
Delta R.T.: -0.045 min
Response: 9049974
Conc: 1.98 ng/ml

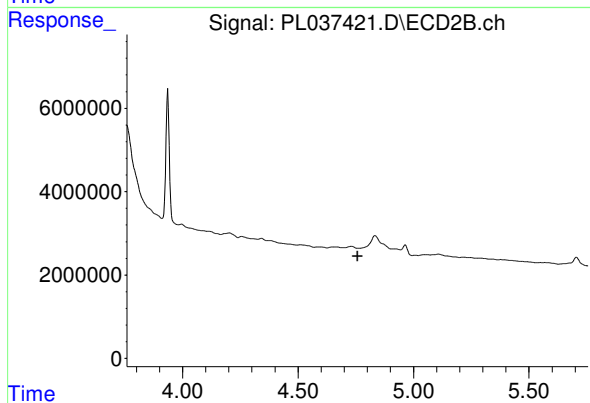

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

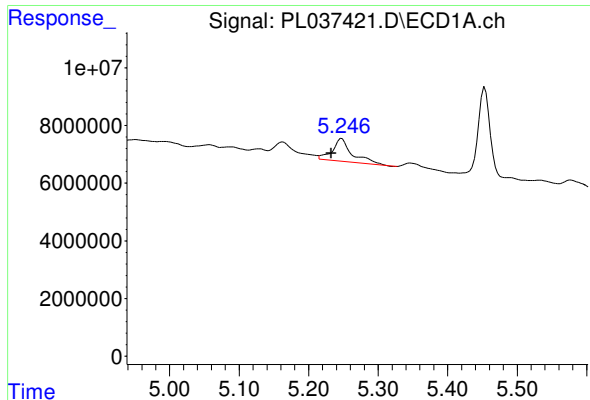

#10 gamma-Chlordane


R.T.: 5.248 min
Delta R.T.: 0.015 min
Response: 15879588
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

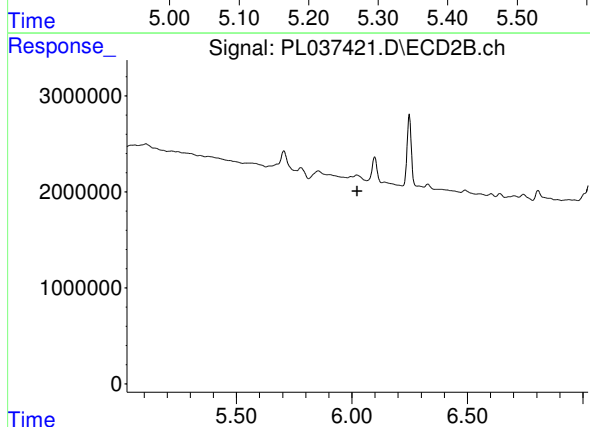


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

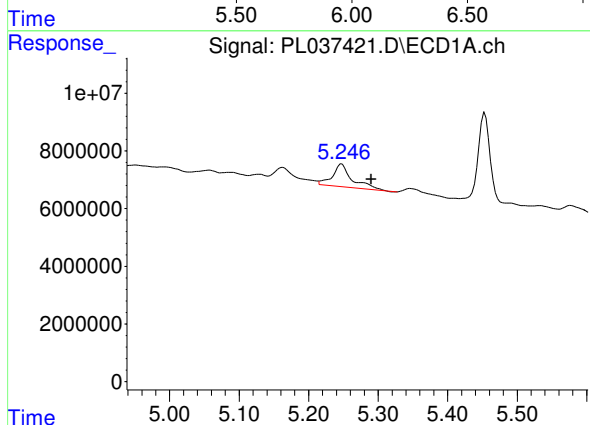


#11 alpha-Chlordane

R.T.: 5.248 min
Delta R.T.: -0.042 min
Response: 15879588
Conc: 1.75 ng/ml

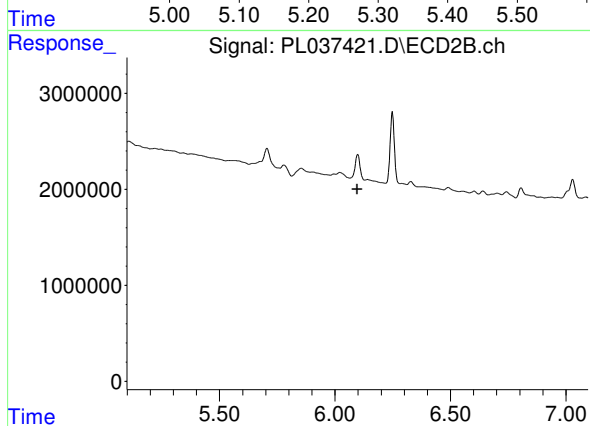

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.097 min
Response: 0
Conc: N.D.

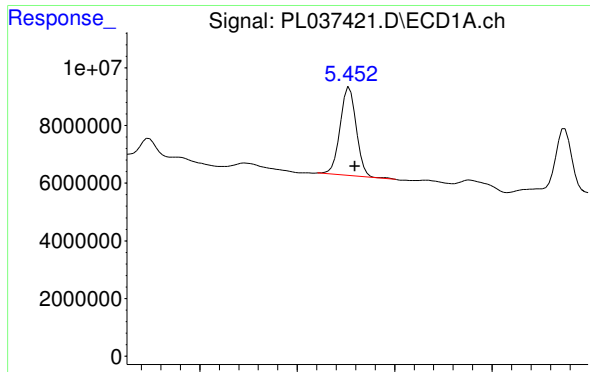

#12 4,4'-DDE


R.T.: 5.454 min
Delta R.T.: -0.005 min
Response: 35175336
Conc: 3.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

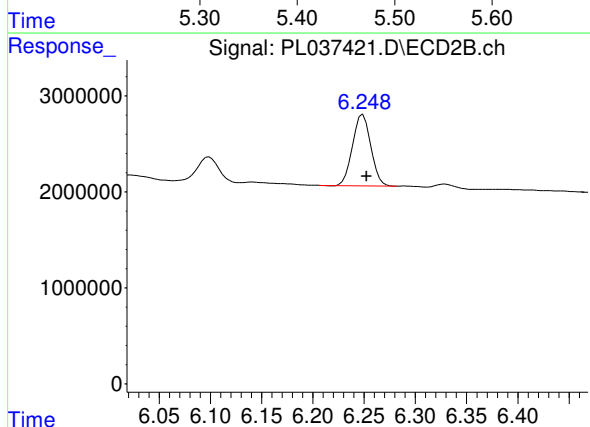


#12 4,4'-DDE

R.T.: 6.249 min
Delta R.T.: -0.004 min
Response: 9227093
Conc: 3.63 ng/ml

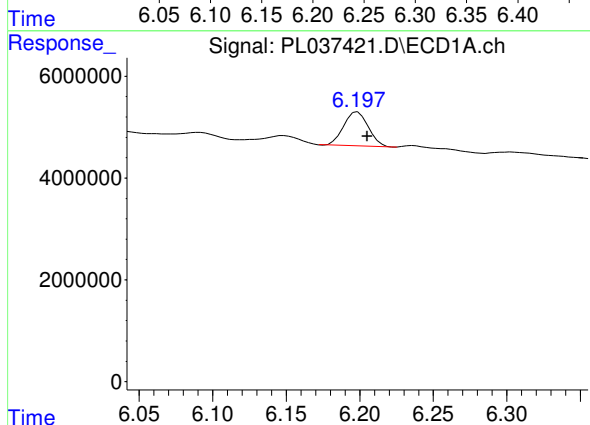


#17 4,4'-DDT

R.T.: 6.199 min
Delta R.T.: -0.006 min
Response: 7736857
Conc: 1.20 ng/ml

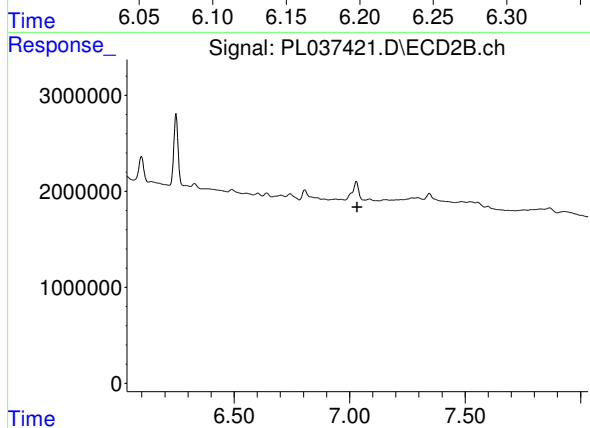

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.033 min
Response: 0
Conc: N.D.

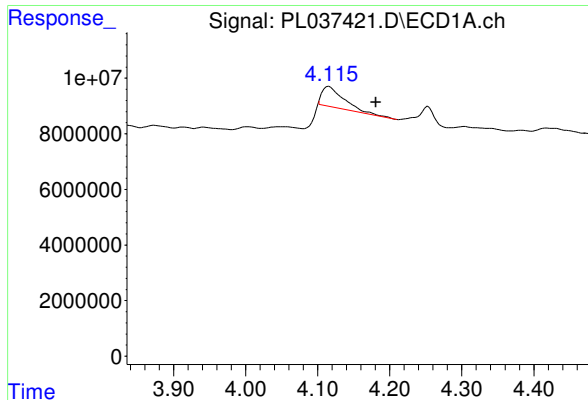

#23 Chlordane-1


R.T.: 4.116 min
Delta R.T.: -0.065 min
Response: 15027292
Conc: 48.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

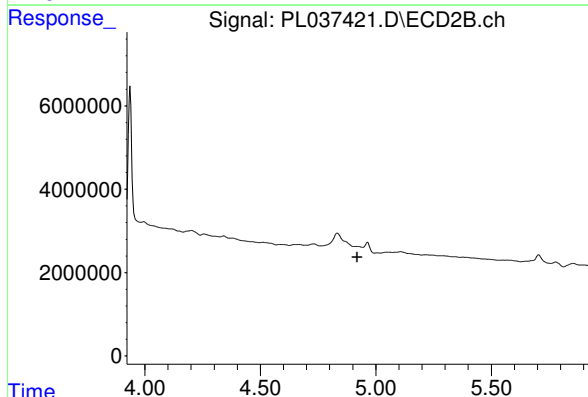


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.921 min
Response: 0
Conc: N.D.

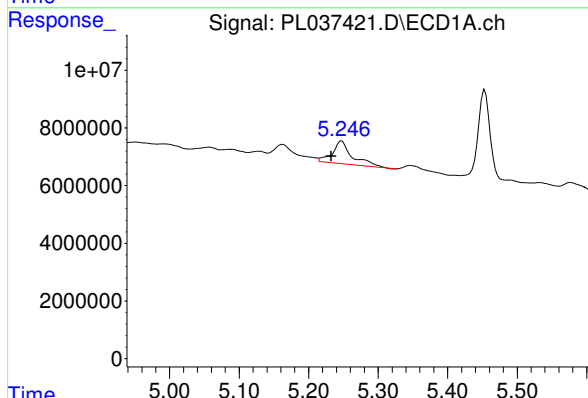


#25 Chlordane-3

R.T.: 5.248 min
Delta R.T.: 0.015 min
Response: 15879588
Conc: 14.94 ng/ml

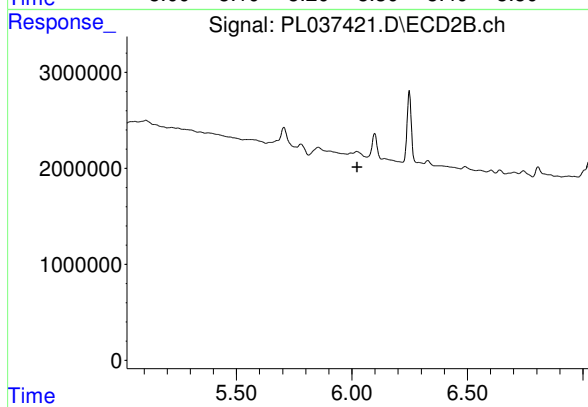

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.022 min
Response: 0
Conc: N.D.

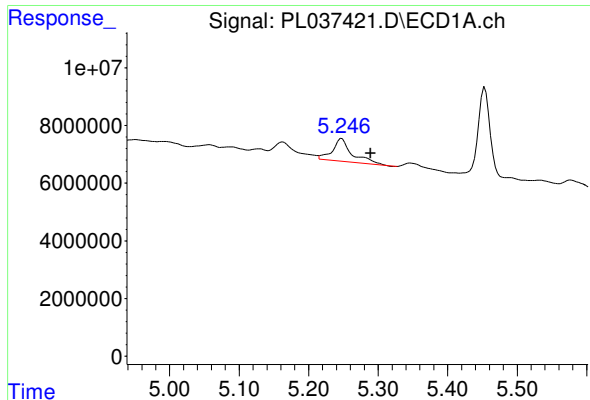

#26 Chlordane-4


R.T.: 5.248 min
Delta R.T.: -0.041 min
Response: 15879588
Conc: 16.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

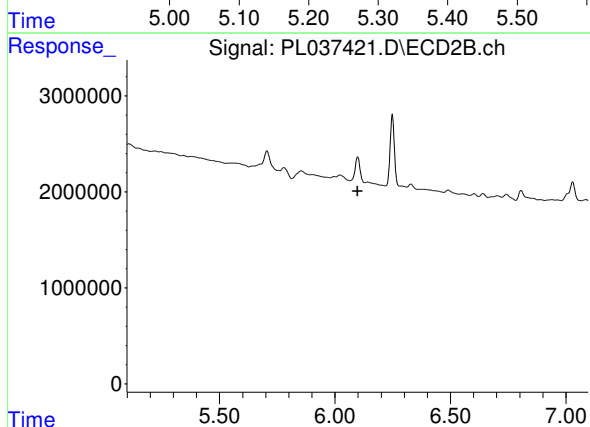


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.098 min
Response: 0
Conc: N.D.

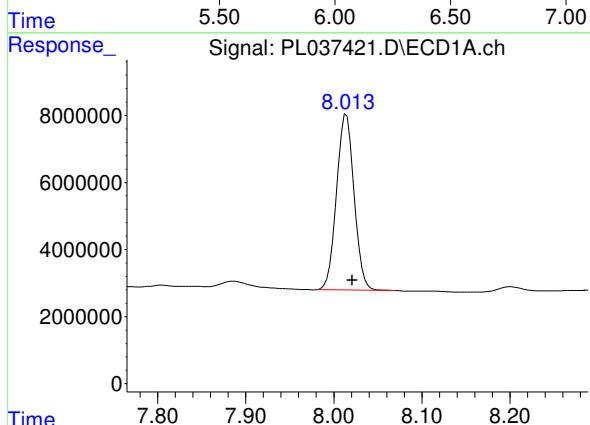

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.006 min
Response: 72655528
Conc: 12.04 ng/ml

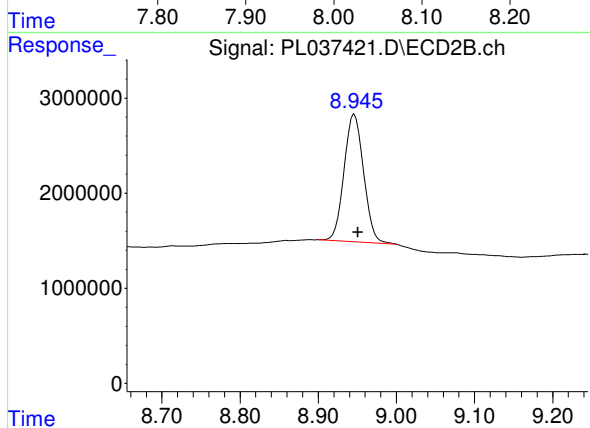

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.004 min
Response: 23224506
Conc: 11.71 ng/ml