

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
 Data File : PL037422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 14:05
 Operator : UA\AJ
 Sample : J3676-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 05:11:56 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.335	3.936	86167468	25110716	10.893	9.076
28) SA Decachlor...	8.014	8.946	35474168	11822411	5.879	5.959
Target Compounds						
6) B beta-BHC	4.253f	0.000	17344511	0	3.803	N.D. #
12) B 4,4'-DDE	5.453	0.000	10230183	0	1.158	N.D. #
13) MA Dieldrin	5.641f	0.000	9350907	0	1.056	N.D. #
17) MA 4,4'-DDT	6.198	0.000	10231424	0	1.585	N.D. #
23) Chlordane-1	4.185	0.000	9352310	0	30.458	N.D. #
24) Chlordane-2	4.705	0.000	4471837	0	12.561	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
Data File : PL037422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 14:05
Operator : UA\AJ
Sample : J3676-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 05:11:56 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

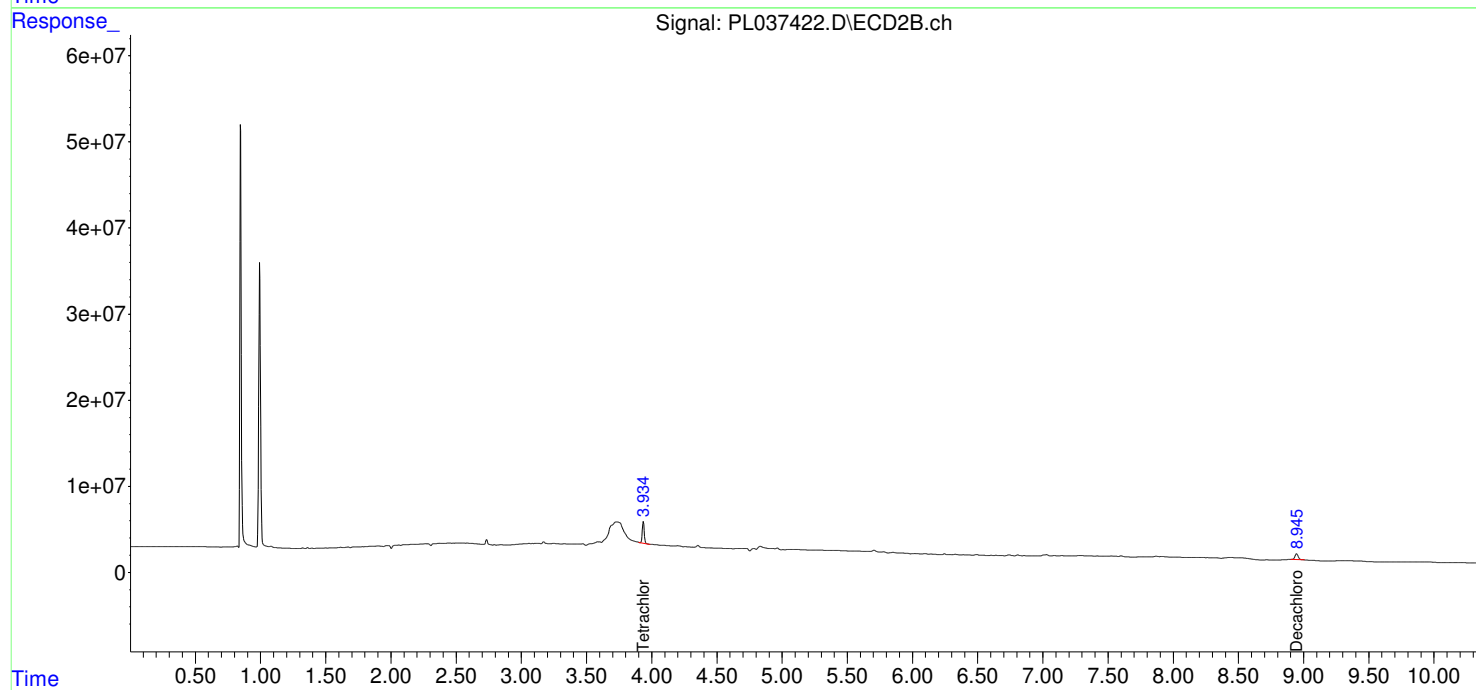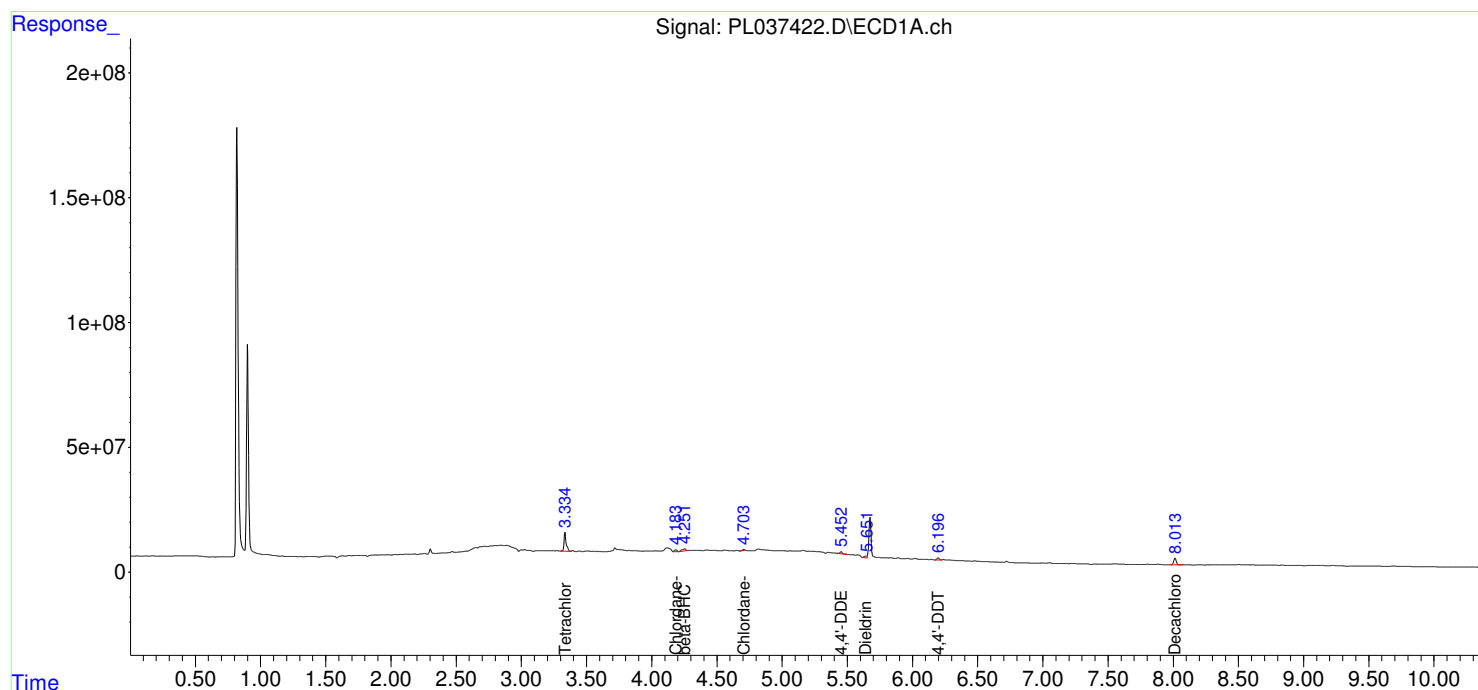


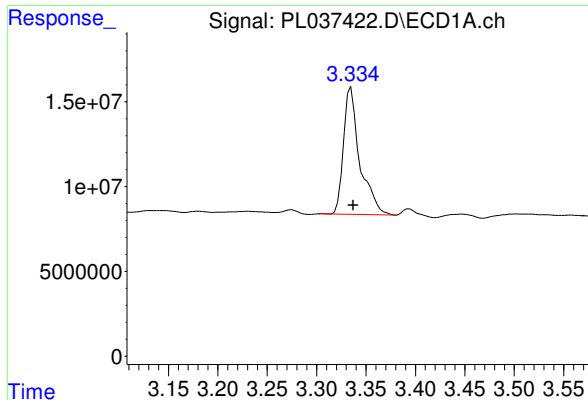

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 86167468
Conc: 10.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

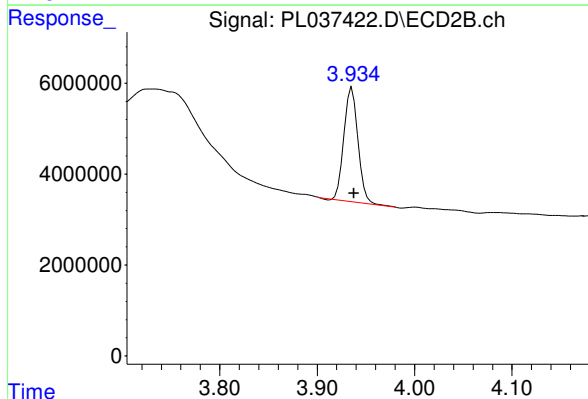


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 25110716
Conc: 9.08 ng/ml

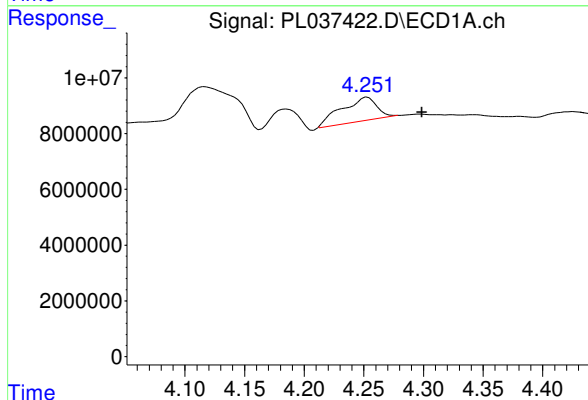


#6 beta-BHC

R.T.: 4.253 min
Delta R.T.: -0.046 min
Response: 17344511
Conc: 3.80 ng/ml

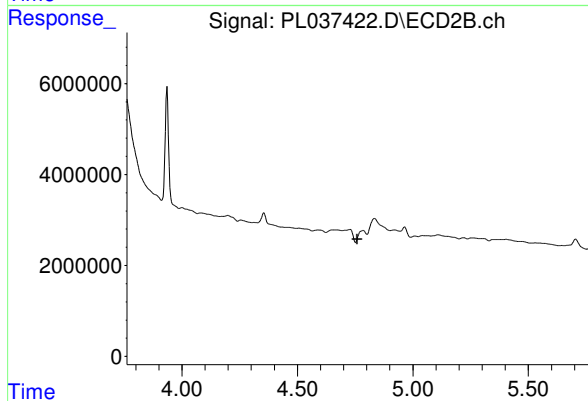

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

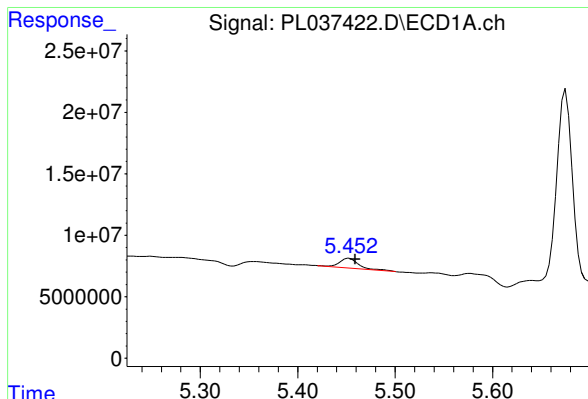

#12 4,4'-DDE


R.T.: 5.453 min
Delta R.T.: -0.006 min
Response: 10230183
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

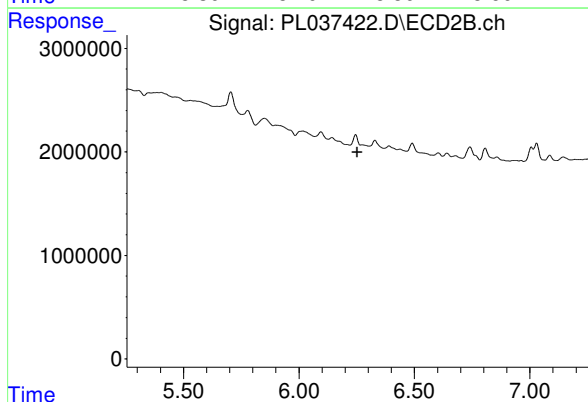


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.252 min
Response: 0
Conc: N.D.

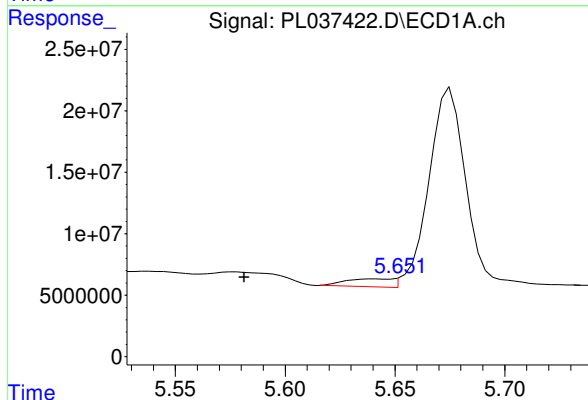


#13 Dieldrin

R.T.: 5.641 min
Delta R.T.: 0.059 min
Response: 9350907
Conc: 1.06 ng/ml

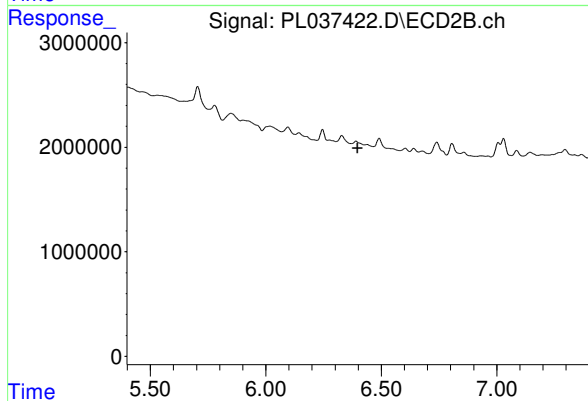

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

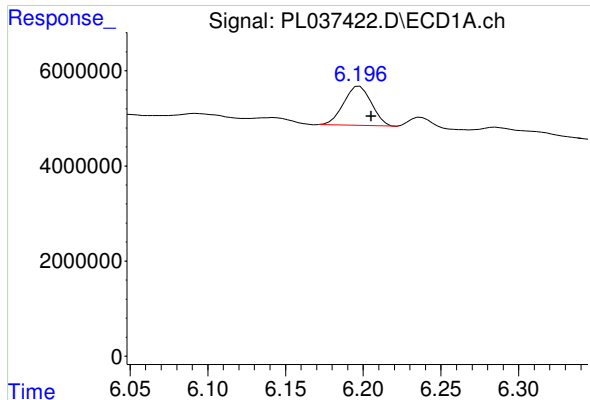

#17 4,4'-DDT


R.T.: 6.198 min
Delta R.T.: -0.007 min
Response: 10231424
Conc: 1.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

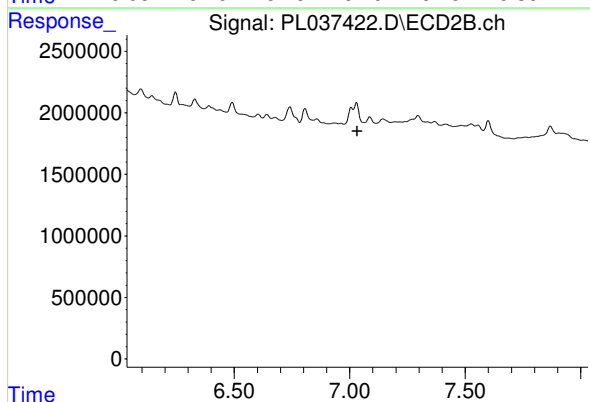


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 7.033 min
Response: 0
Conc: N.D.

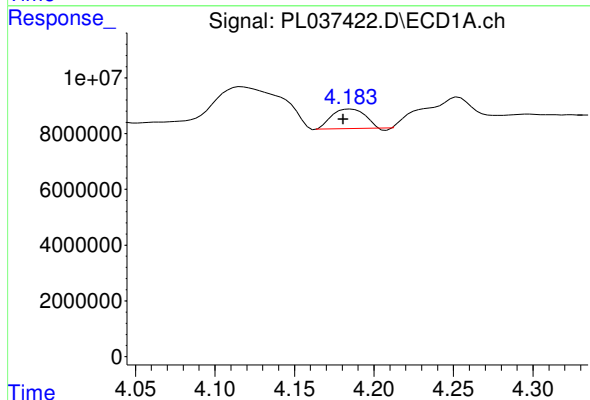


#23 Chlordane-1

R.T.: 4.185 min
Delta R.T.: 0.004 min
Response: 9352310
Conc: 30.46 ng/ml

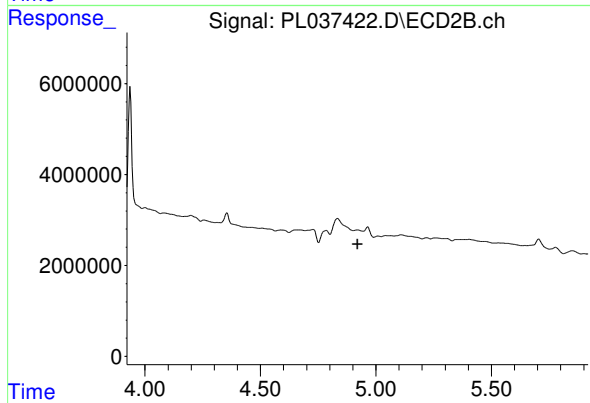

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.921 min
Response: 0
Conc: N.D.

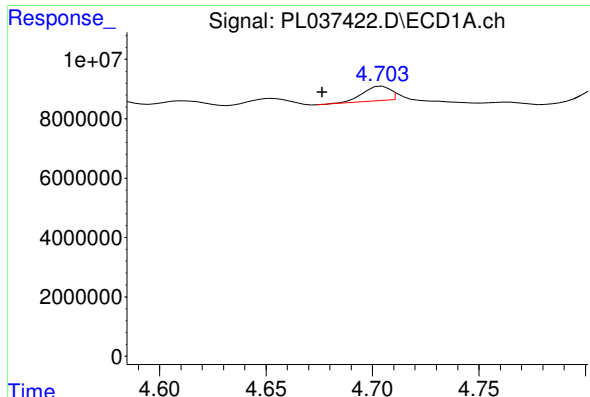

#24 Chlordane-2


R.T.: 4.705 min
Delta R.T.: 0.028 min
Response: 4471837
Conc: 12.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

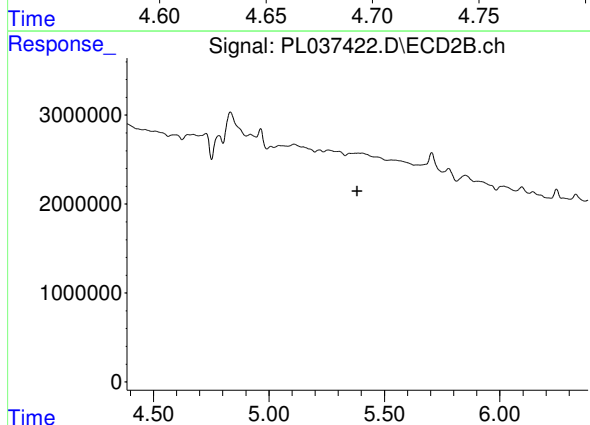


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.382 min
Response: 0
Conc: N.D.

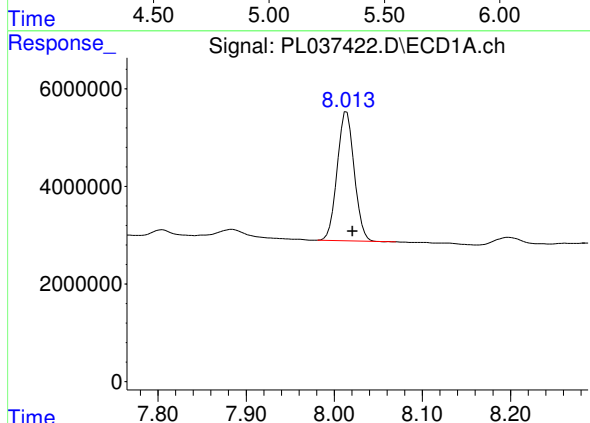

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.007 min
Response: 35474168
Conc: 5.88 ng/ml

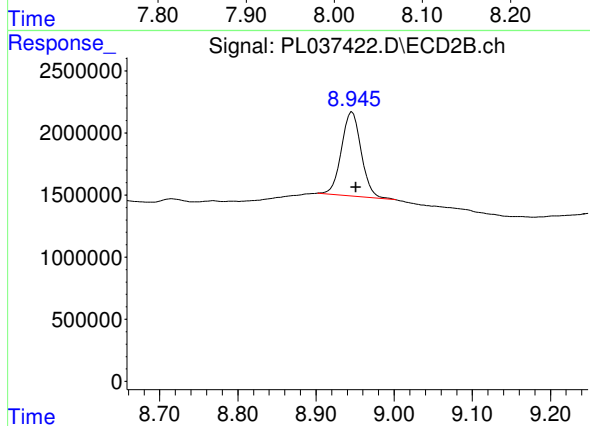

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.004 min
Response: 11822411
Conc: 5.96 ng/ml