

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
 Data File : PL037441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 18:32
 Operator : UA\AJ
 Sample : J3709-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 05:13:14 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.936	74914234	25983699	9.470	9.391
28)	SA Decachlor...	8.015	8.947	40238076	13100476	6.669	6.603
Target Compounds							
6)	B beta-BHC	4.253f	0.000	6219382	0	1.364	N.D. #
10)	B gamma-Chl...	5.163f	0.000	10435573	0	1.114	N.D. #
23)	Chlordane-1	4.119	0.000	6900369	0	22.473	N.D. #
25)	Chlordane-3	5.163	0.000	10435573	0	9.818	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
Data File : PL037441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 18:32
Operator : UA\AJ
Sample : J3709-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 05:13:14 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

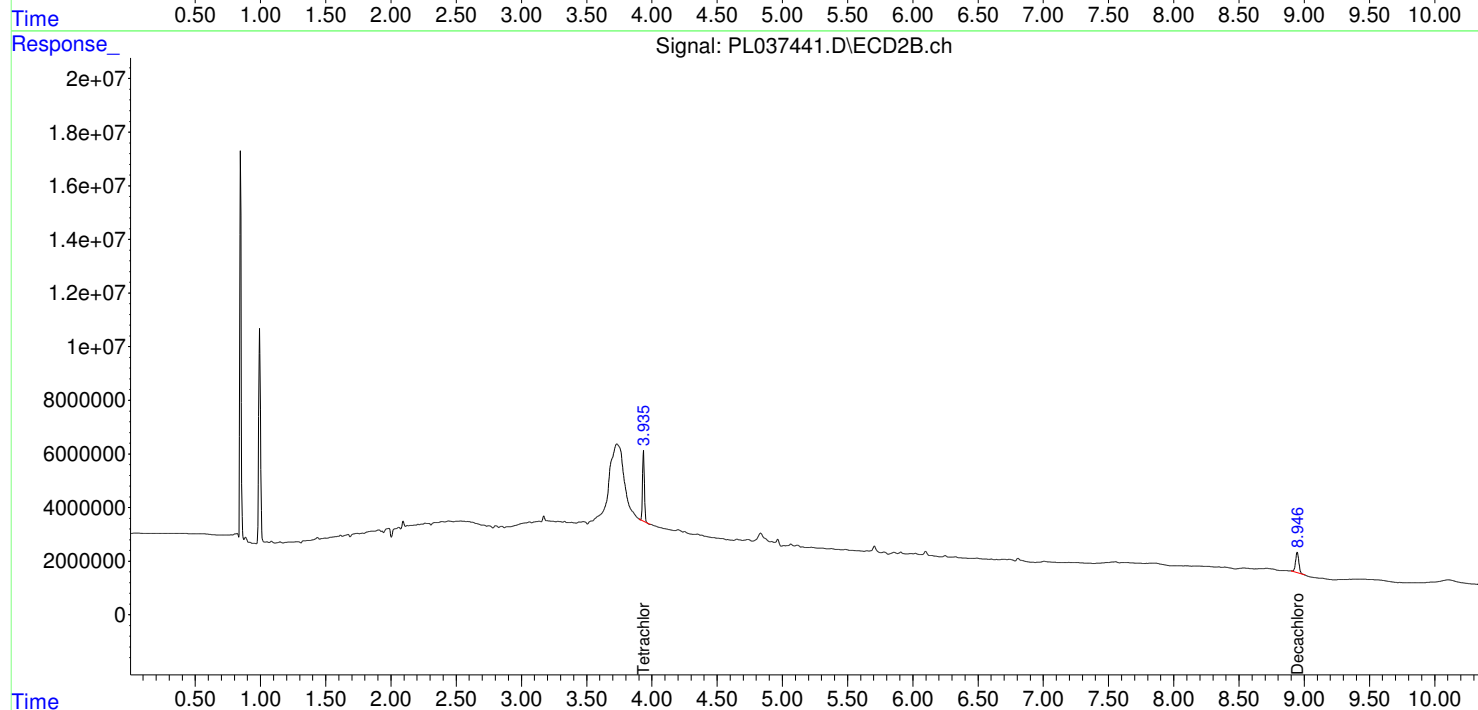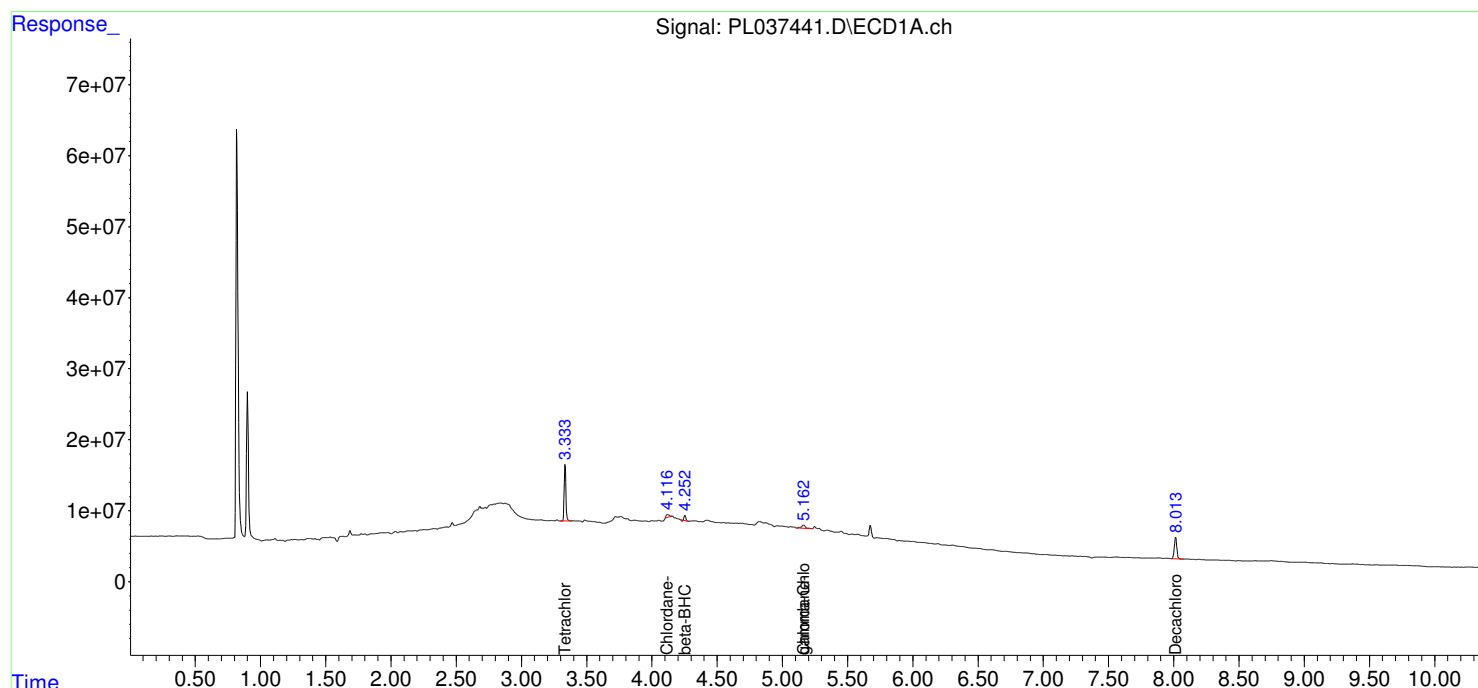


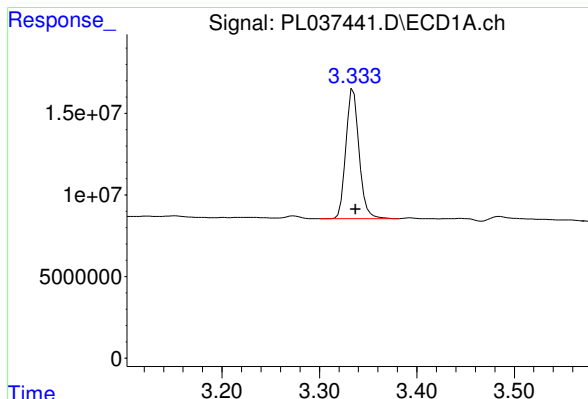

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 74914234
Conc: 9.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

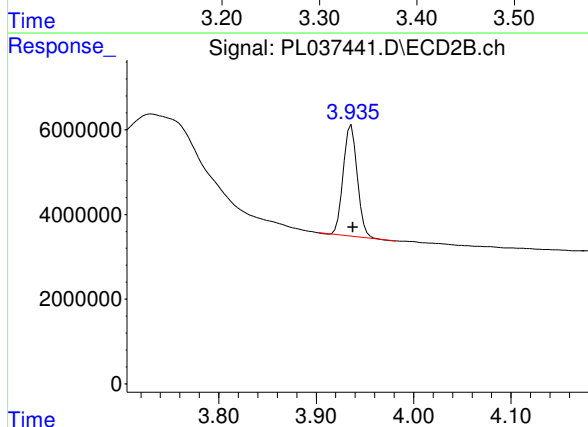


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 25983699
Conc: 9.39 ng/ml

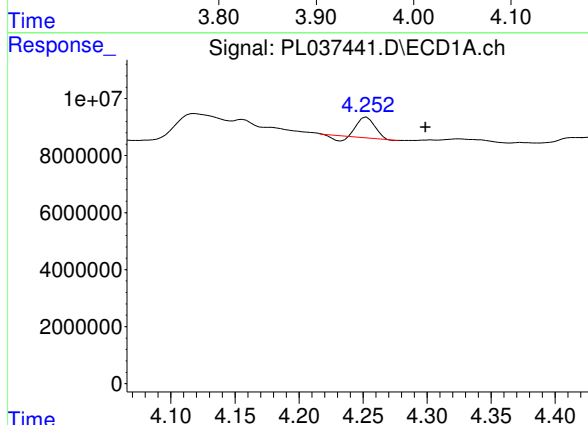


#6 beta-BHC

R.T.: 4.253 min
Delta R.T.: -0.046 min
Response: 6219382
Conc: 1.36 ng/ml

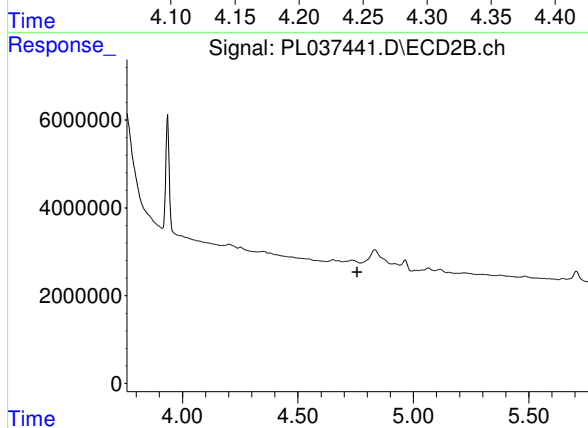

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

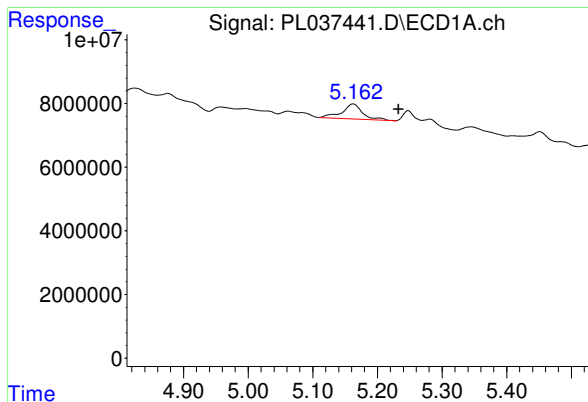

#10 gamma-Chlordane


R.T.: 5.163 min
Delta R.T.: -0.069 min
Response: 10435573
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

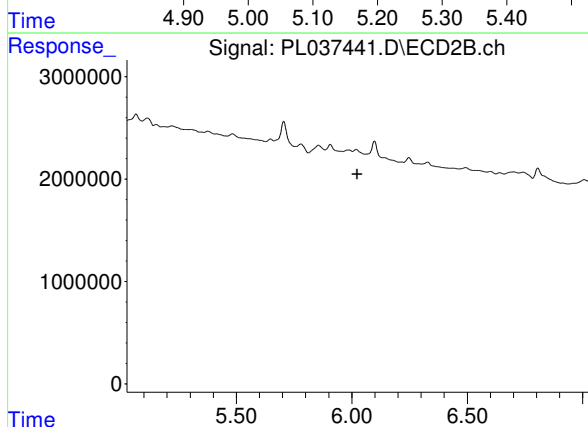


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

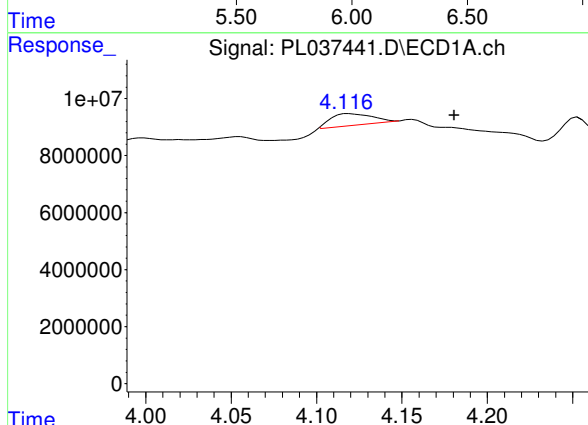


#23 Chlordane-1

R.T.: 4.119 min
Delta R.T.: -0.061 min
Response: 6900369
Conc: 22.47 ng/ml

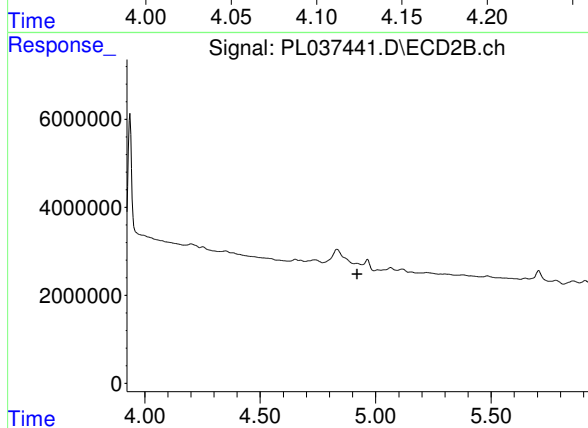

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.921 min
Response: 0
Conc: N.D.

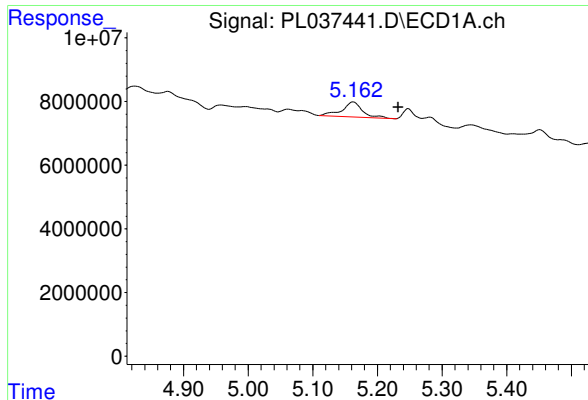

#25 Chlordane-3


R.T.: 5.163 min
Delta R.T.: -0.069 min
Response: 10435573
Conc: 9.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

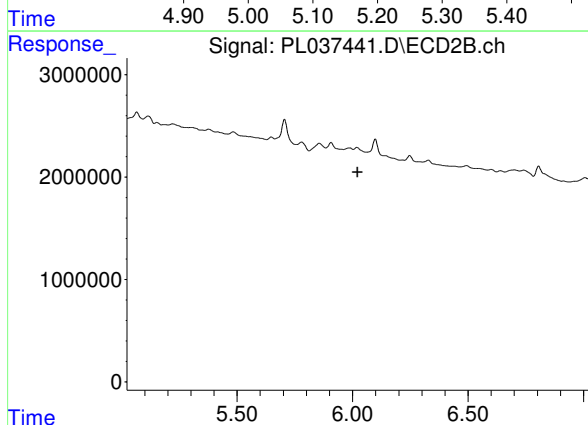


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.022 min
Response: 0
Conc: N.D.

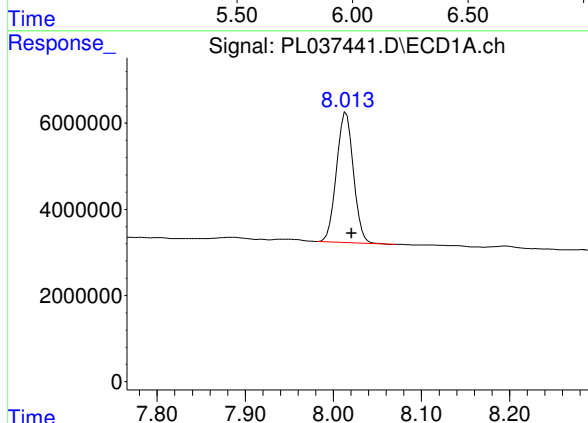

#28 Decachlorobiphenyl

R.T.: 8.015 min
Delta R.T.: -0.006 min
Response: 40238076
Conc: 6.67 ng/ml

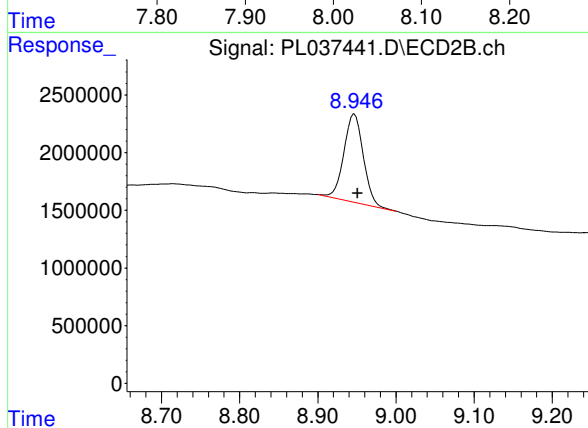

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 13100476
Conc: 6.60 ng/ml