

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
 Data File : PL037442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 18:46
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 05:13:18 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.335	3.936	126.3E6	44416142	15.972	16.054
28) SA Decachlor...	8.014	8.947	115.7E6	36974719	19.181	18.637
Target Compounds						
8) B Heptachlo...	0.000	5.780	0	8832544	N.D.	3.098 #
14) MA Endrin	5.849	0.000	9881083	0	1.254	N.D. #
21) B Endrin ke...	6.934f	0.000	162.7E6	0	22.884	N.D. #
23) Chlordane-1	4.115	0.000	11767021	0	38.323	N.D. #
24) Chlordane-2	0.000	5.316	0	8844090	N.D.	69.886 #
27) Chlordane-5	5.849	0.000	9881083	0	75.504	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
Data File : PL037442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 18:46
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 05:13:18 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

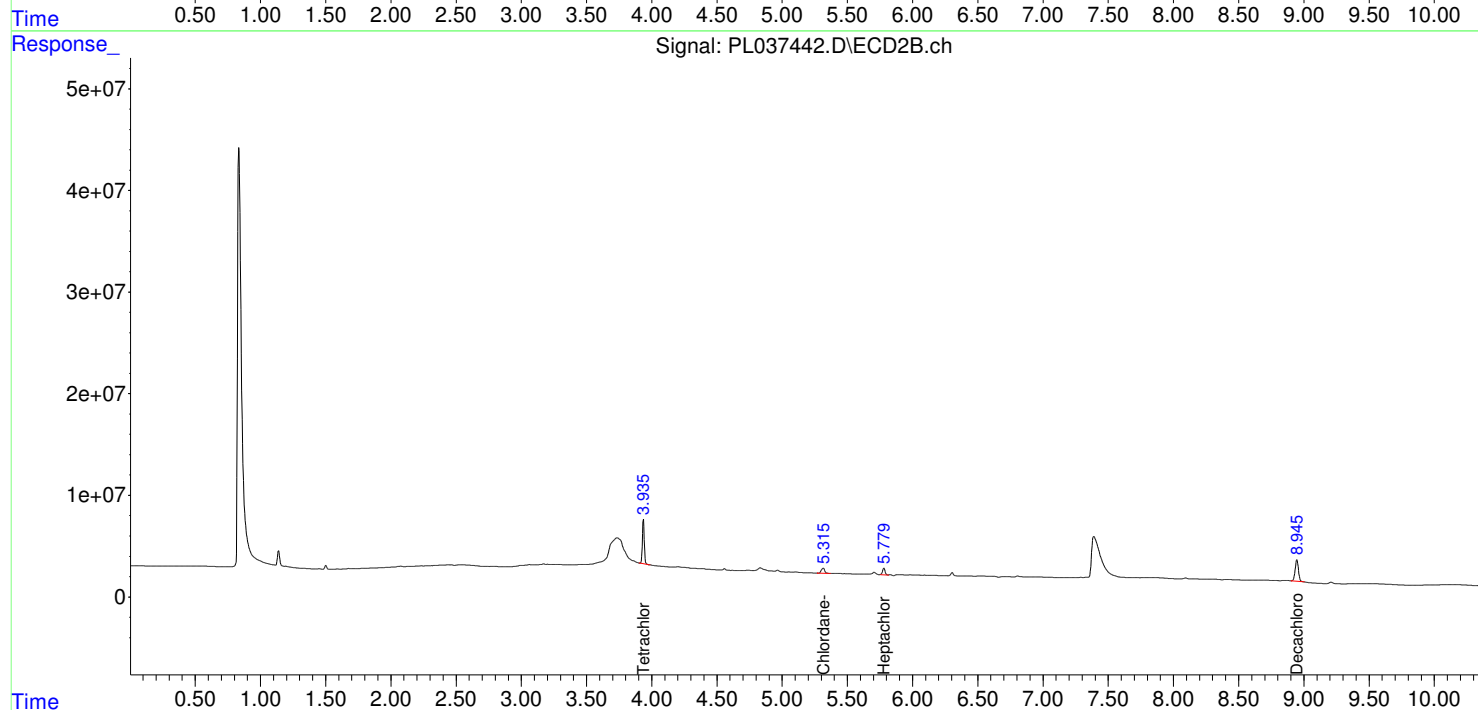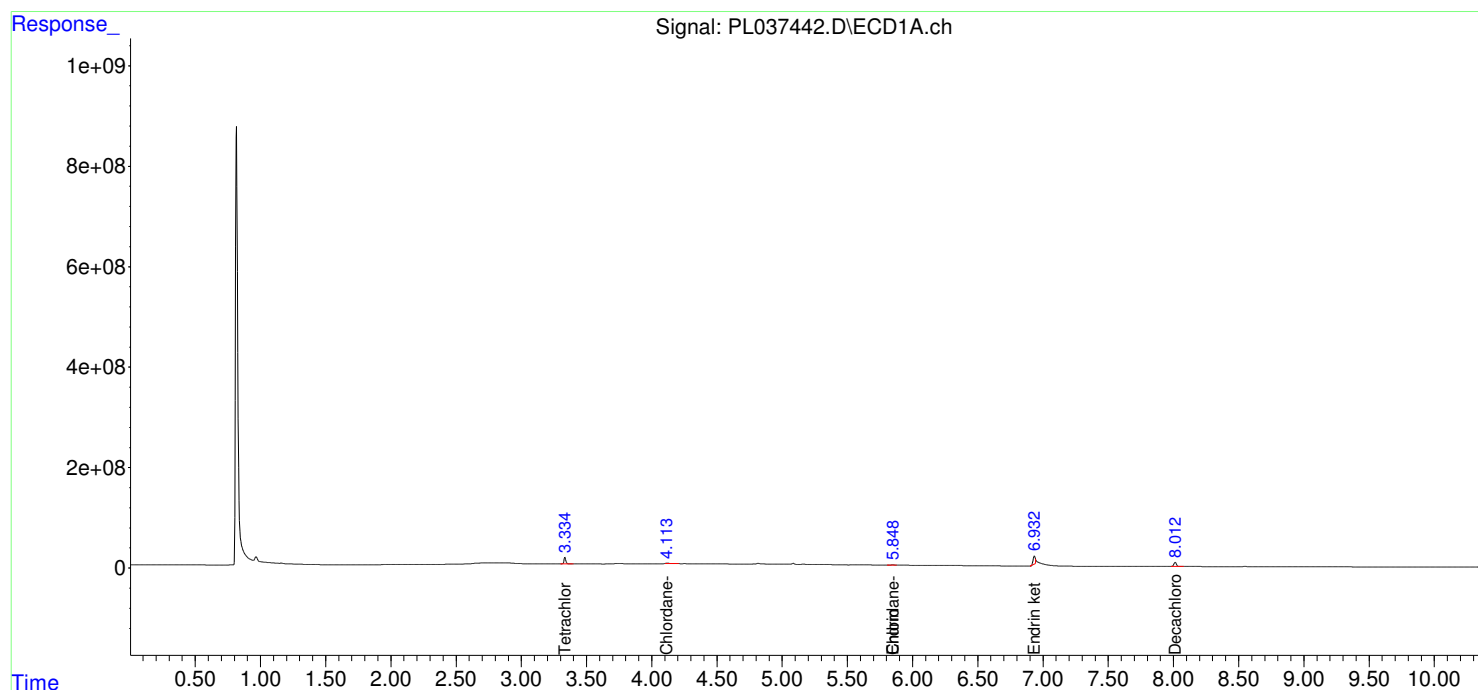


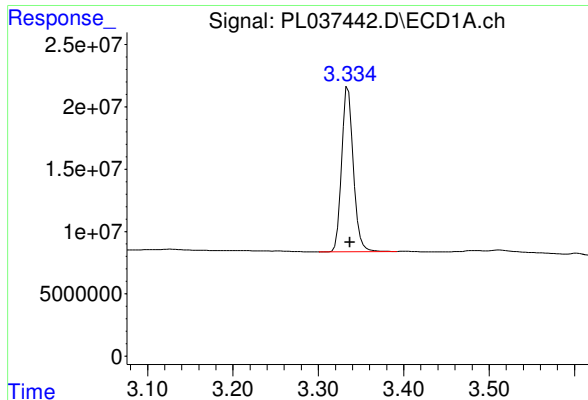

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 126341430
Conc: 15.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

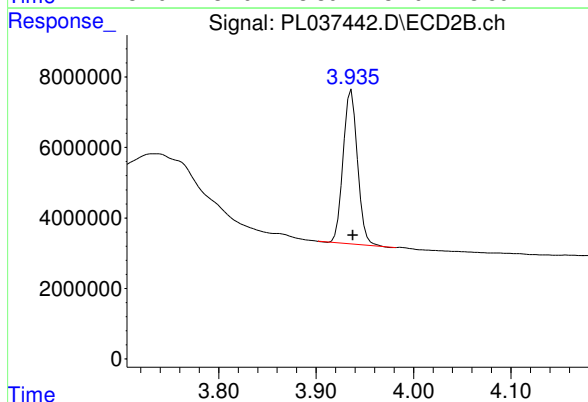


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.001 min
Response: 44416142
Conc: 16.05 ng/ml

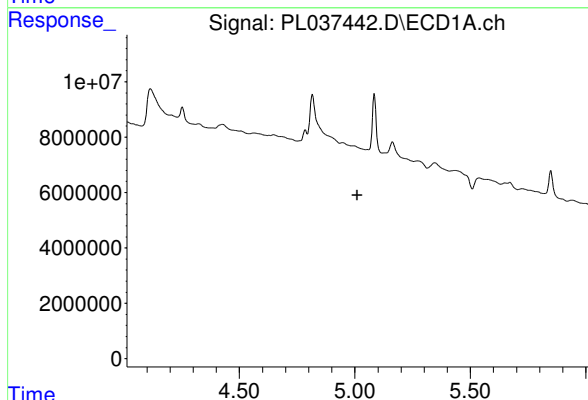


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.010 min
Response: 0
Conc: N.D.

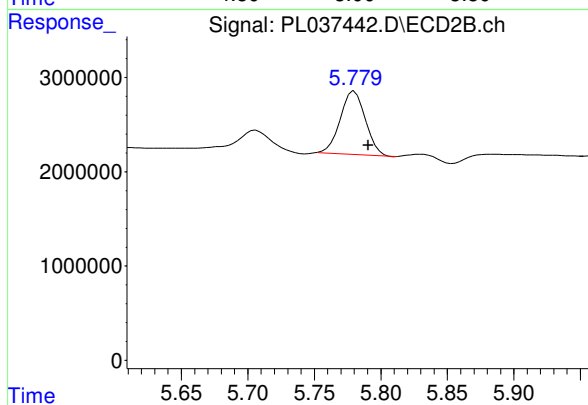

#8 Heptachlor epoxide


R.T.: 5.780 min
Delta R.T.: -0.010 min
Response: 8832544
Conc: 3.10 ng/ml

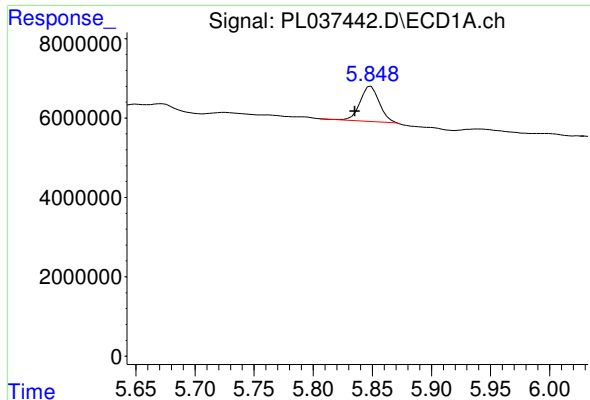

#14 Endrin


R.T.: 5.849 min
Delta R.T.: 0.014 min
Response: 9881083
Conc: 1.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

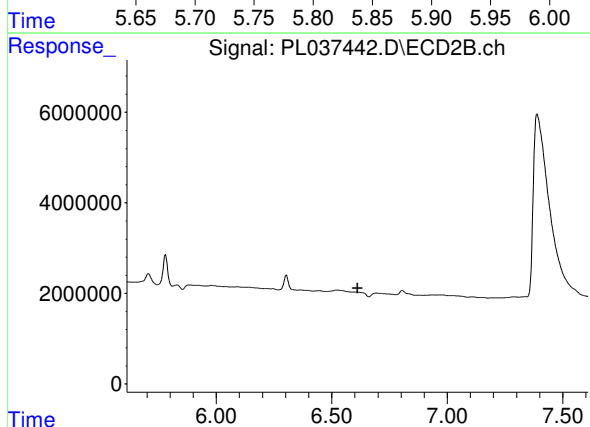


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

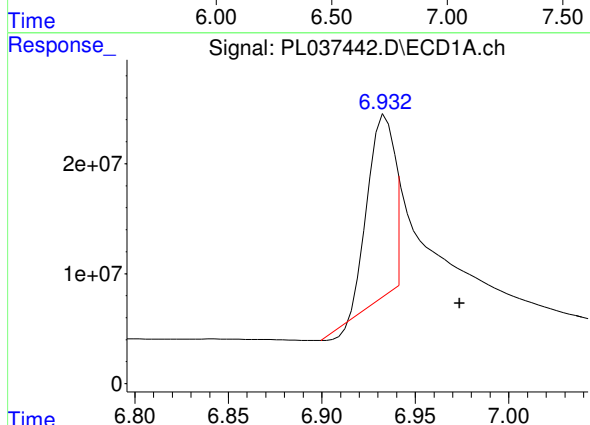


#21 Endrin ketone

R.T.: 6.934 min
Delta R.T.: -0.039 min
Response: 162740218
Conc: 22.88 ng/ml

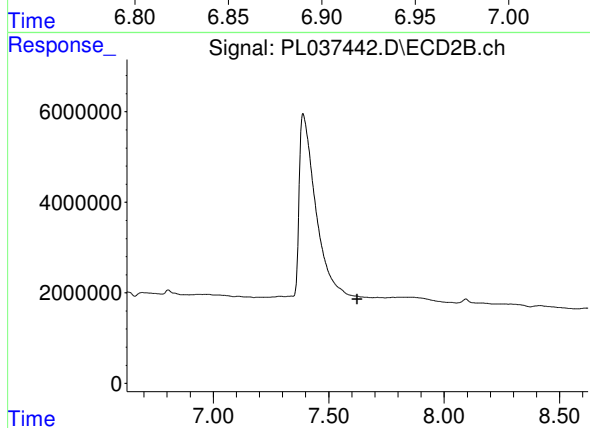

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.623 min
Response: 0
Conc: N.D.

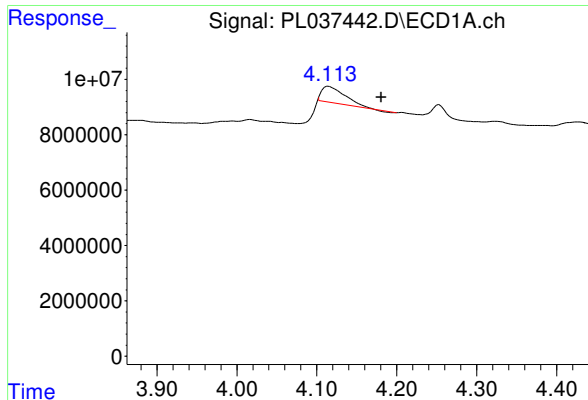

#23 Chlordane-1


R.T.: 4.115 min
Delta R.T.: -0.066 min
Response: 11767021
Conc: 38.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

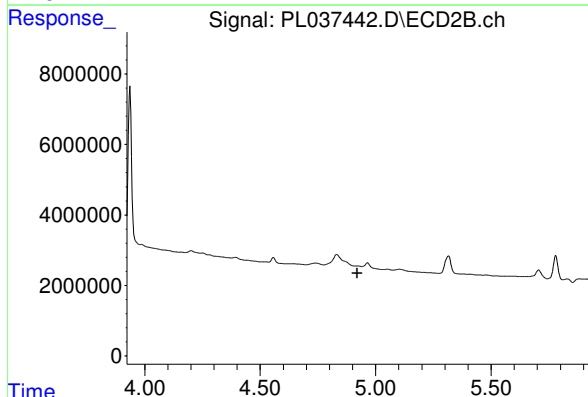


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

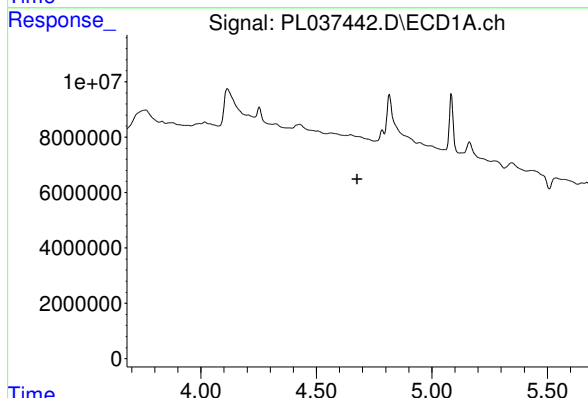


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.676 min
Response: 0
Conc: N.D.

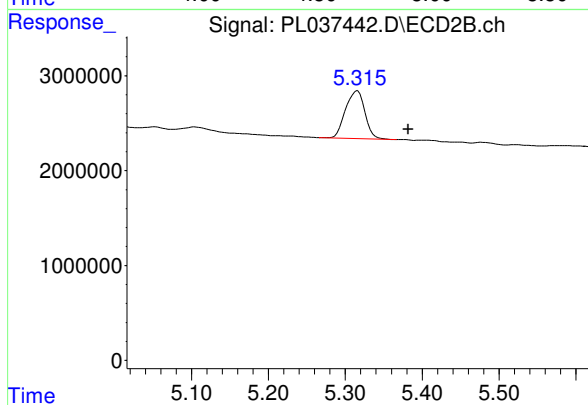

#24 Chlordane-2


R.T.: 5.316 min
Delta R.T.: -0.066 min
Response: 8844090
Conc: 69.89 ng/ml

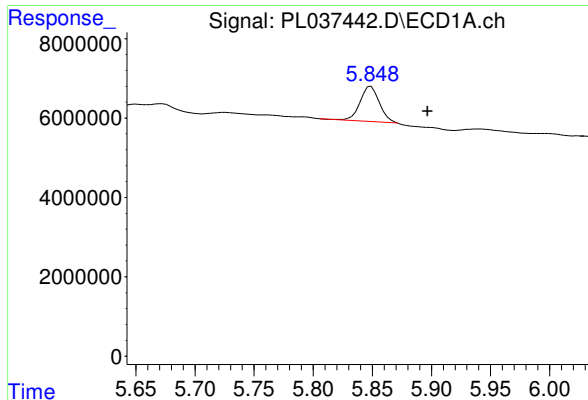

#27 Chlordane-5


R.T.: 5.849 min
Delta R.T.: -0.048 min
Response: 9881083
Conc: 75.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

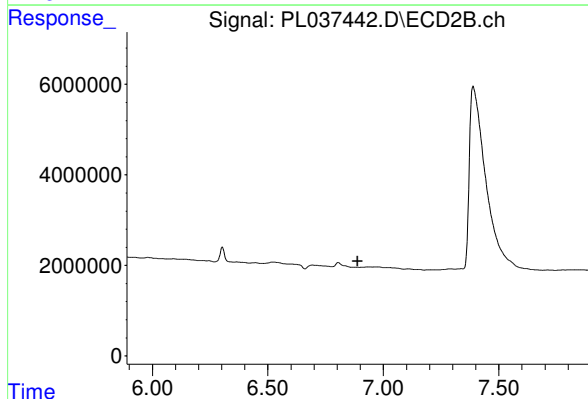


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.889 min
Response: 0
Conc: N.D.

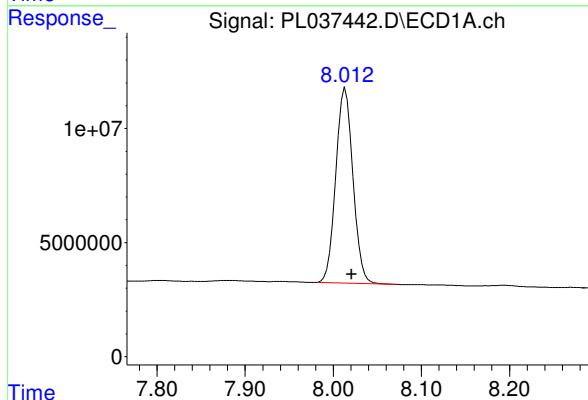

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.007 min
Response: 115737965
Conc: 19.18 ng/ml

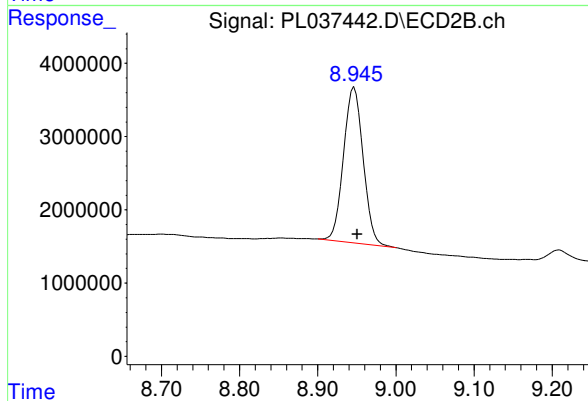

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 36974719
Conc: 18.64 ng/ml