

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL062618\  
 Data File : PL037445.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 26 Jun 2018 19:28  
 Operator : UA\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 27 05:13:31 2018  
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD\_L\methods\PL062018.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jun 21 02:27:11 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml    |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|----------|
| -----                       |                 |        |       |          |          |        |          |
| System Monitoring Compounds |                 |        |       |          |          |        |          |
| 1)                          | SA Tetrachlo... | 3.335  | 3.936 | 116.7E6  | 42483673 | 14.747 | 15.355   |
| 28)                         | SA Decachlor... | 8.014  | 8.946 | 100.1E6  | 33221926 | 16.597 | 16.745   |
| Target Compounds            |                 |        |       |          |          |        |          |
| 8)                          | B Heptachlo...  | 0.000  | 5.780 | 0        | 10723046 | N.D.   | 3.762 #  |
| 14)                         | MA Endrin       | 5.849  | 0.000 | 11143781 | 0        | 1.415  | N.D. #   |
| 21)                         | B Endrin ke...  | 6.935f | 0.000 | 191.3E6  | 0        | 26.904 | N.D. #   |
| 24)                         | Chlordane-2     | 0.000  | 5.317 | 0        | 12654013 | N.D.   | 99.992 # |
| 27)                         | Chlordane-5     | 5.849  | 0.000 | 11143781 | 0        | 85.153 | N.D. #   |
| -----                       |                 |        |       |          |          |        |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL062618\  
Data File : PL037445.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 26 Jun 2018 19:28  
Operator : UA\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 27 05:13:31 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD\_L\methods\PL062018.M  
Quant Title : GC Extractables  
QLast Update : Thu Jun 21 02:27:11 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

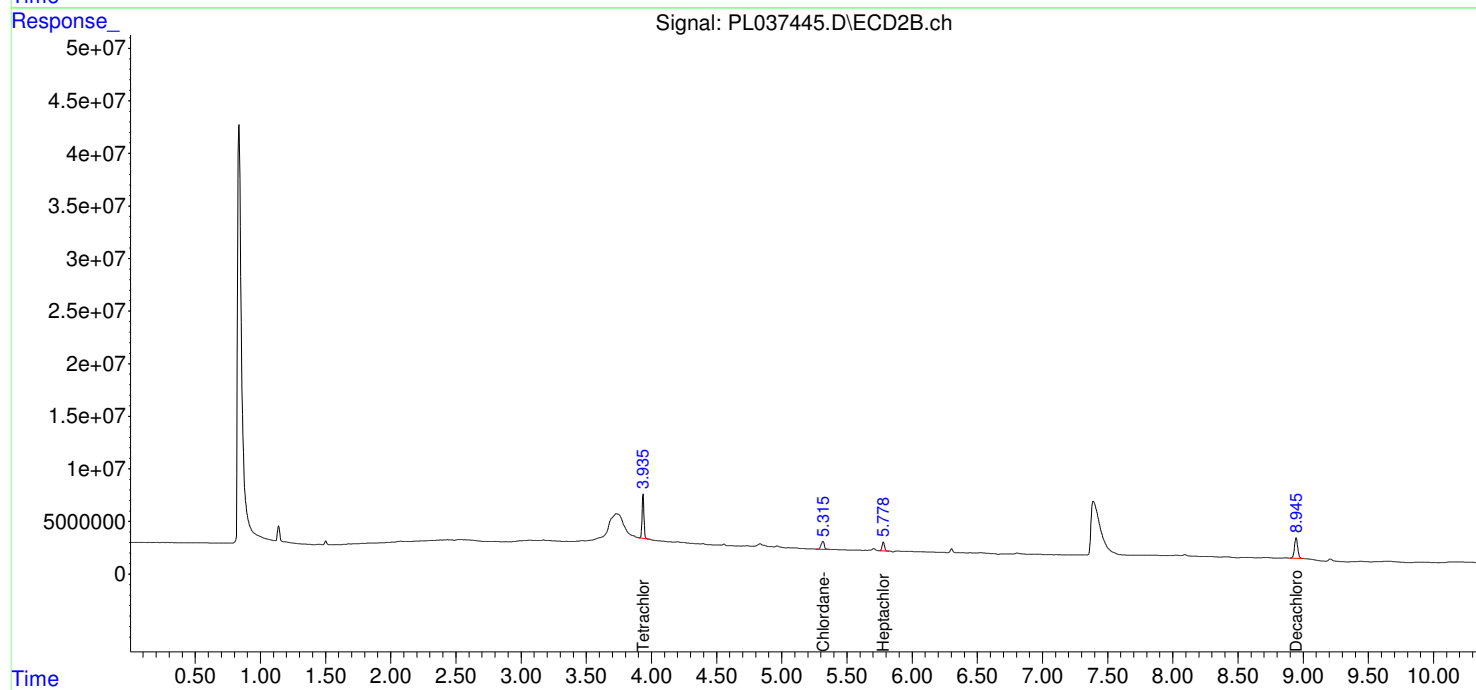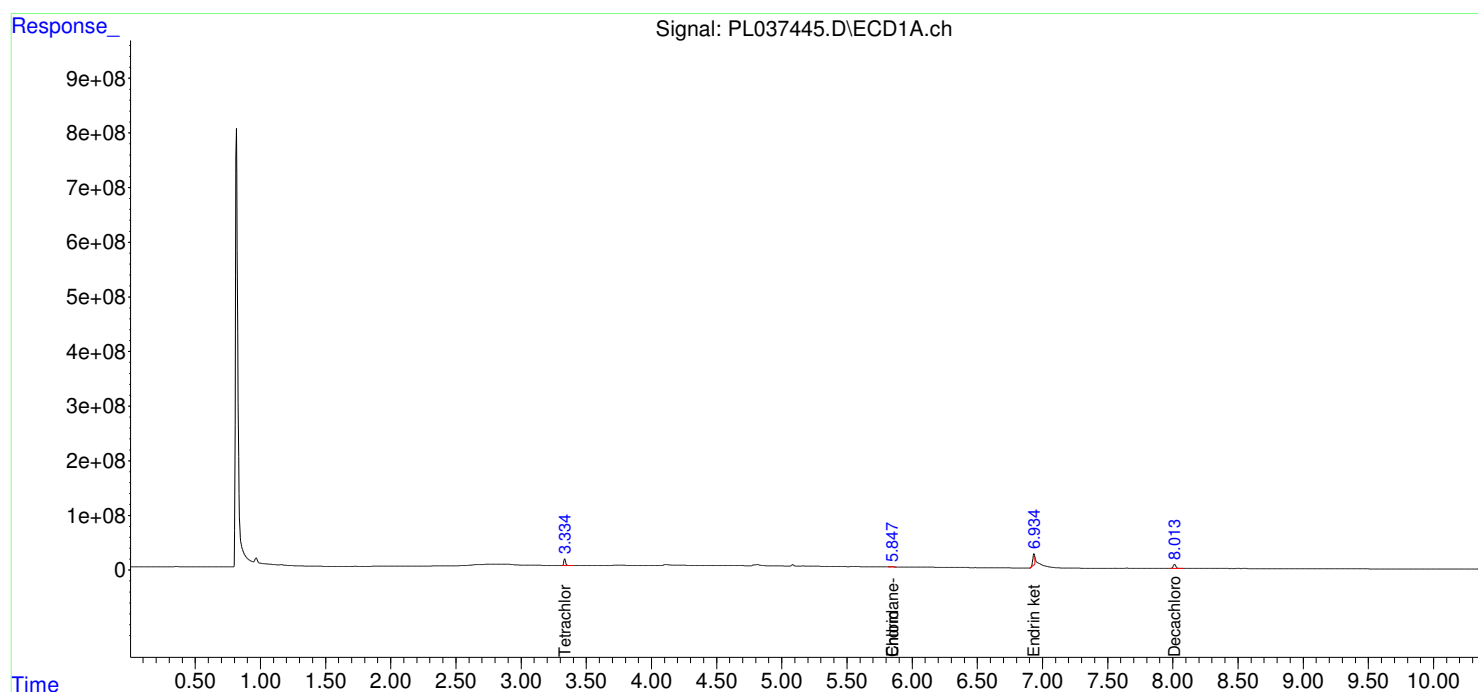


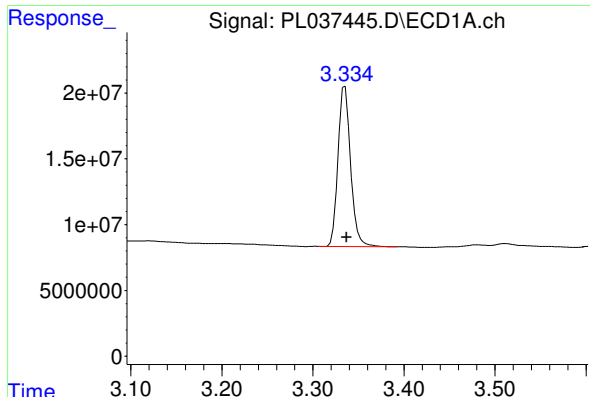

#1 Tetrachloro-m-xylene


R.T.: 3.335 min  
Delta R.T.: -0.002 min  
Response: 116651477  
Conc: 14.75 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

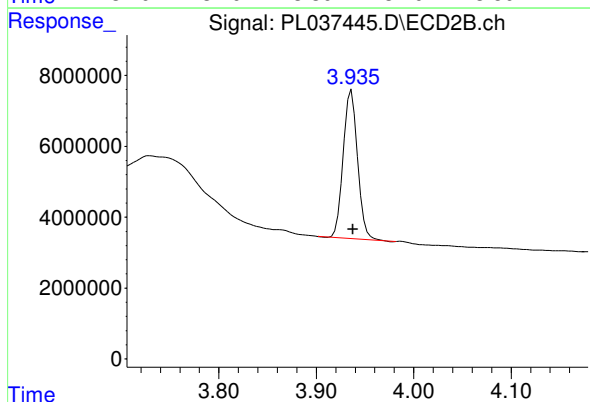


#1 Tetrachloro-m-xylene

R.T.: 3.936 min  
Delta R.T.: -0.001 min  
Response: 42483673  
Conc: 15.36 ng/ml

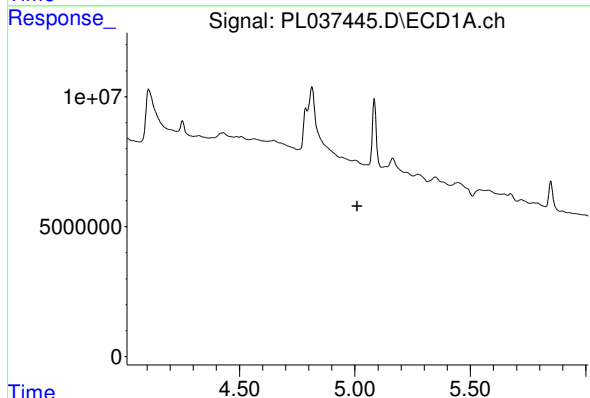


#8 Heptachlor epoxide

R.T.: 0.000 min  
Exp R.T.: 5.010 min  
Response: 0  
Conc: N.D.

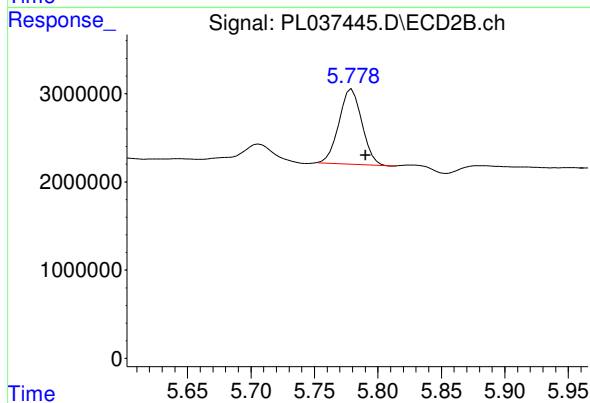

#8 Heptachlor epoxide


R.T.: 5.780 min  
Delta R.T.: -0.011 min  
Response: 10723046  
Conc: 3.76 ng/ml

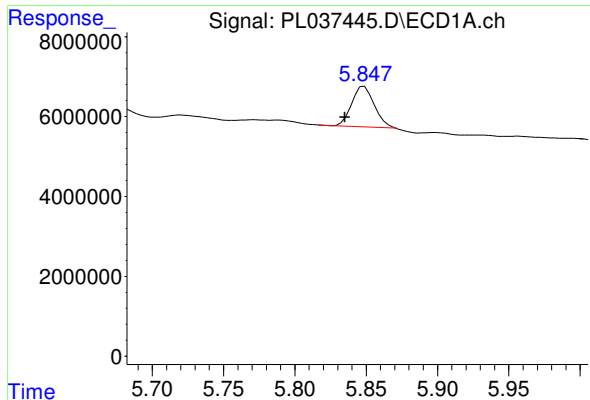

#14 Endrin


R.T.: 5.849 min  
Delta R.T.: 0.014 min  
Response: 11143781  
Conc: 1.41 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

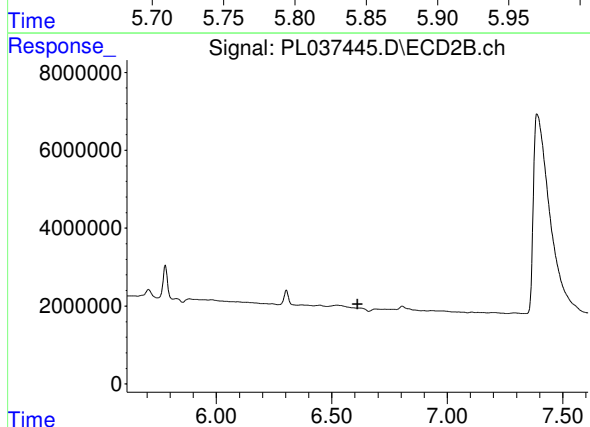


#14 Endrin

R.T.: 0.000 min  
Exp R.T. : 6.612 min  
Response: 0  
Conc: N.D.

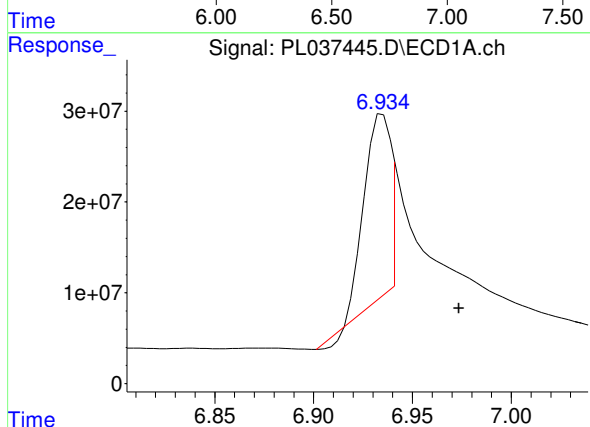


#21 Endrin ketone

R.T.: 6.935 min  
Delta R.T.: -0.038 min  
Response: 191333226  
Conc: 26.90 ng/ml

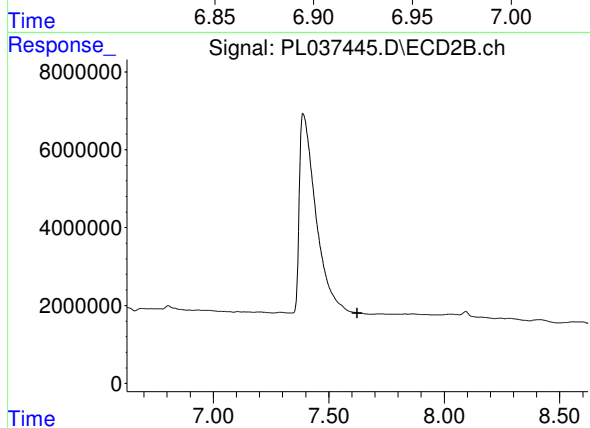

#21 Endrin ketone


R.T.: 0.000 min  
Exp R.T. : 7.623 min  
Response: 0  
Conc: N.D.

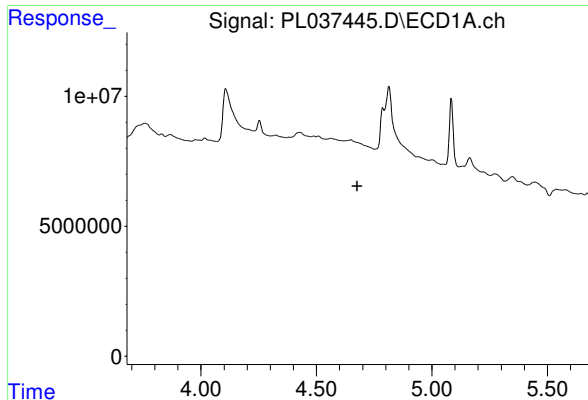

#24 Chlordane-2


R.T.: 0.000 min  
Exp R.T.: 4.676 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

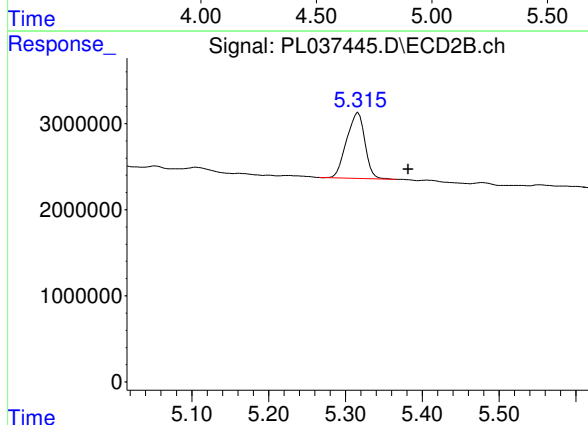


#24 Chlordane-2

R.T.: 5.317 min  
Delta R.T.: -0.065 min  
Response: 12654013  
Conc: 99.99 ng/ml

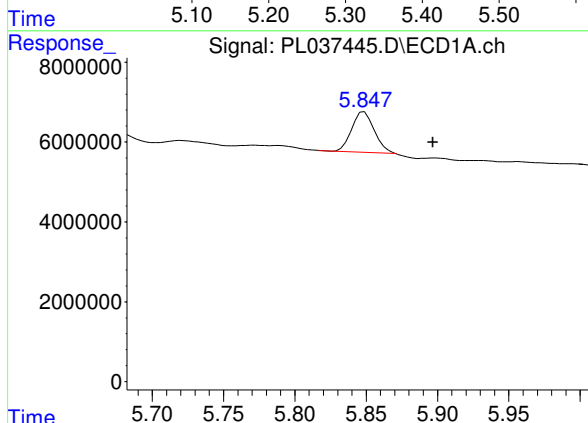


#27 Chlordane-5

R.T.: 5.849 min  
Delta R.T.: -0.048 min  
Response: 11143781  
Conc: 85.15 ng/ml

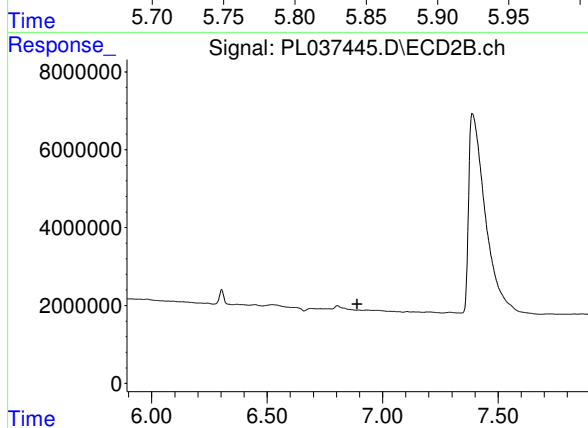

#27 Chlordane-5


R.T.: 0.000 min  
Exp R.T.: 6.889 min  
Response: 0  
Conc: N.D.

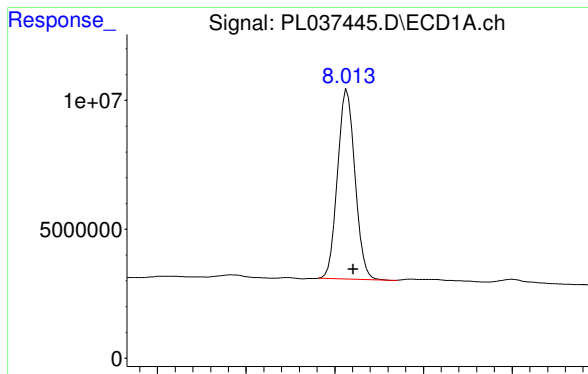

#28 Decachlorobiphenyl

R.T.: 8.014 min  
Delta R.T.: -0.007 min  
Response: 100148941  
Conc: 16.60 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

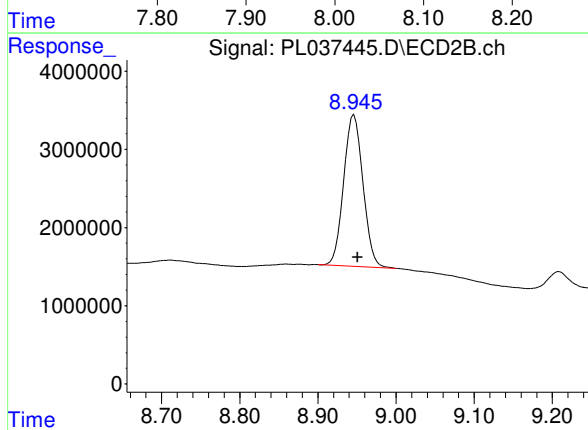

#28 Decachlorobiphenyl

R.T.: 8.946 min  
Delta R.T.: -0.005 min  
Response: 33221926  
Conc: 16.75 ng/ml