

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
 Data File : PL037447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 19:56
 Operator : UA\AJ
 Sample : J3709-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 05:13:40 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.335	3.936	52216007	18931981	6.601	6.843
28) SA Decachlor...	8.014	8.947	40968787	12906162	6.790	6.505
Target Compounds						
6) B beta-BHC	4.253f	0.000	10079678	0	2.210	N.D. #
23) Chlordane-1	4.120	0.000	15620665	0	50.873	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
Data File : PL037447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 19:56
Operator : UA\AJ
Sample : J3709-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 05:13:40 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

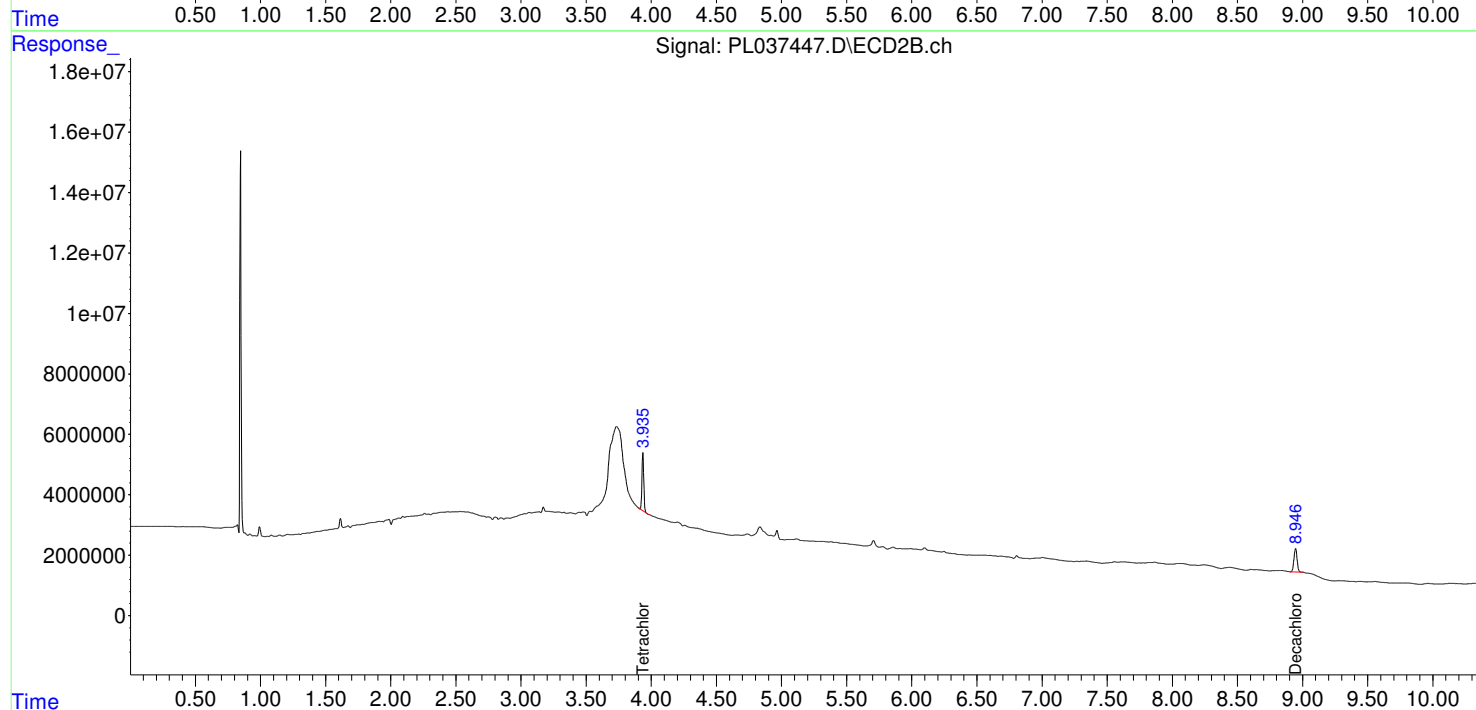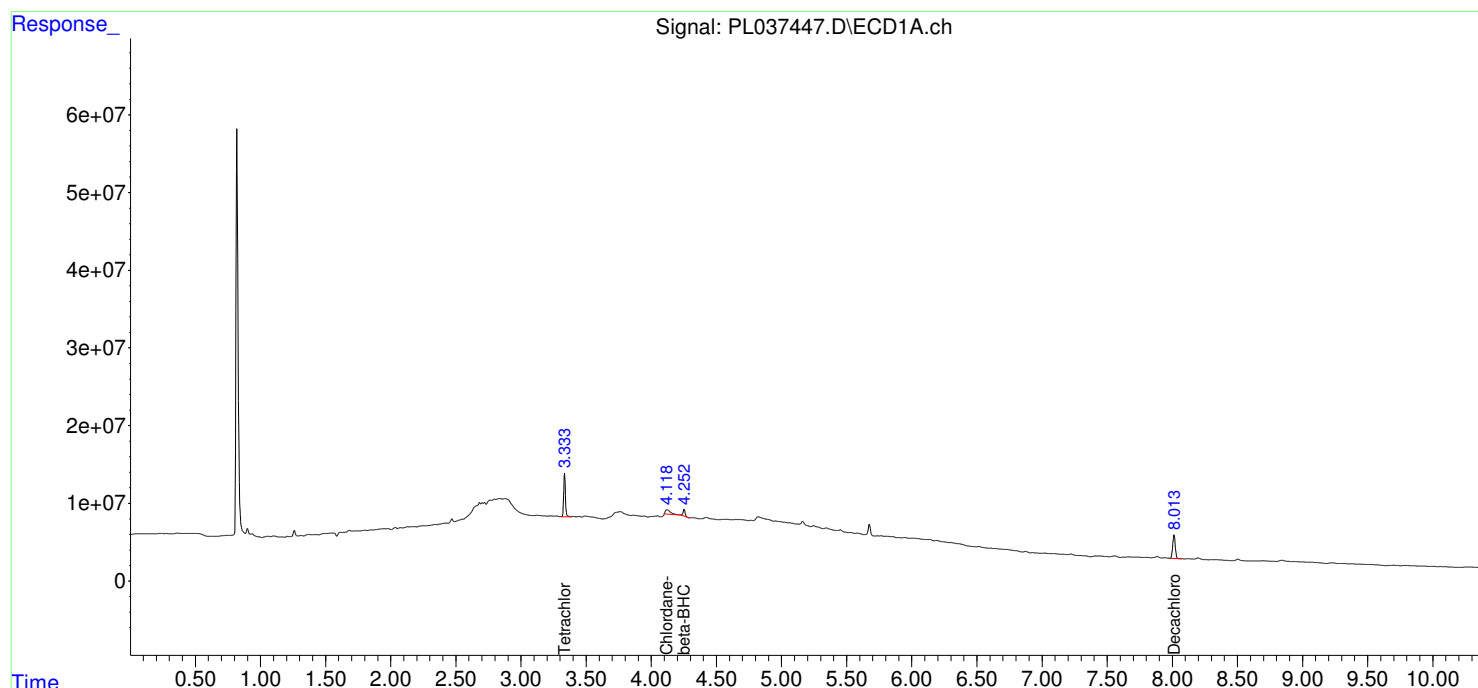


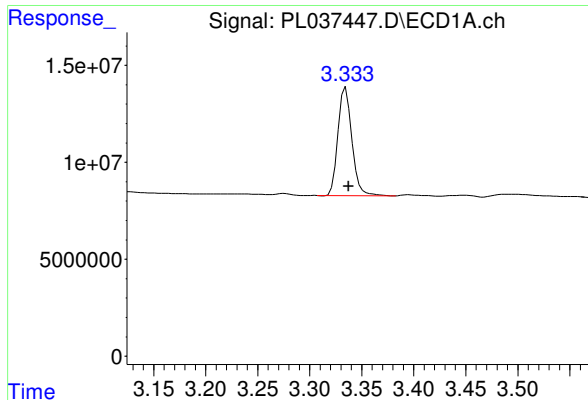

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 52216007
Conc: 6.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

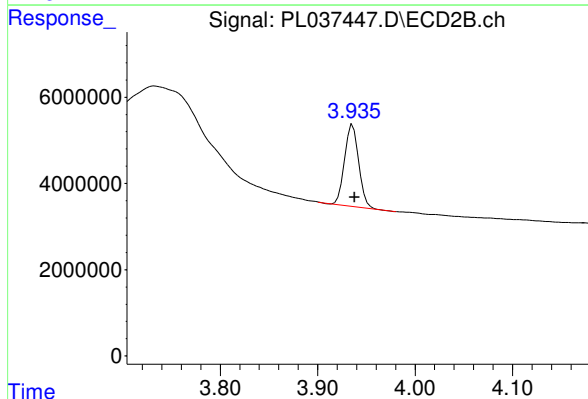


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 18931981
Conc: 6.84 ng/ml

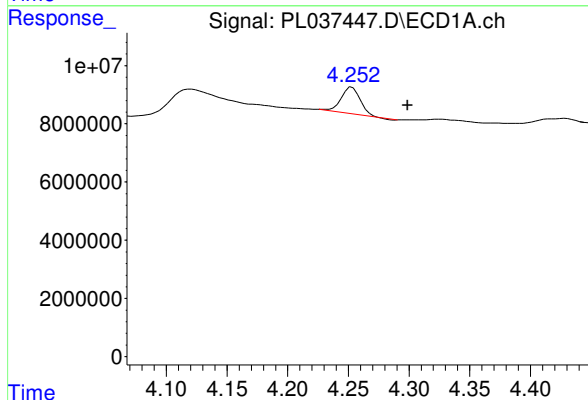


#6 beta-BHC

R.T.: 4.253 min
Delta R.T.: -0.046 min
Response: 10079678
Conc: 2.21 ng/ml

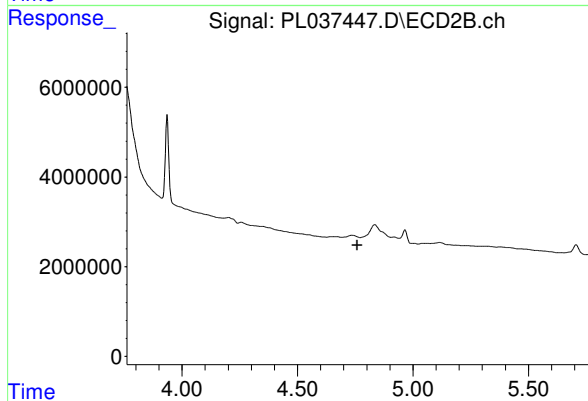

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

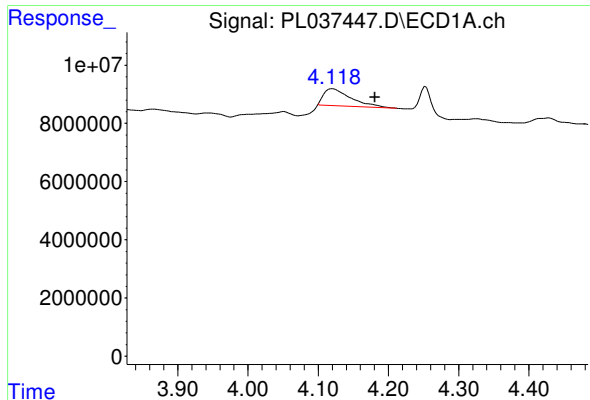

#23 Chlordane-1


R.T.: 4.120 min
Delta R.T.: -0.061 min
Response: 15620665
Conc: 50.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

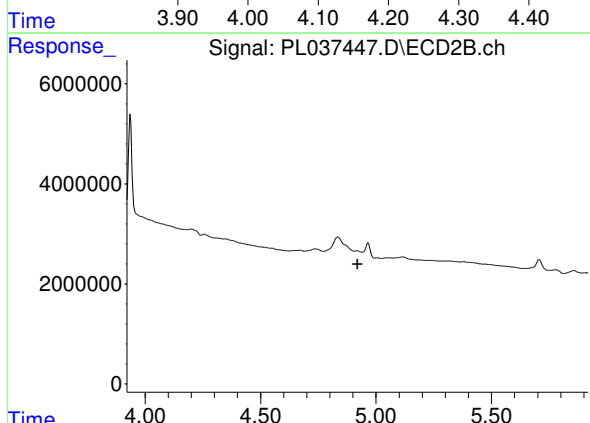


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.921 min
Response: 0
Conc: N.D.

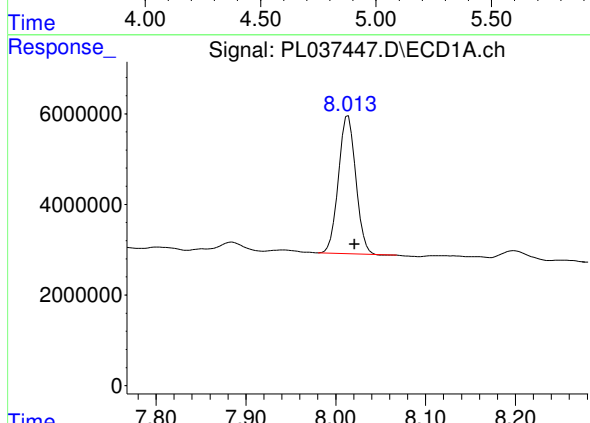

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.007 min
Response: 40968787
Conc: 6.79 ng/ml

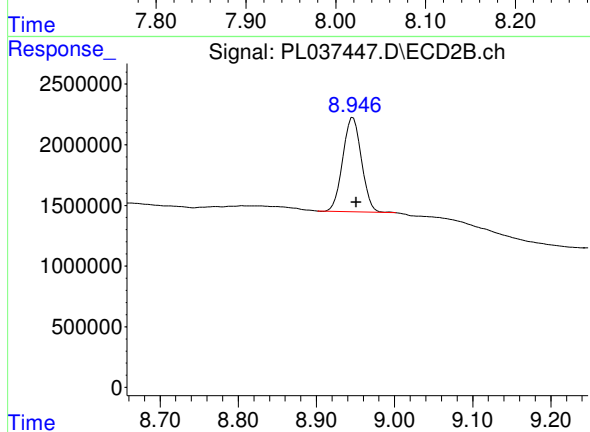

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 12906162
Conc: 6.51 ng/ml