

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
 Data File : PL037450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 20:38
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 05:13:54 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.335	3.936	122.7E6	42753334	15.516	15.453
28) SA Decachlor...	8.015	8.948	97617006	32922316	16.178	16.594
Target Compounds						
8) B Heptachlo...	0.000	5.780	0	16381953	N.D.	5.747 #
12) B 4,4'-DDE	0.000	6.304f	0	236597	N.D.	0.093 #
14) MA Endrin	5.850	0.000	17758142	0	2.254	N.D. #
21) B Endrin ke...	6.935f	0.000	304.2E6	0	42.777	N.D. #
24) Chlordane-2	0.000	5.317	0	21481805	N.D.	169.749 #
27) Chlordane-5	5.850	0.000	17758142	0	135.695	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
Data File : PL037450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 20:38
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 05:13:54 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

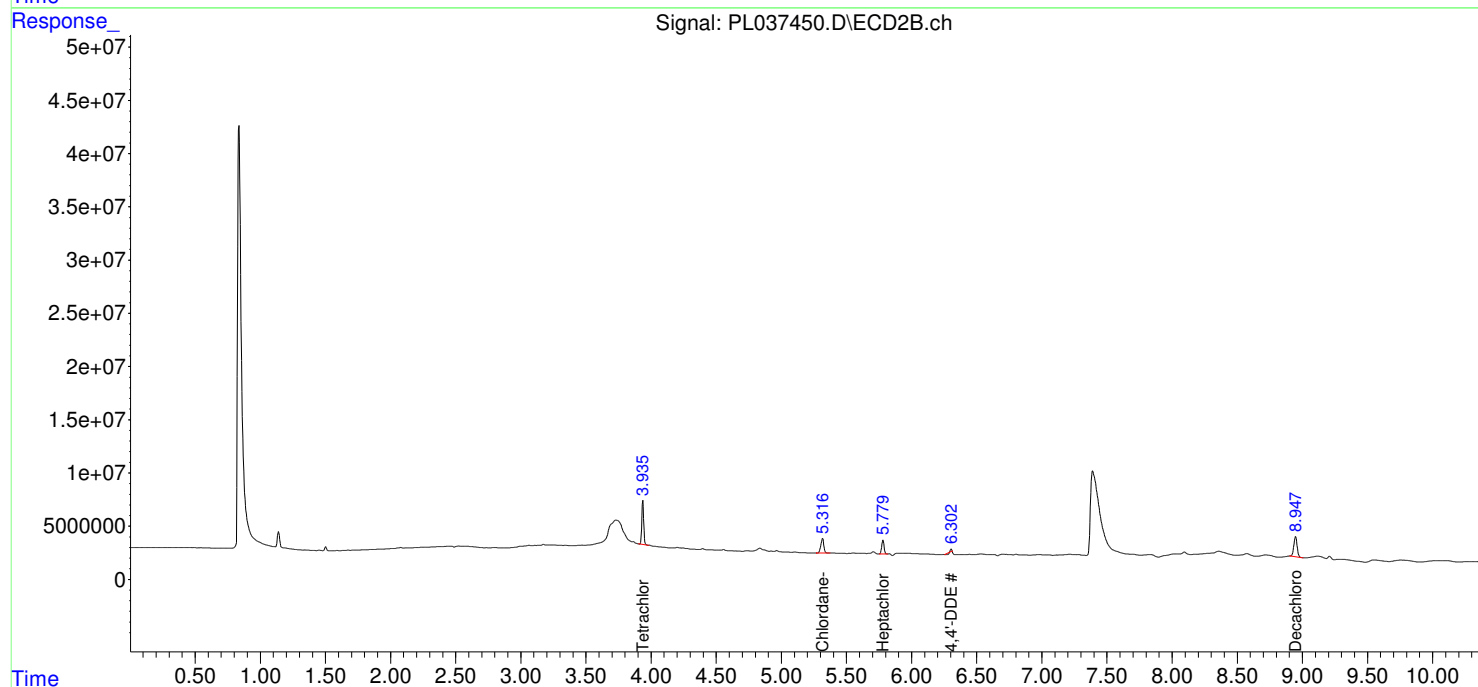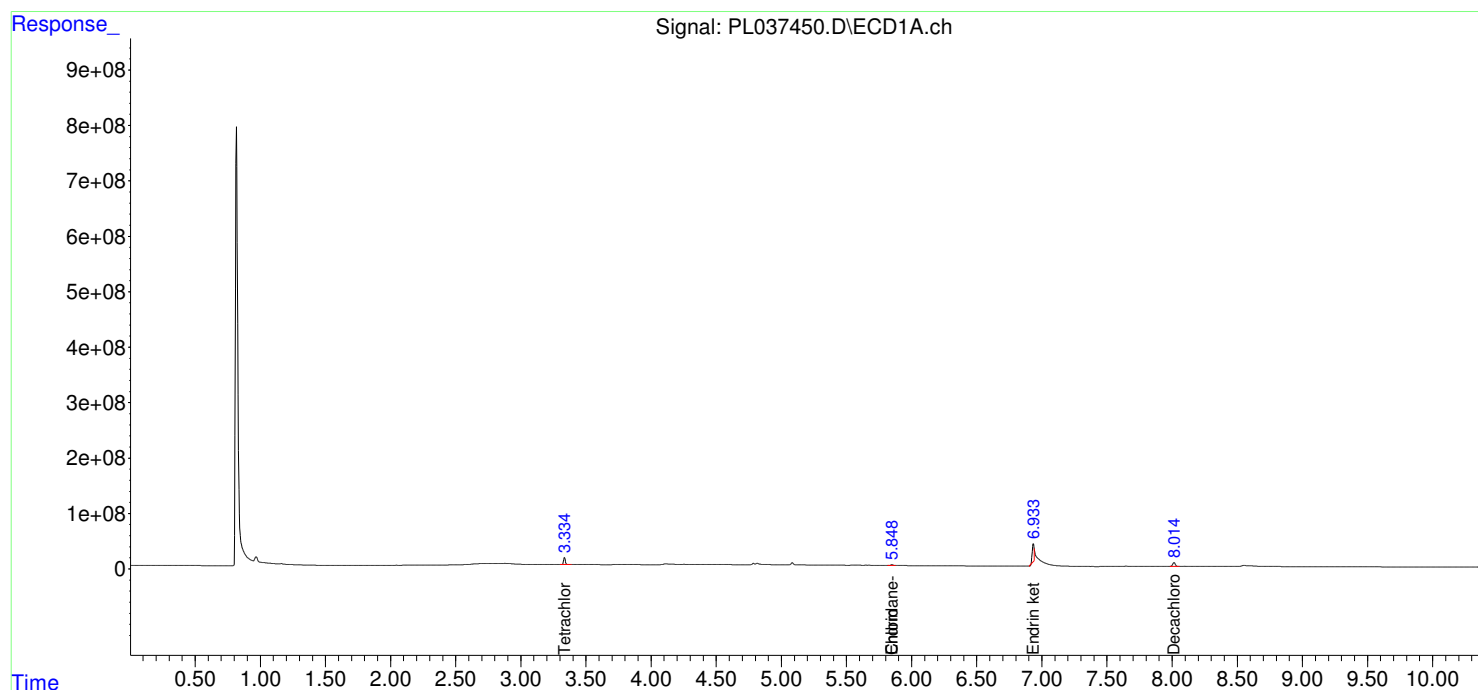


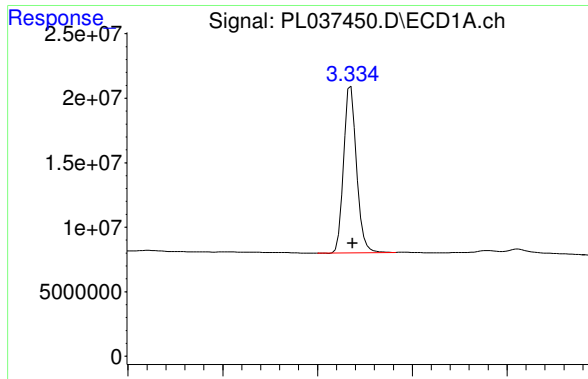

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 122736255
Conc: 15.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

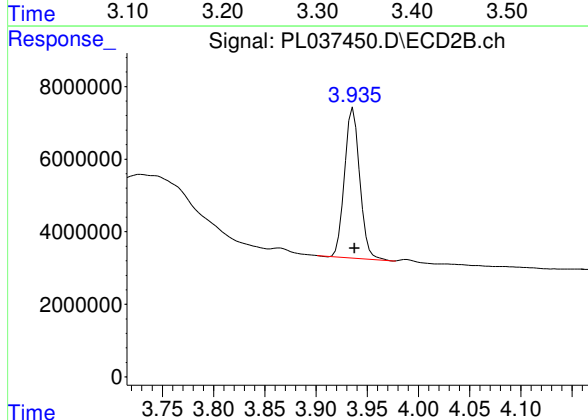


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.001 min
Response: 42753334
Conc: 15.45 ng/ml

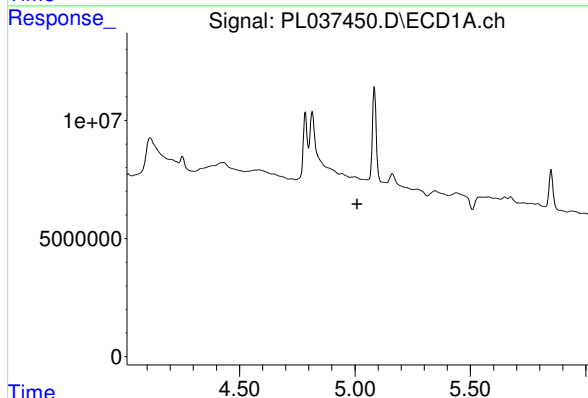


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.010 min
Response: 0
Conc: N.D.

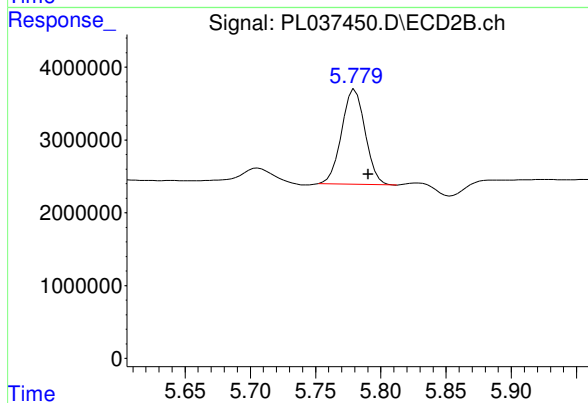

#8 Heptachlor epoxide


R.T.: 5.780 min
Delta R.T.: -0.010 min
Response: 16381953
Conc: 5.75 ng/ml

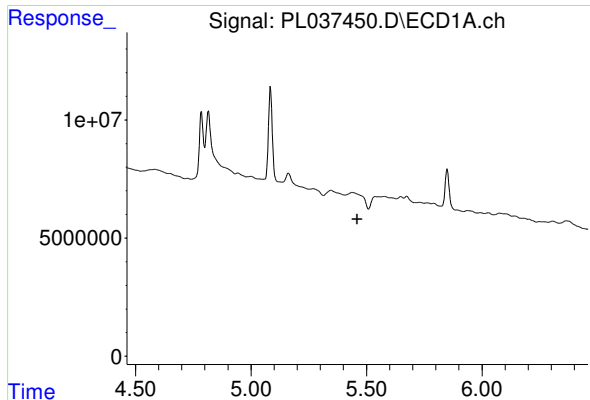

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

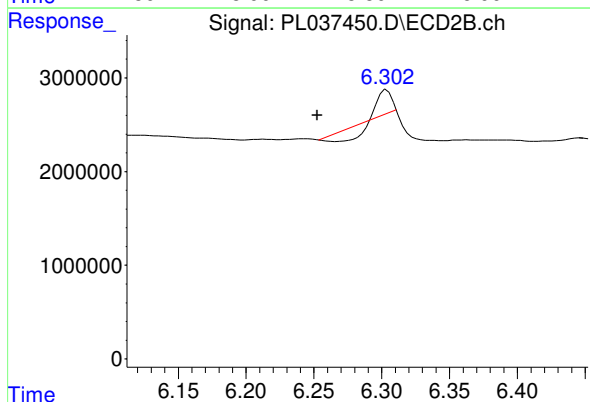


#12 4,4'-DDE

R.T.: 6.304 min
Delta R.T.: 0.051 min
Response: 236597
Conc: 0.09 ng/ml

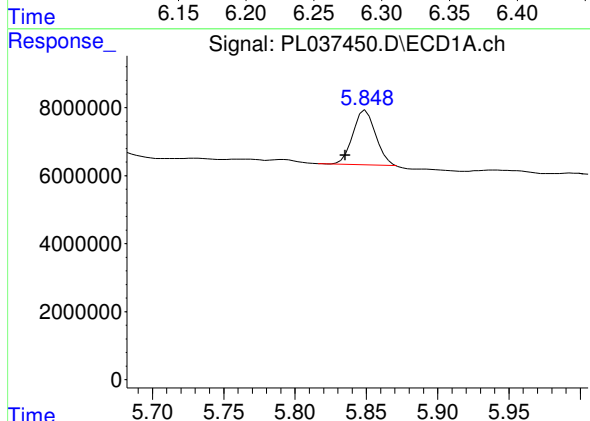


#14 Endrin

R.T.: 5.850 min
Delta R.T.: 0.015 min
Response: 17758142
Conc: 2.25 ng/ml

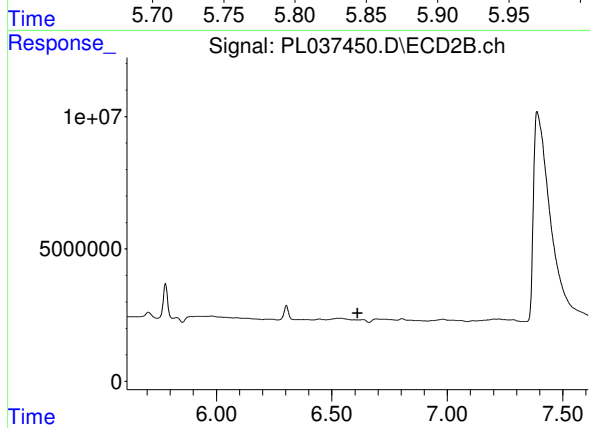

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

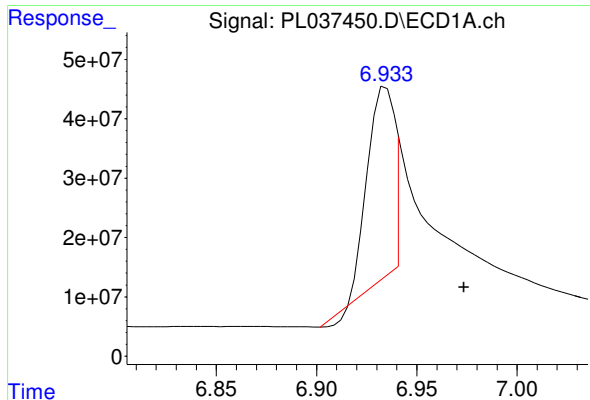

#21 Endrin ketone


R.T.: 6.935 min
Delta R.T.: -0.039 min
Response: 304215287
Conc: 42.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

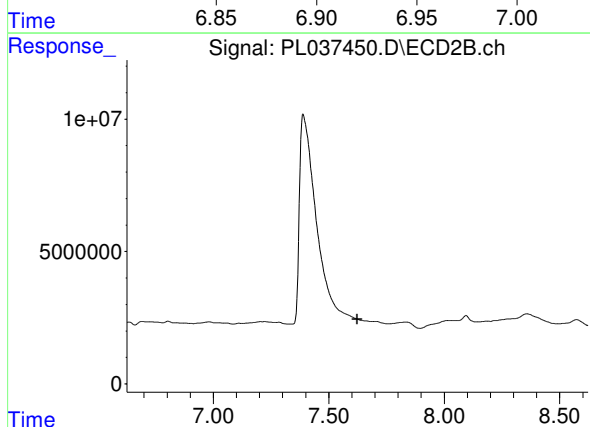


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.623 min
Response: 0
Conc: N.D.

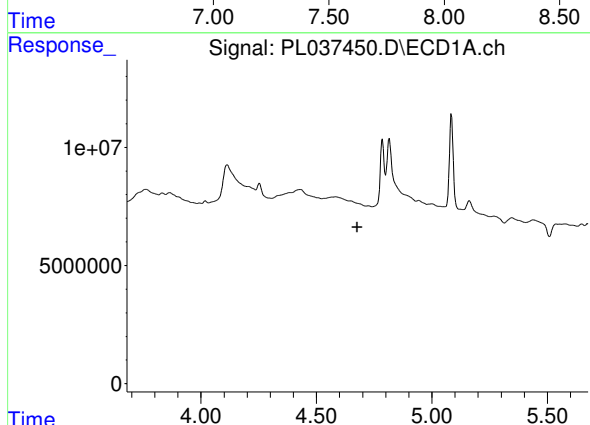


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.676 min
Response: 0
Conc: N.D.

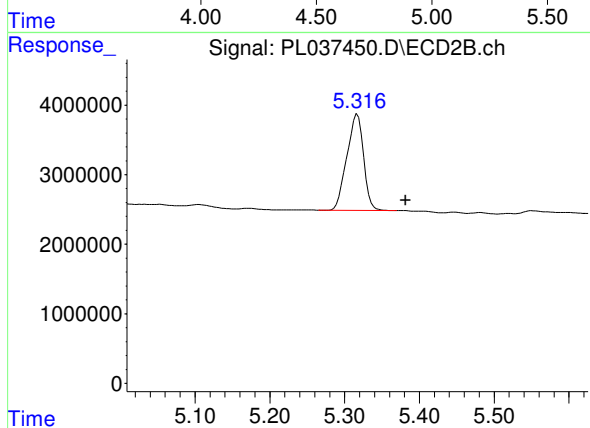

#24 Chlordane-2


R.T.: 5.317 min
Delta R.T.: -0.065 min
Response: 21481805
Conc: 169.75 ng/ml

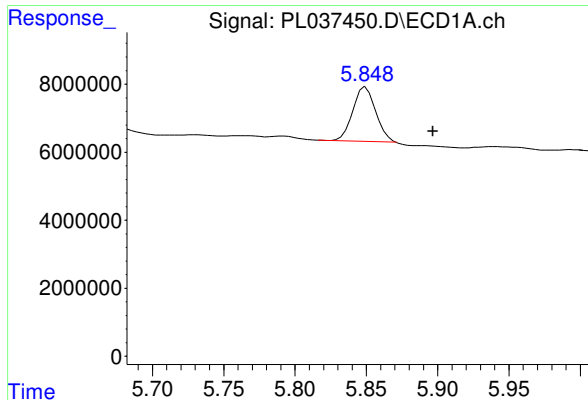

#27 Chlordane-5


R.T.: 5.850 min
Delta R.T.: -0.047 min
Response: 17758142
Conc: 135.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

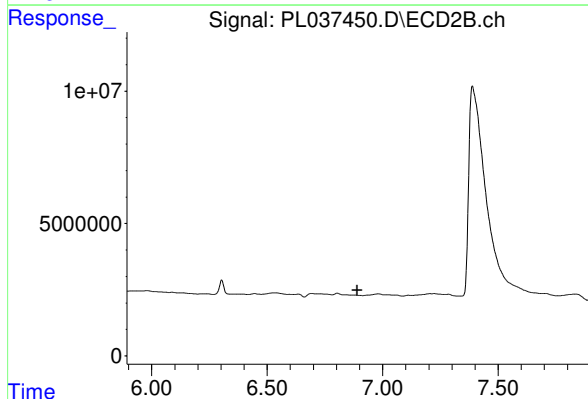


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.889 min
Response: 0
Conc: N.D.

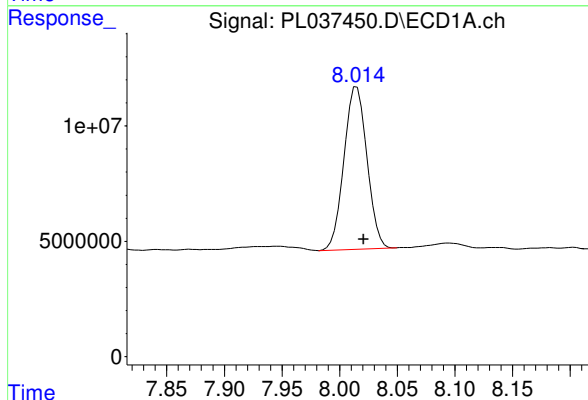

#28 Decachlorobiphenyl

R.T.: 8.015 min
Delta R.T.: -0.006 min
Response: 97617006
Conc: 16.18 ng/ml

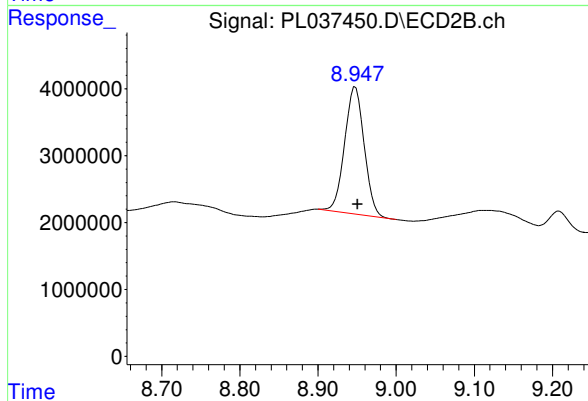

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 32922316
Conc: 16.59 ng/ml