

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
 Data File : PL037431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 16:12
 Operator : UA\AJ
 Sample : J3684-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2-S

Manual Integrations
 APPROVED

ugo
 6/27/2018 10:53:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 05:12:33 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.335	3.936	82113497	27815868	10.381	10.054
28) SA Decachlor...	8.014	8.947	57290483	18944769	9.495	9.549
Target Compounds						
12) B 4,4'-DDE	5.453	6.249	25383839	5937999	2.874	2.334
17) MA 4,4'-DDT	6.198	7.029	23322656	7933688	3.612m	3.746

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
Data File : PL037431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 16:12
Operator : UA\AJ
Sample : J3684-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-2-S


Manual Integrations
APPROVED

ugo
6/27/2018 10:53:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 05:12:33 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

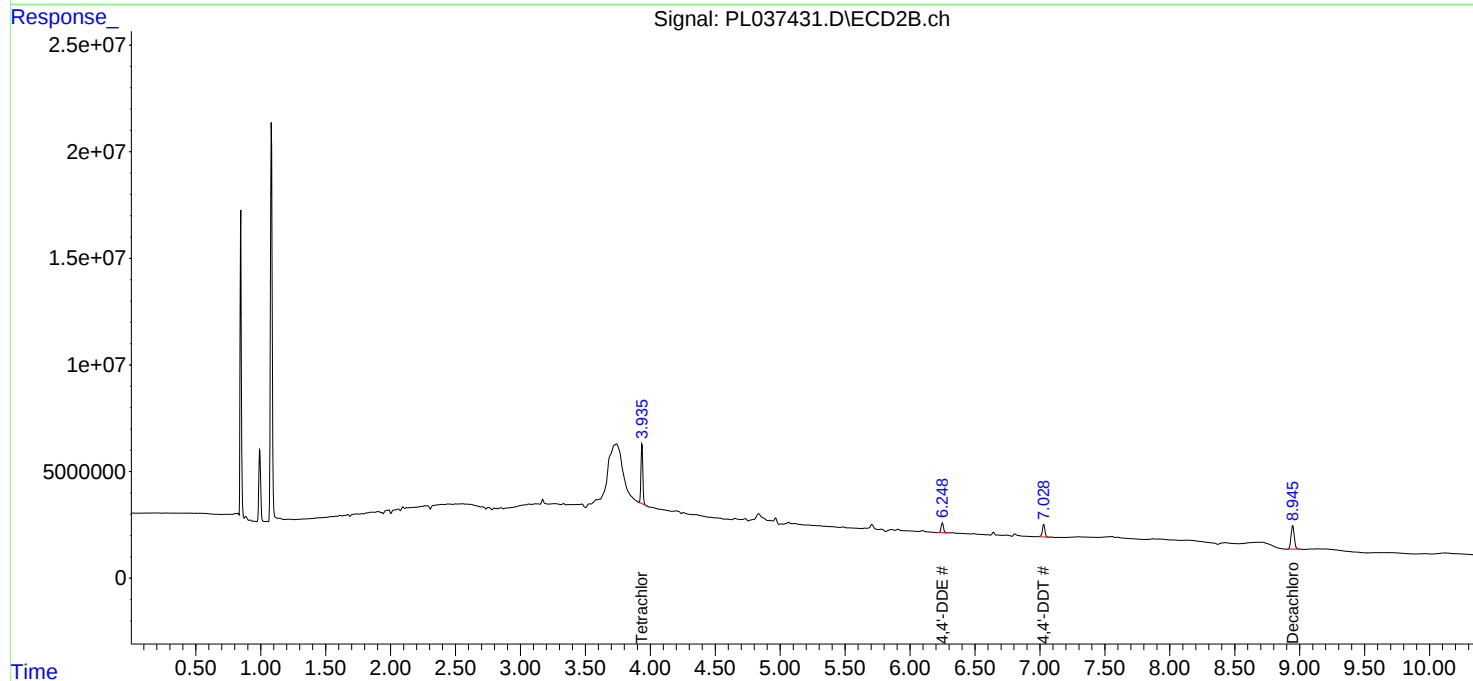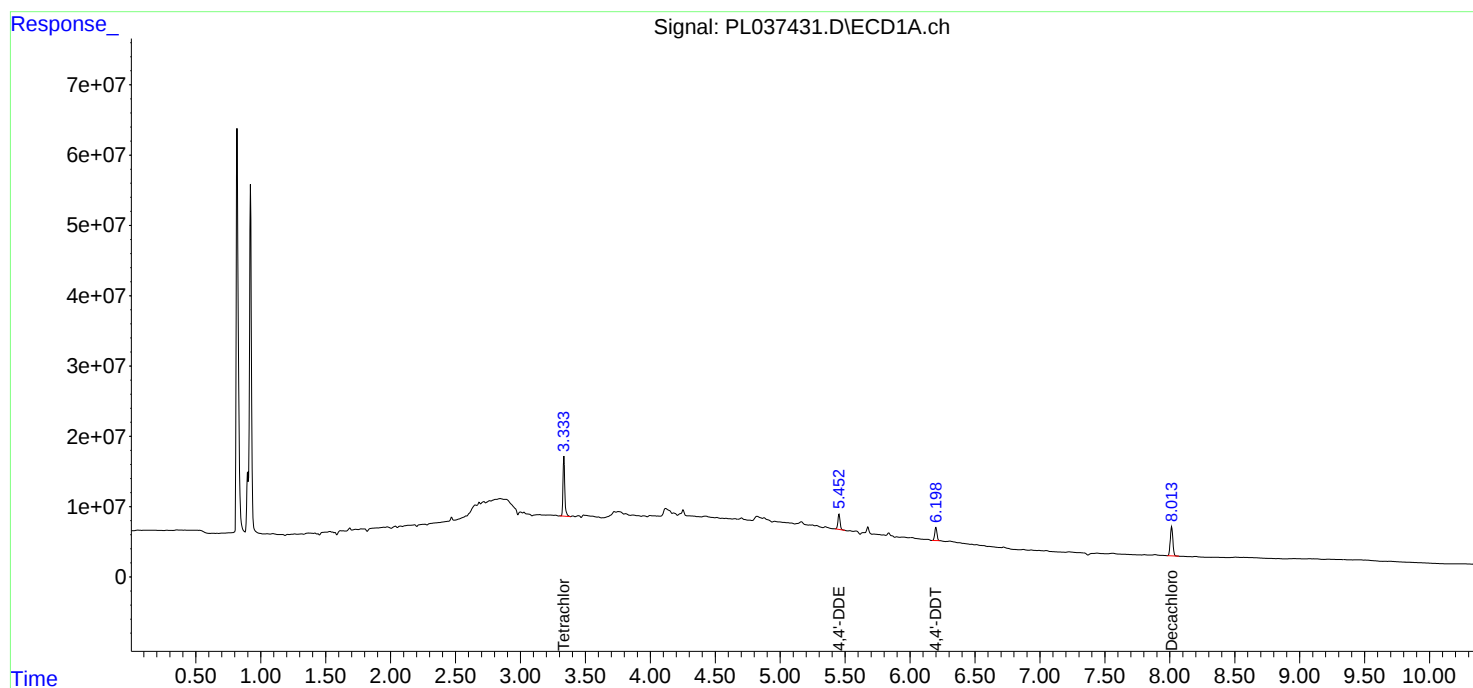

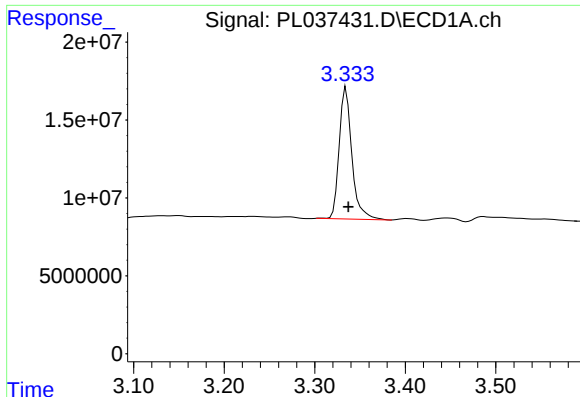


#1 Tetrachloro-m-xylene

R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 82113497
Conc: 10.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-S


Manual Integrations
APPROVED

ugo
6/27/2018 10:53:13 AM

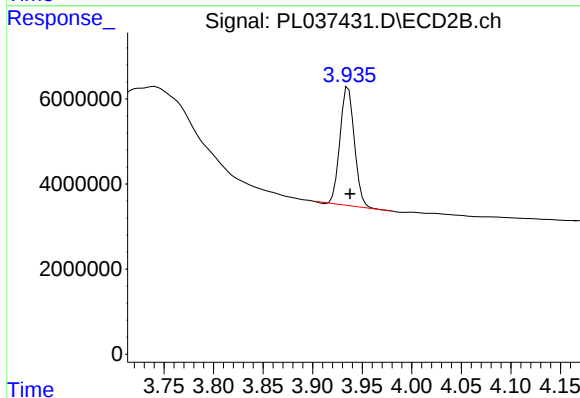


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 27815868
Conc: 10.05 ng/ml

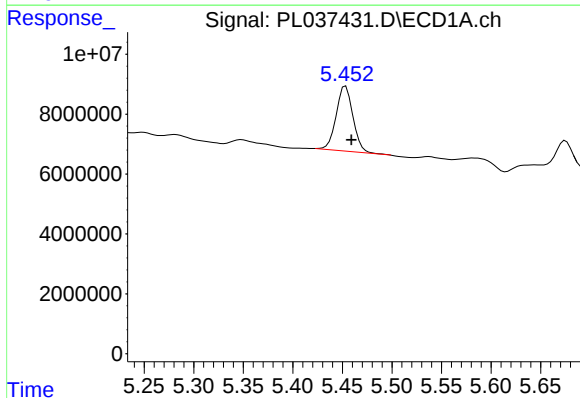


#12 4,4'-DDE

R.T.: 5.453 min
Delta R.T.: -0.006 min
Response: 25383839
Conc: 2.87 ng/ml

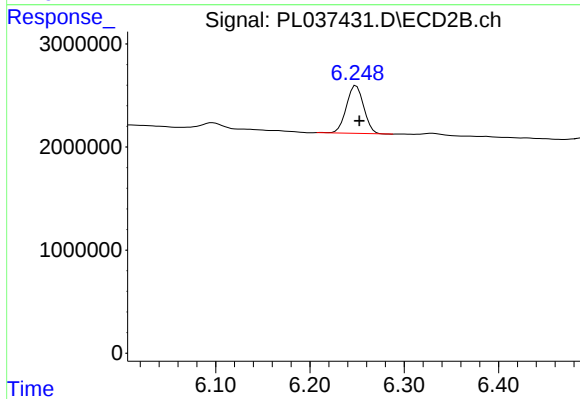

#12 4,4'-DDE

R.T.: 6.249 min
Delta R.T.: -0.003 min
Response: 5937999
Conc: 2.33 ng/ml

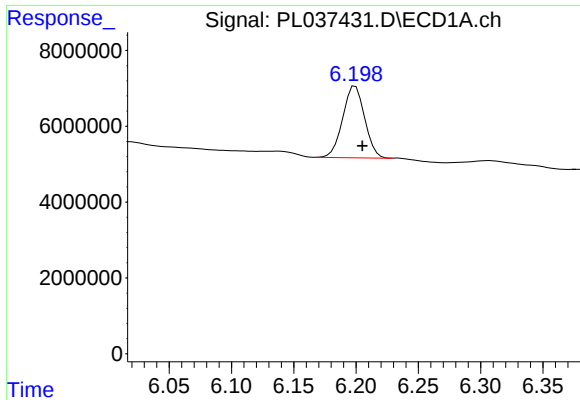


#17 4,4'-DDT

R.T.: 6.198 min
Delta R.T.: -0.007 min
Response: 23322656
Conc: 3.61 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-2-S


Manual Integrations
APPROVED

ugo
6/27/2018 10:53:13 AM

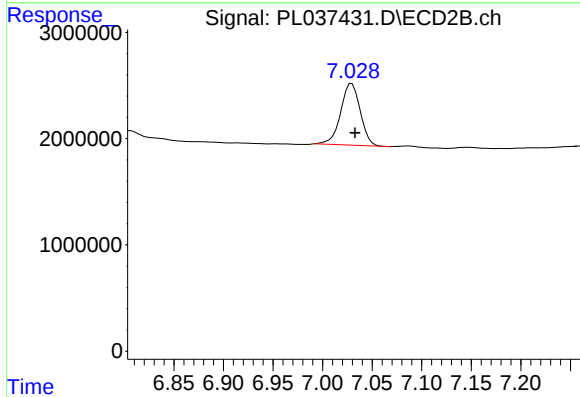


#17 4,4'-DDT

R.T.: 7.029 min
Delta R.T.: -0.003 min
Response: 7933688
Conc: 3.75 ng/ml

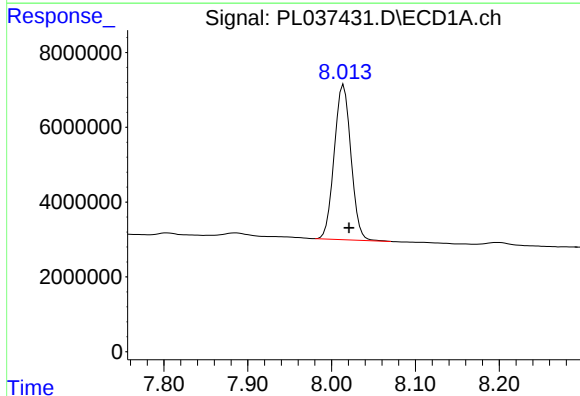

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.006 min
Response: 57290483
Conc: 9.49 ng/ml

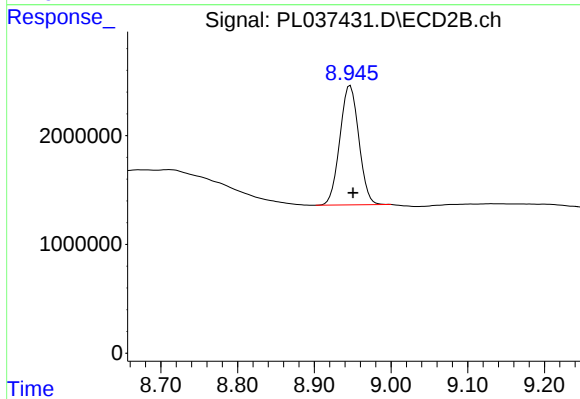

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 18944769
Conc: 9.55 ng/ml