

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
 Data File : PL037439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 18:04
 Operator : UA\AJ
 Sample : J3712-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-031

Manual Integrations
 APPROVED

ugo
 6/27/2018 10:54:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 05:13:06 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.936	153.2E6	53936540	19.364	19.495
28)	SA Decachlor...	8.014	8.947	100.9E6	31328838	16.722	15.791
Target Compounds							
10)	B gamma-Chl...	5.228	6.018	8819729	2535905	0.942	0.900m
11)	B alpha-Chl...	5.283	6.095	11221222	5811667	1.236	2.019m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062618\
Data File : PL037439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 18:04
Operator : UA\AJ
Sample : J3712-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FK-PS-01-031


Manual Integrations
APPROVED

ugo
6/27/2018 10:54:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 05:13:06 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

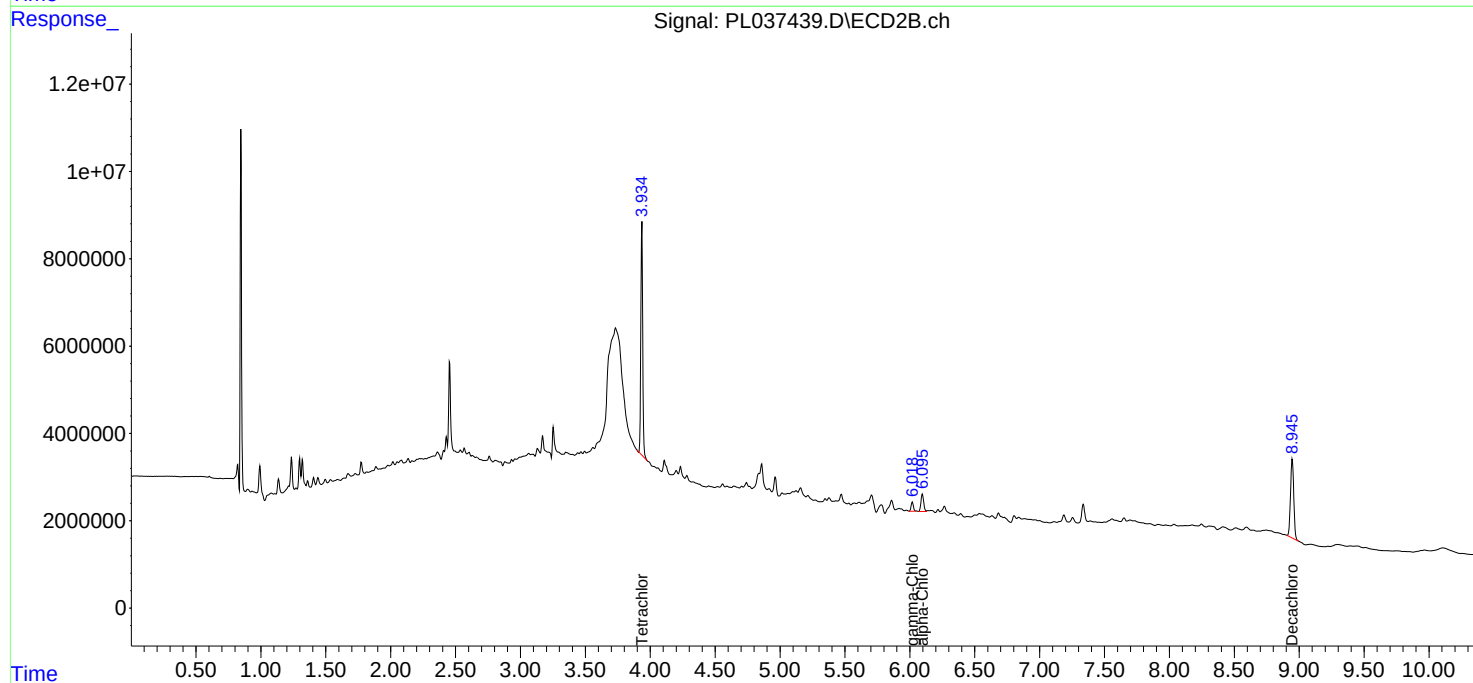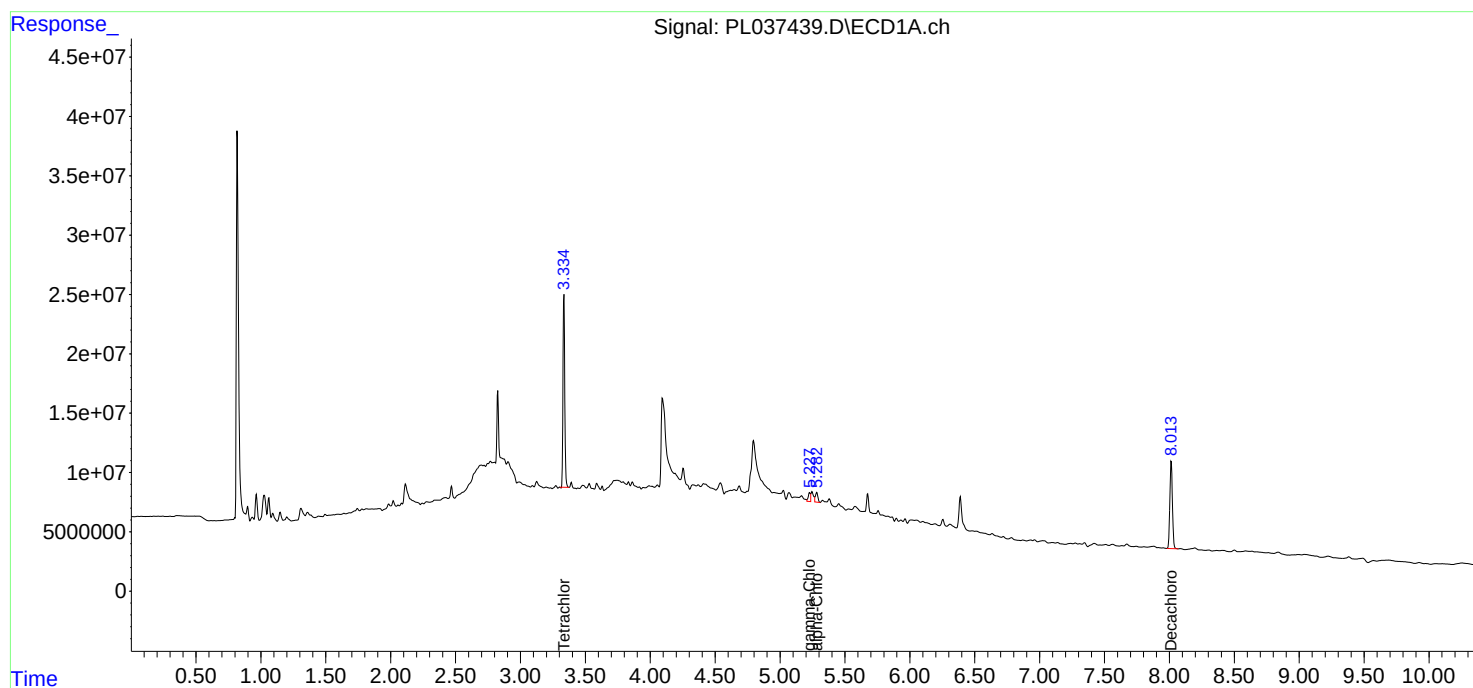

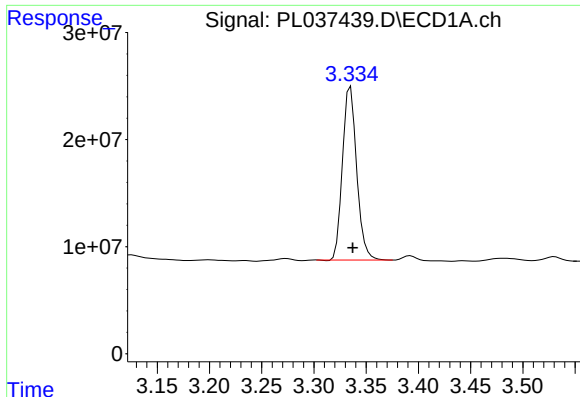


#1 Tetrachloro-m-xylene

R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 153173861
Conc: 19.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-031


Manual Integrations
APPROVED

ugo
6/27/2018 10:54:28 AM

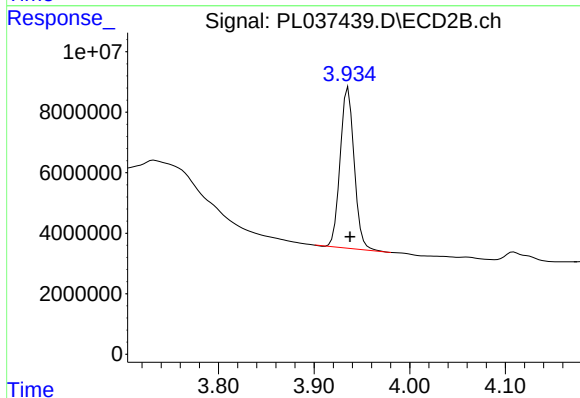


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 53936540
Conc: 19.49 ng/ml

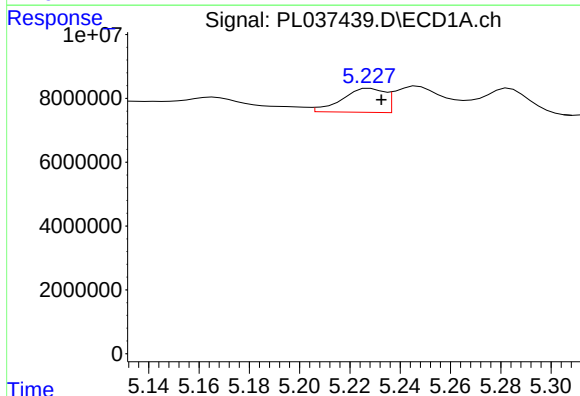


#10 gamma-Chlordane

R.T.: 5.228 min
Delta R.T.: -0.004 min
Response: 8819729
Conc: 0.94 ng/ml

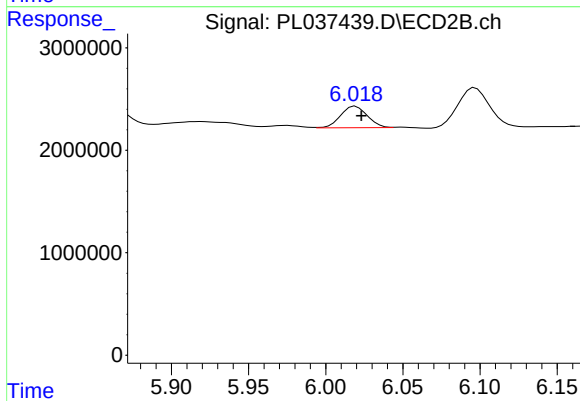

#10 gamma-Chlordane

R.T.: 6.018 min
Delta R.T.: -0.005 min
Response: 2535905
Conc: 0.90 ng/ml m

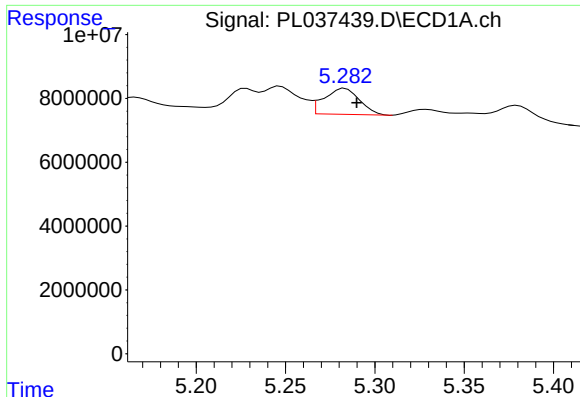


#11 alpha-Chlordane

R.T.: 5.283 min
Delta R.T.: -0.006 min
Response: 11221222
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-031


Manual Integrations
APPROVED

ugo
6/27/2018 10:54:28 AM

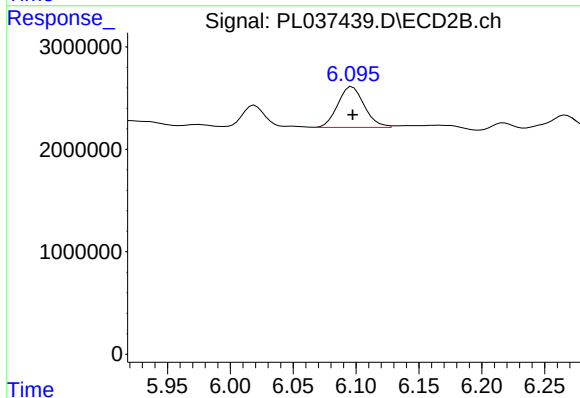


#11 alpha-Chlordane

R.T.: 6.095 min
Delta R.T.: -0.002 min
Response: 5811667
Conc: 2.02 ng/ml m

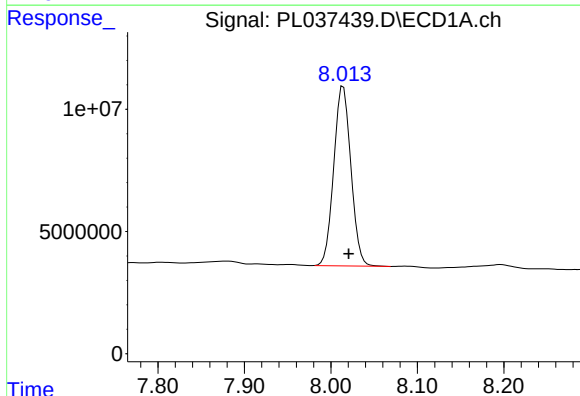

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.006 min
Response: 100899476
Conc: 16.72 ng/ml

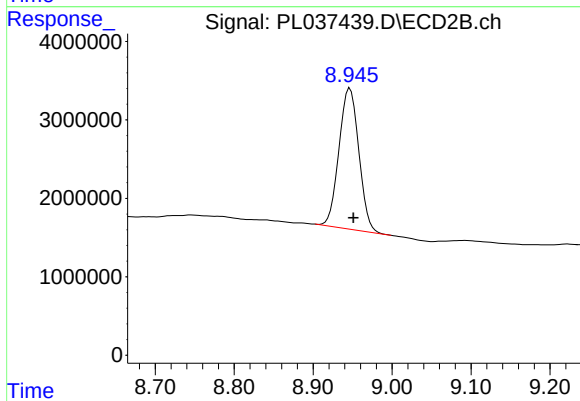

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 31328838
Conc: 15.79 ng/ml