

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062619\
 Data File : PL049883.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2019 17:44
 Operator : SM\AJ
 Sample : K3505-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-013-B212-062019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 01:00:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.936	239.4E6	62777484	21.228	20.504
28)	SA Decachlor...	7.987	8.966	231.4E6	65287356	18.210	19.448
Target Compounds							
9)	A Endosulfan I	5.347f	0.000	31140885	0	2.013	N.D. #
10)	B gamma-Chl...	0.000	6.024	0	7526620	N.D.	2.020 #
25)	Chlordane-3	0.000	6.024	0	7526620	N.D.	15.125 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062619\
Data File : PL049883.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2019 17:44
Operator : SM\AJ
Sample : K3505-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-013-B212-062019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 01:00:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

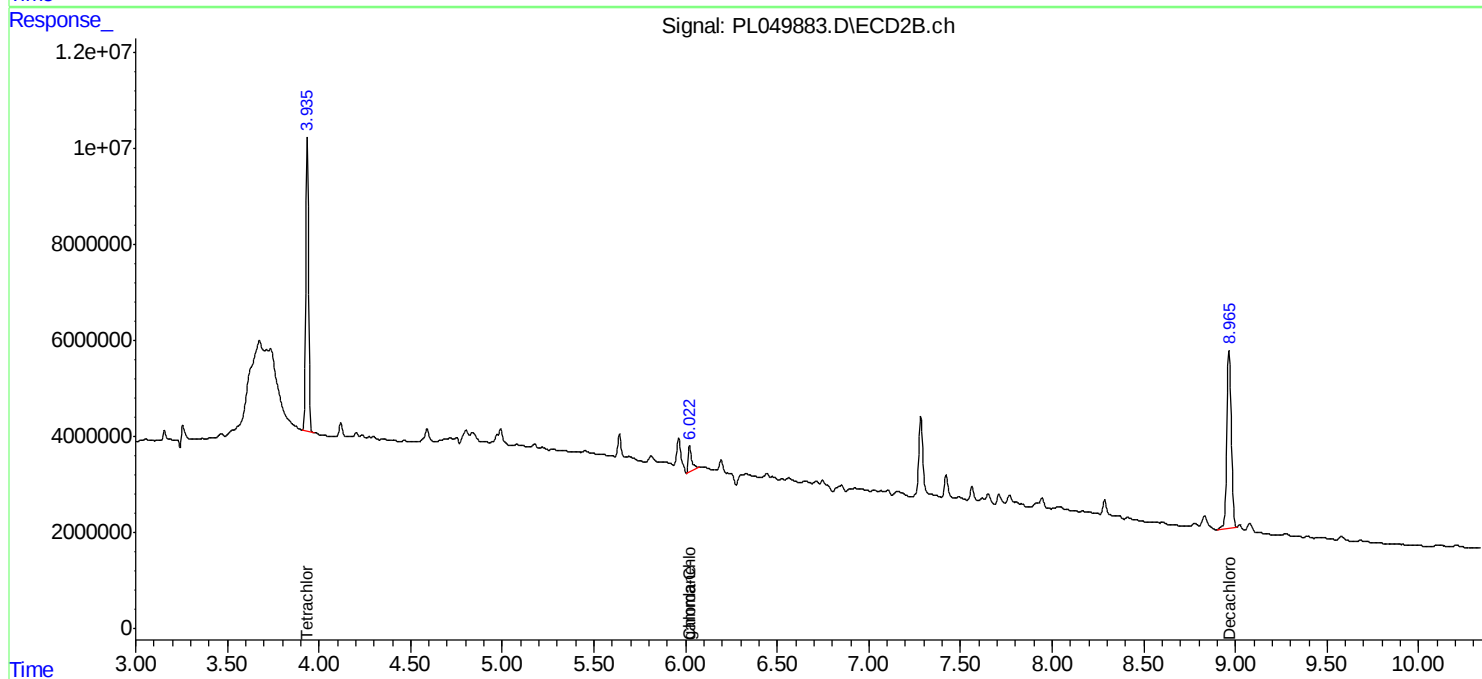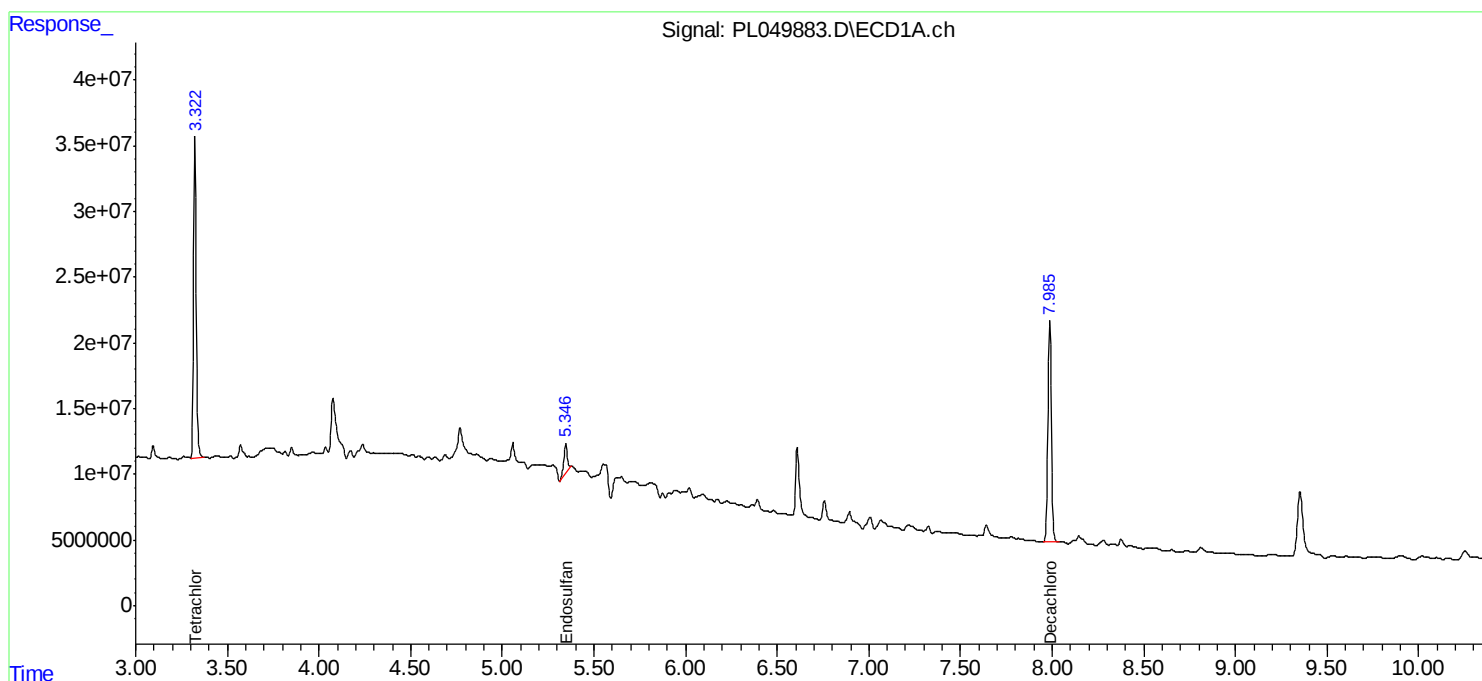


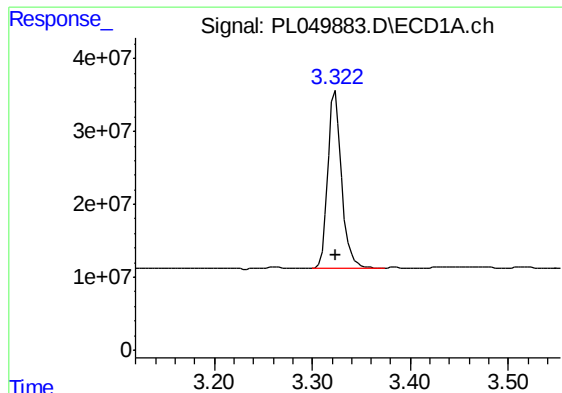

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 239398871
Conc: 21.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-B212-062019

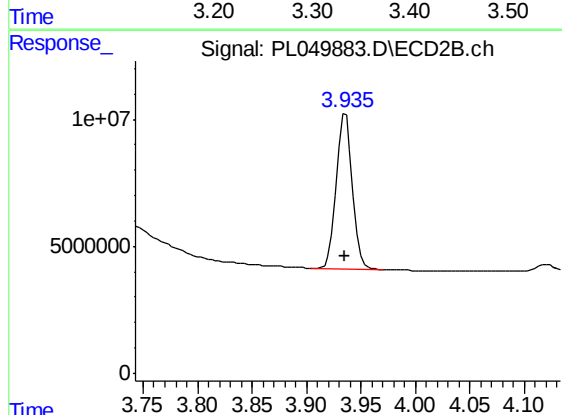


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 62777484
Conc: 20.50 ng/ml

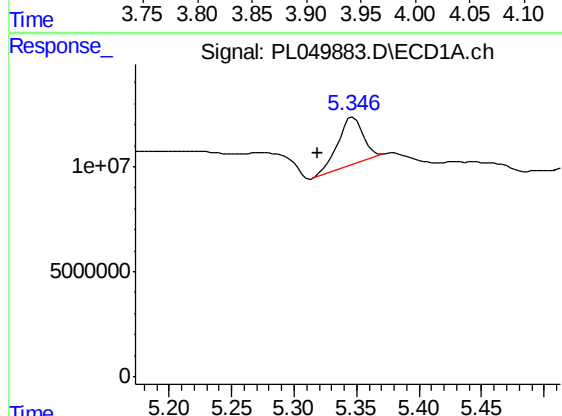


#9 Endosulfan I

R.T.: 5.347 min
Delta R.T.: 0.029 min
Response: 31140885
Conc: 2.01 ng/ml

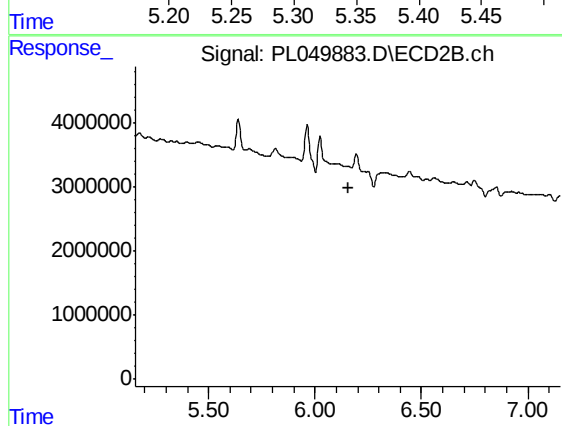

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

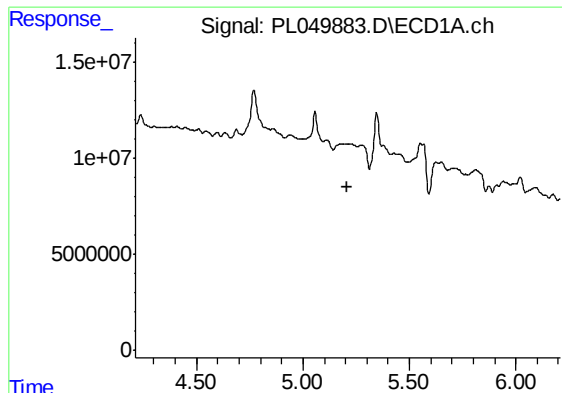

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-013-B212-062019

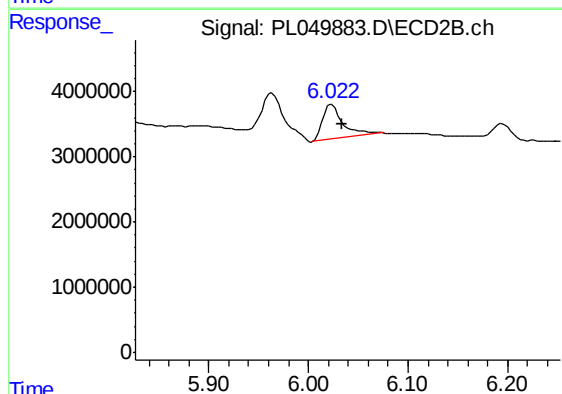


#10 gamma-Chlordane

R.T.: 6.024 min
Delta R.T.: -0.010 min
Response: 7526620
Conc: 2.02 ng/ml

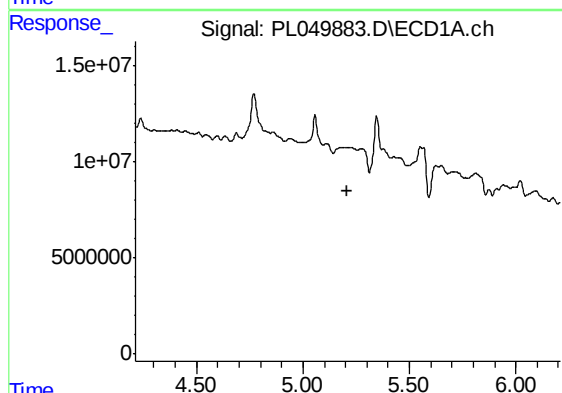


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.211 min
Response: 0
Conc: N.D.

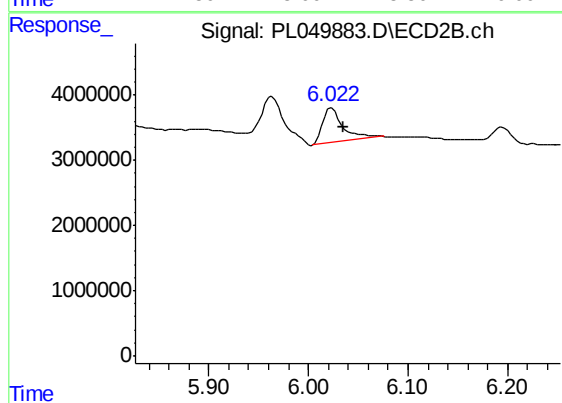

#25 Chlordane-3


R.T.: 6.024 min
Delta R.T.: -0.011 min
Response: 7526620
Conc: 15.13 ng/ml

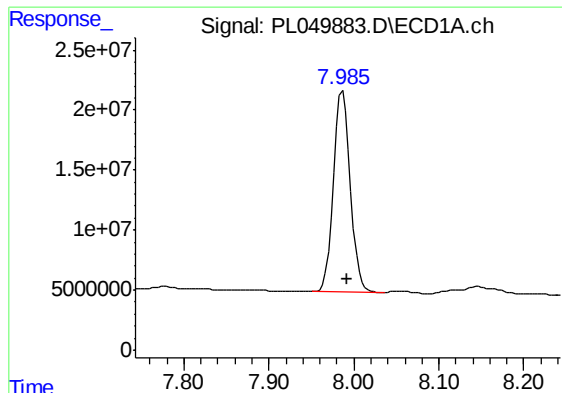

#28 Decachlorobiphenyl

R.T.: 7.987 min
Delta R.T.: -0.005 min
Response: 231383596
Conc: 18.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-B212-062019

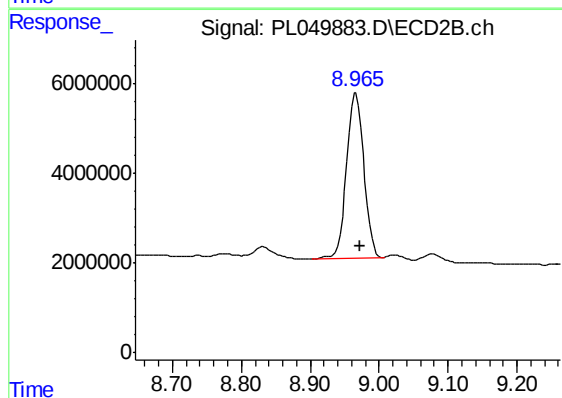

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: -0.007 min
Response: 65287356
Conc: 19.45 ng/ml