

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062619\
 Data File : PL049898.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2019 21:30
 Operator : SM\AJ
 Sample : K3531-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-GF-02-043-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 01:04:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.933	101.8E6	27498527	9.030	8.981
28)	SA Decachlor...	7.986	8.967	98238931	30709807	7.731	9.148
Target Compounds							
10)	B gamma-Chl...	5.227f	0.000	21921384	0	1.283	N.D. #
11)	B alpha-Chl...	0.000	6.104	0	10602469	N.D.	2.867 #
23)	Chlordane-1	4.162	0.000	20695067	0	36.334	N.D. #
25)	Chlordane-3	5.227f	0.000	21921384	0	11.671	N.D. #
26)	Chlordane-4	0.000	6.104	0	10602469	N.D.	17.839 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062619\
Data File : PL049898.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2019 21:30
Operator : SM\AJ
Sample : K3531-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
FK-GF-02-043-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 01:04:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

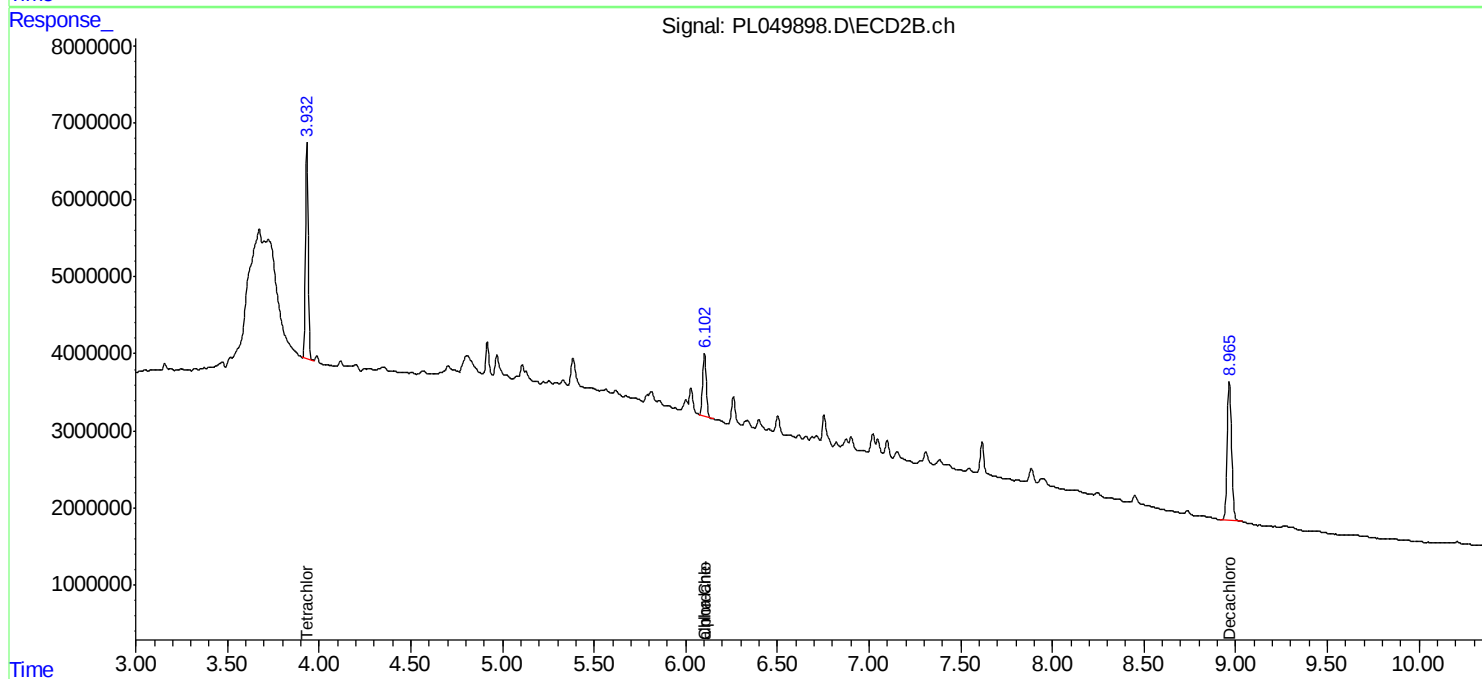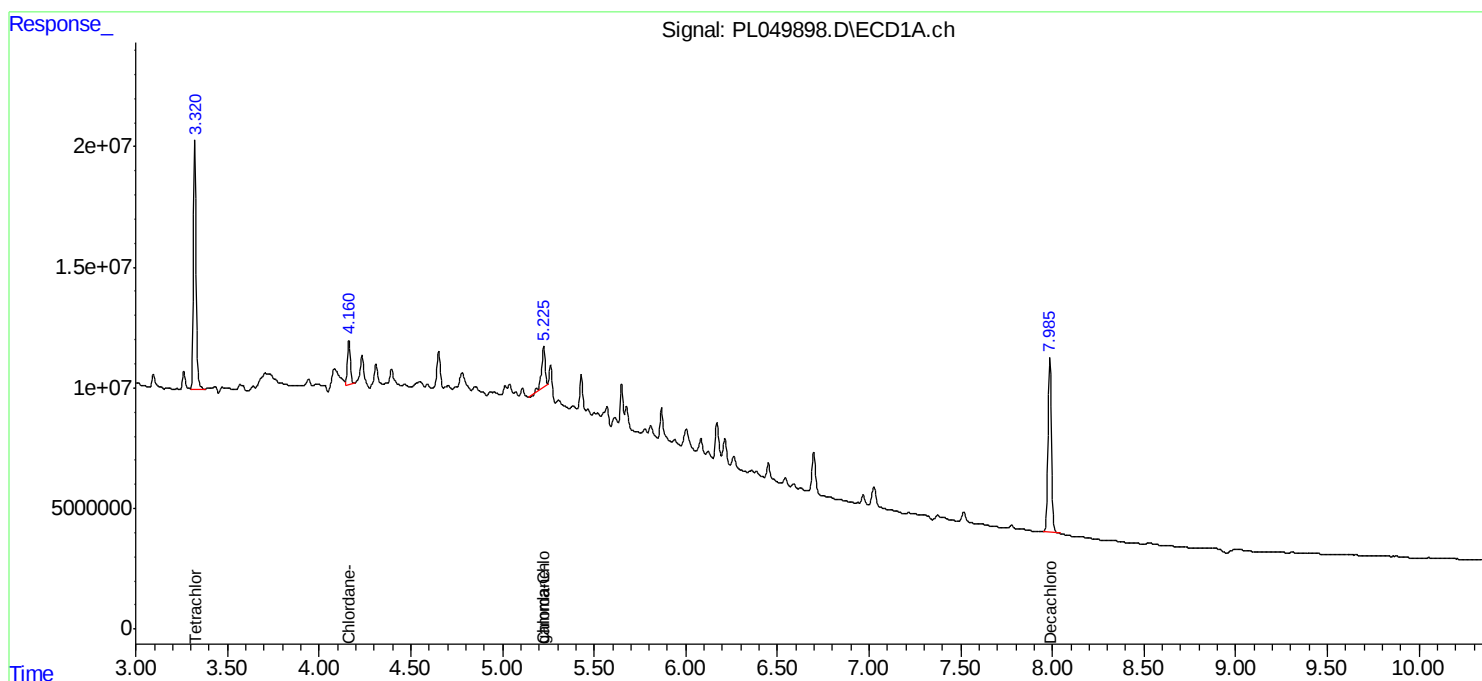


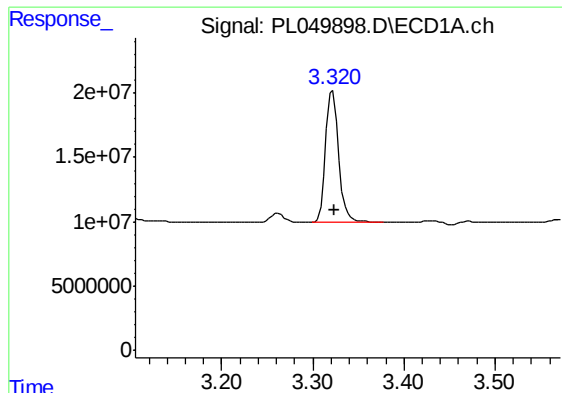

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 101832408
Conc: 9.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-GF-02-043-A

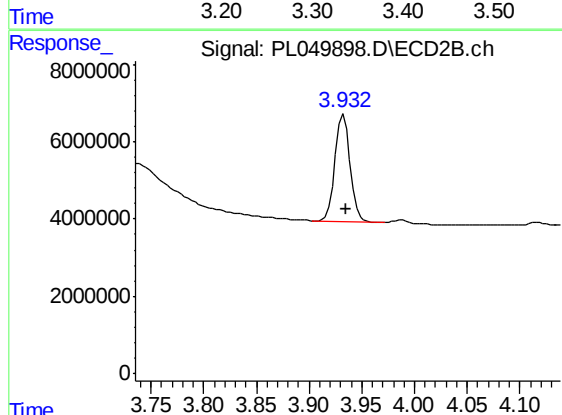


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.002 min
Response: 27498527
Conc: 8.98 ng/ml

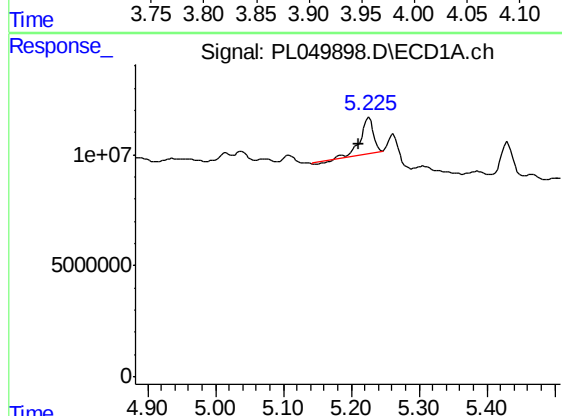


#10 gamma-Chlordane

R.T.: 5.227 min
Delta R.T.: 0.016 min
Response: 21921384
Conc: 1.28 ng/ml

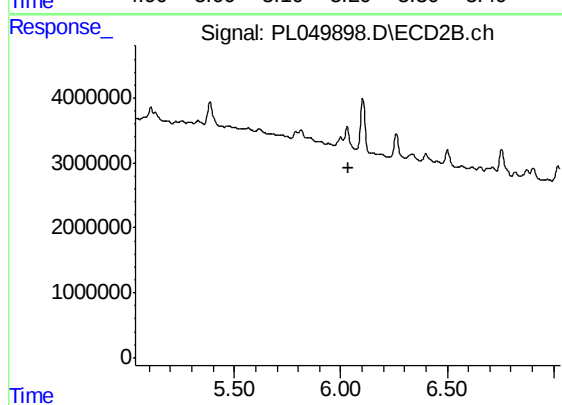

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.034 min
Response: 0
Conc: N.D.

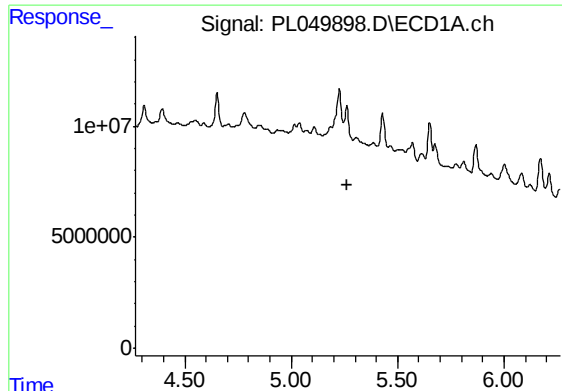

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-GF-02-043-A

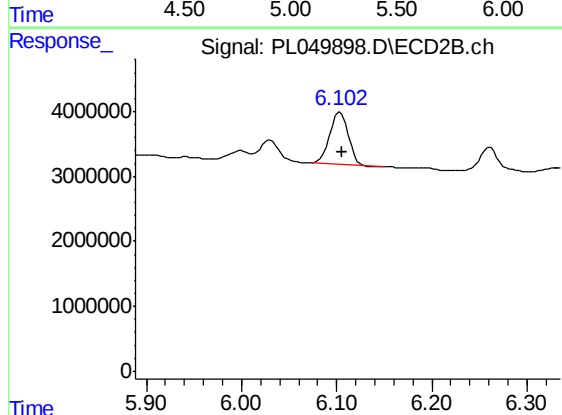


#11 alpha-Chlordane

R.T.: 6.104 min
Delta R.T.: -0.002 min
Response: 10602469
Conc: 2.87 ng/ml

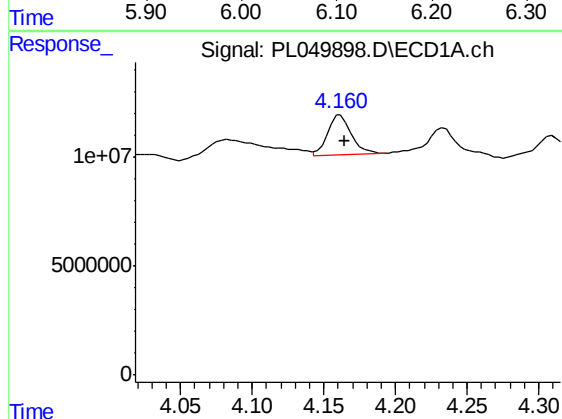


#23 Chlordane-1

R.T.: 4.162 min
Delta R.T.: -0.002 min
Response: 20695067
Conc: 36.33 ng/ml

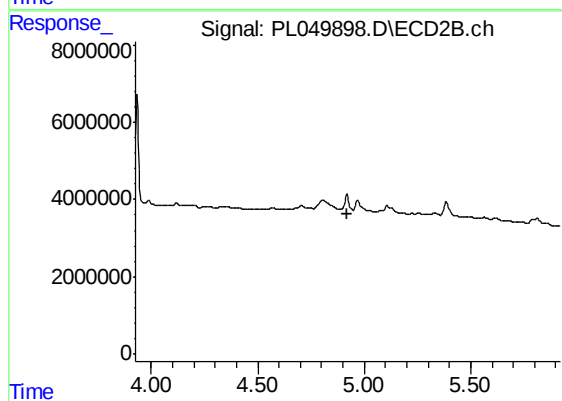

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

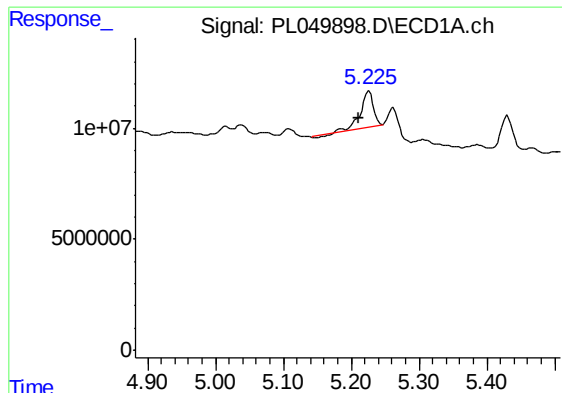

#25 Chlordane-3


R.T.: 5.227 min
Delta R.T.: 0.016 min
Response: 21921384
Conc: 11.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-GF-02-043-A

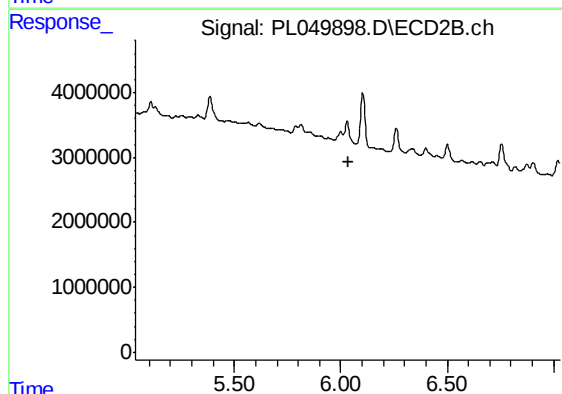


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

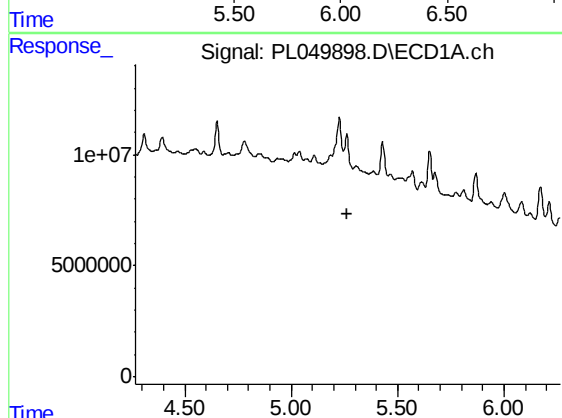


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.266 min
Response: 0
Conc: N.D.

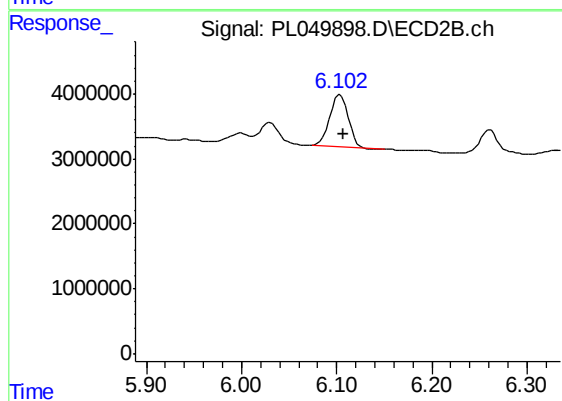

#26 Chlordane-4


R.T.: 6.104 min
Delta R.T.: -0.004 min
Response: 10602469
Conc: 17.84 ng/ml

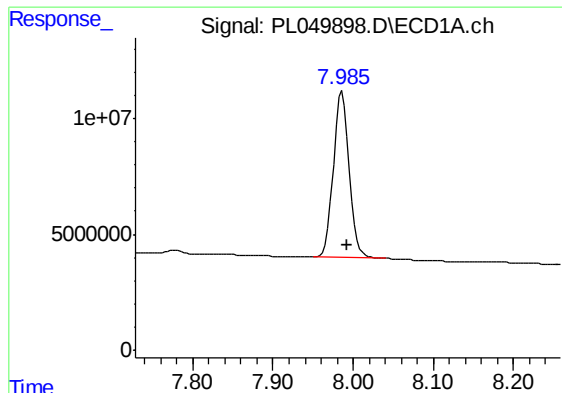

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.006 min
Response: 98238931
Conc: 7.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-GF-02-043-A

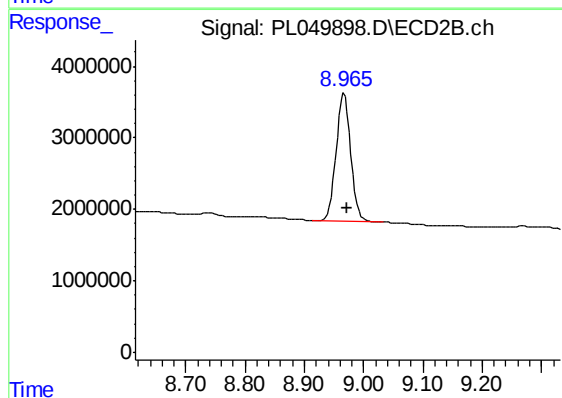

#28 Decachlorobiphenyl

R.T.: 8.967 min
Delta R.T.: -0.006 min
Response: 30709807
Conc: 9.15 ng/ml