

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062620\
 Data File : PL059543.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2020 16:54
 Operator : AJ\MA
 Sample : L2810-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-062420

Manual Integrations
 APPROVED

Ankita
 6/29/2020 2:31:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 23:49:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 22 14:09:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.069	37148174	54734406	20.671	21.207m
28)	SA Decachlor...	8.287	9.183	31992151	44046688	18.788	19.238

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062620\
Data File : PL059543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2020 16:54
Operator : AJ\MA
Sample : L2810-16
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
CL-01-062420


Manual Integrations
APPROVED

Ankita
6/29/2020 2:31:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 23:49:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062220.M
Quant Title : GC Extractables
QLast Update : Mon Jun 22 14:09:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

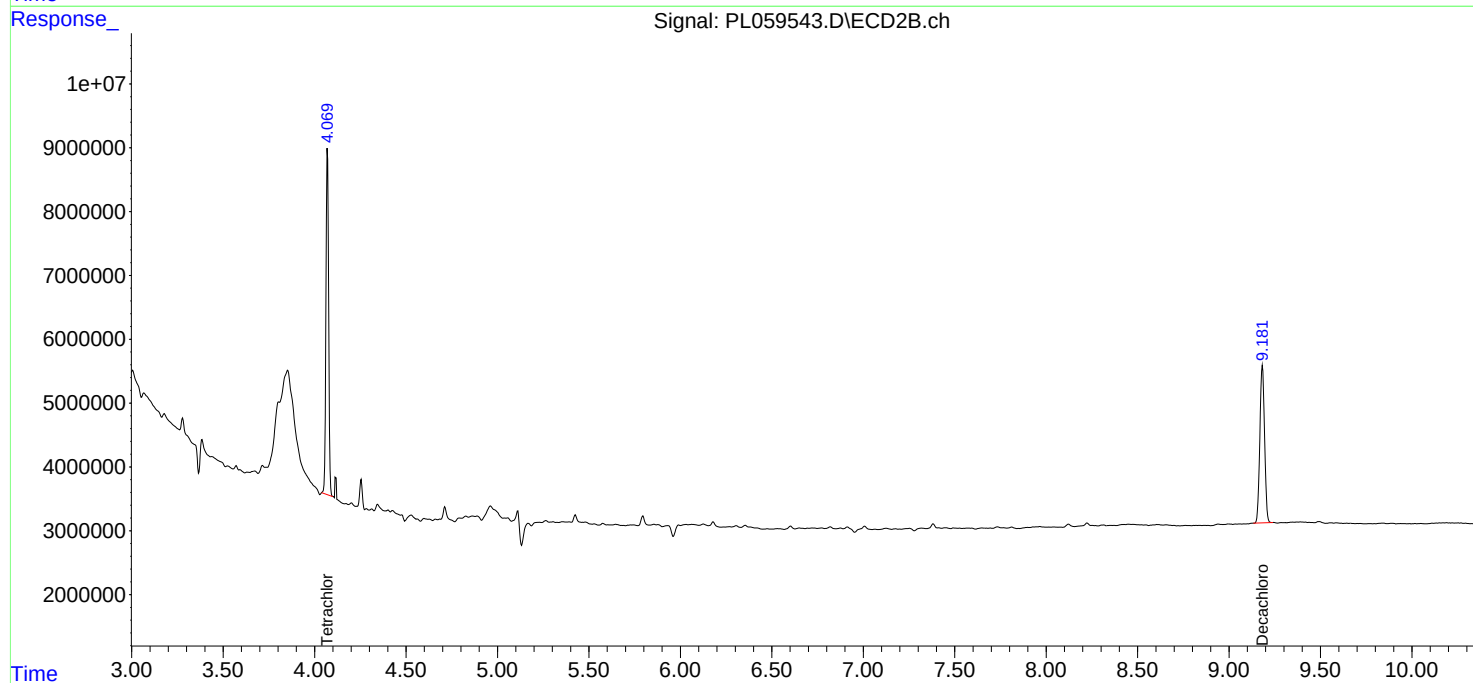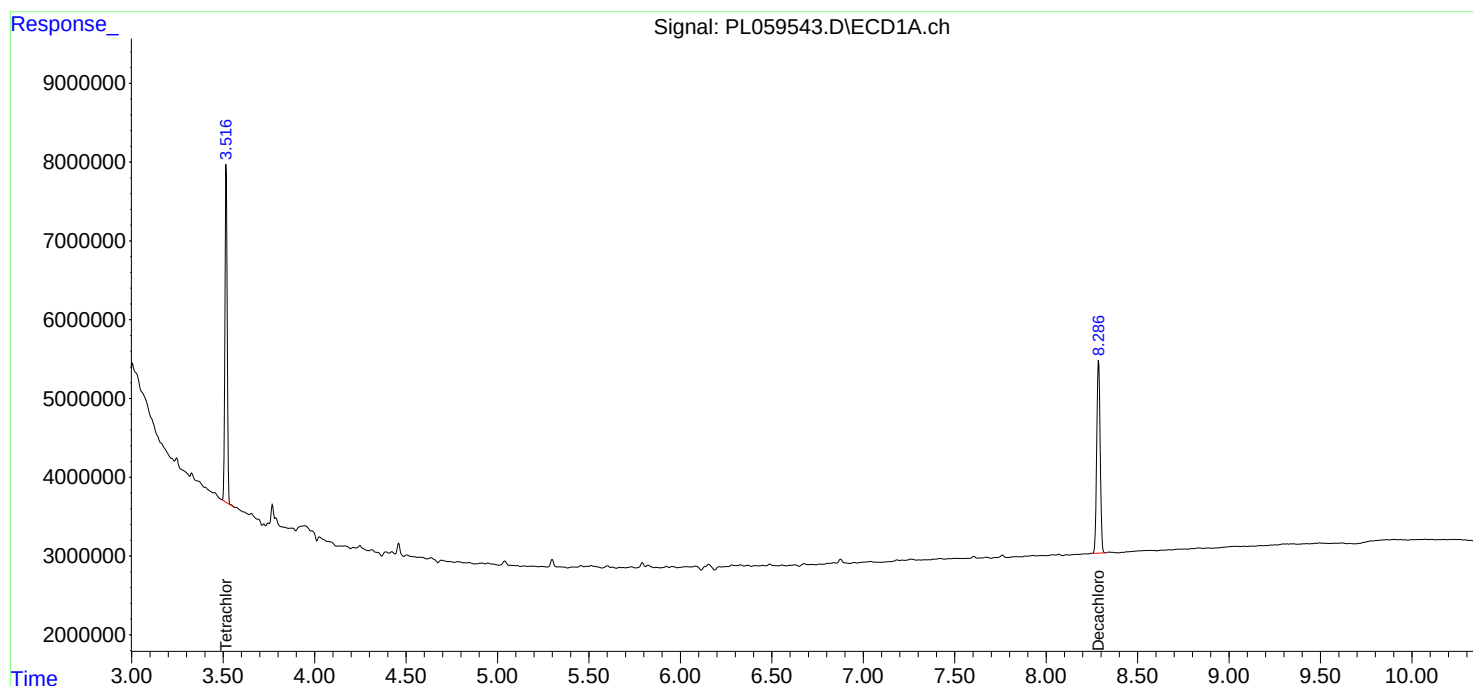

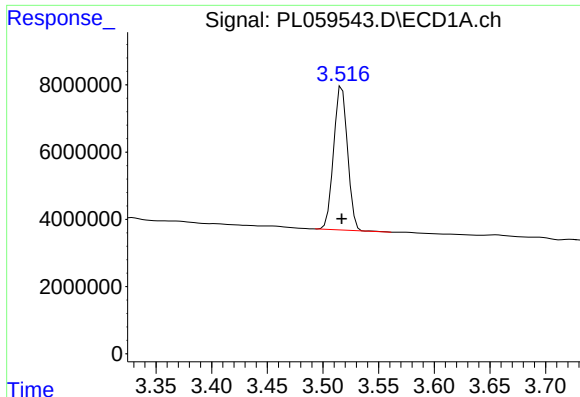


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 37148174
Conc: 20.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-062420


Manual Integrations
APPROVED

Ankita
6/29/2020 2:31:40 PM

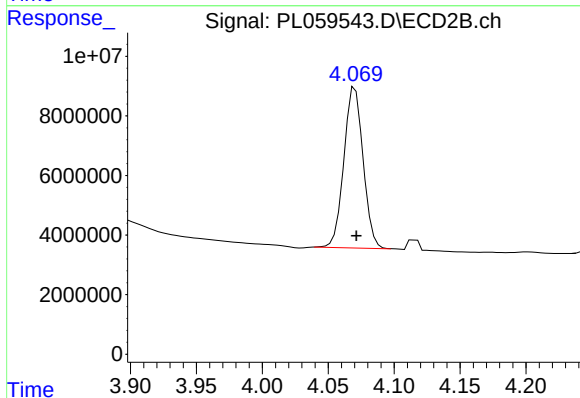


#1 Tetrachloro-m-xylene

R.T.: 4.069 min
Delta R.T.: -0.002 min
Response: 54734406
Conc: 21.21 ng/ml m

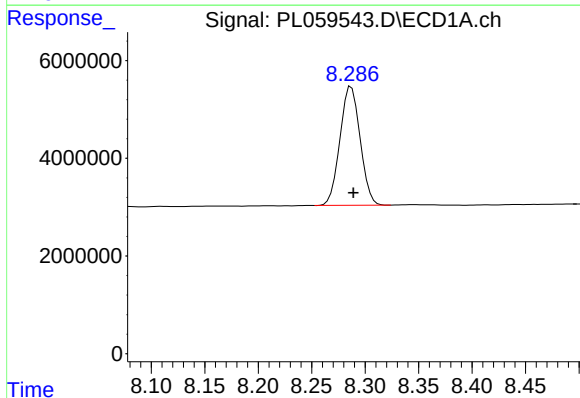

#28 Decachlorobiphenyl

R.T.: 8.287 min
Delta R.T.: -0.002 min
Response: 31992151
Conc: 18.79 ng/ml

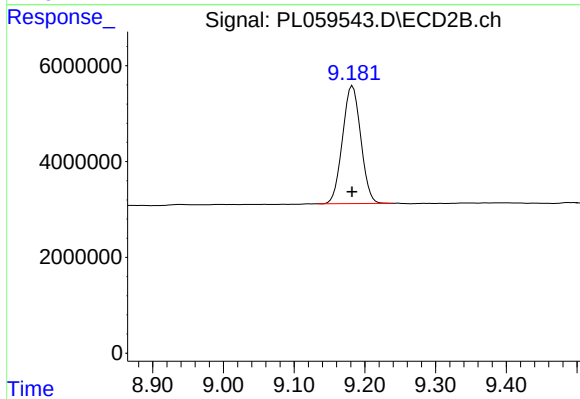

#28 Decachlorobiphenyl

R.T.: 9.183 min
Delta R.T.: 0.000 min
Response: 44046688
Conc: 19.24 ng/ml