

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062623\
 Data File : PL083717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2023 18:16
 Operator : AR\AJ
 Sample : 03362-20
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMPOSIT-SB-25

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/27/2023
 Supervised By :Ankita Jodhani 06/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 21:42:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 26 10:45:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	2.692	22763611	28010549	9.162	9.647
28)	SA Decachlor...	8.972	7.880	24994137	37281256	14.634	15.078
Target Compounds							
11)	B alpha-Chl...	5.926	4.974	31604777	31834397	9.589m	9.400

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062623\
Data File : PL083717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2023 18:16
Operator : AR\AJ
Sample : 03362-20
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMPOSIT-SB-25


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/27/2023
Supervised By : Ankita Jodhani 06/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 21:42:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
Quant Title : GC Extractables
QLast Update : Mon Jun 26 10:45:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

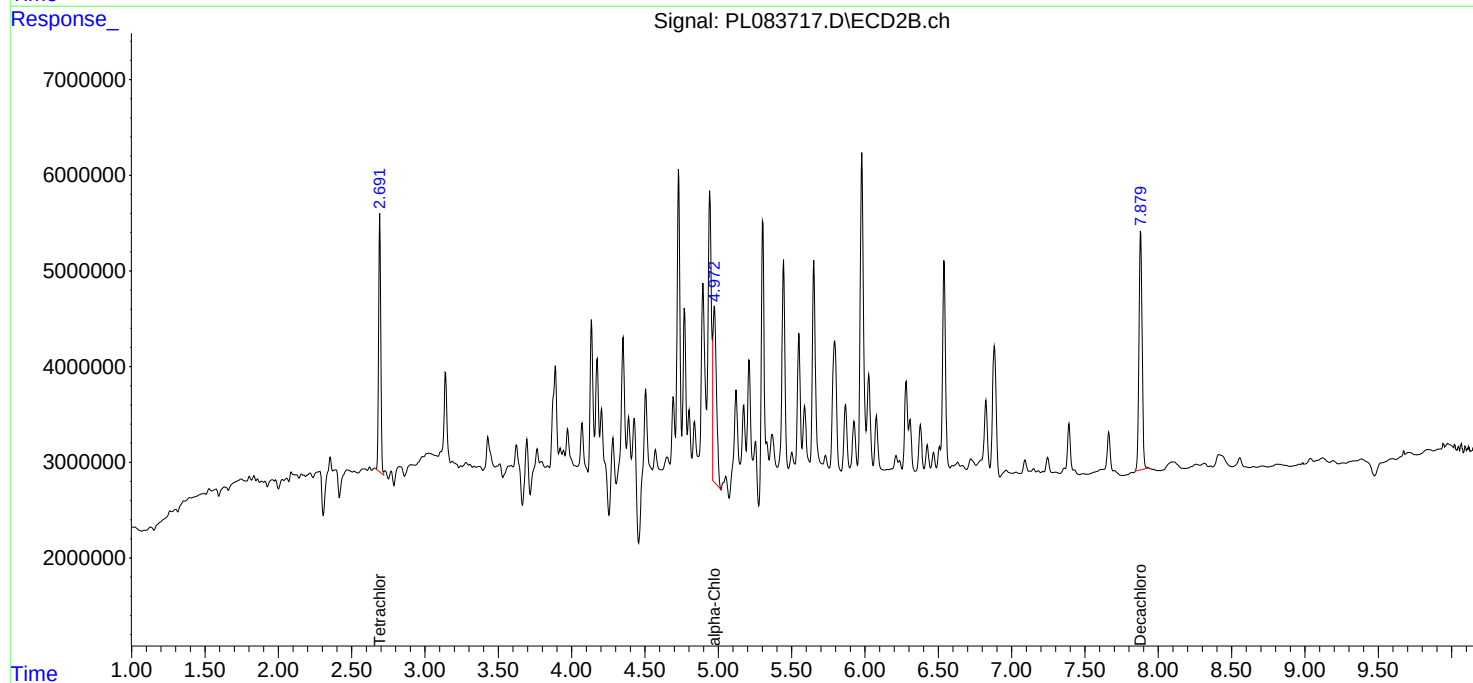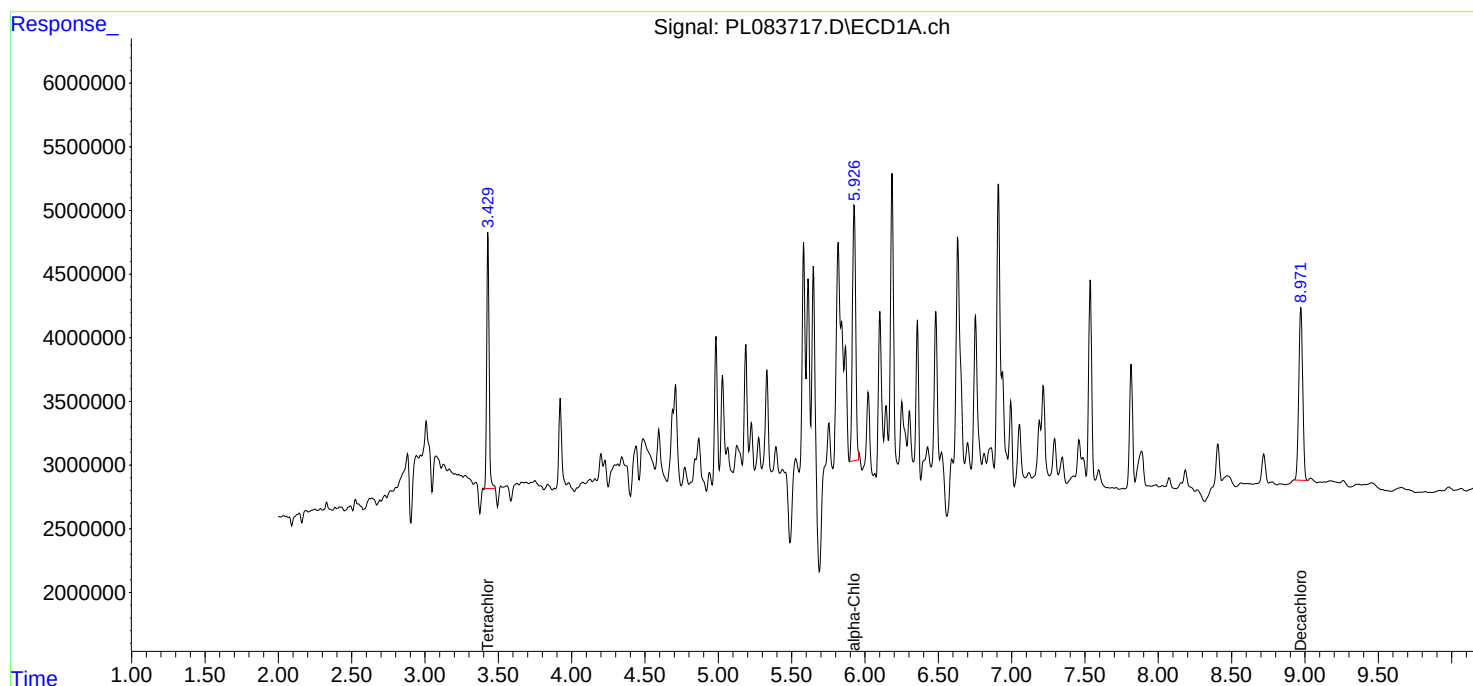

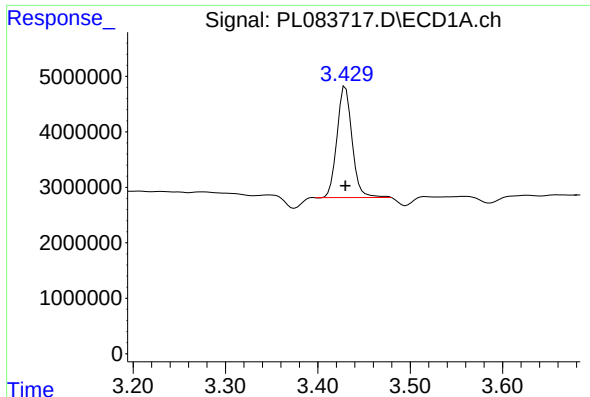


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: 0.000 min
Response: 22763611
Conc: 9.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMPOSIT-SB-25


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/27/2023
Supervised By :Ankita Jodhani 06/27/2023

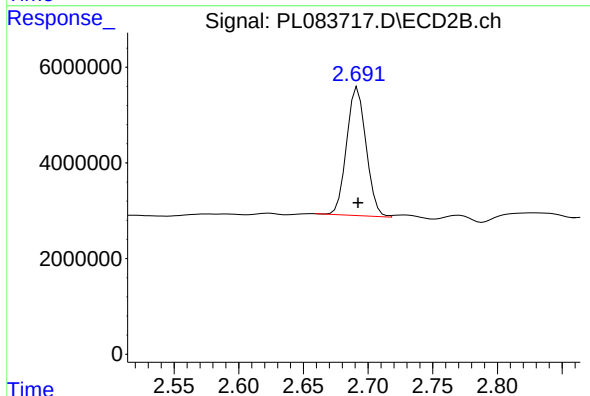


#1 Tetrachloro-m-xylene

R.T.: 2.692 min
Delta R.T.: 0.000 min
Response: 28010549
Conc: 9.65 ng/ml

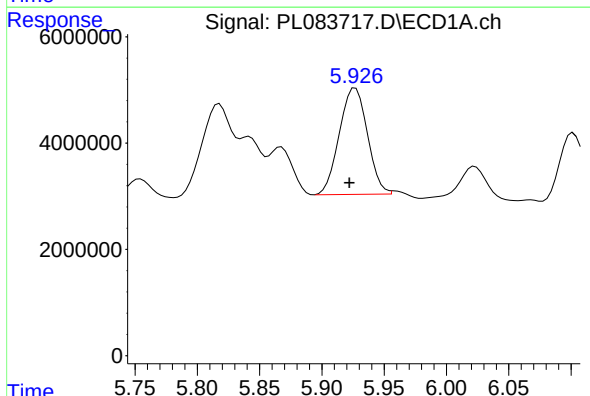


#11 alpha-Chlordane

R.T.: 5.926 min
Delta R.T.: 0.003 min
Response: 31604777
Conc: 9.59 ng/ml m

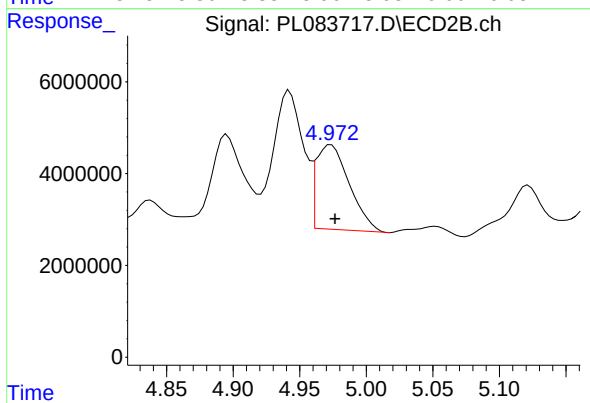

#11 alpha-Chlordane

R.T.: 4.974 min
Delta R.T.: -0.003 min
Response: 31834397
Conc: 9.40 ng/ml

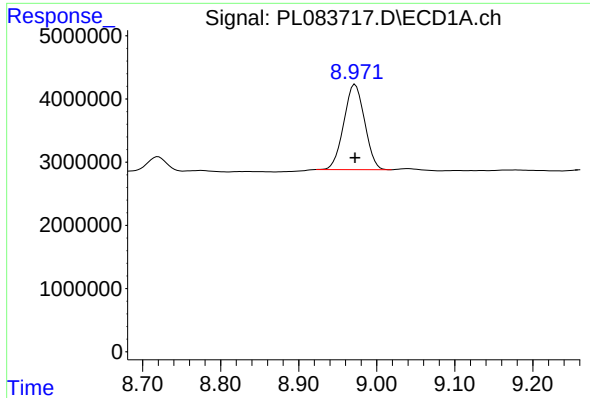


#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: 0.000 min
Response: 24994137
Conc: 14.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMPOSIT-SB-25

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/27/2023
Supervised By :Ankita Jodhani 06/27/2023

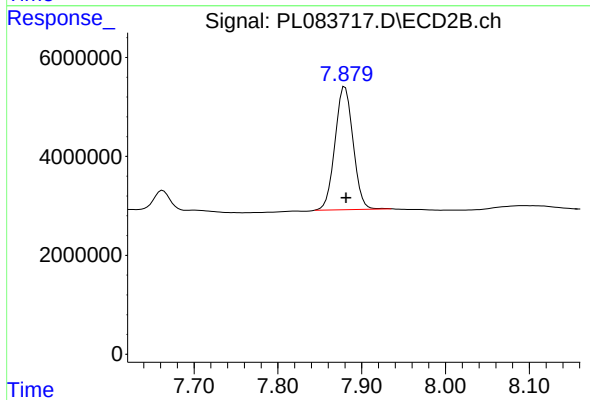

#28 Decachlorobiphenyl

R.T.: 7.880 min
Delta R.T.: -0.001 min
Response: 37281256
Conc: 15.08 ng/ml