

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062625\
 Data File : PL096181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2025 13:29
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 13:43:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062625.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 26 13:42:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.879	162.3E6	285.2E6	50.000	50.000
28)	SA Decachlor...	9.126	8.066	124.1E6	285.8E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.734	3.897	83772758	97985978	500.000	500.000
24)	Chlordane-2	5.262	4.477	85169058	110.0E6	500.000	500.000
25)	Chlordane-3	5.967	5.112	330.1E6	339.6E6	500.000	500.000
26)	Chlordane-4	6.052	5.177	390.0E6	300.7E6	500.000	500.000
27)	Chlordane-5	6.894	6.076	70742153	128.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062625\
Data File : PL096181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2025 13:29
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 13:43:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062625.M
Quant Title : GC Extractables
QLast Update : Thu Jun 26 13:42:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

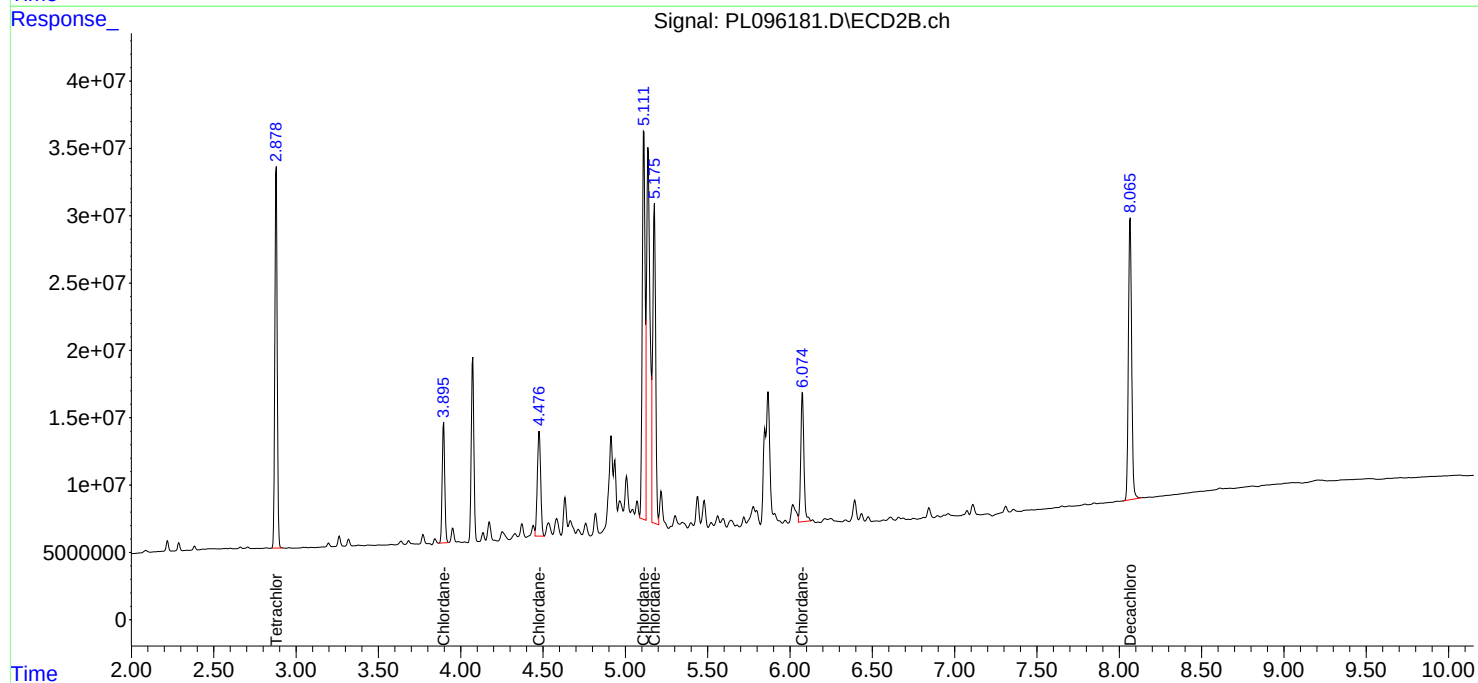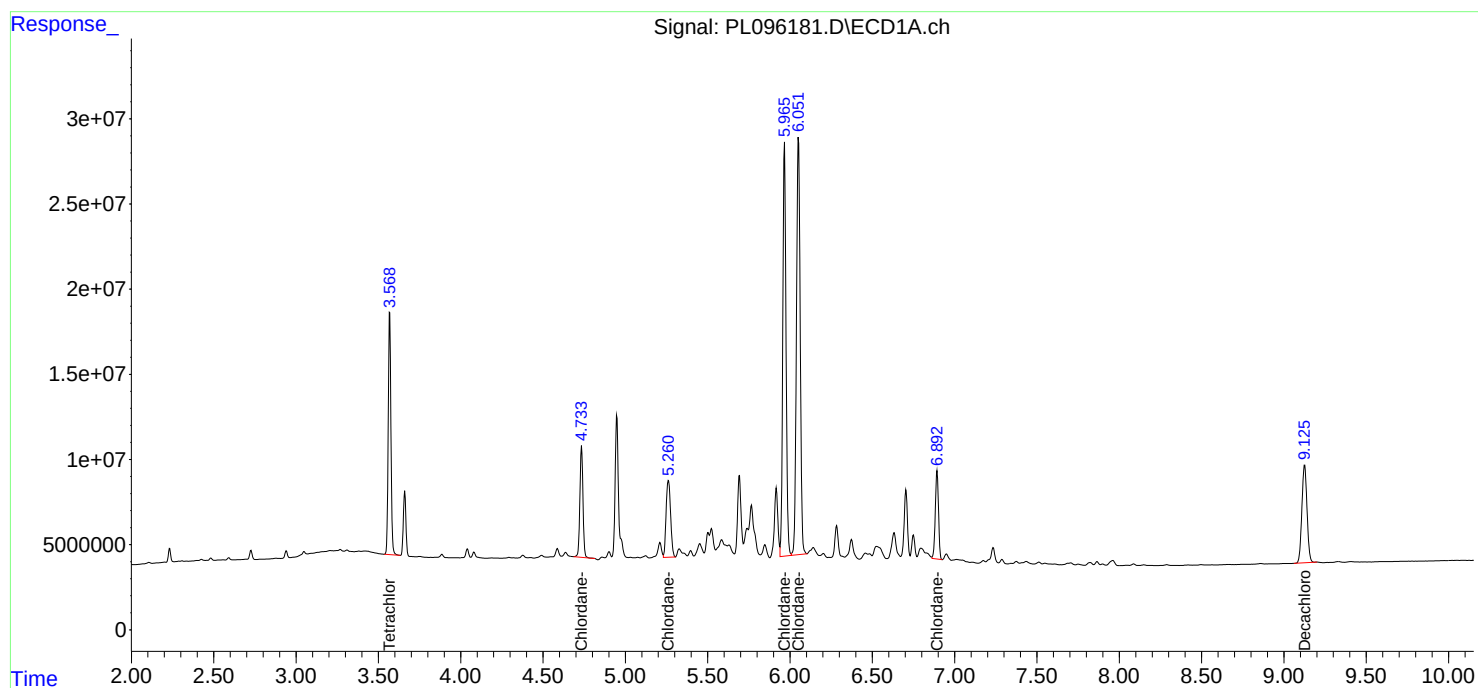


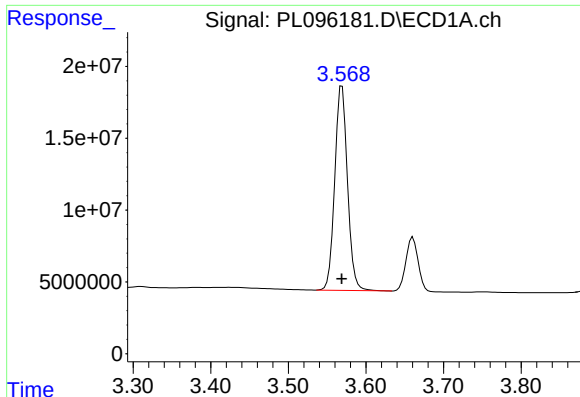

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 162309925
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

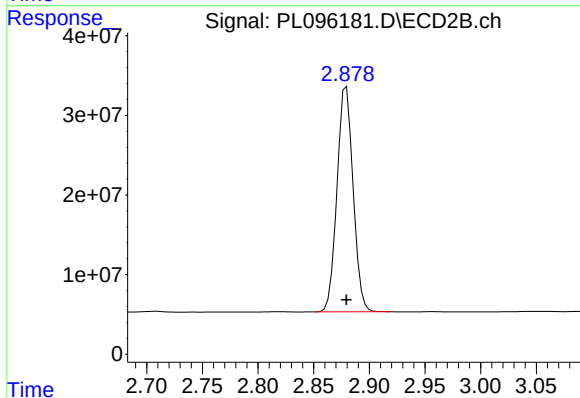


#1 Tetrachloro-m-xylene

R.T.: 2.879 min
Delta R.T.: 0.000 min
Response: 285203774
Conc: 50.00 ng/ml

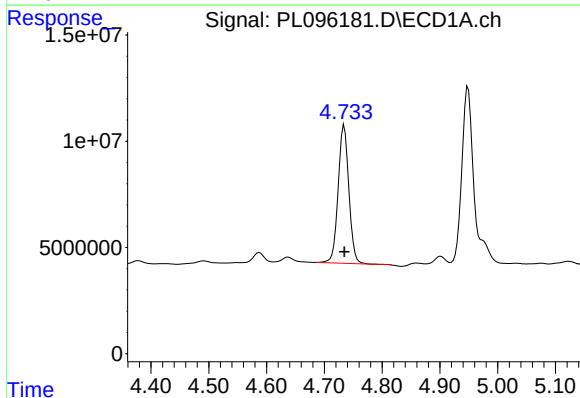


#23 Chlordane-1

R.T.: 4.734 min
Delta R.T.: 0.000 min
Response: 83772758
Conc: 500.00 ng/ml

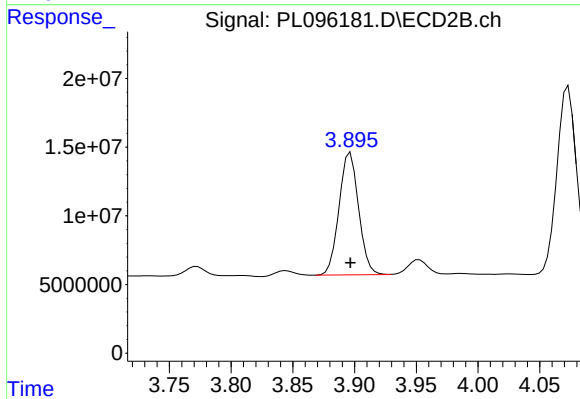

#23 Chlordane-1


R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 97985978
Conc: 500.00 ng/ml

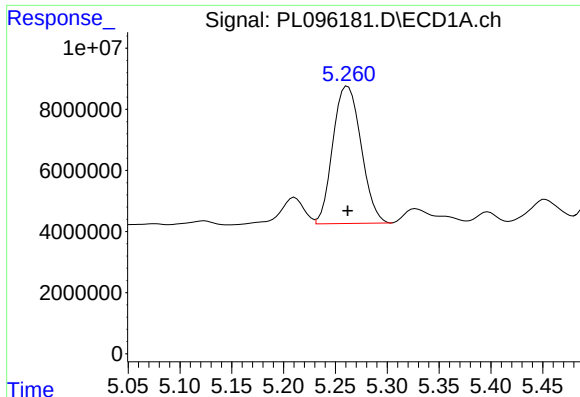

#24 Chlordane-2


R.T.: 5.262 min
Delta R.T.: 0.000 min
Response: 85169058
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

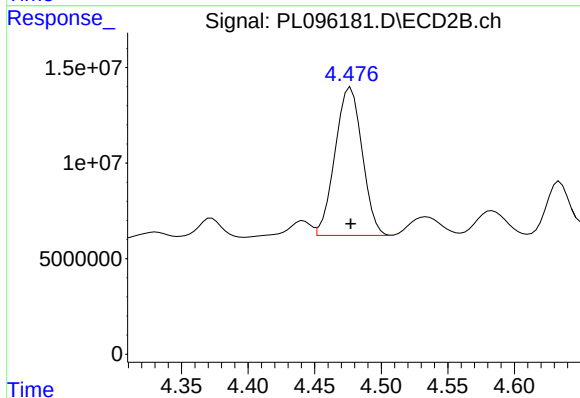


#24 Chlordane-2

R.T.: 4.477 min
Delta R.T.: 0.000 min
Response: 110043375
Conc: 500.00 ng/ml

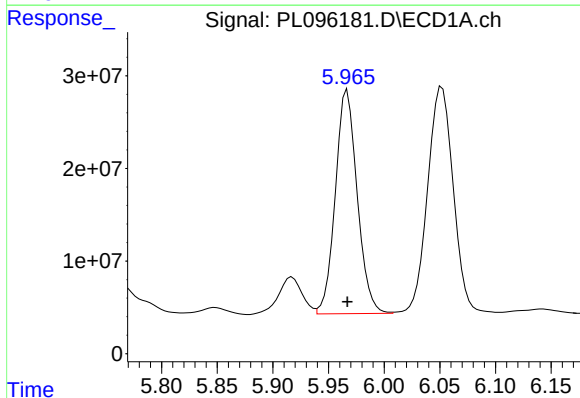


#25 Chlordane-3

R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 330117951
Conc: 500.00 ng/ml

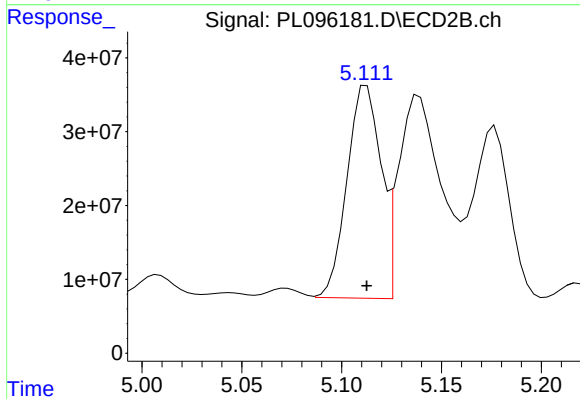

#25 Chlordane-3


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 339633305
Conc: 500.00 ng/ml

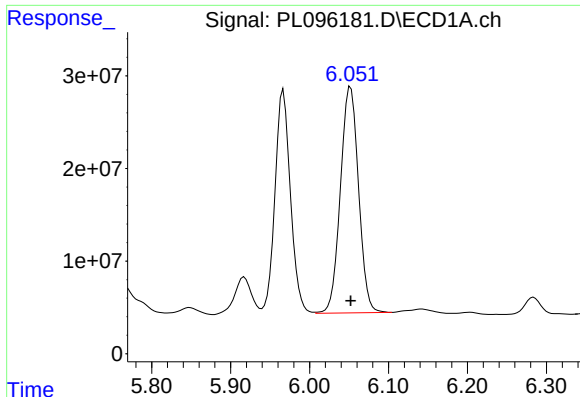

#26 Chlordane-4


R.T.: 6.052 min
Delta R.T.: 0.000 min
Response: 389984538
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

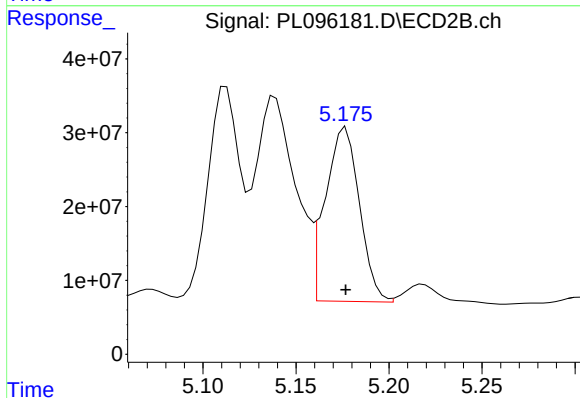


#26 Chlordane-4

R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 300669812
Conc: 500.00 ng/ml

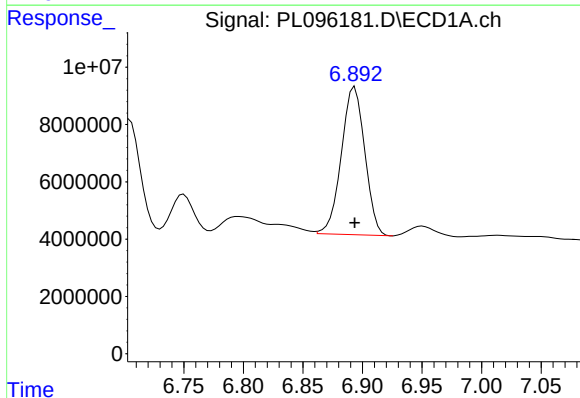


#27 Chlordane-5

R.T.: 6.894 min
Delta R.T.: 0.000 min
Response: 70742153
Conc: 500.00 ng/ml

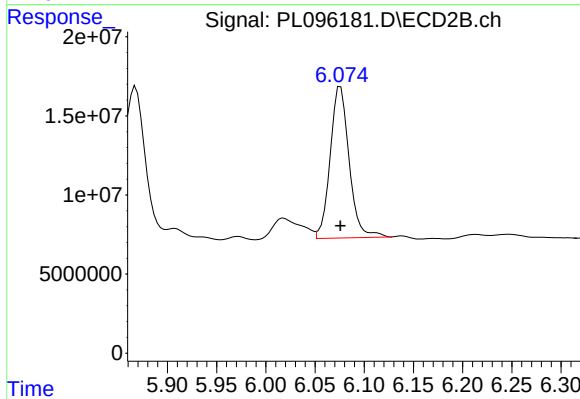

#27 Chlordane-5


R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 128452849
Conc: 500.00 ng/ml

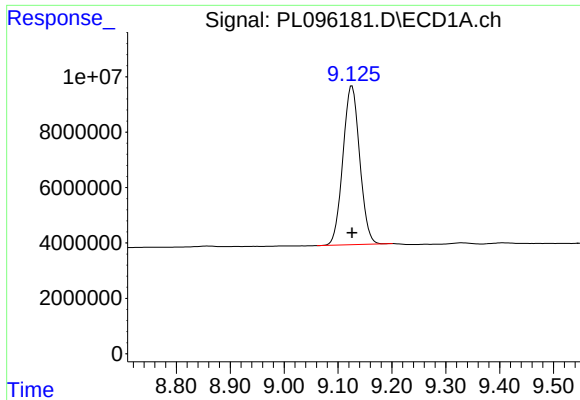

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 124137930
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

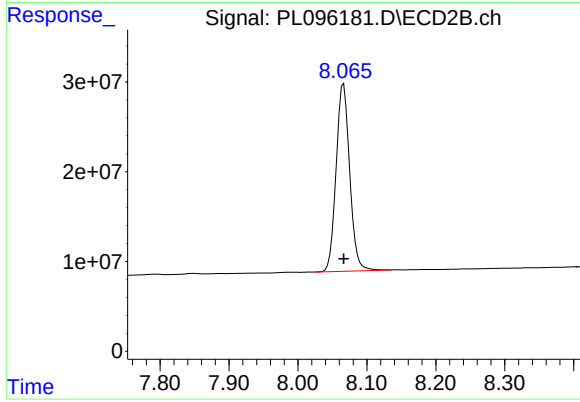

#28 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: 0.000 min
Response: 285849211
Conc: 50.00 ng/ml