

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
 Data File : PL037453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2018 12:53
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:30:12 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.936	129.6E6	45205071	16.388	16.339
28)	SA Decachlor...	8.016	8.947	122.9E6	37313215	20.370	18.808
Target Compounds							
23)	Chlordane-1	4.131	0.000	13847607	0	45.099	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
Data File : PL037453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2018 12:53
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:30:12 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

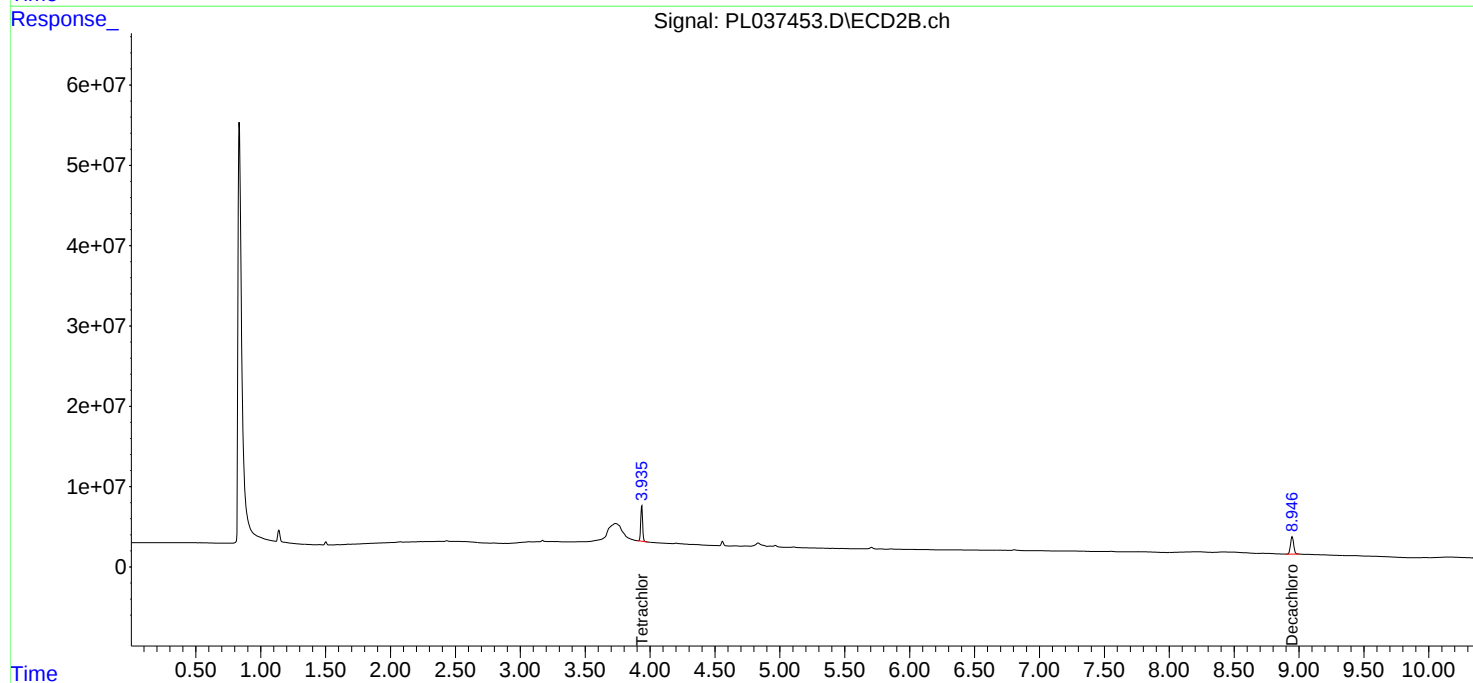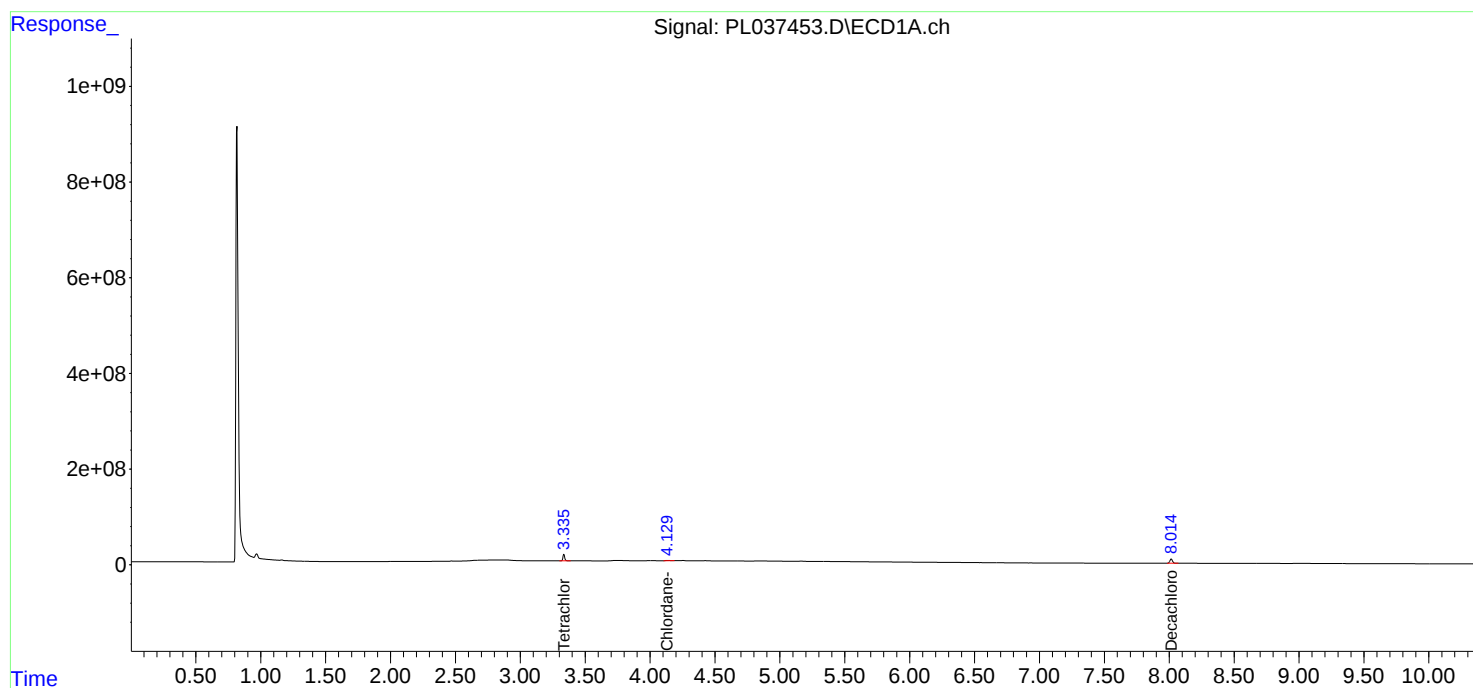


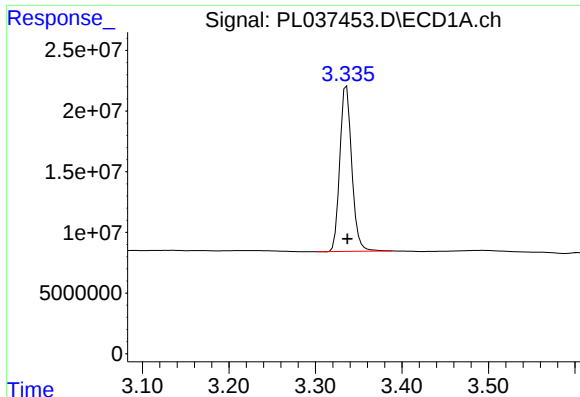

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 129635632
Conc: 16.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

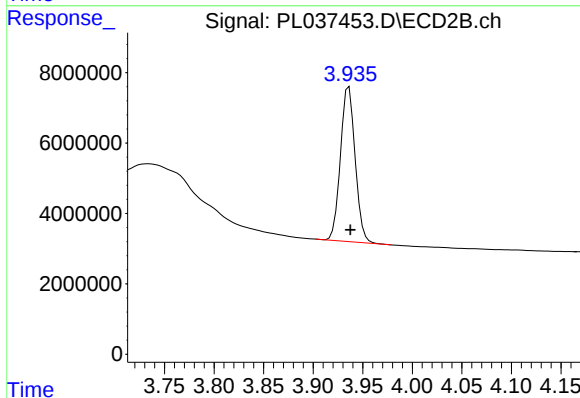


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 45205071
Conc: 16.34 ng/ml

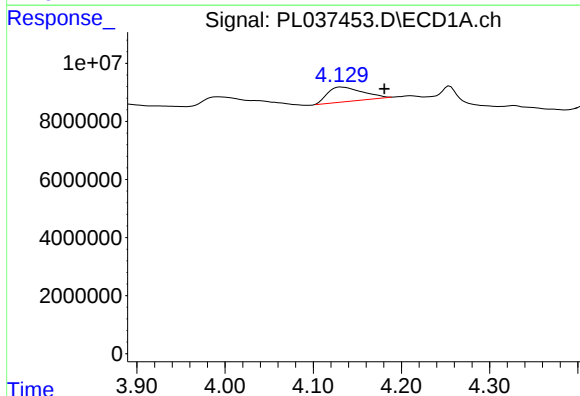


#23 Chlordane-1

R.T.: 4.131 min
Delta R.T.: -0.049 min
Response: 13847607
Conc: 45.10 ng/ml

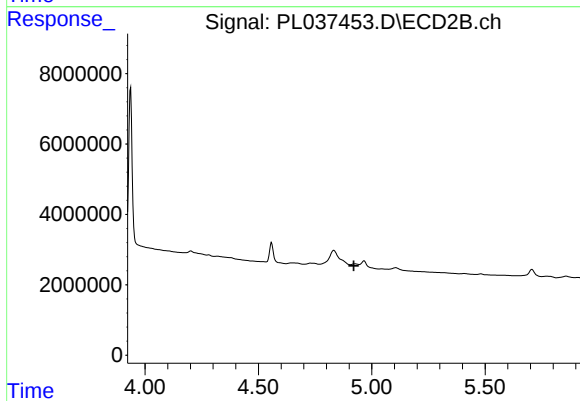

#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

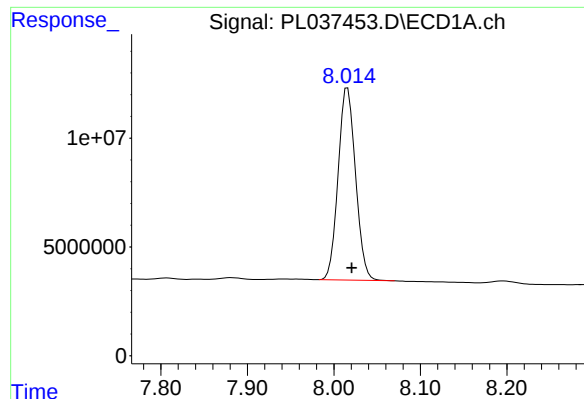

#28 Decachlorobiphenyl


R.T.: 8.016 min

Delta R.T.: -0.005 min

Response: 122914669

Conc: 20.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

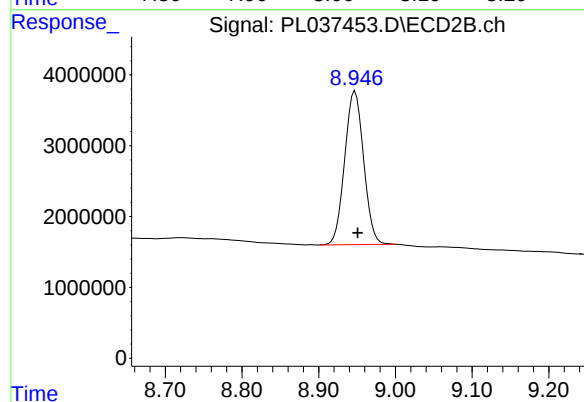

#28 Decachlorobiphenyl

R.T.: 8.947 min

Delta R.T.: -0.003 min

Response: 37313215

Conc: 18.81 ng/ml