

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
 Data File : PL037462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2018 16:32
 Operator : UA\AJ
 Sample : J3242-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:32:41 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.936	60659355	19086546	7.668	6.899
28)	SA Decachlor...	8.015	8.948	75150305	24057507	12.454	12.126
Target Compounds							
2)	A alpha-BHC	3.727f	0.000	10556439	0	0.862	N.D. #
3)	MA gamma-BHC...	4.015f	0.000	551935	0	0.054	N.D. #
10)	B gamma-Chl...	5.248	0.000	8595590	0	0.918	N.D. #
11)	B alpha-Chl...	5.248f	0.000	8595590	0	0.947	N.D. #
17)	MA 4,4'-DDT	6.197	0.000	5584529	0	0.865	N.D. #
23)	Chlordane-1	4.180	0.000	4880982	0	15.896	N.D. #
25)	Chlordane-3	5.248	0.000	8595590	0	8.087	N.D. #
26)	Chlordane-4	5.248	0.000	8595590	0	8.921	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
Data File : PL037462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2018 16:32
Operator : UA\AJ
Sample : J3242-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:32:41 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

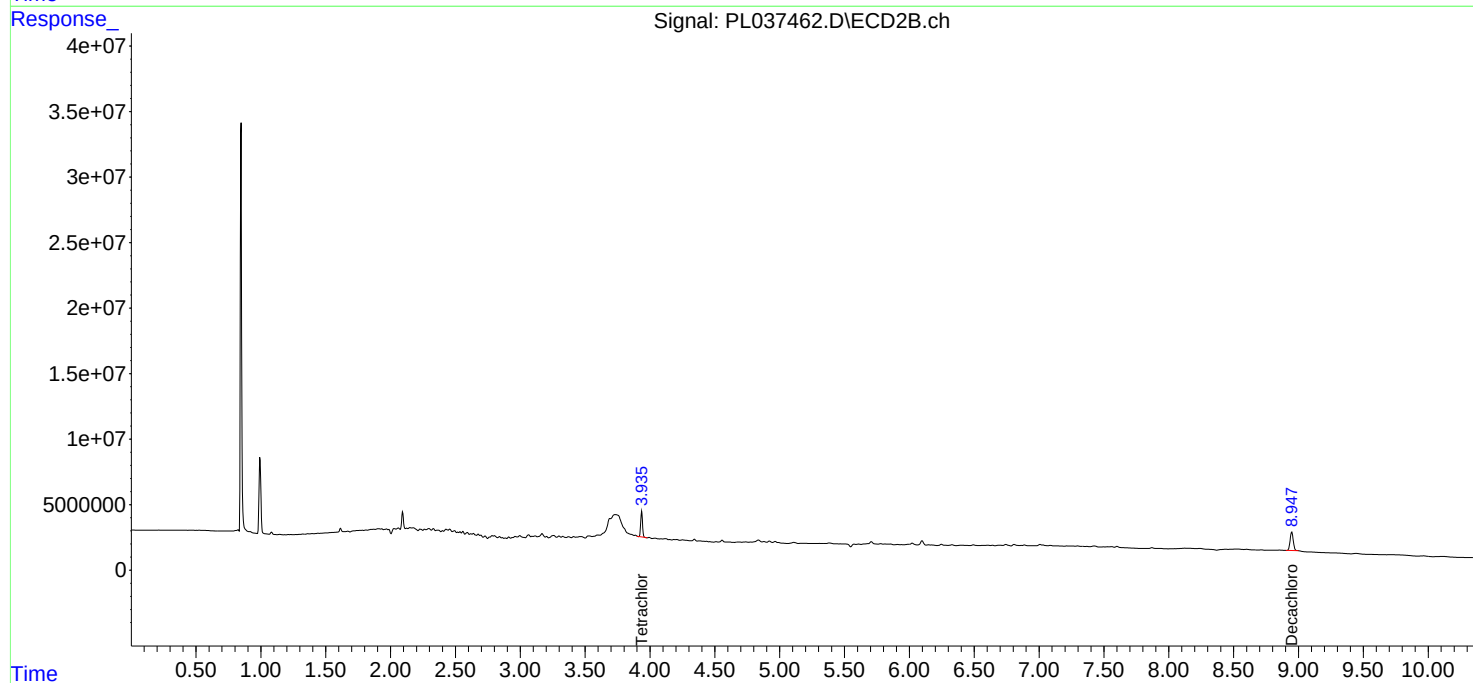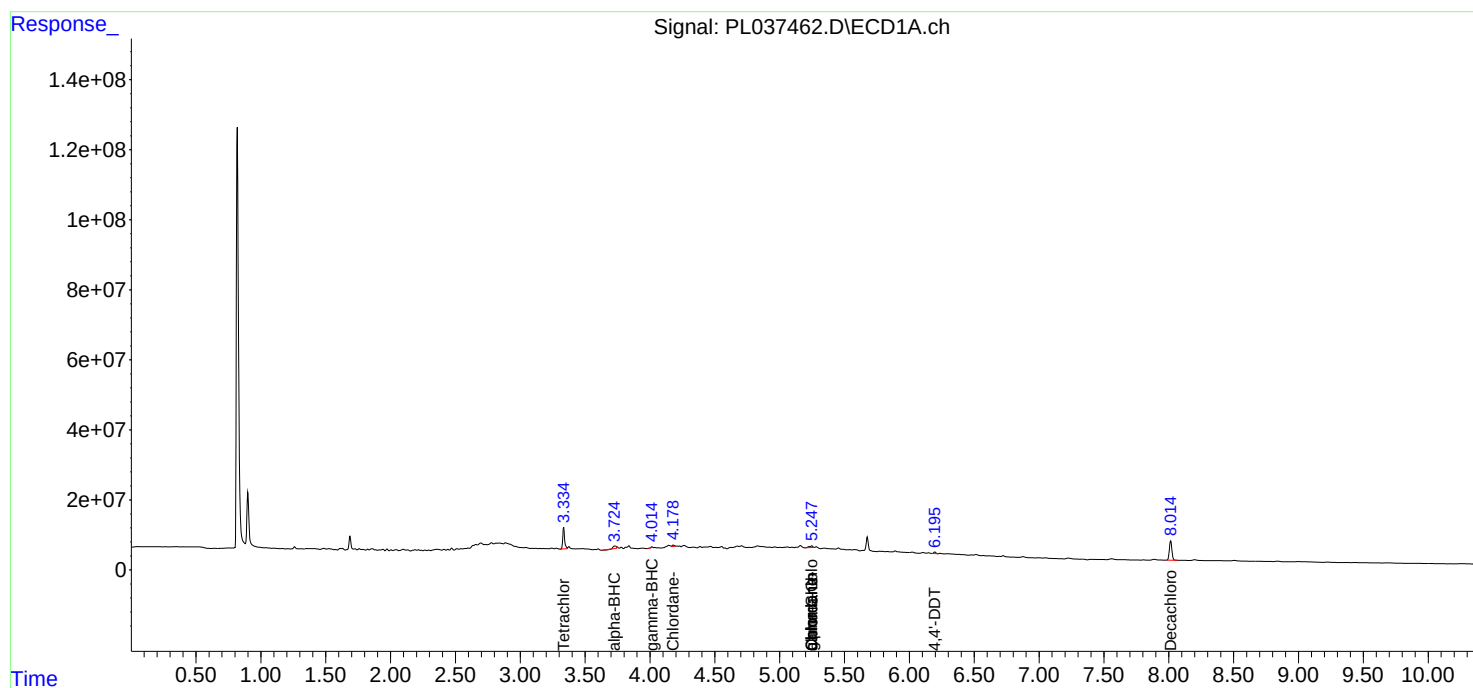


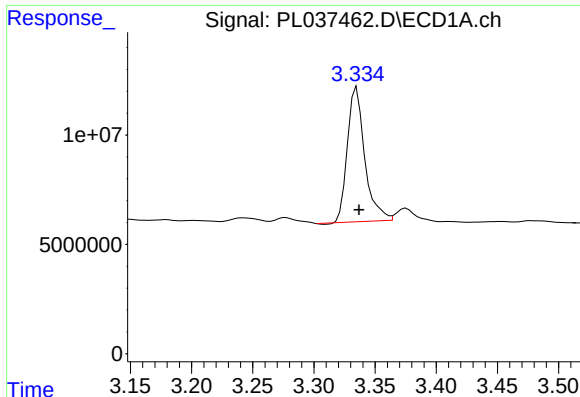

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 60659355
Conc: 7.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

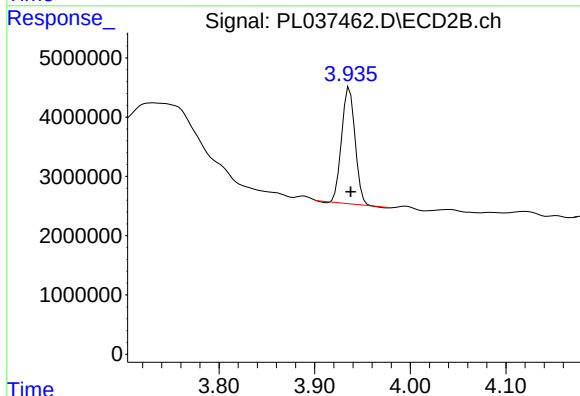


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.001 min
Response: 19086546
Conc: 6.90 ng/ml

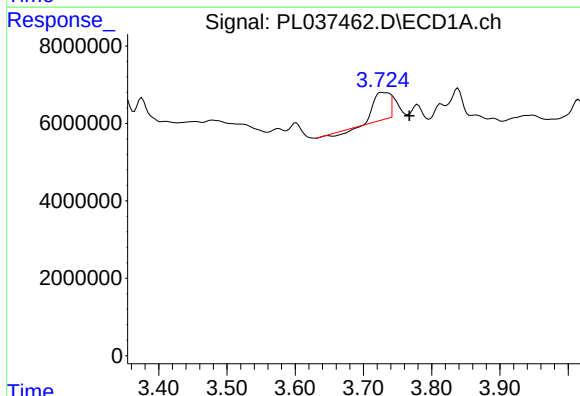


#2 alpha-BHC

R.T.: 3.727 min
Delta R.T.: -0.041 min
Response: 10556439
Conc: 0.86 ng/ml

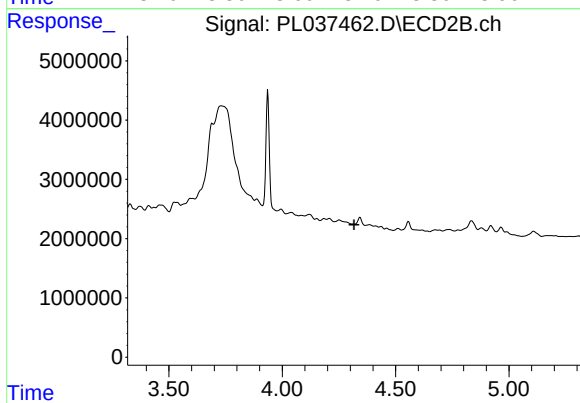

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

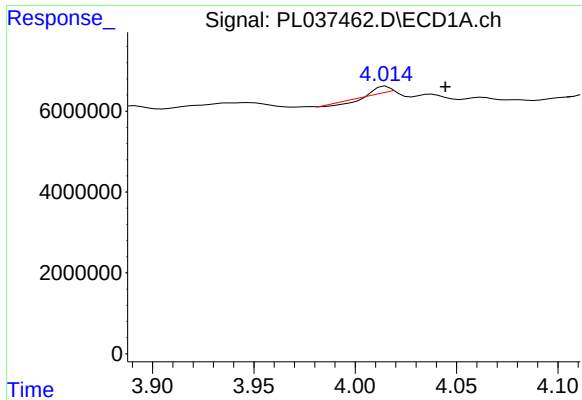

#3 gamma-BHC (Lindane)


R.T.: 4.015 min
Delta R.T.: -0.029 min
Response: 551935
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

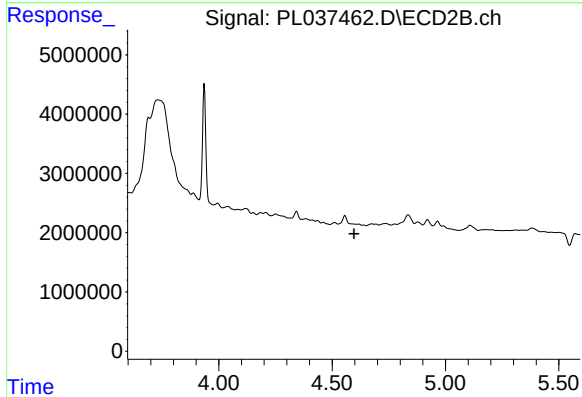


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.597 min
Response: 0
Conc: N.D.

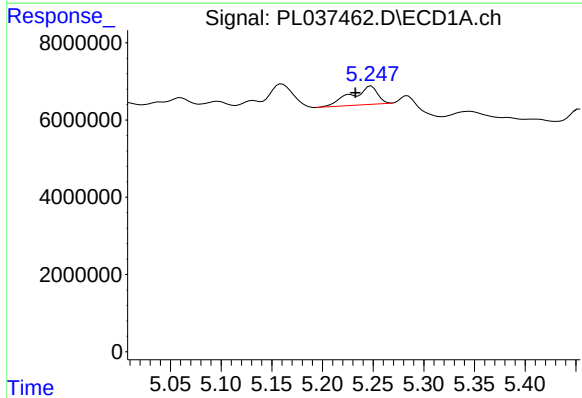


#10 gamma-Chlordane

R.T.: 5.248 min
Delta R.T.: 0.016 min
Response: 8595590
Conc: 0.92 ng/ml

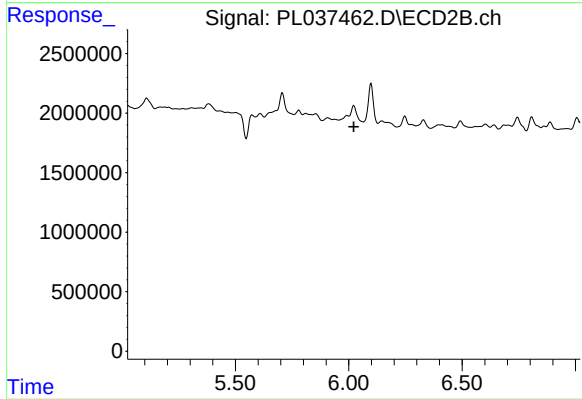

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

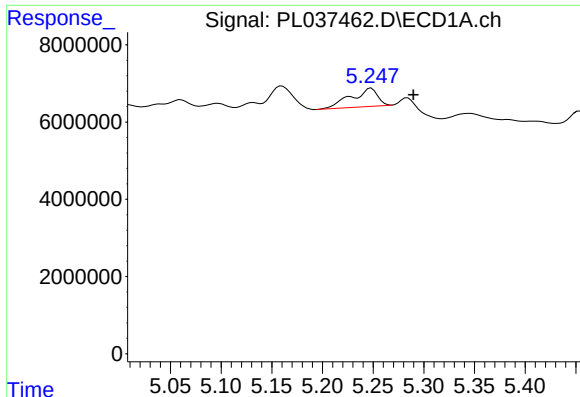

#11 alpha-Chlordane


R.T.: 5.248 min
Delta R.T.: -0.042 min
Response: 8595590
Conc: 0.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

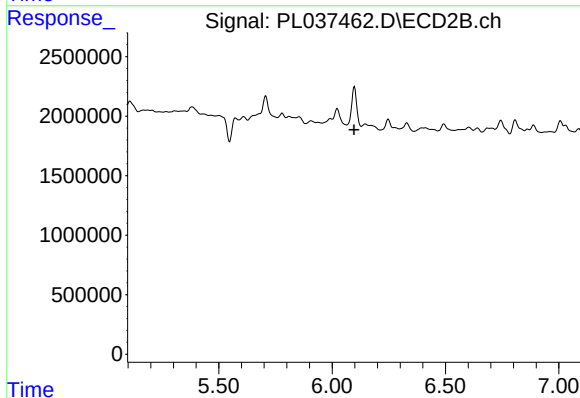


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

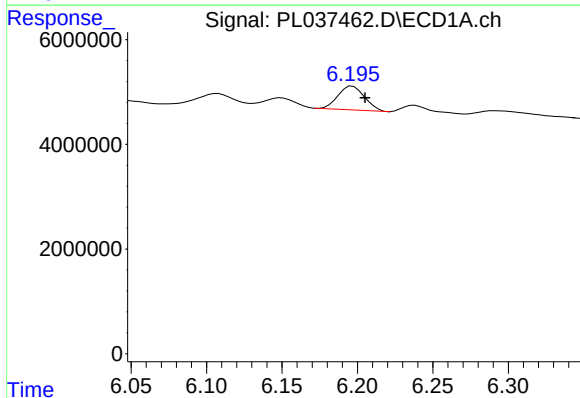


#17 4,4'-DDT

R.T.: 6.197 min
Delta R.T.: -0.008 min
Response: 5584529
Conc: 0.86 ng/ml

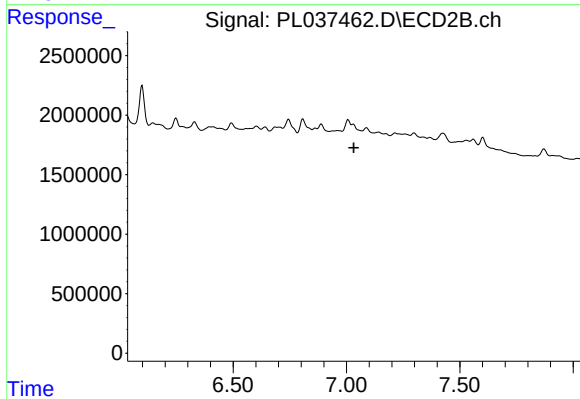

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

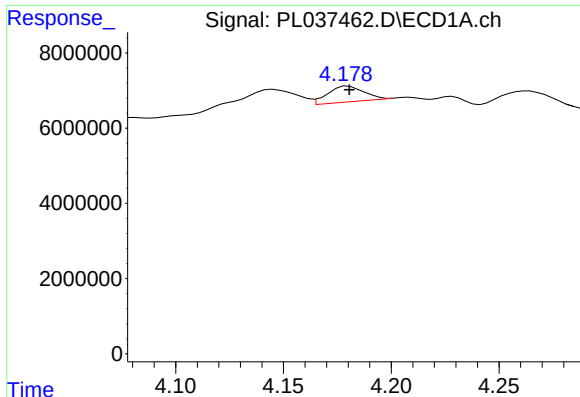

#23 Chlordane-1


R.T.: 4.180 min
Delta R.T.: 0.000 min
Response: 4880982
Conc: 15.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

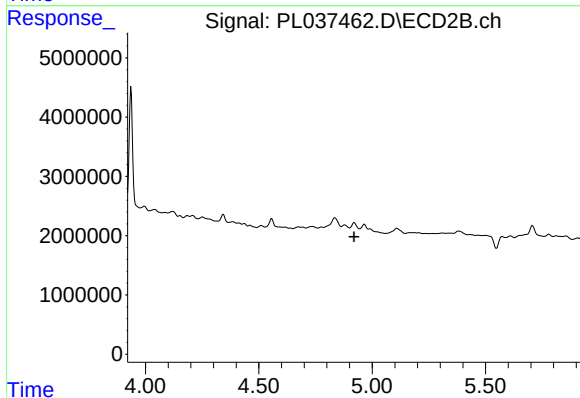


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

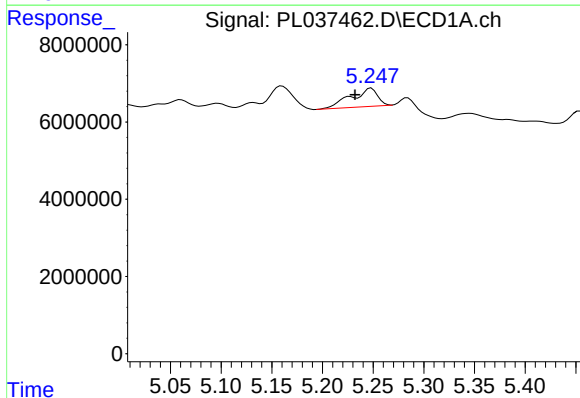


#25 Chlordane-3

R.T.: 5.248 min
Delta R.T.: 0.016 min
Response: 8595590
Conc: 8.09 ng/ml

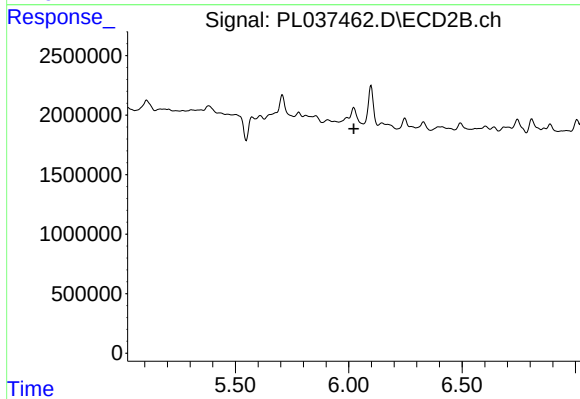

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

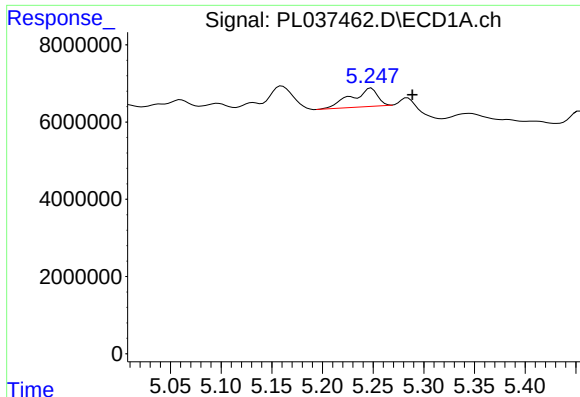

#26 Chlordane-4


R.T.: 5.248 min
Delta R.T.: -0.041 min
Response: 8595590
Conc: 8.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

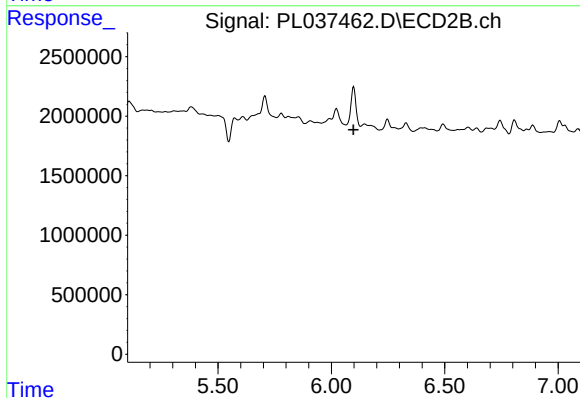


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

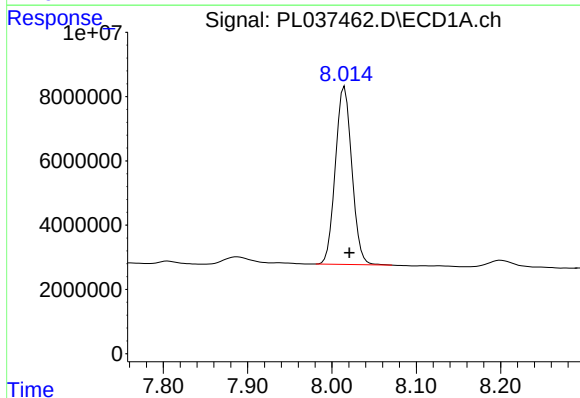

#28 Decachlorobiphenyl

R.T.: 8.015 min
Delta R.T.: -0.006 min
Response: 75150305
Conc: 12.45 ng/ml

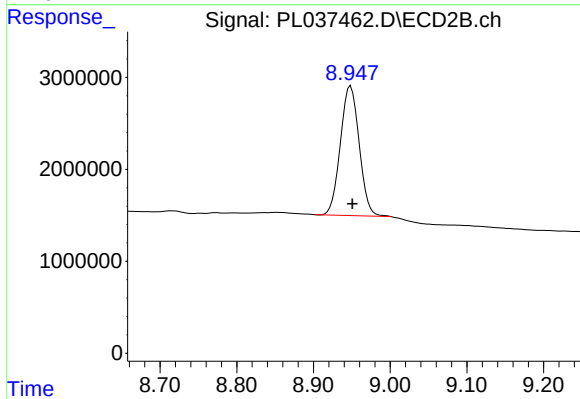

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.002 min
Response: 24057507
Conc: 12.13 ng/ml