

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
 Data File : PL037475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2018 19:35
 Operator : UA\AJ
 Sample : J3242-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:34:59 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.937	151.0E6	55858981	19.086	20.190
28)	SA Decachlor...	8.016	8.949	121.4E6	41479445	20.124	20.908
Target Compounds							
6)	B beta-BHC	4.253f	0.000	7644879	0	1.676	N.D. #
10)	B gamma-Chl...	5.256	0.000	12912024	0	1.379	N.D. #
11)	B alpha-Chl...	5.256	0.000	12912024	0	1.422	N.D. #
15)	B Endosulfa...	6.049f	0.000	9718274	0	1.322	N.D. #
25)	Chlordane-3	5.256	0.000	12912024	0	12.148	N.D. #
26)	Chlordane-4	5.256	0.000	12912024	0	13.401	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
Data File : PL037475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2018 19:35
Operator : UA\AJ
Sample : J3242-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:34:59 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

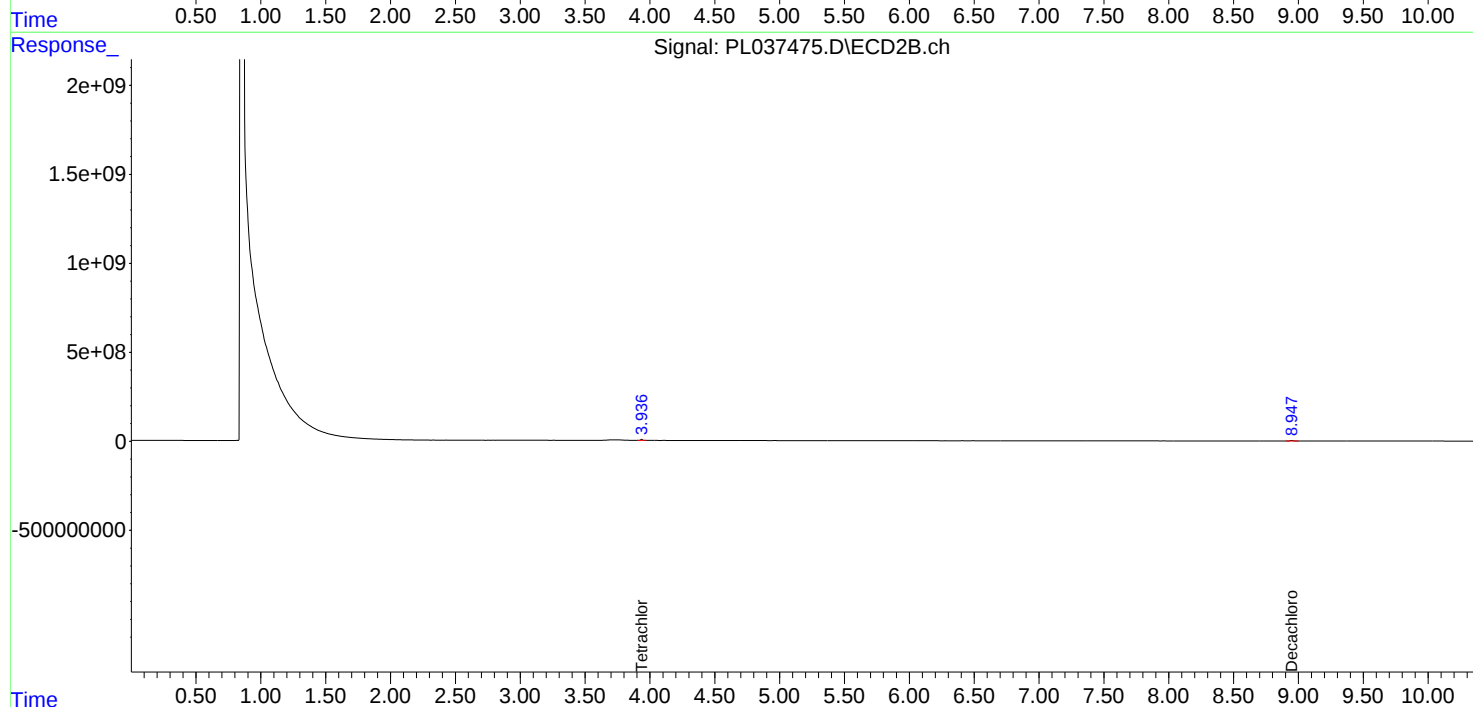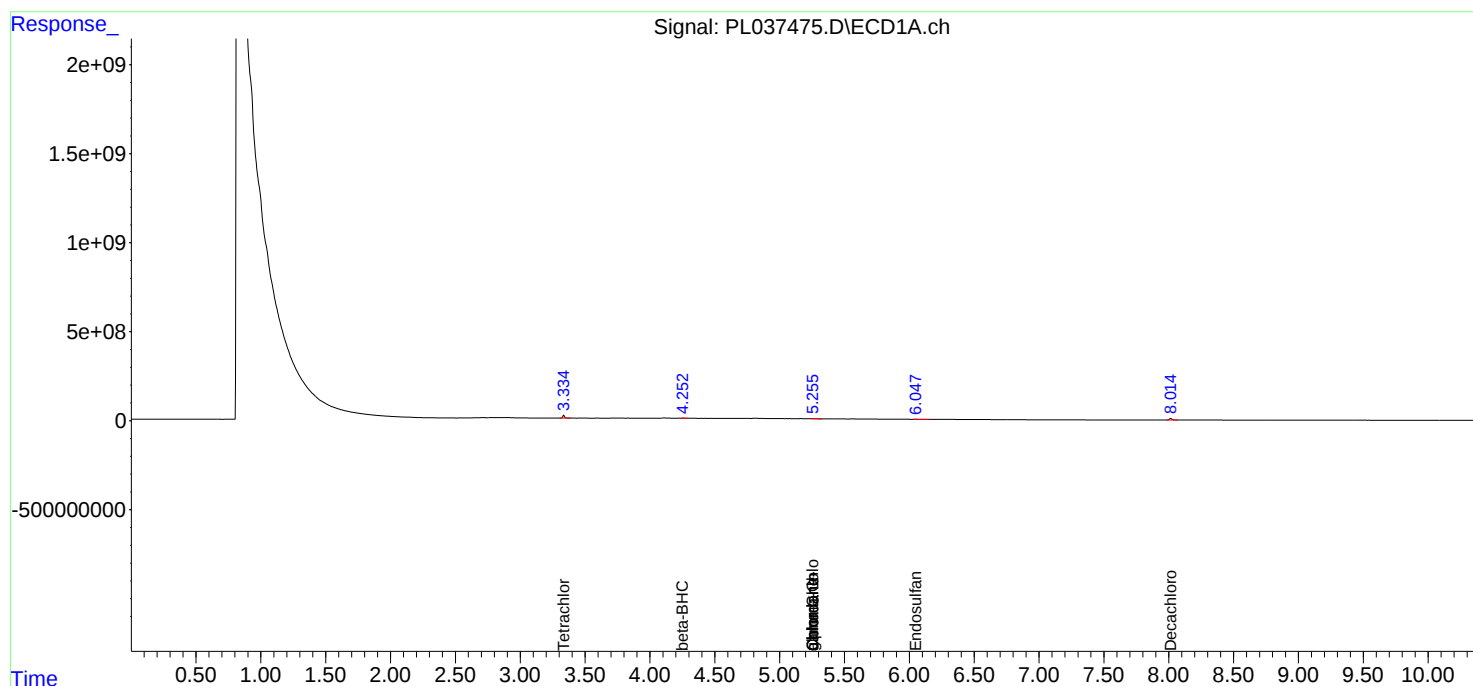


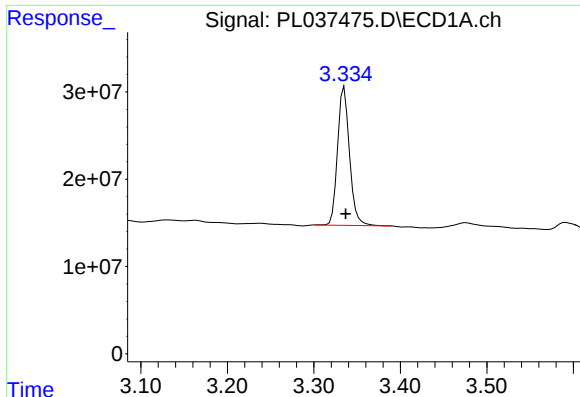

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 150974620
Conc: 19.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

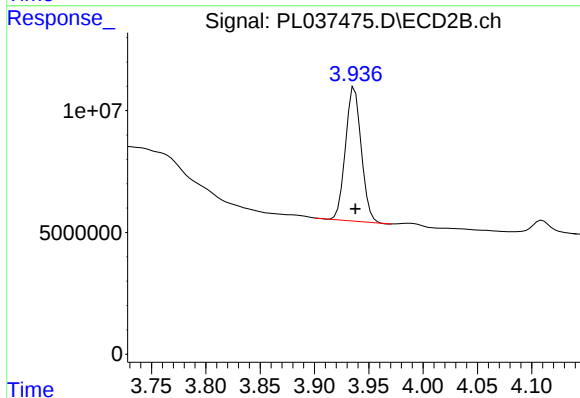


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 55858981
Conc: 20.19 ng/ml

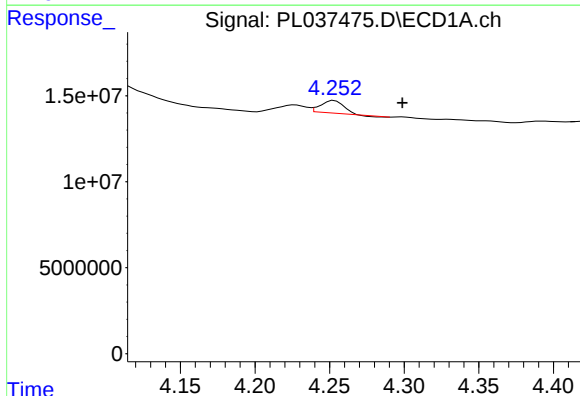


#6 beta-BHC

R.T.: 4.253 min
Delta R.T.: -0.046 min
Response: 7644879
Conc: 1.68 ng/ml

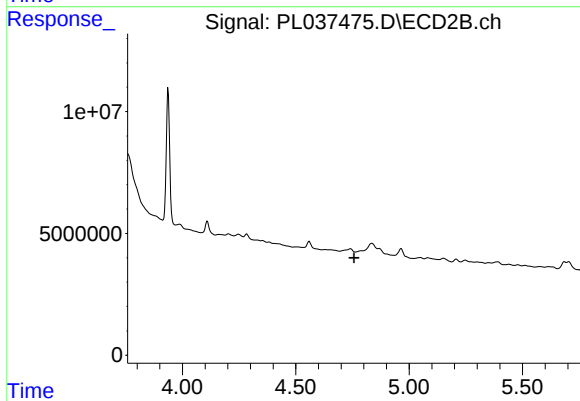

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

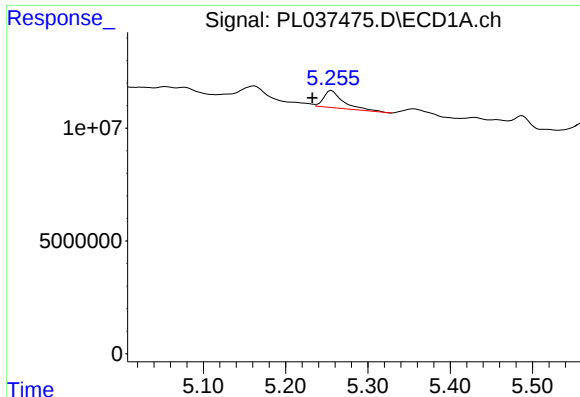

#10 gamma-Chlordane


R.T.: 5.256 min
Delta R.T.: 0.023 min
Response: 12912024
Conc: 1.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

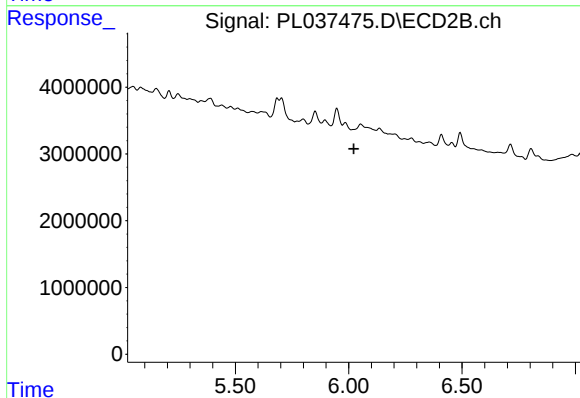


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

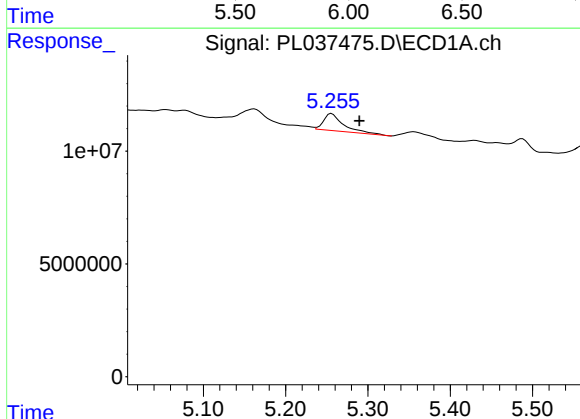


#11 alpha-Chlordane

R.T.: 5.256 min
Delta R.T.: -0.034 min
Response: 12912024
Conc: 1.42 ng/ml

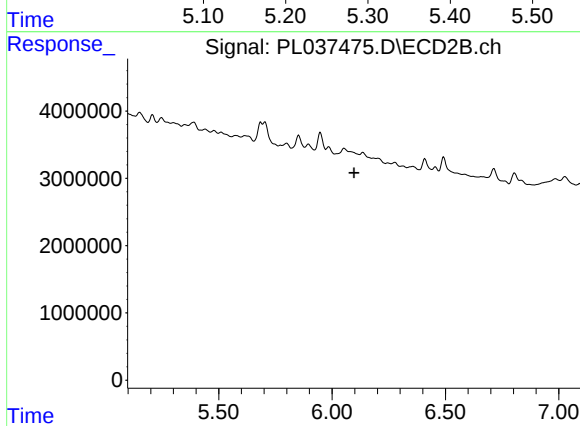

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

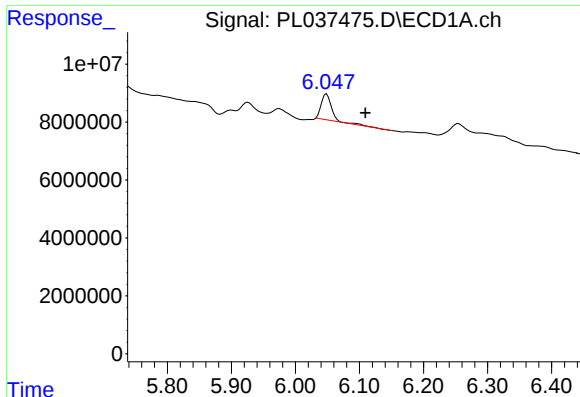

#15 Endosulfan II


R.T.: 6.049 min
Delta R.T.: -0.061 min
Response: 9718274
Conc: 1.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

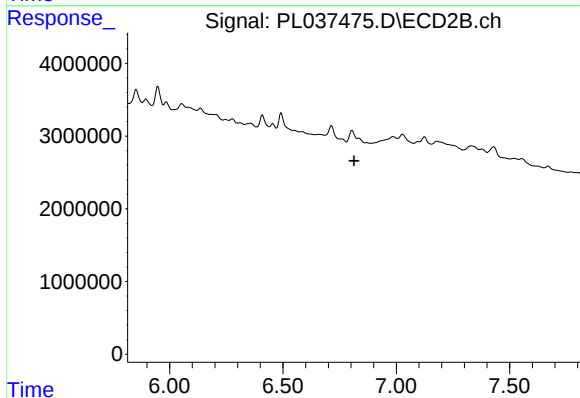


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.814 min
Response: 0
Conc: N.D.

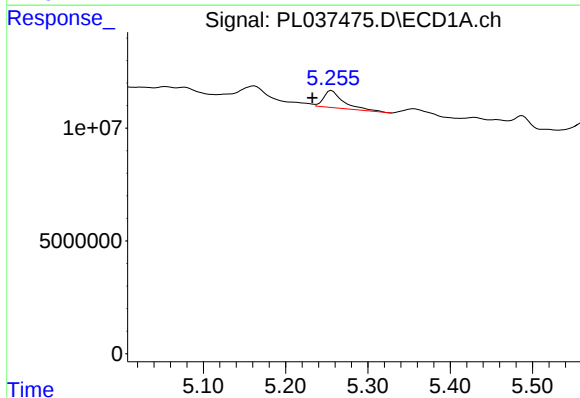


#25 Chlordane-3

R.T.: 5.256 min
Delta R.T.: 0.024 min
Response: 12912024
Conc: 12.15 ng/ml

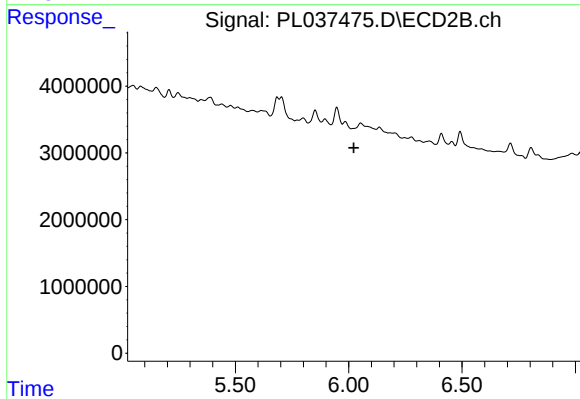

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

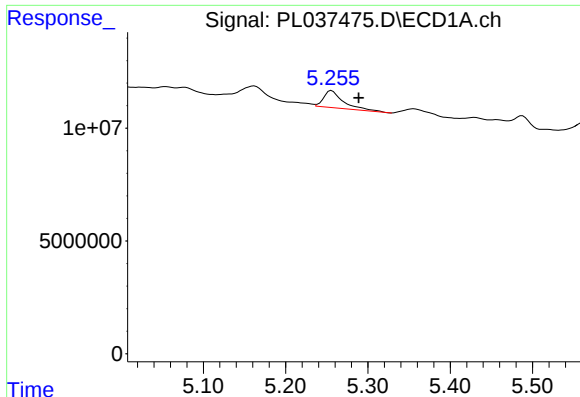

#26 Chlordane-4


R.T.: 5.256 min
Delta R.T.: -0.033 min
Response: 12912024
Conc: 13.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

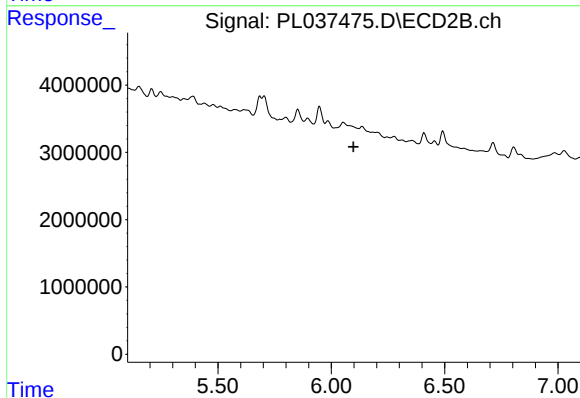


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

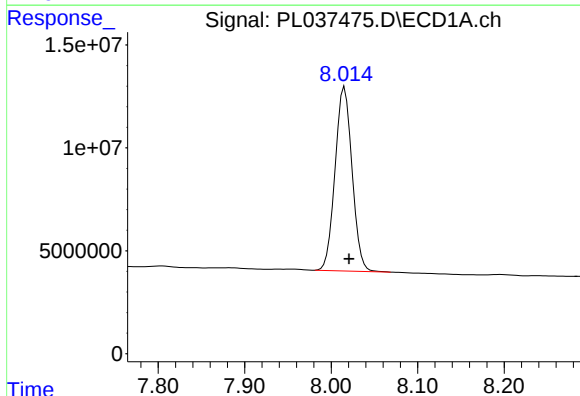

#28 Decachlorobiphenyl

R.T.: 8.016 min
Delta R.T.: -0.005 min
Response: 121432010
Conc: 20.12 ng/ml

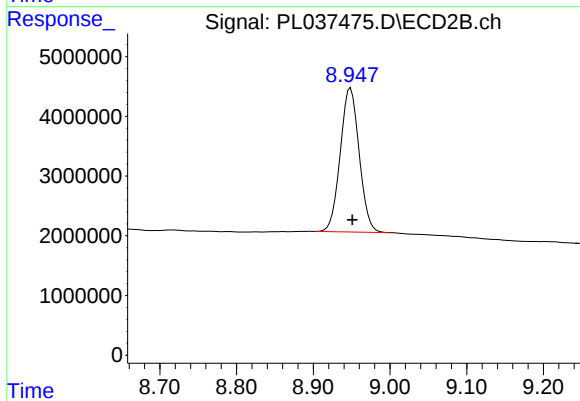

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.002 min
Response: 41479445
Conc: 20.91 ng/ml