

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
 Data File : PL037487.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2018 22:23
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:37:24 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.937	129.5E6	46467072	16.371	16.795
28)	SA Decachlor...	8.015	8.949	127.0E6	39283811	21.048	19.801
Target Compounds							
6)	B beta-BHC	4.253f	0.000	6817902	0	1.495	N.D. #
8)	B Heptachlo...	0.000	5.781	0	6589127	N.D.	2.311 #
10)	B gamma-Chl...	5.163f	0.000	9369485	0	1.000	N.D. #
13)	MA Dieldrin	5.537f	0.000	269431	0	0.030	N.D. #
14)	MA Endrin	5.849	0.000	7643712	0	0.970	N.D. #
21)	B Endrin ke...	6.935f	0.000	94058761	0	13.226	N.D. #
23)	Chlordane-1	4.132	0.000	9908737	0	32.271	N.D. #
25)	Chlordane-3	5.163	0.000	9369485	0	8.815	N.D. #
27)	Chlordane-5	5.849	0.000	7643712	0	58.408	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
Data File : PL037487.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2018 22:23
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:37:24 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

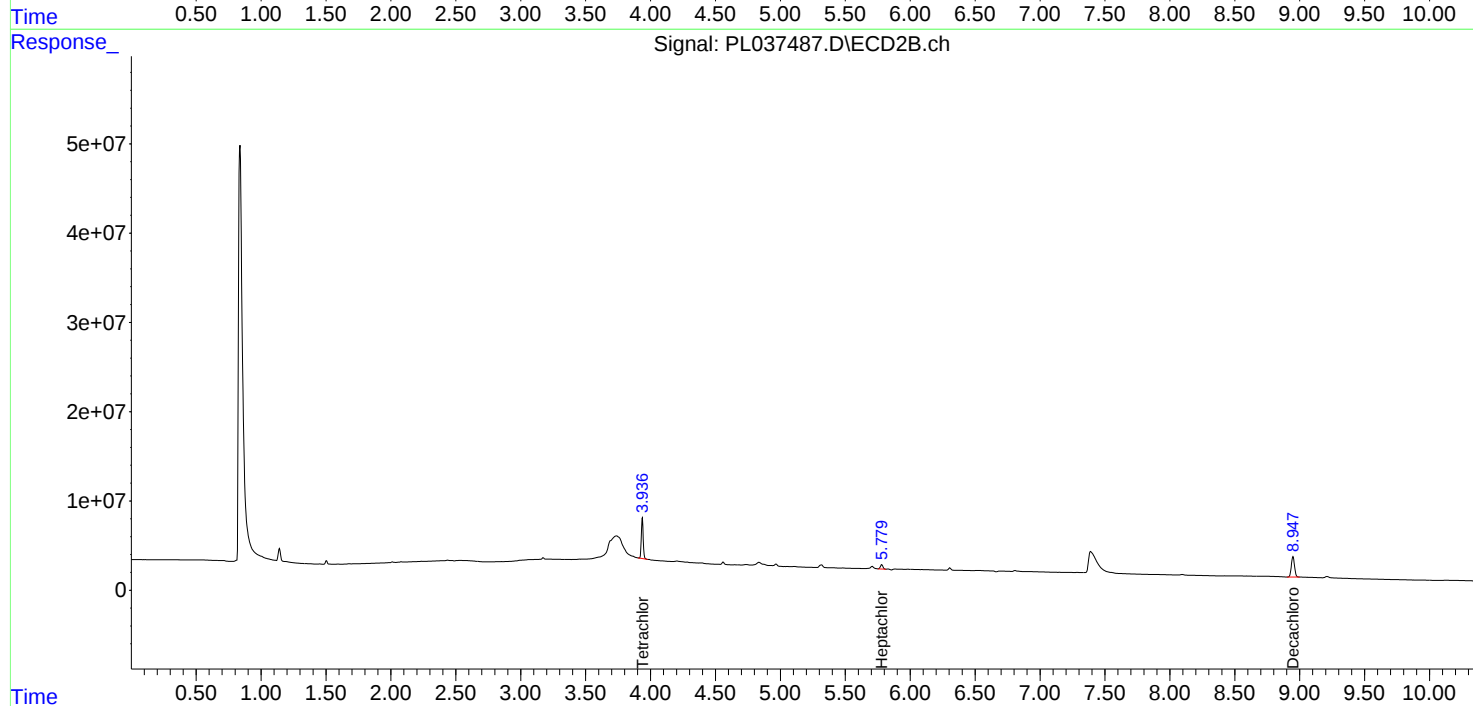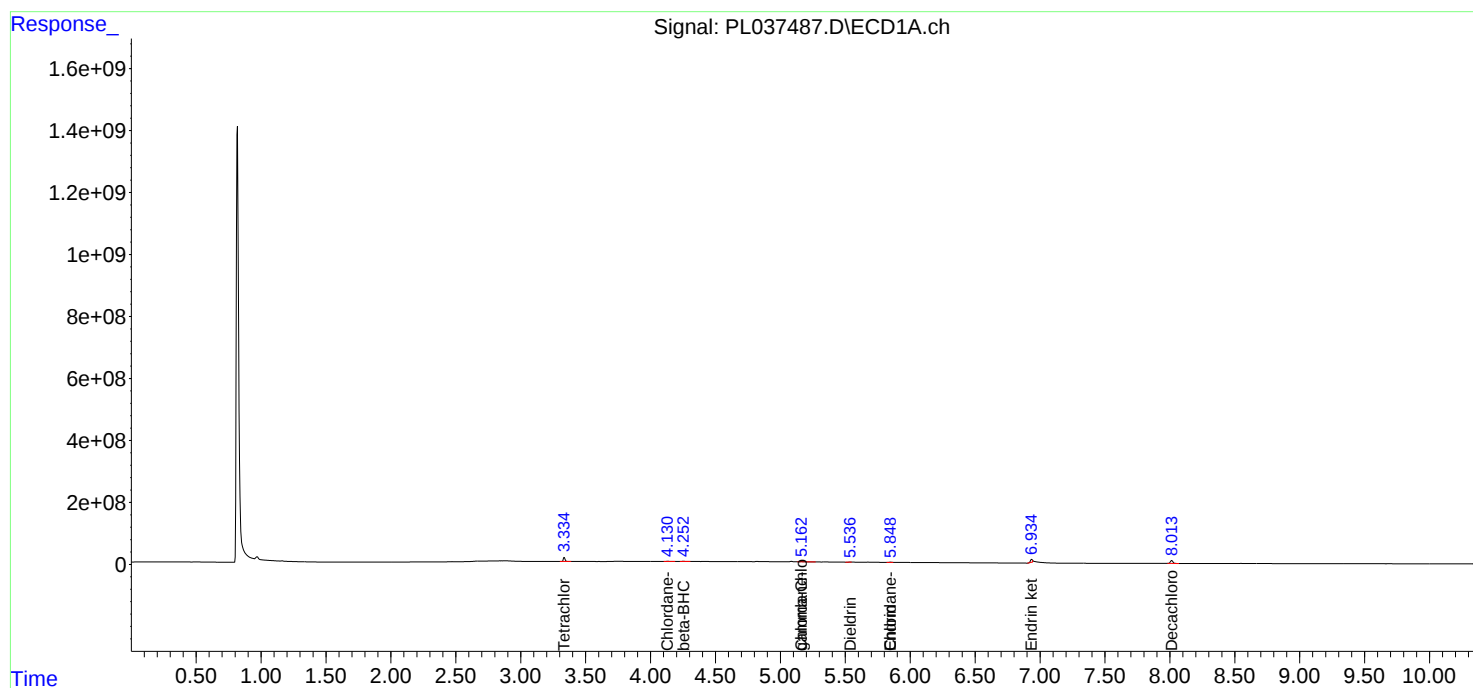


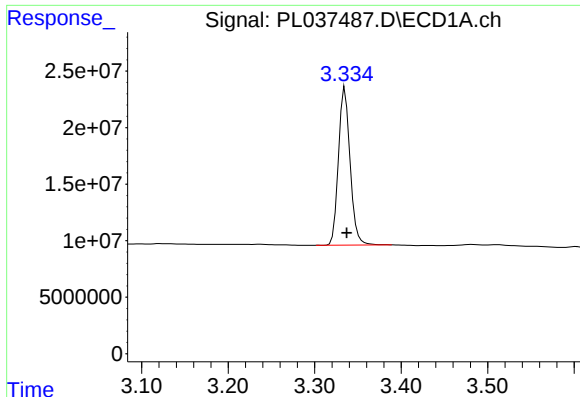

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 129500071
Conc: 16.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

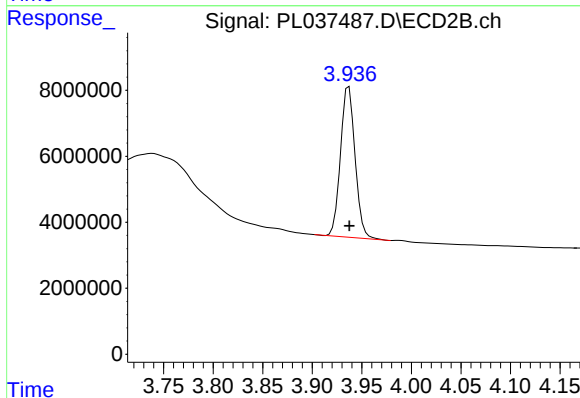


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 46467072
Conc: 16.79 ng/ml

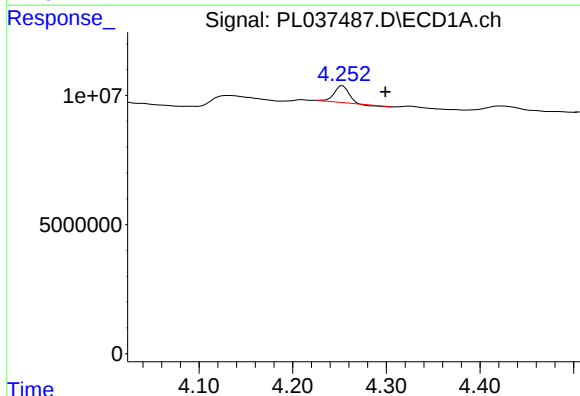


#6 beta-BHC

R.T.: 4.253 min
Delta R.T.: -0.045 min
Response: 6817902
Conc: 1.49 ng/ml

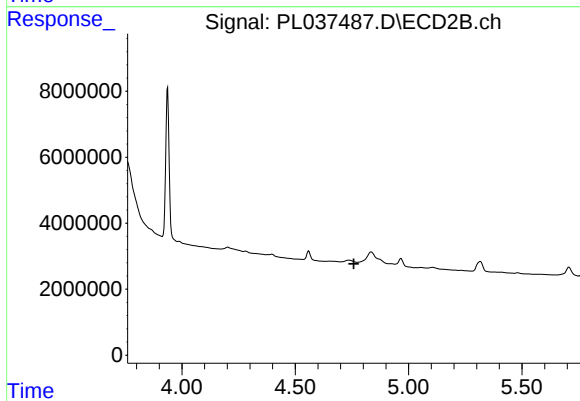

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

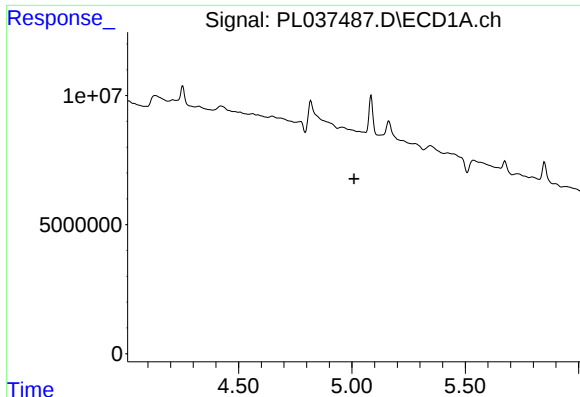

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.010 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

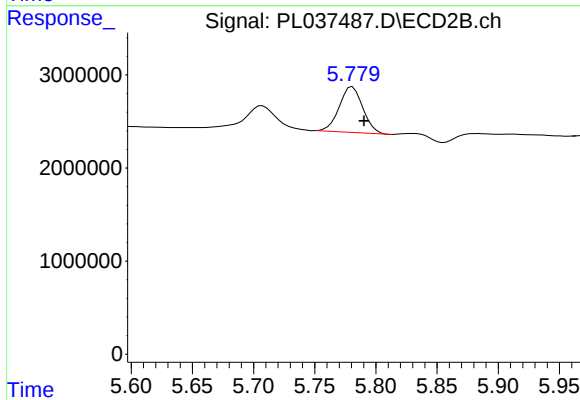


#8 Heptachlor epoxide

R.T.: 5.781 min
Delta R.T.: -0.010 min
Response: 6589127
Conc: 2.31 ng/ml

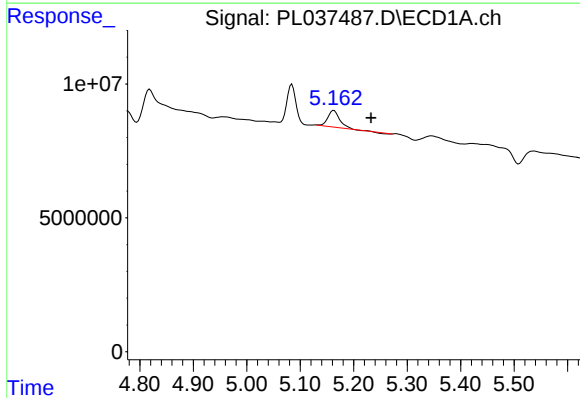


#10 gamma-Chlordane

R.T.: 5.163 min
Delta R.T.: -0.070 min
Response: 9369485
Conc: 1.00 ng/ml

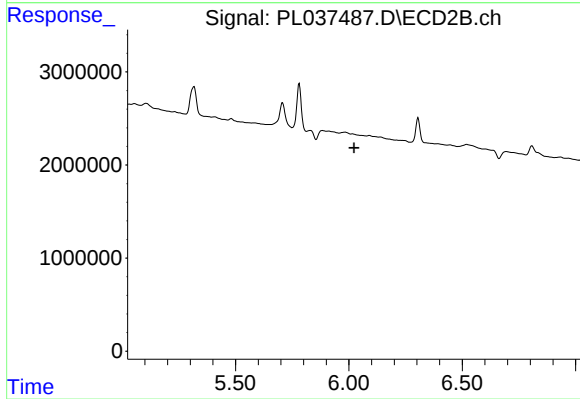

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

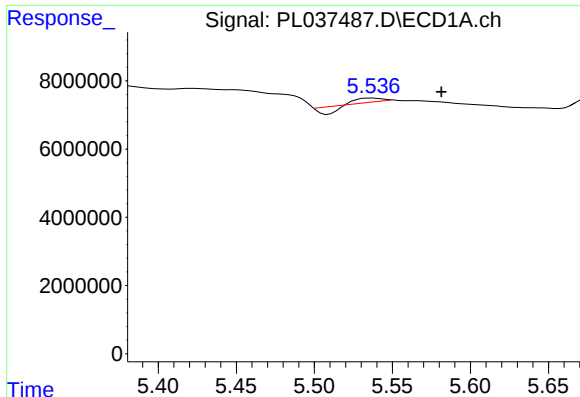

#13 Dieldrin


R.T.: 5.537 min
Delta R.T.: -0.044 min
Response: 269431
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

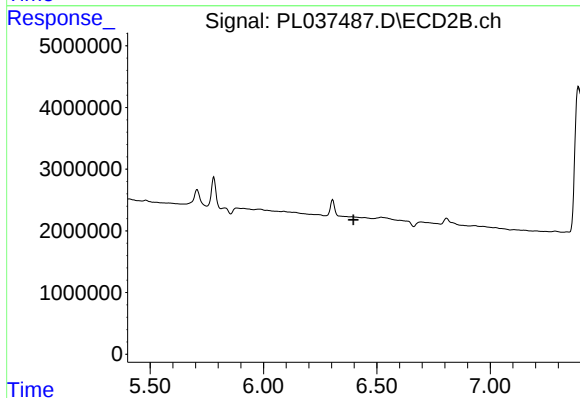


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.398 min
Response: 0
Conc: N.D.

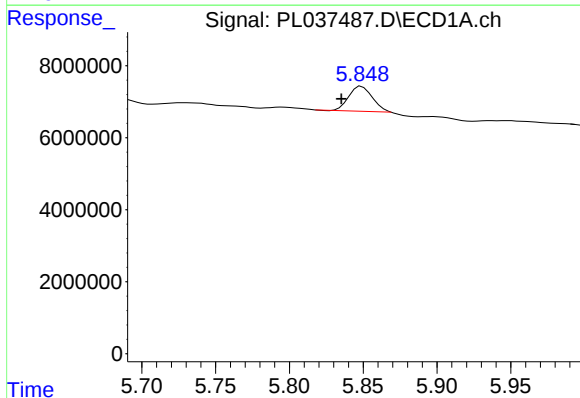


#14 Endrin

R.T.: 5.849 min
Delta R.T.: 0.014 min
Response: 7643712
Conc: 0.97 ng/ml

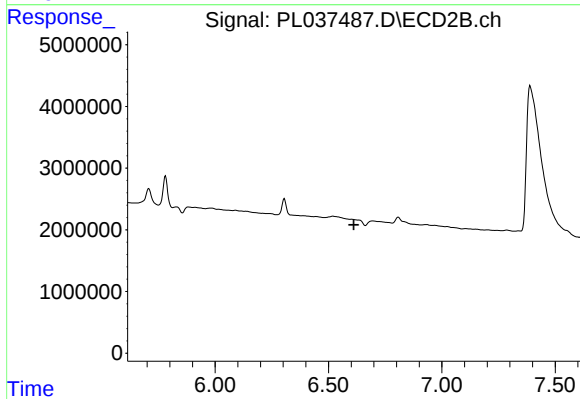

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

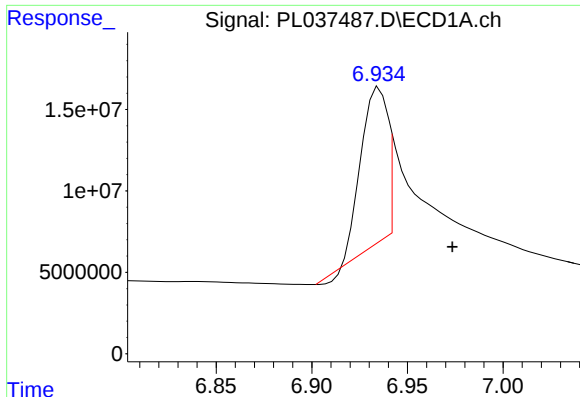

#21 Endrin ketone


R.T.: 6.935 min
Delta R.T.: -0.038 min
Response: 94058761
Conc: 13.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

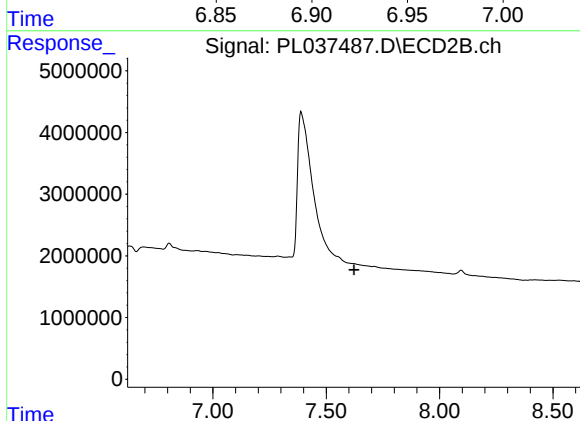


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.623 min
Response: 0
Conc: N.D.

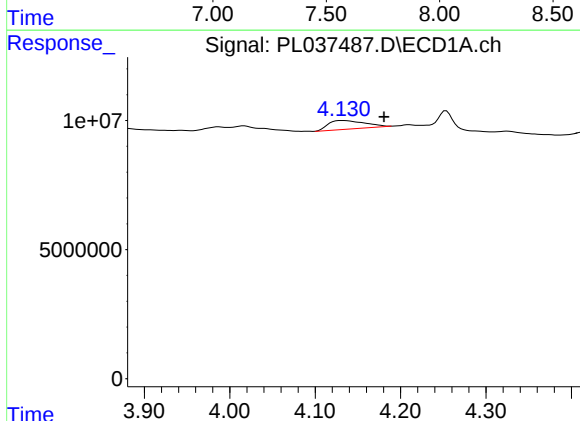


#23 Chlordane-1

R.T.: 4.132 min
Delta R.T.: -0.048 min
Response: 9908737
Conc: 32.27 ng/ml

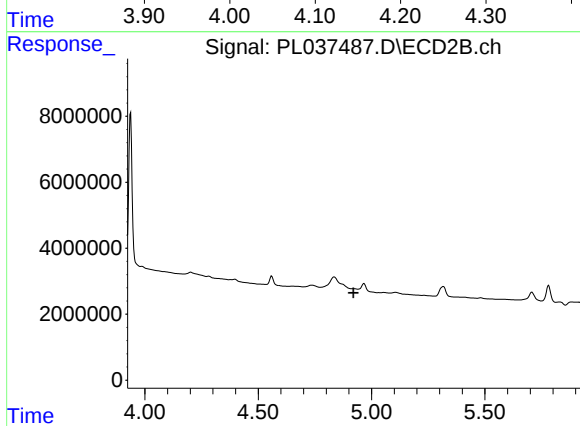

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

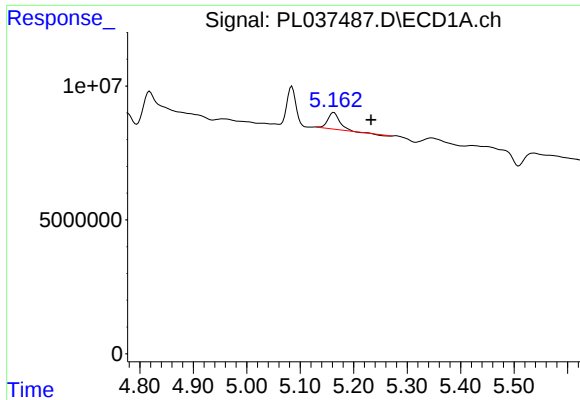

#25 Chlordane-3


R.T.: 5.163 min
Delta R.T.: -0.069 min
Response: 9369485
Conc: 8.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

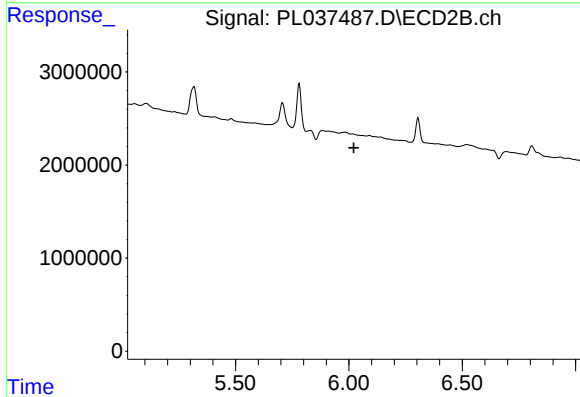


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

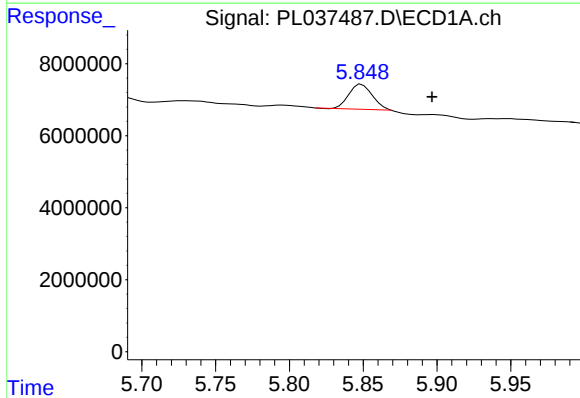


#27 Chlordane-5

R.T.: 5.849 min
Delta R.T.: -0.048 min
Response: 7643712
Conc: 58.41 ng/ml

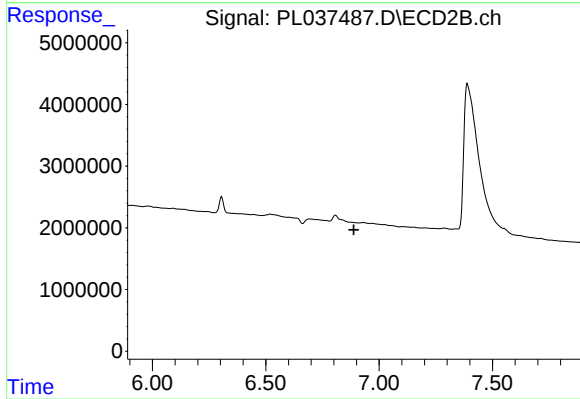

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

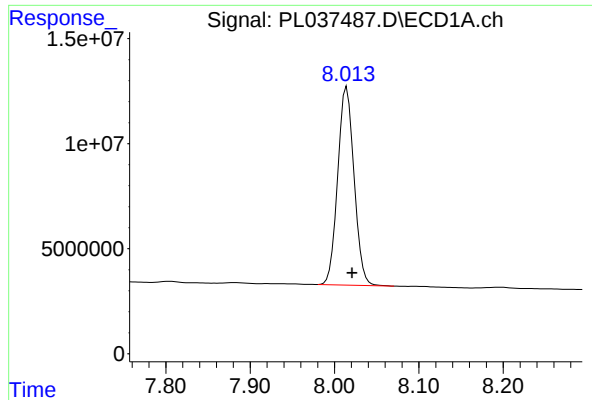

#28 Decachlorobiphenyl

R.T.: 8.015 min
Delta R.T.: -0.006 min
Response: 127006855
Conc: 21.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

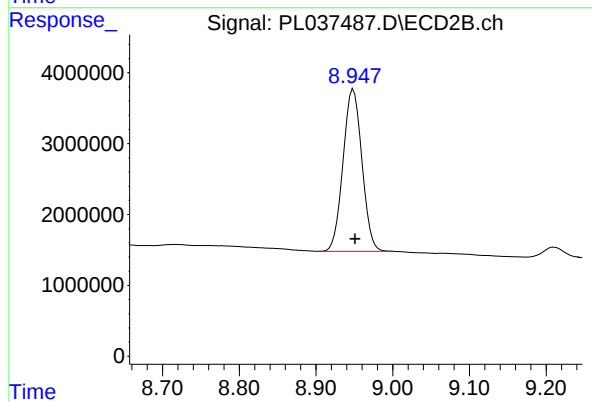

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.002 min
Response: 39283811
Conc: 19.80 ng/ml