

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
 Data File : PL037492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2018 23:33
 Operator : UA\AJ
 Sample : J3242-15
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:38:33 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.937	79650662	26409873	10.069	9.546
28)	SA Decachlor...	8.016	8.950	67988628	23228413	11.268	11.708
Target Compounds							
2)	A alpha-BHC	3.720f	0.000	9118178	0	0.745	N.D. #
6)	B beta-BHC	4.254f	0.000	17839781	0	3.911	N.D. #
10)	B gamma-Chl...	5.164f	0.000	7206263	0	0.769	N.D. #
25)	Chlordane-3	5.164	0.000	7206263	0	6.780	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
Data File : PL037492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2018 23:33
Operator : UA\AJ
Sample : J3242-15
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:38:33 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

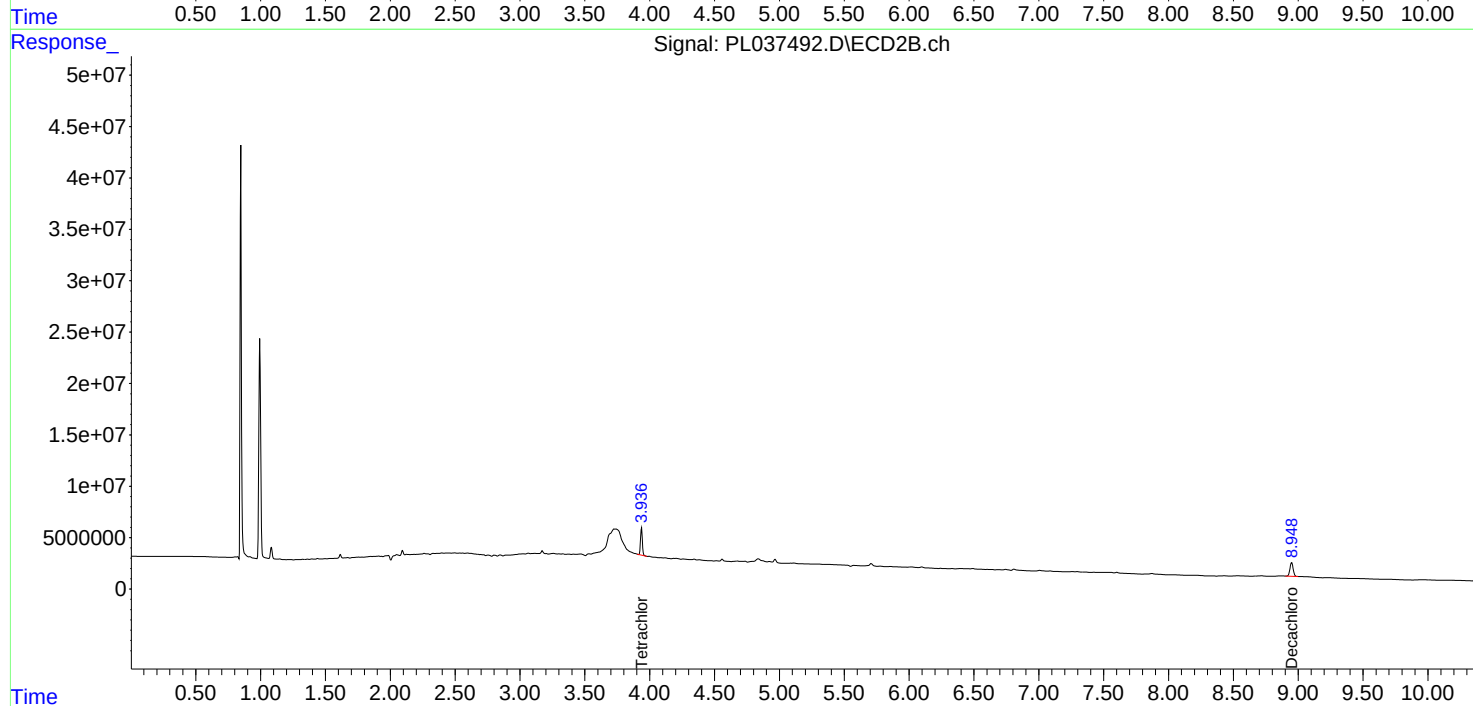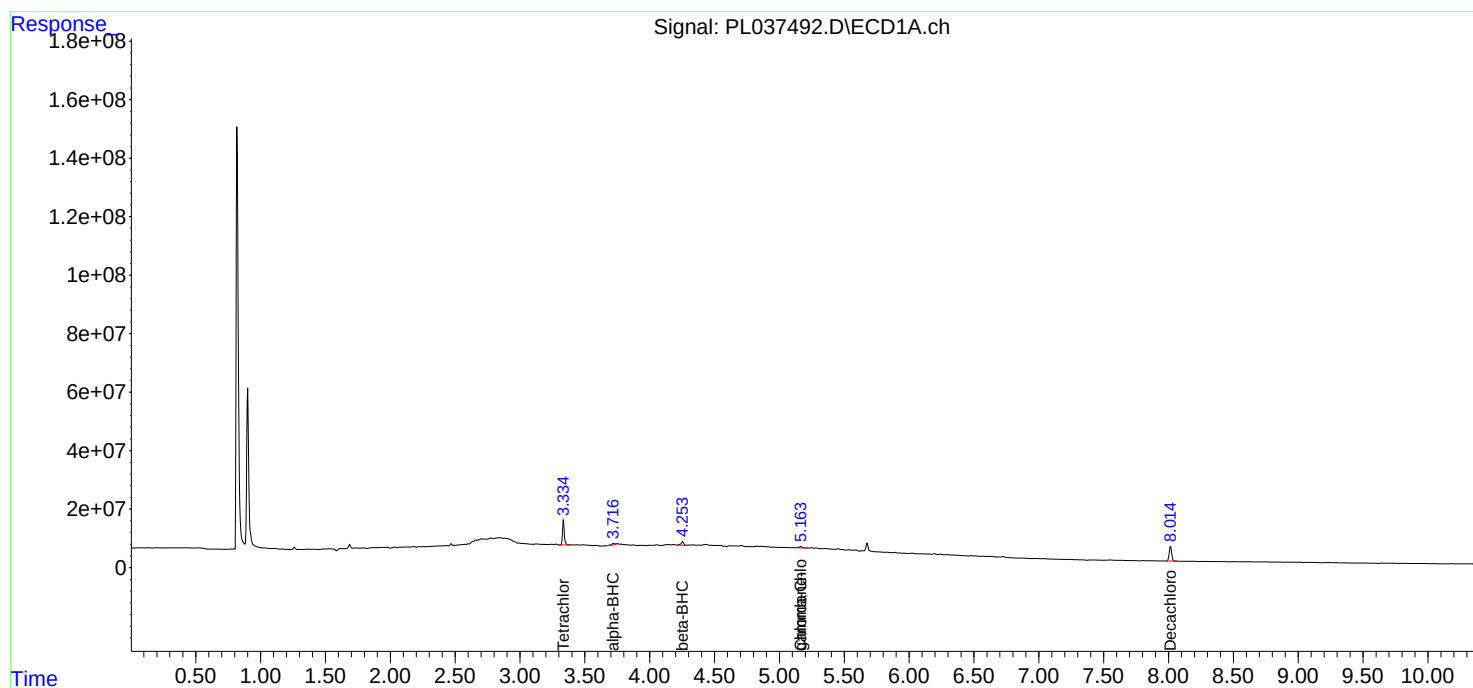


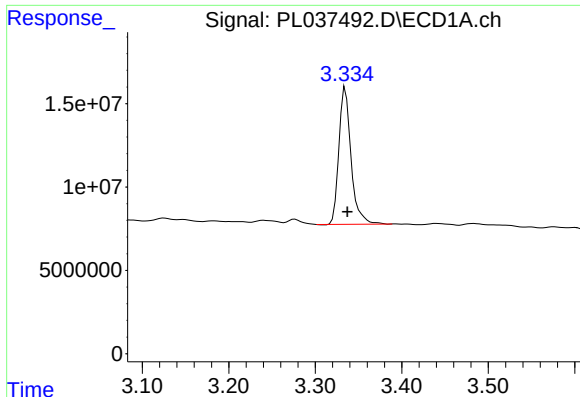

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 79650662
Conc: 10.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

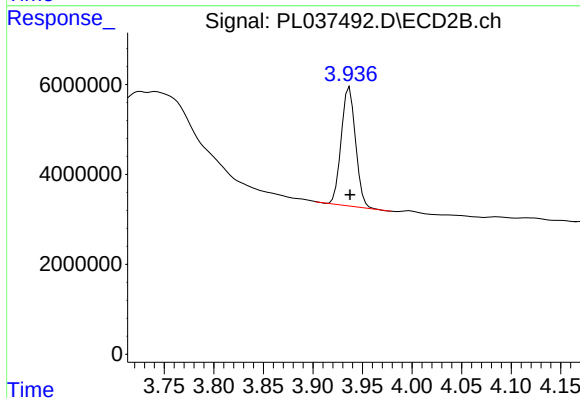


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 26409873
Conc: 9.55 ng/ml

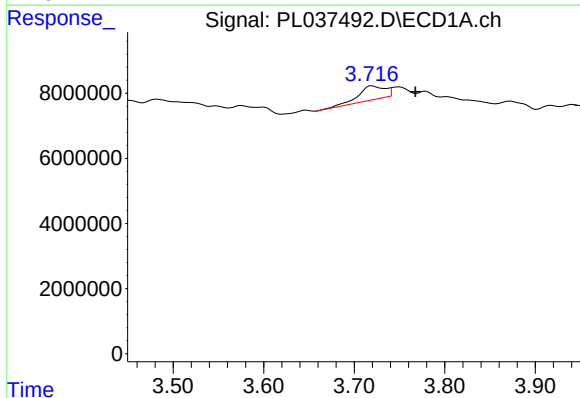


#2 alpha-BHC

R.T.: 3.720 min
Delta R.T.: -0.048 min
Response: 9118178
Conc: 0.74 ng/ml

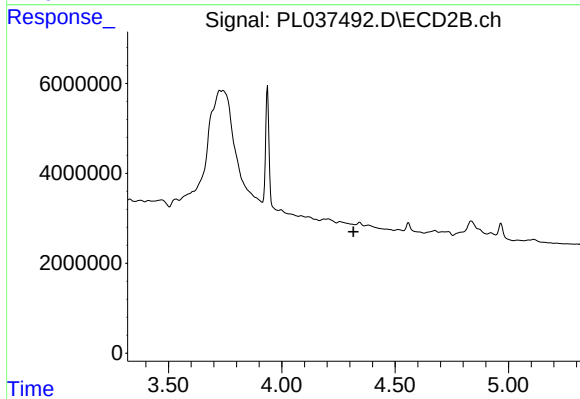

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

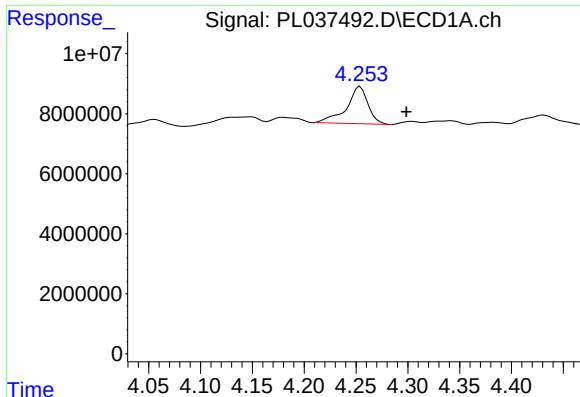

#6 beta-BHC


R.T.: 4.254 min
Delta R.T.: -0.045 min
Response: 17839781
Conc: 3.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

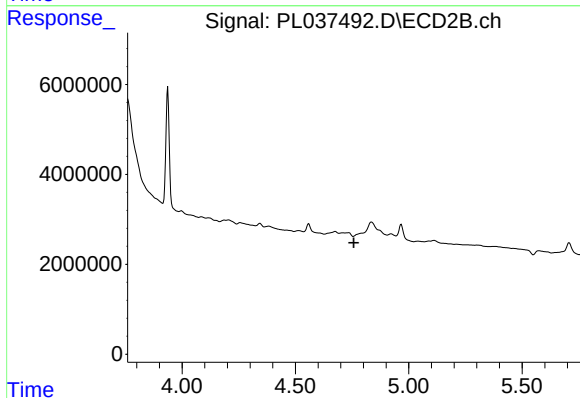


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

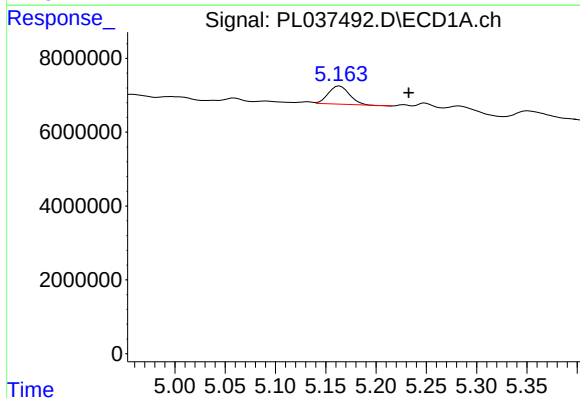


#10 gamma-Chlordane

R.T.: 5.164 min
Delta R.T.: -0.069 min
Response: 7206263
Conc: 0.77 ng/ml

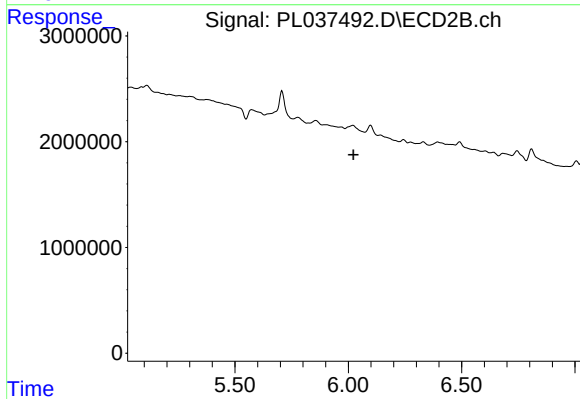

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

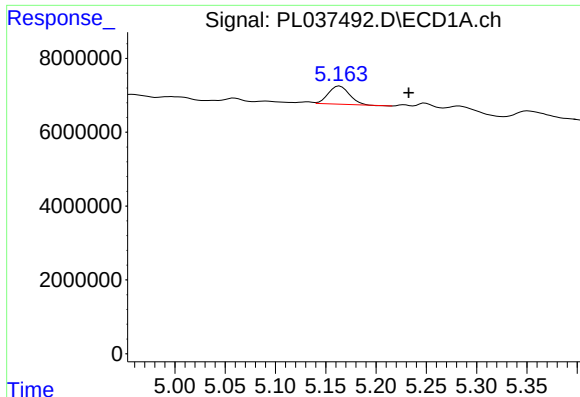

#25 Chlordane-3


R.T.: 5.164 min
Delta R.T.: -0.068 min
Response: 7206263
Conc: 6.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

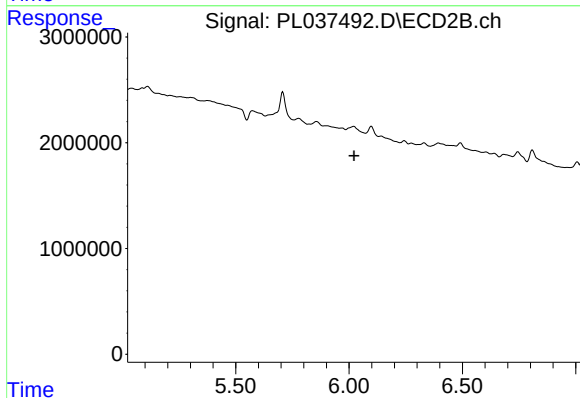


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

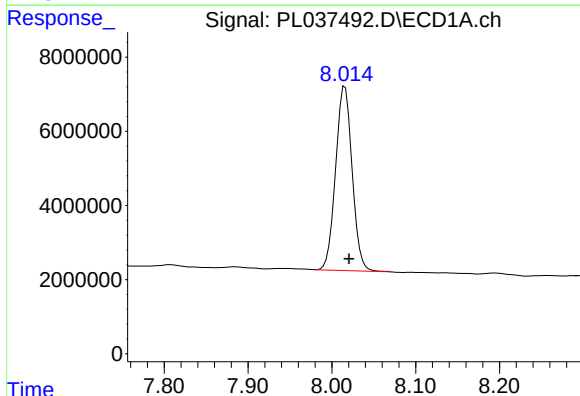

#28 Decachlorobiphenyl

R.T.: 8.016 min
Delta R.T.: -0.005 min
Response: 67988628
Conc: 11.27 ng/ml

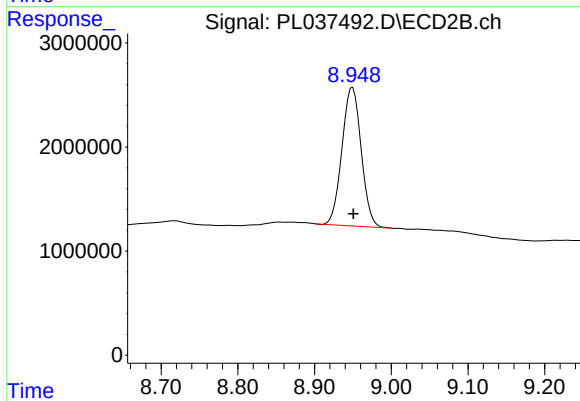

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: -0.001 min
Response: 23228413
Conc: 11.71 ng/ml