

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
 Data File : PL037510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2018 08:19
 Operator : UA\AJ
 Sample : J3682-01
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 09:11:23 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.346	3.936	114.4E6	44004343	14.462	15.905
28)	SA Decachlor...	8.030	8.955	92668022	29893265	15.358	15.068
Target Compounds							
2)	A alpha-BHC	3.757	0.000	43209272	0	3.529	N.D. #
4)	MA Heptachlor	4.276f	0.000	62571775	0	6.107	N.D. #
5)	MB Aldrin	4.543f	0.000	23305715	0	2.290	N.D. #
6)	B beta-BHC	4.276	0.000	62571775	0	13.719	N.D. #
7)	B delta-BHC	4.506	4.964	24577825	20211840	2.323	7.167 #
12)	B 4,4'-DDE	5.468	0.000	8987549	0	1.018	N.D. #
19)	B Endosulfa...	6.523	0.000	14002046	0	2.096	N.D. #
20)	A Methoxychlor	6.701f	0.000	7527429	0	2.215	N.D. #
23)	Chlordane-1	0.000	4.964	0	20211840	N.D.	168.206 #
24)	Chlordane-2	4.662	0.000	6946670	0	19.513	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
Data File : PL037510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2018 08:19
Operator : UA\AJ
Sample : J3682-01
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 09:11:23 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

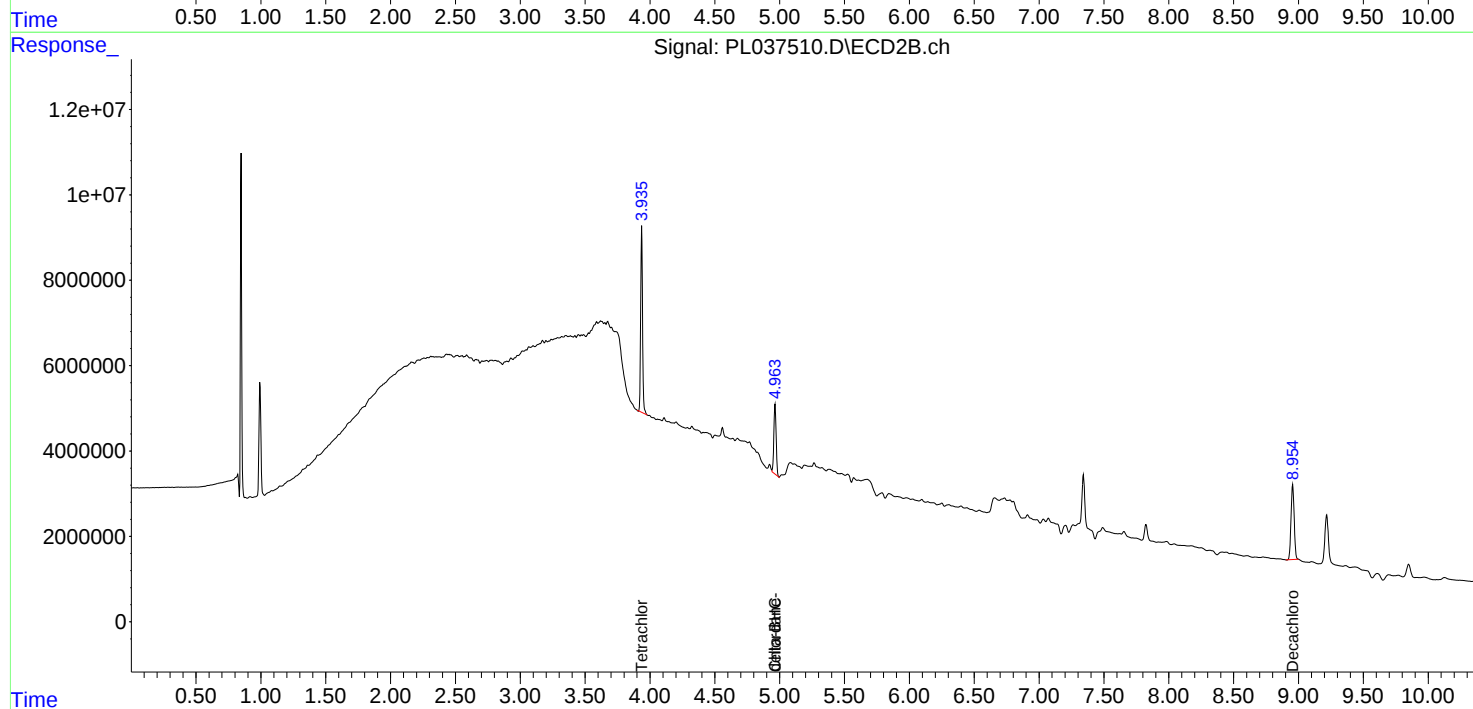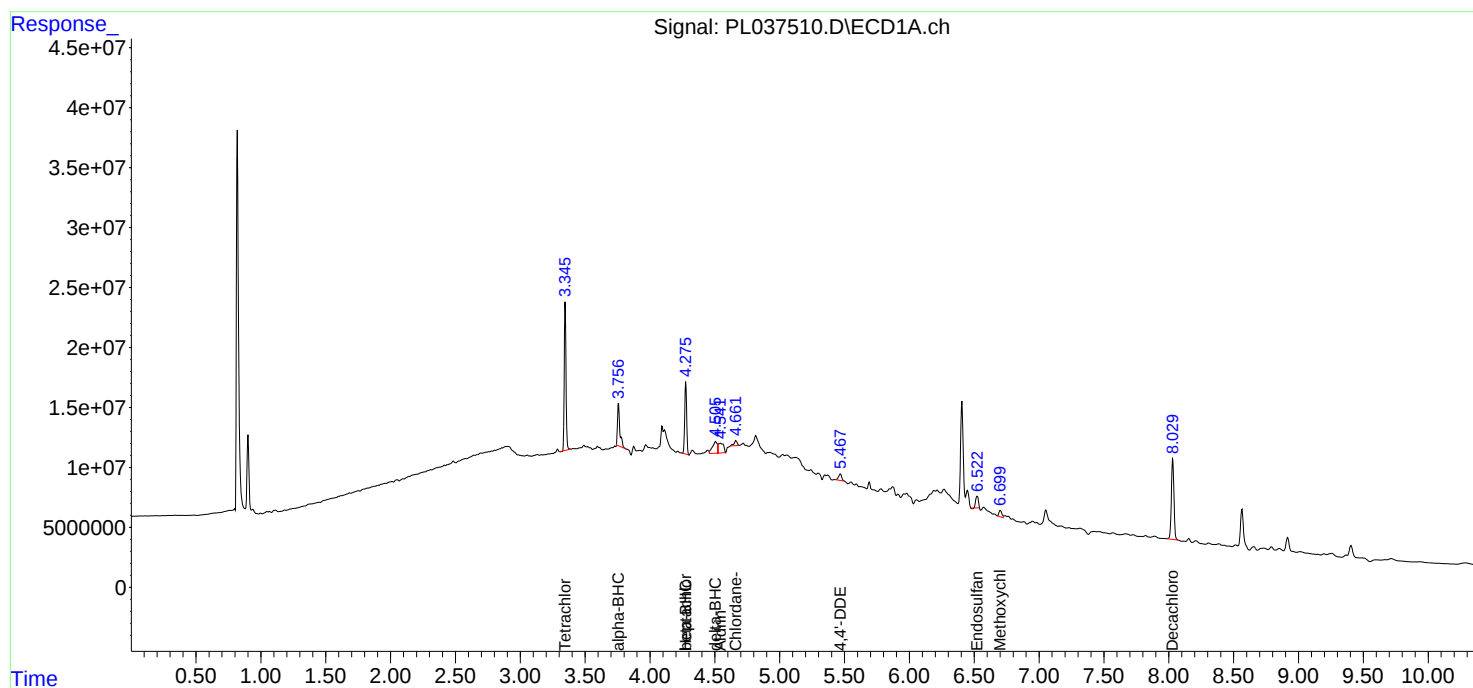


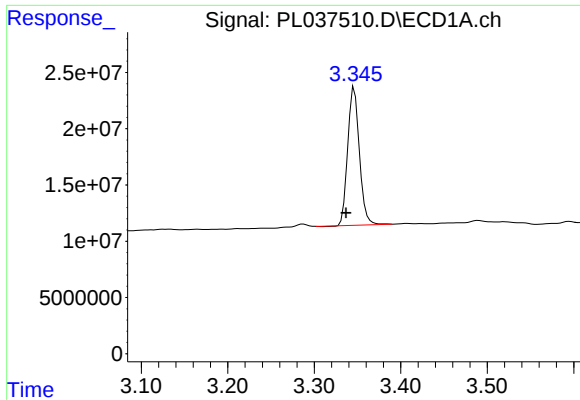

#1 Tetrachloro-m-xylene


R.T.: 3.346 min
Delta R.T.: 0.009 min
Response: 114399537
Conc: 14.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

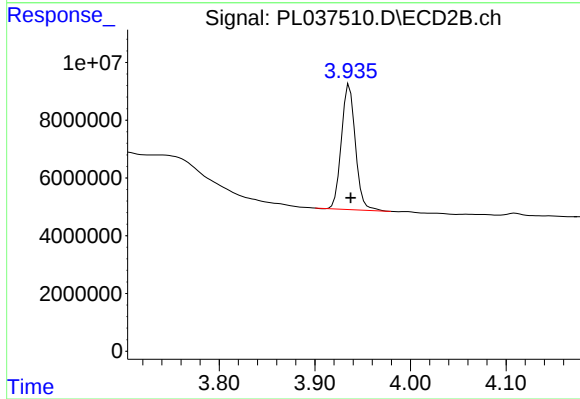


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.001 min
Response: 44004343
Conc: 15.90 ng/ml

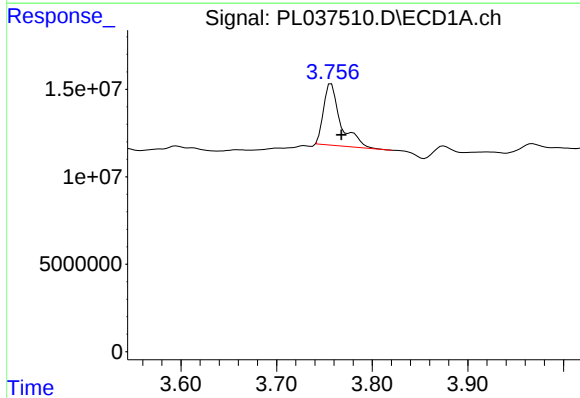


#2 alpha-BHC

R.T.: 3.757 min
Delta R.T.: -0.010 min
Response: 43209272
Conc: 3.53 ng/ml

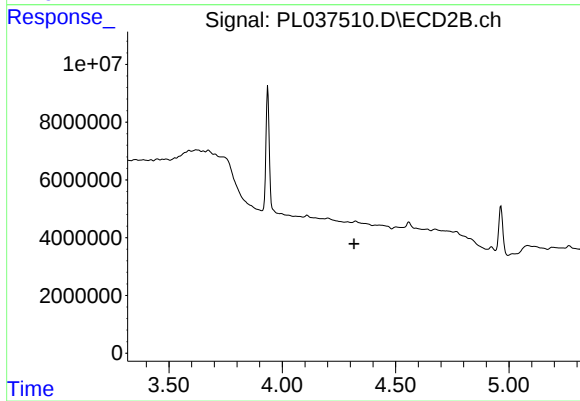

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

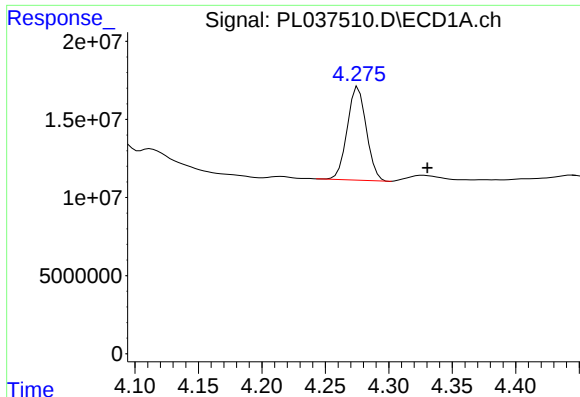

#4 Heptachlor


R.T.: 4.276 min
Delta R.T.: -0.054 min
Response: 62571775
Conc: 6.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

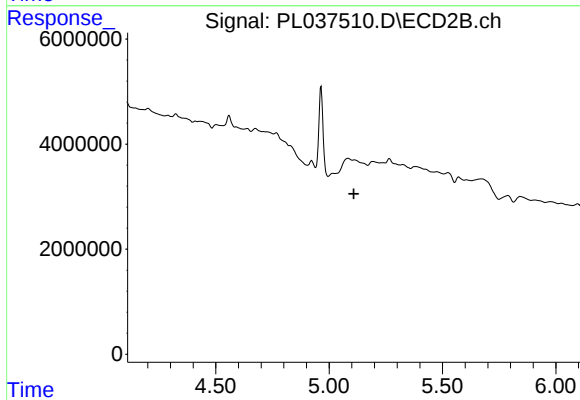


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

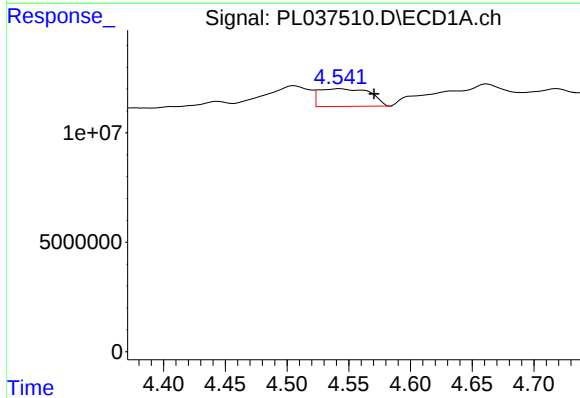


#5 Aldrin

R.T.: 4.543 min
Delta R.T.: -0.028 min
Response: 23305715
Conc: 2.29 ng/ml

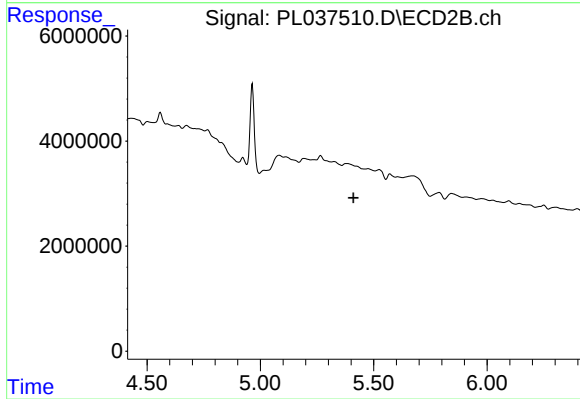

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.411 min
Response: 0
Conc: N.D.

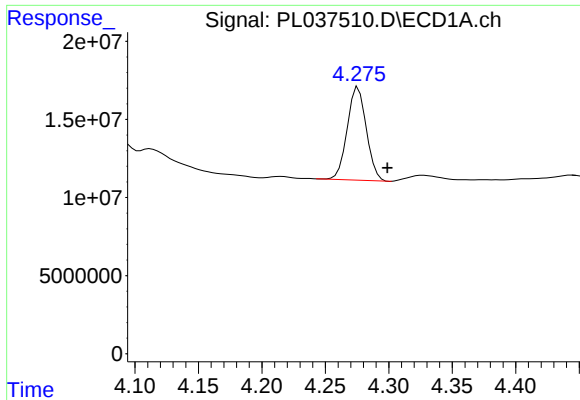

#6 beta-BHC


R.T.: 4.276 min
Delta R.T.: -0.023 min
Response: 62571775
Conc: 13.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

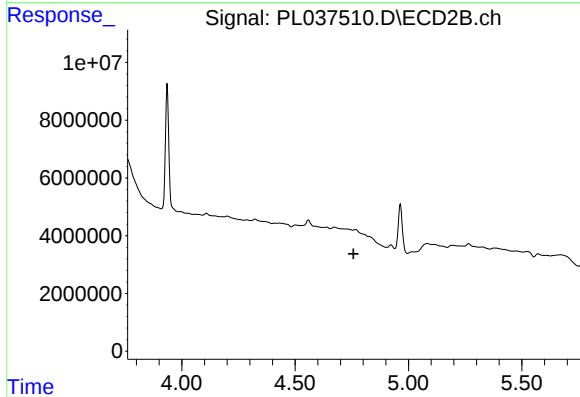


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

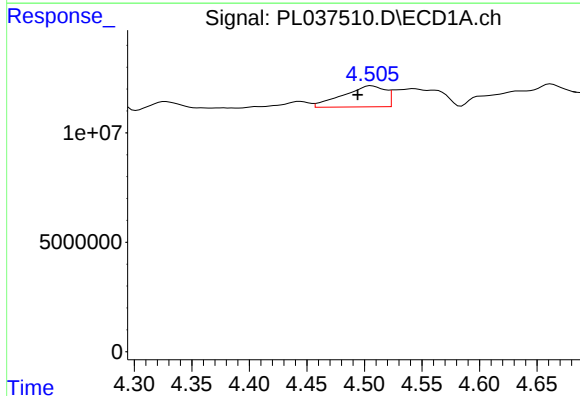


#7 delta-BHC

R.T.: 4.506 min
Delta R.T.: 0.012 min
Response: 24577825
Conc: 2.32 ng/ml

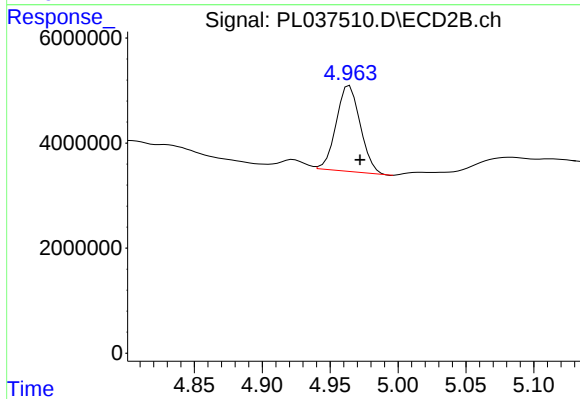

#7 delta-BHC


R.T.: 4.964 min
Delta R.T.: -0.008 min
Response: 20211840
Conc: 7.17 ng/ml

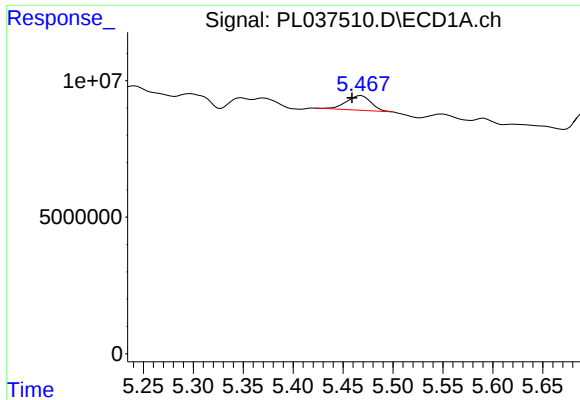

#12 4,4'-DDE


R.T.: 5.468 min
Delta R.T.: 0.009 min
Response: 8987549
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

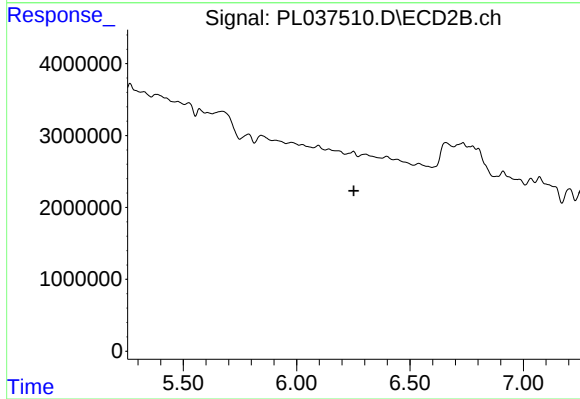


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

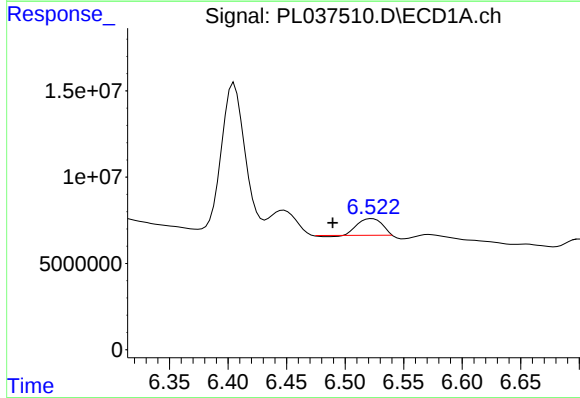


#19 Endosulfan Sulfate

R.T.: 6.523 min
Delta R.T.: 0.034 min
Response: 14002046
Conc: 2.10 ng/ml

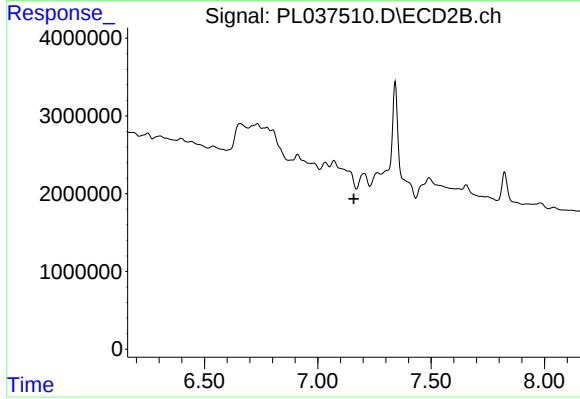

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.159 min
Response: 0
Conc: N.D.

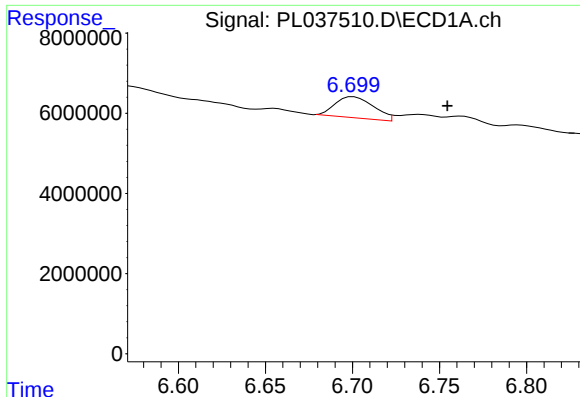

#20 Methoxychlor


R.T.: 6.701 min
Delta R.T.: -0.054 min
Response: 7527429
Conc: 2.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

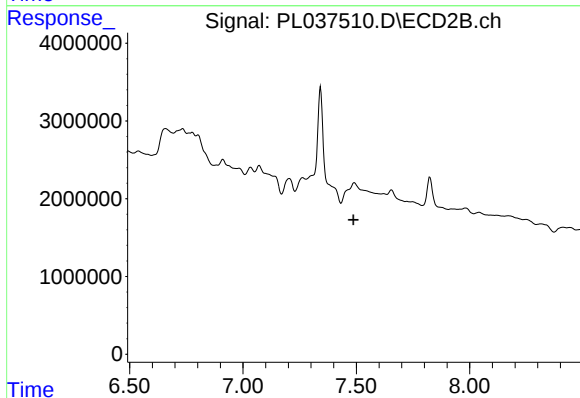


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.488 min
Response: 0
Conc: N.D.

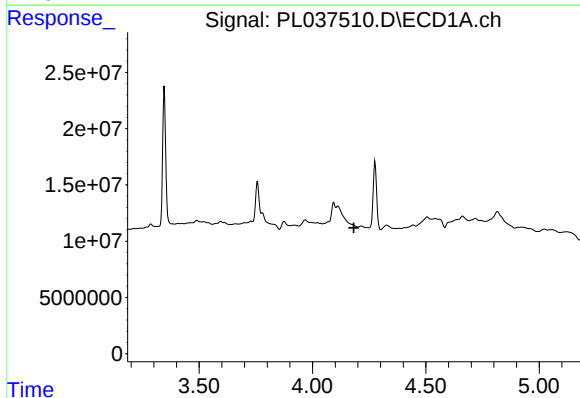


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.182 min
Response: 0
Conc: N.D.

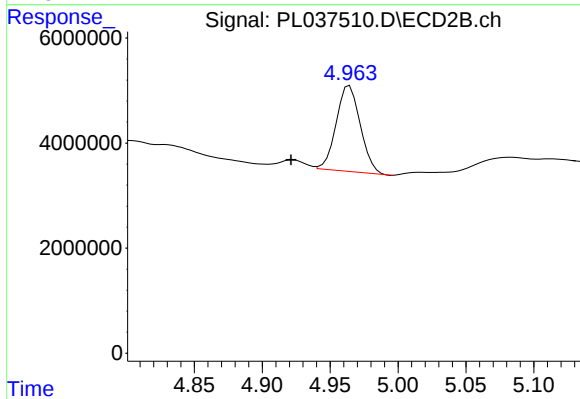

#23 Chlordane-1


R.T.: 4.964 min
Delta R.T.: 0.043 min
Response: 20211840
Conc: 168.21 ng/ml

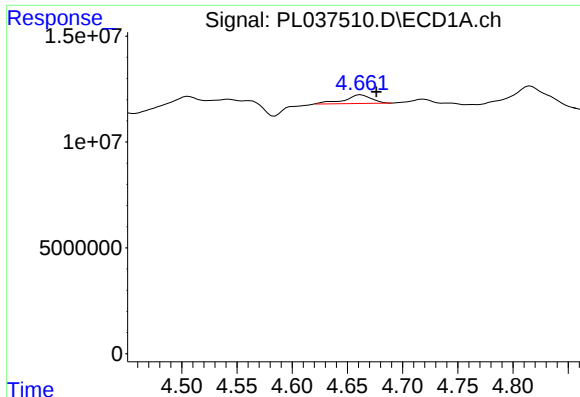

#24 Chlordane-2


R.T.: 4.662 min
Delta R.T.: -0.014 min
Response: 6946670
Conc: 19.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

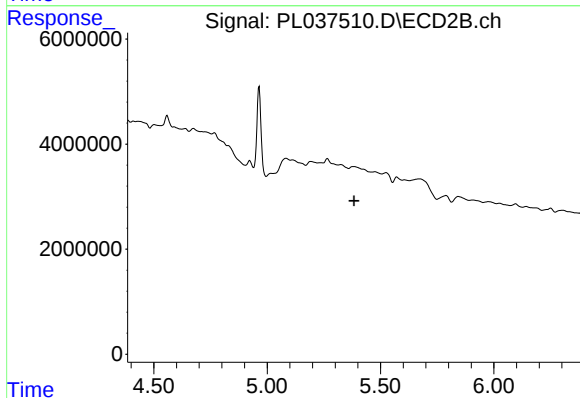


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.384 min
Response: 0
Conc: N.D.

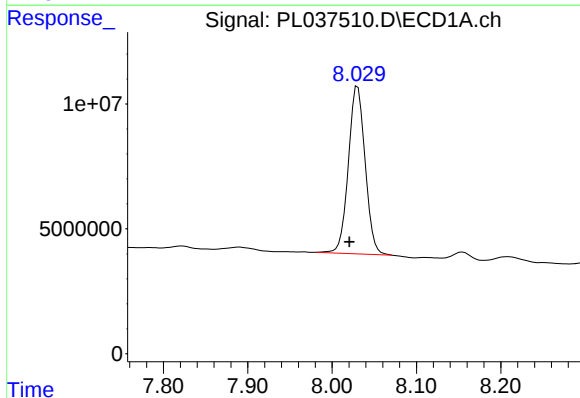

#28 Decachlorobiphenyl

R.T.: 8.030 min
Delta R.T.: 0.010 min
Response: 92668022
Conc: 15.36 ng/ml

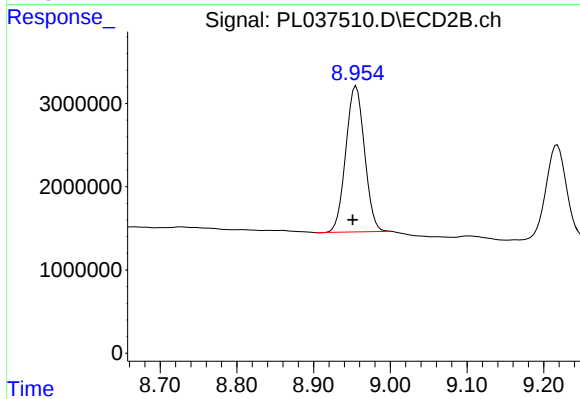

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: 0.004 min
Response: 29893265
Conc: 15.07 ng/ml