

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
 Data File : PL037511.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2018 08:34
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 09:12:01 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.936	135.4E6	48267656	17.117	17.446
28)	SA Decachlor...	8.023	8.951	127.5E6	40557476	21.137	20.443
Target Compounds							
3)	MA gamma-BHC...	3.998f	0.000	1795755	0	0.174	N.D. #
6)	B beta-BHC	4.259f	0.000	9268564	0	2.032	N.D. #
7)	B delta-BHC	4.516	0.000	5501654	0	0.520	N.D. #
8)	B Heptachlo...	0.000	5.782	0	26718529	N.D.	9.373 #
10)	B gamma-Chl...	5.166f	0.000	37959491	0	4.053	N.D. #
14)	MA Endrin	5.856	0.000	39004136	0	4.951	N.D. #
23)	Chlordane-1	4.128	0.000	21675018	0	71.791	N.D. #
24)	Chlordane-2	0.000	5.319	0	32581790	N.D.	257.460 #
25)	Chlordane-3	5.166	0.000	37959491	0	35.712	N.D. #
27)	Chlordane-5	5.856	0.000	39004136	0	300.889	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
Data File : PL037511.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2018 08:34
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 09:12:01 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

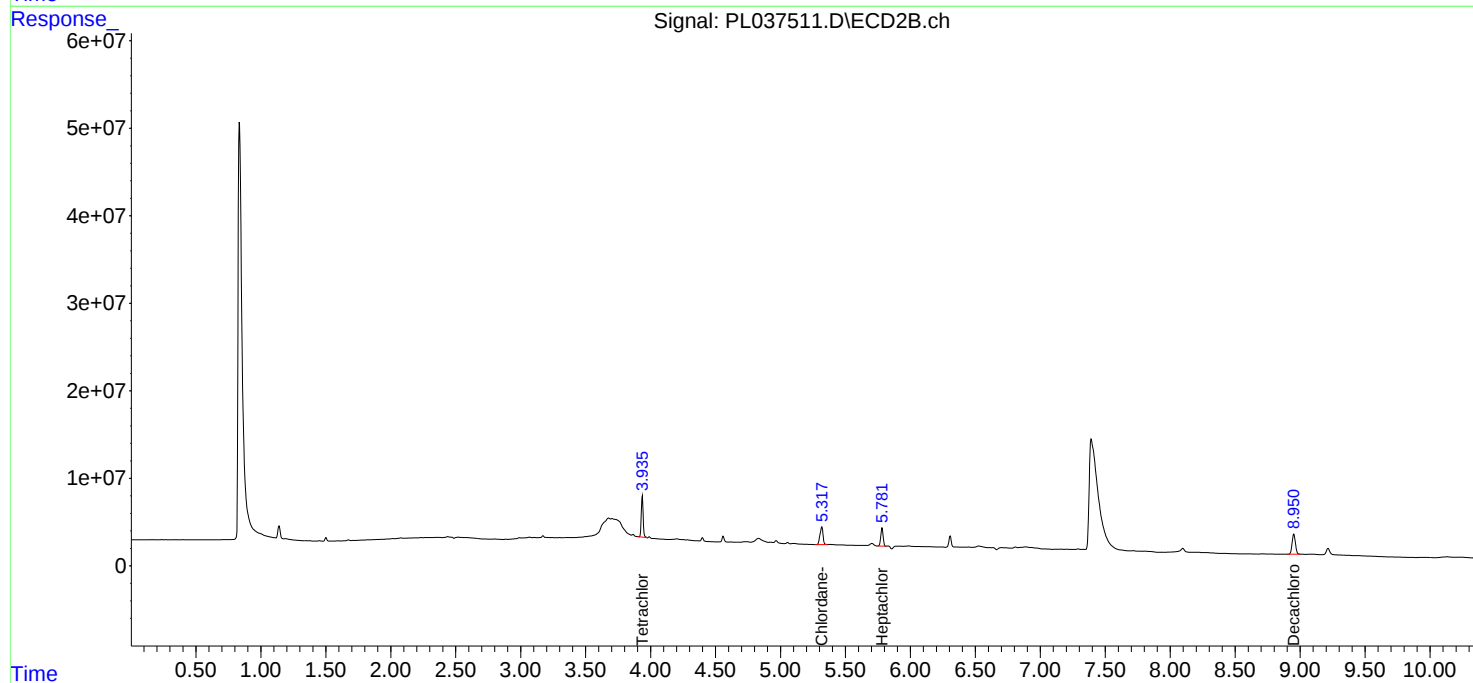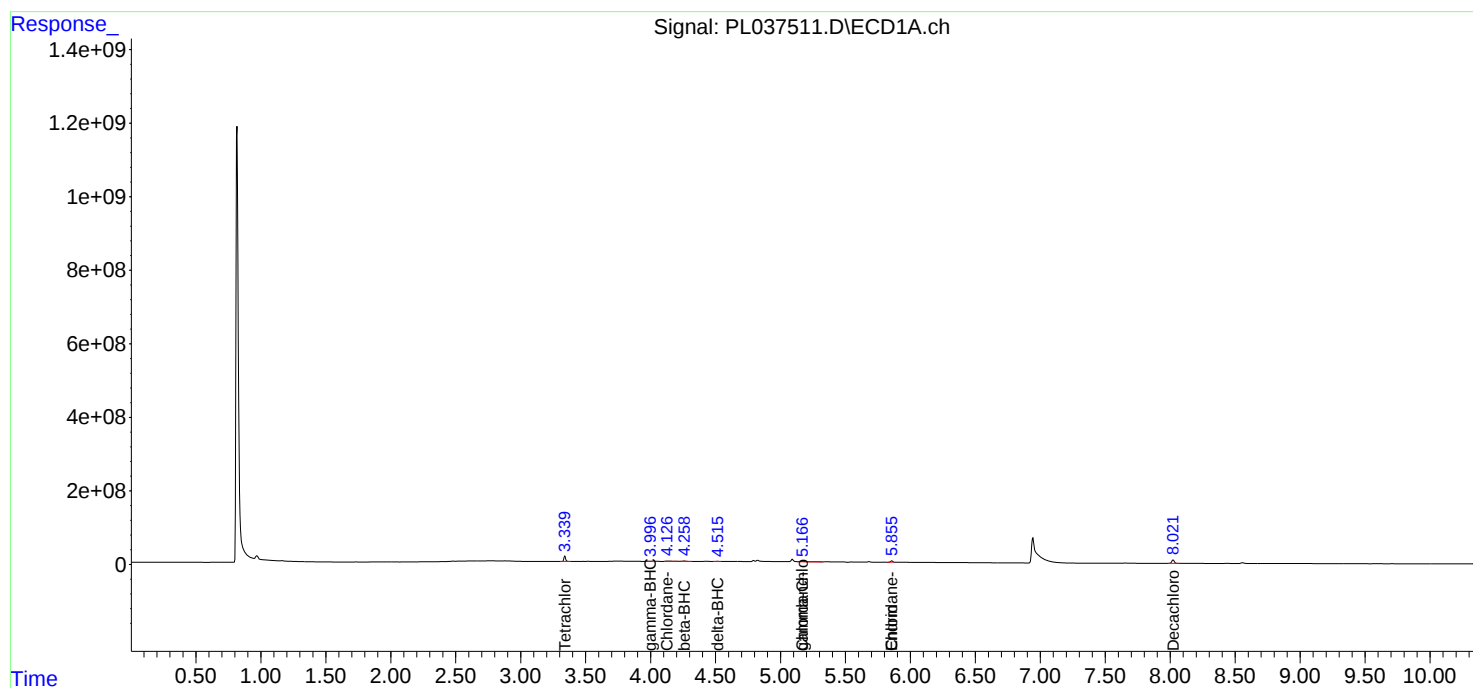


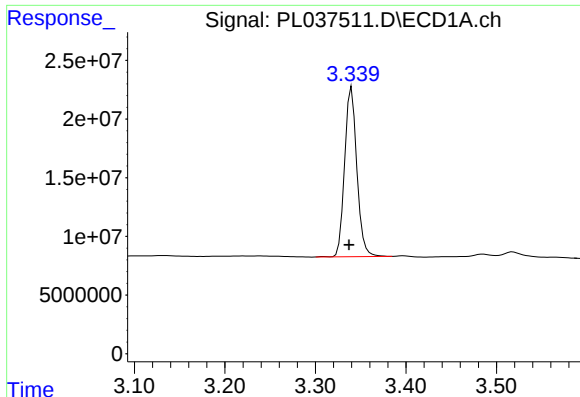

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: 0.003 min
Response: 135403447
Conc: 17.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

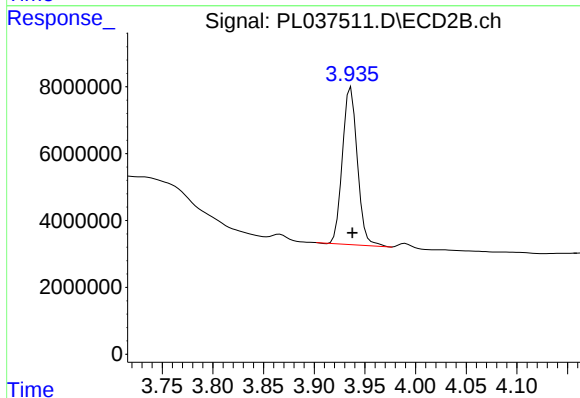


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.001 min
Response: 48267656
Conc: 17.45 ng/ml

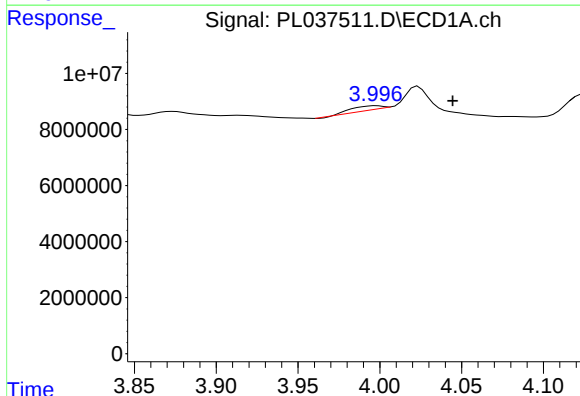


#3 gamma-BHC (Lindane)

R.T.: 3.998 min
Delta R.T.: -0.047 min
Response: 1795755
Conc: 0.17 ng/ml

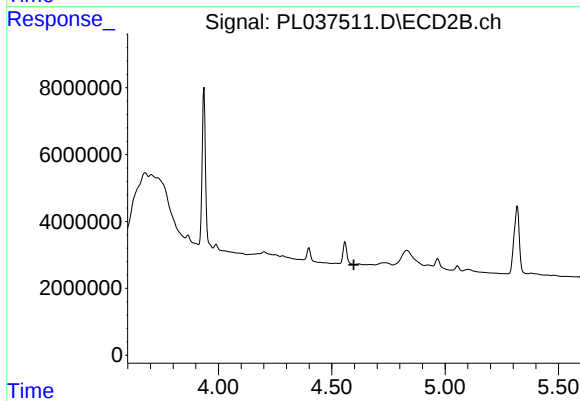

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

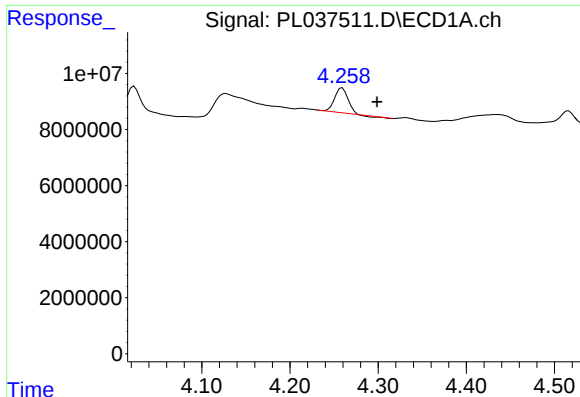

#6 beta-BHC


R.T.: 4.259 min
Delta R.T.: -0.039 min
Response: 9268564
Conc: 2.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

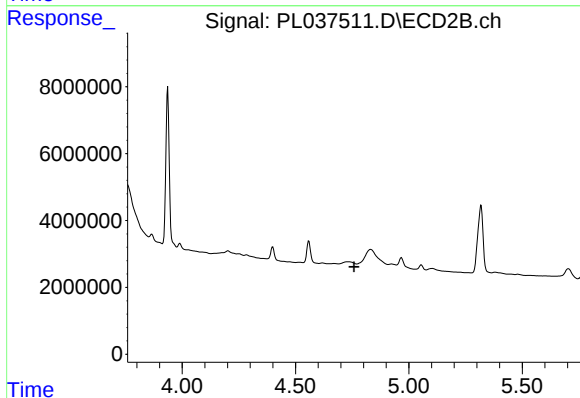


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

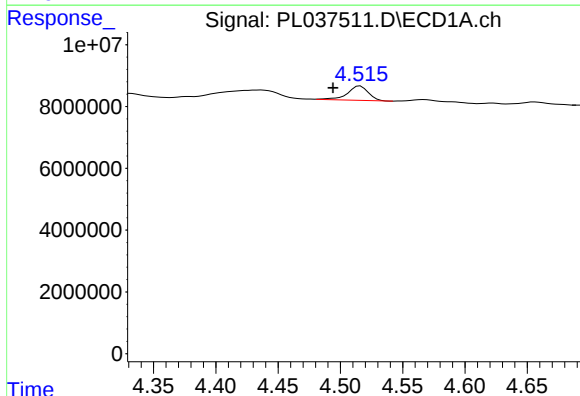


#7 delta-BHC

R.T.: 4.516 min
Delta R.T.: 0.022 min
Response: 5501654
Conc: 0.52 ng/ml

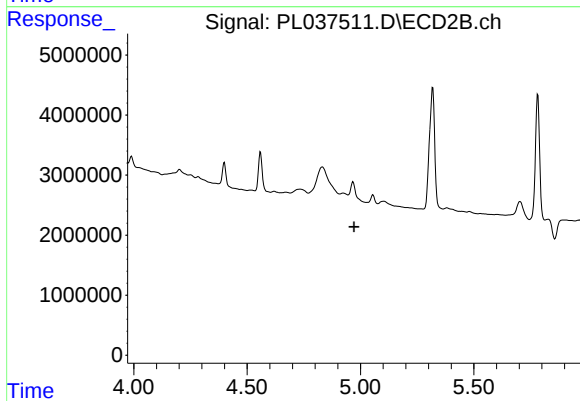

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.972 min
Response: 0
Conc: N.D.

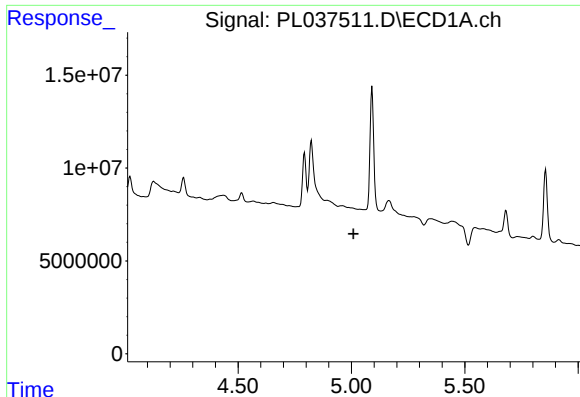

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.010 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

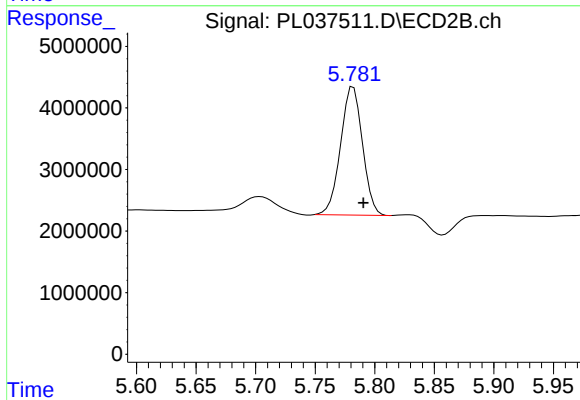


#8 Heptachlor epoxide

R.T.: 5.782 min
Delta R.T.: -0.008 min
Response: 26718529
Conc: 9.37 ng/ml

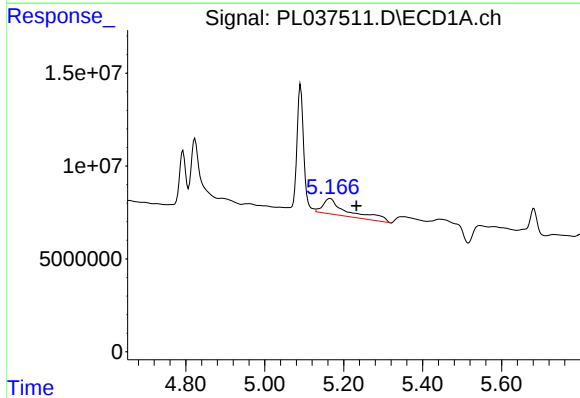


#10 gamma-Chlordane

R.T.: 5.166 min
Delta R.T.: -0.067 min
Response: 37959491
Conc: 4.05 ng/ml

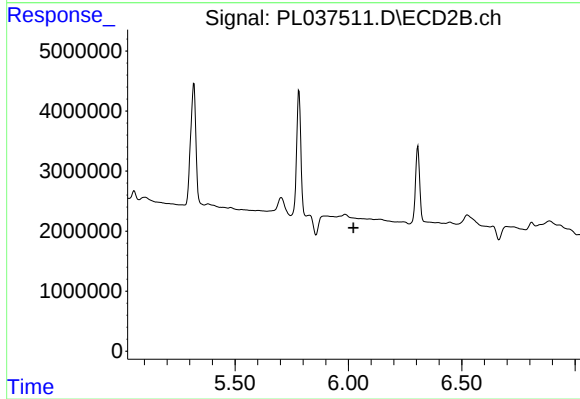

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

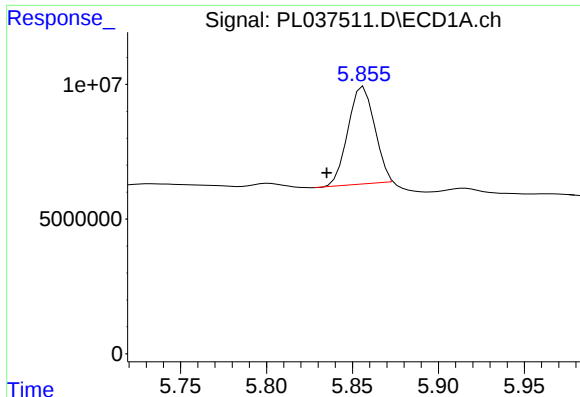

#14 Endrin


R.T.: 5.856 min
Delta R.T.: 0.021 min
Response: 39004136
Conc: 4.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

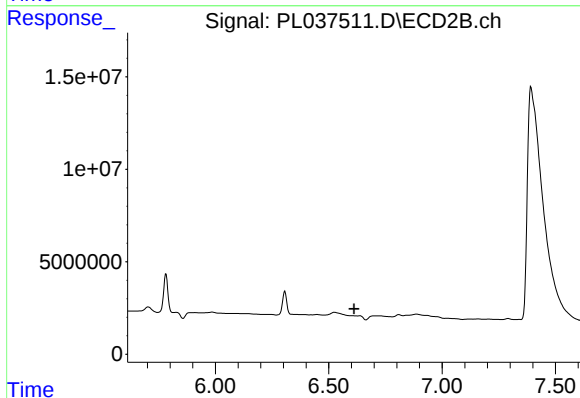


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

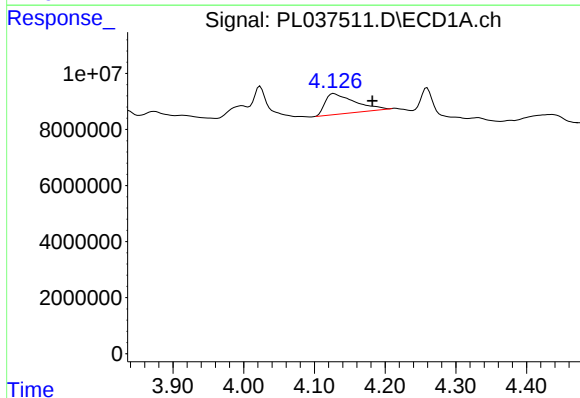


#23 Chlordane-1

R.T.: 4.128 min
Delta R.T.: -0.054 min
Response: 21675018
Conc: 71.79 ng/ml

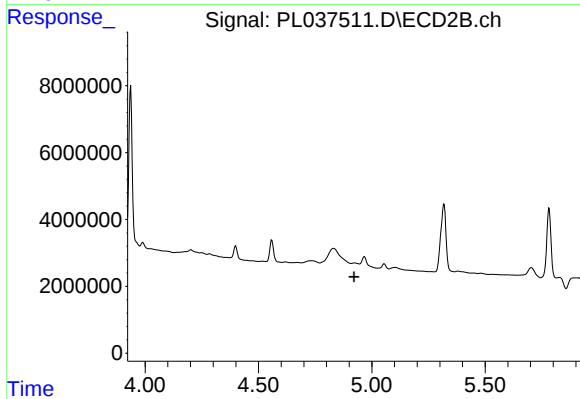

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

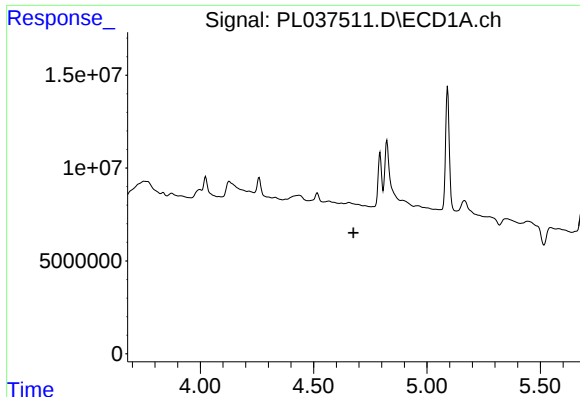

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.676 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

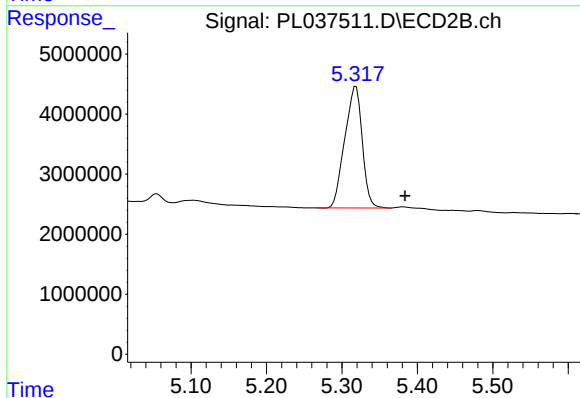


#24 Chlordane-2

R.T.: 5.319 min
Delta R.T.: -0.065 min
Response: 32581790
Conc: 257.46 ng/ml

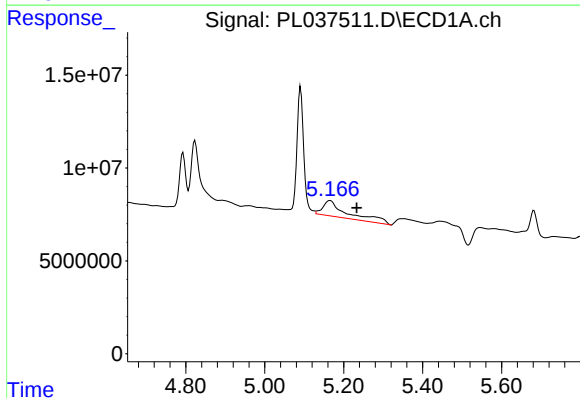


#25 Chlordane-3

R.T.: 5.166 min
Delta R.T.: -0.067 min
Response: 37959491
Conc: 35.71 ng/ml

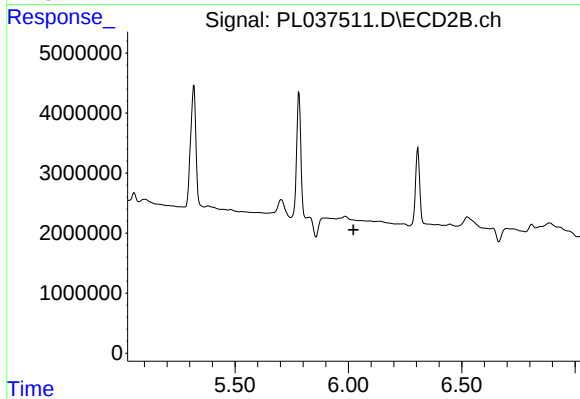

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

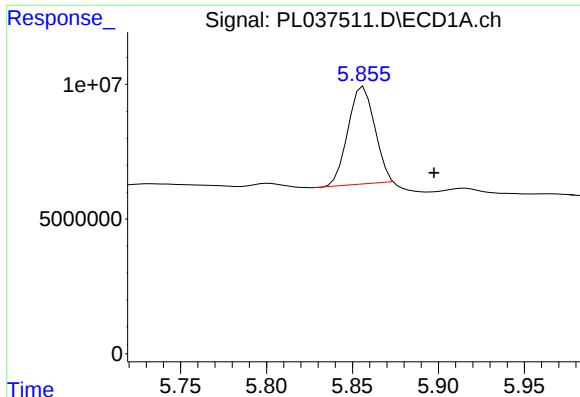

#27 Chlordane-5


R.T.: 5.856 min
Delta R.T.: -0.041 min
Response: 39004136
Conc: 300.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

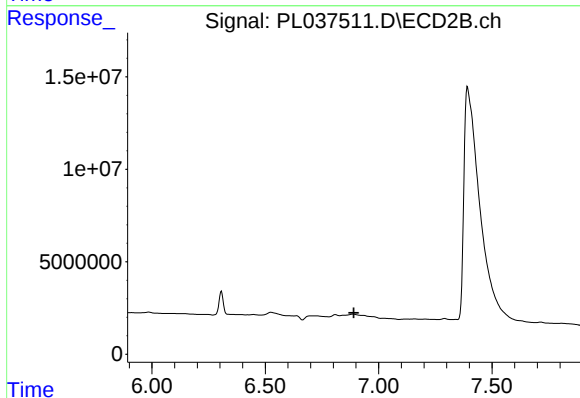


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.890 min
Response: 0
Conc: N.D.

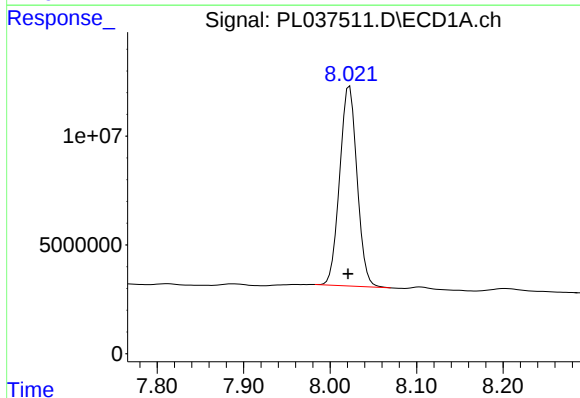

#28 Decachlorobiphenyl

R.T.: 8.023 min
Delta R.T.: 0.002 min
Response: 127541116
Conc: 21.14 ng/ml

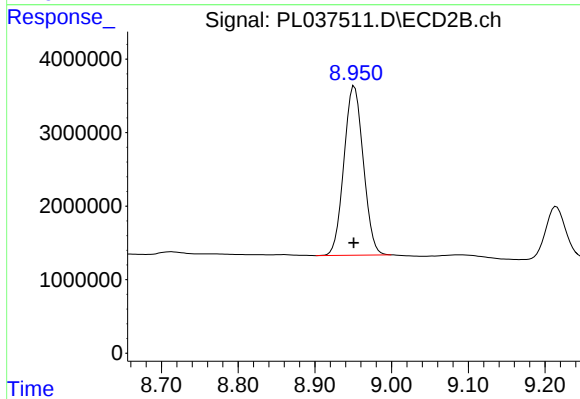

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: 0.000 min
Response: 40557476
Conc: 20.44 ng/ml