

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
 Data File : PL037458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2018 15:36
 Operator : UA\AJ
 Sample : J3048-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3-S

Manual Integrations
 APPROVED

UGO
 6/28/2018 11:30:22 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:31:16 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.936	54340906	16570194	6.870	5.989
28)	SA Decachlor...	8.017	8.948	67241983	20254702	11.144	10.209
Target Compounds							
12)	B 4,4'-DDE	5.453	6.248	31174205	10256878	3.529m	4.031m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
Data File : PL037458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2018 15:36
Operator : UA\AJ
Sample : J3048-06
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-3-S


Manual Integrations
APPROVED

UGO
6/28/2018 11:30:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:31:16 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

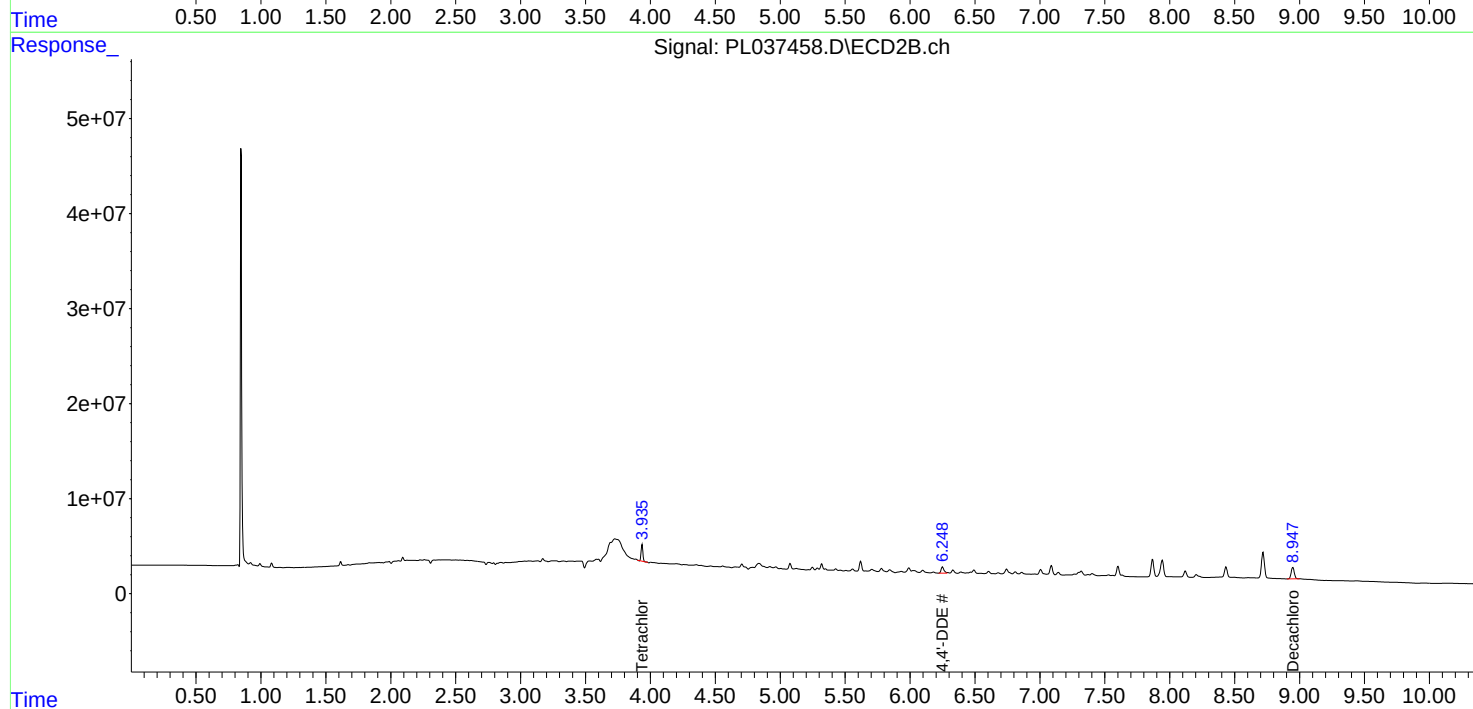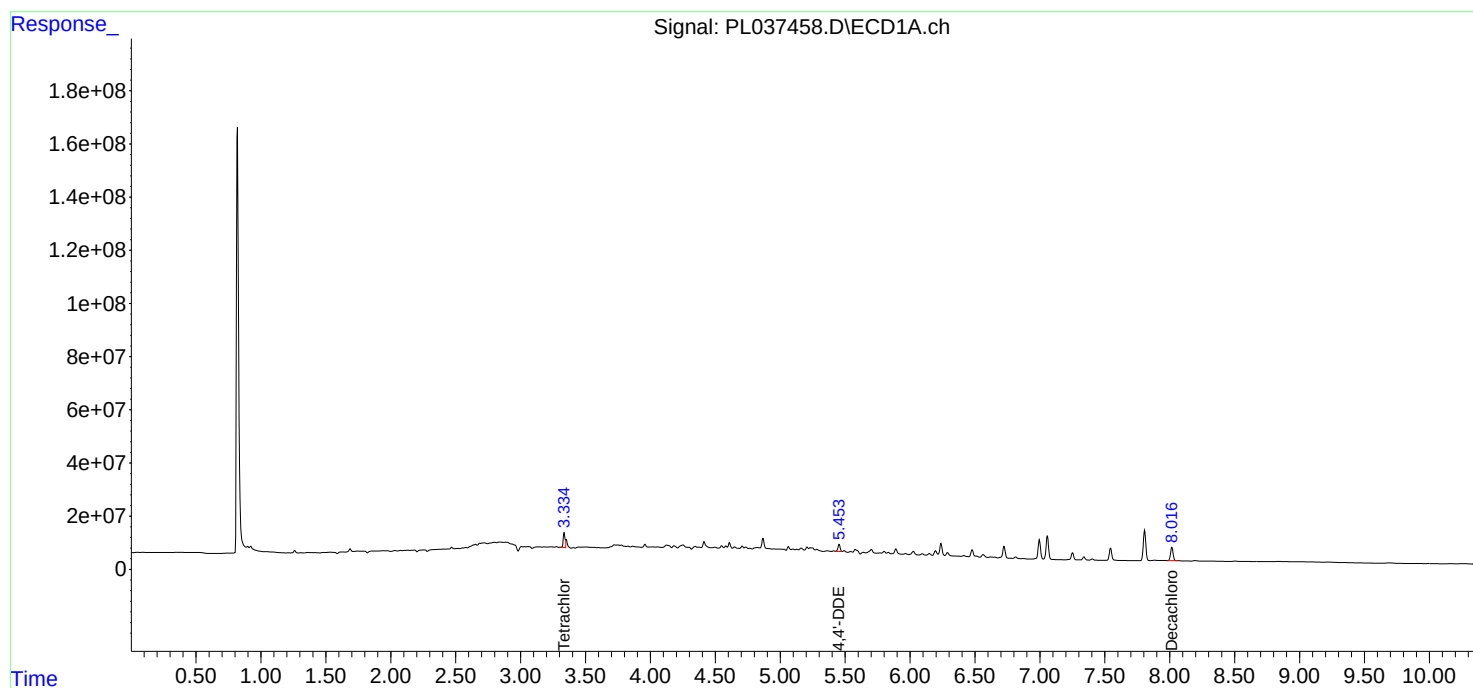

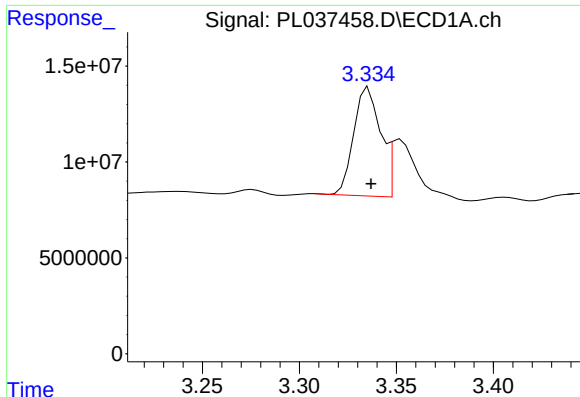


#1 Tetrachloro-m-xylene

R.T.: 3.336 min
Delta R.T.: -0.001 min
Response: 54340906
Conc: 6.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-S


Manual Integrations
APPROVED

UGO
6/28/2018 11:30:22 AM

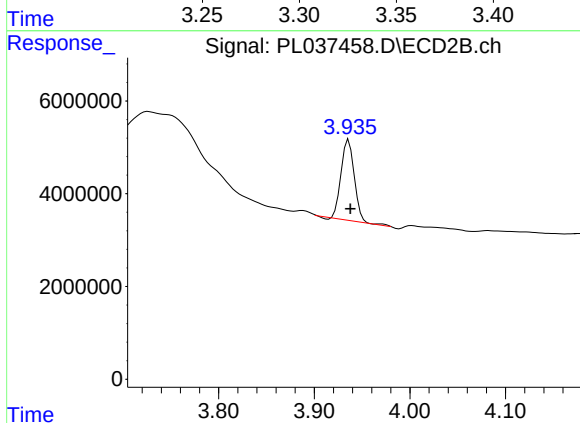


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 16570194
Conc: 5.99 ng/ml

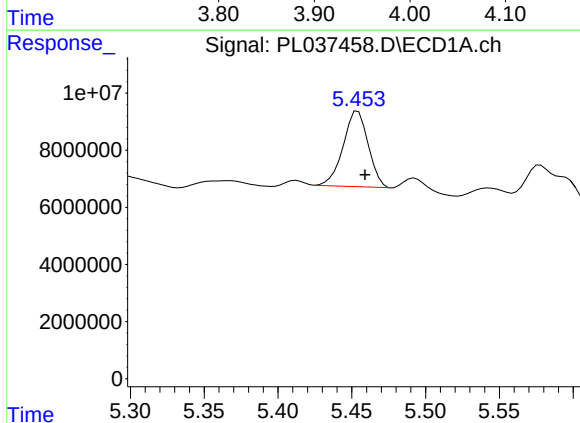


#12 4,4'-DDE

R.T.: 5.453 min
Delta R.T.: -0.006 min
Response: 31174205
Conc: 3.53 ng/ml m

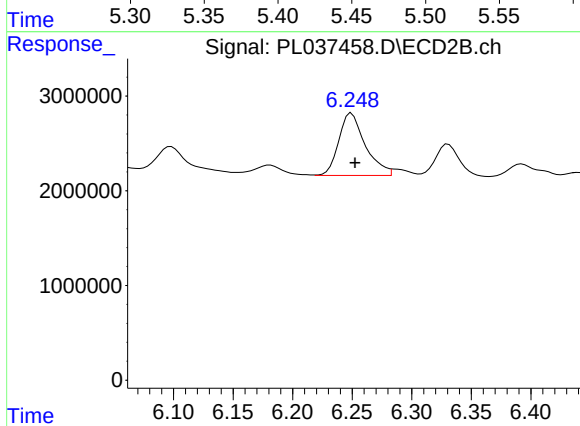

#12 4,4'-DDE

R.T.: 6.248 min
Delta R.T.: -0.004 min
Response: 10256878
Conc: 4.03 ng/ml m

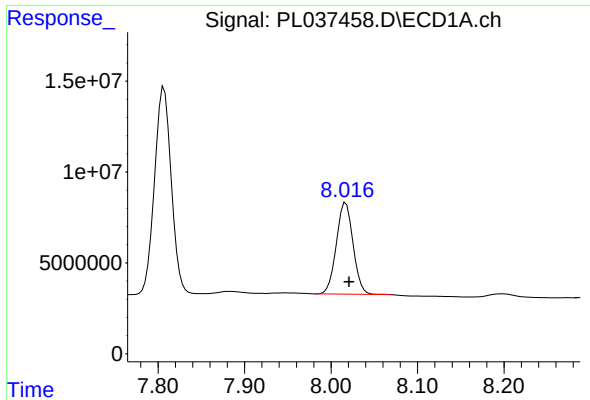


#28 Decachlorobiphenyl

R.T.: 8.017 min
Delta R.T.: -0.004 min
Response: 67241983
Conc: 11.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-S

Manual Integrations
APPROVED

UGO
6/28/2018 11:30:22 AM

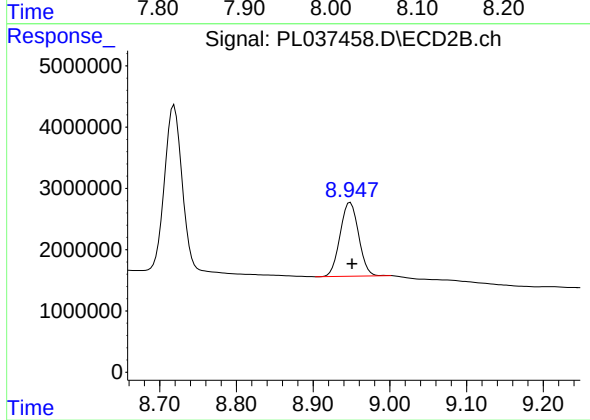

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.002 min
Response: 20254702
Conc: 10.21 ng/ml