

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
 Data File : PL037459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2018 15:50
 Operator : UA\AJ
 Sample : J3048-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3-D

Manual Integrations
 APPROVED

UGO
 6/28/2018 11:30:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:32:05 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.334	3.934	67208097	22347750	8.496m	8.077m
28)	SA Decachlor...	8.016	8.948	66748745	20566577	11.062	10.366
Target Compounds							
10)	B gamma-Chl...	5.228	6.020	18946426	5611134	2.023m	1.992m
11)	B alpha-Chl...	5.282	6.096	10264023	2967580	1.130m	1.031m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
Data File : PL037459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2018 15:50
Operator : UA\AJ
Sample : J3048-10
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
TP-3-D


Manual Integrations
APPROVED

UGO
6/28/2018 11:30:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:32:05 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

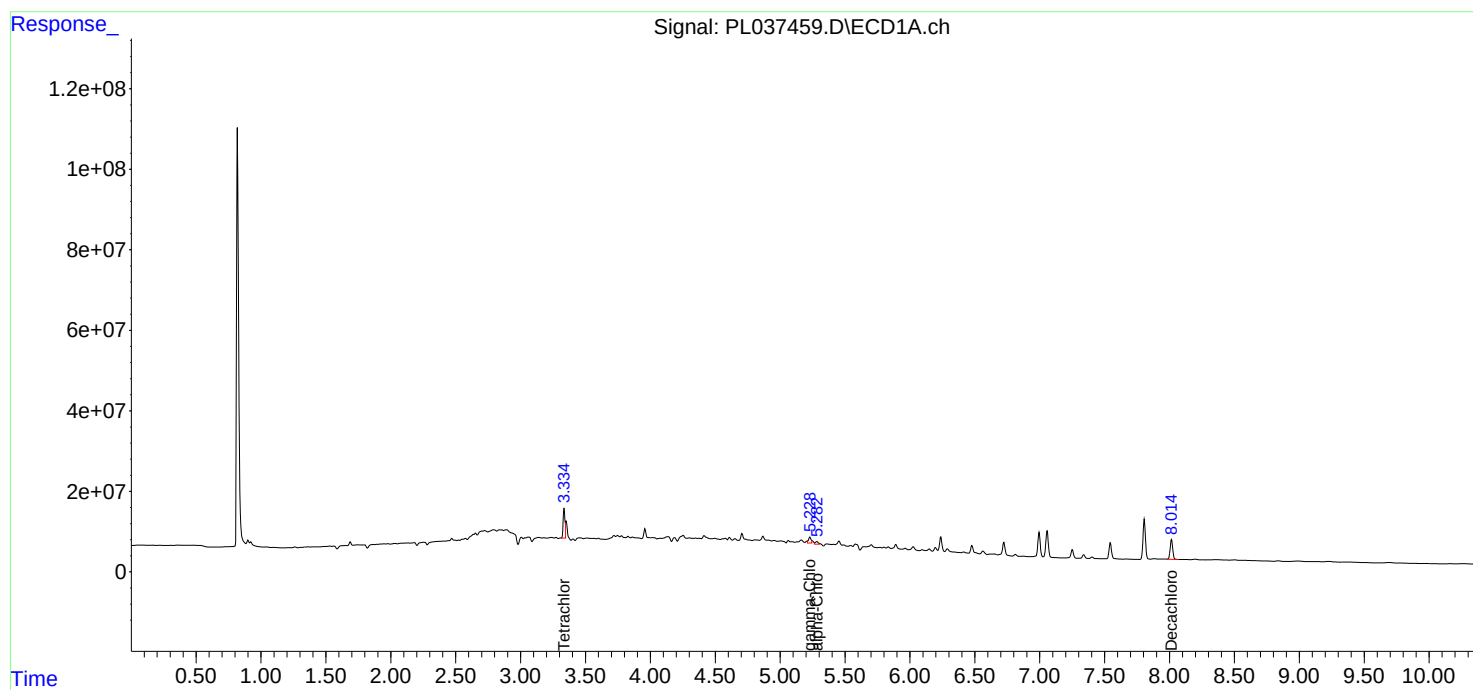

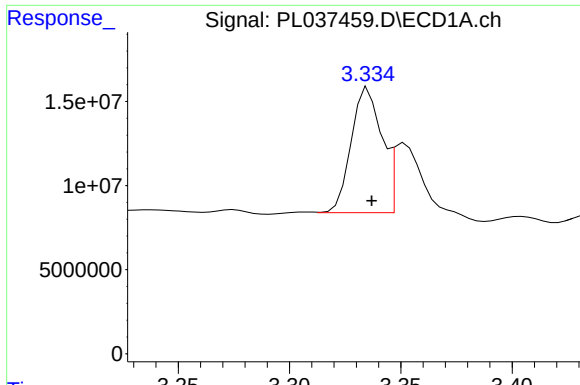


#1 Tetrachloro-m-xylene

R.T.: 3.334 min
Delta R.T.: -0.003 min
Response: 67208097
Conc: 8.50 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-3-D


Manual Integrations
APPROVED

UGO
6/28/2018 11:30:25 AM

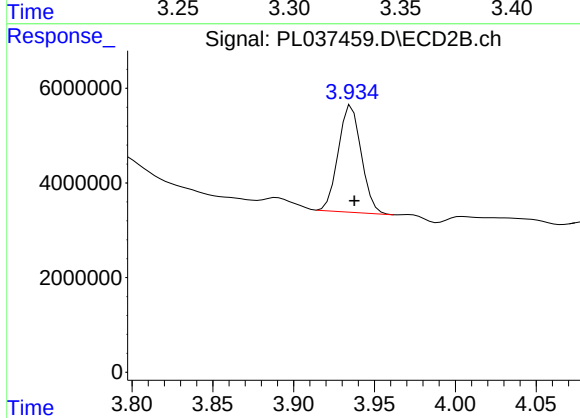


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.003 min
Response: 22347750
Conc: 8.08 ng/ml m

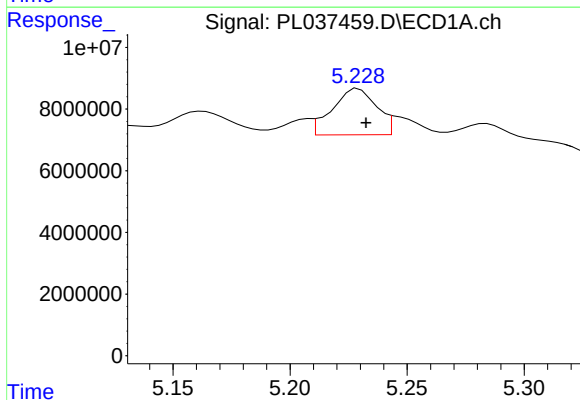


#10 gamma-Chlordane

R.T.: 5.228 min
Delta R.T.: -0.005 min
Response: 18946426
Conc: 2.02 ng/ml m

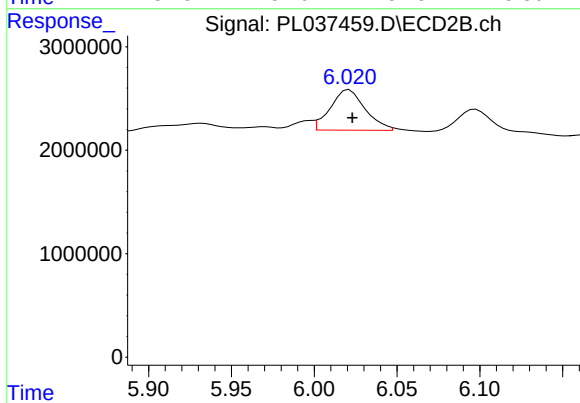

#10 gamma-Chlordane

R.T.: 6.020 min
Delta R.T.: -0.003 min
Response: 5611134
Conc: 1.99 ng/ml m

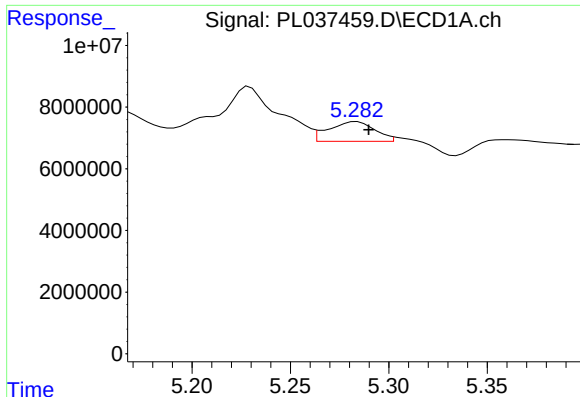


#11 alpha-Chlordane

R.T.: 5.282 min
Delta R.T.: -0.007 min
Response: 10264023
Conc: 1.13 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-3-D


Manual Integrations
APPROVED

UGO
6/28/2018 11:30:25 AM

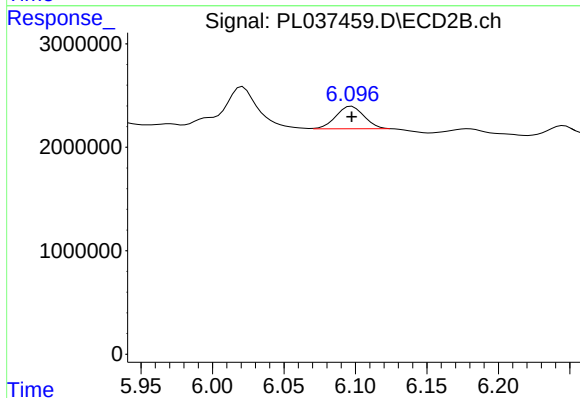


#11 alpha-Chlordane

R.T.: 6.096 min
Delta R.T.: -0.001 min
Response: 2967580
Conc: 1.03 ng/ml m

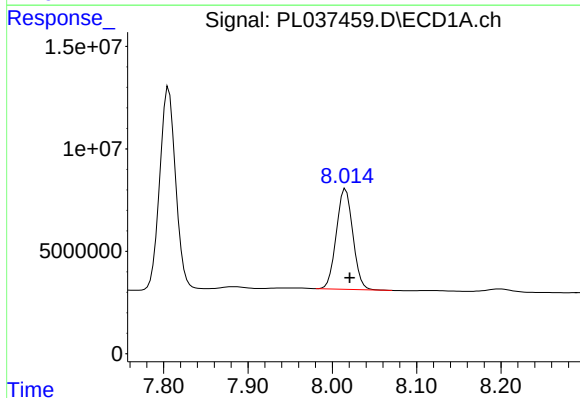

#28 Decachlorobiphenyl

R.T.: 8.016 min
Delta R.T.: -0.005 min
Response: 66748745
Conc: 11.06 ng/ml

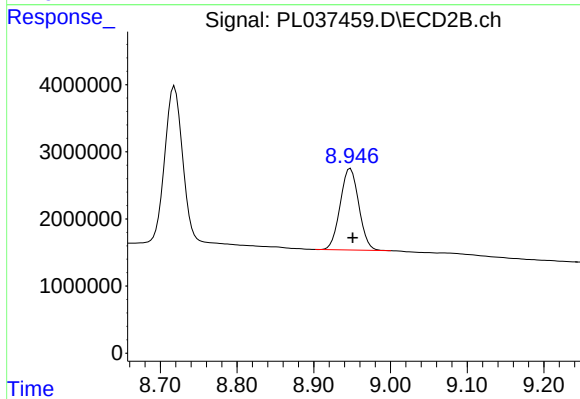

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 20566577
Conc: 10.37 ng/ml