

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
 Data File : PL037460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2018 16:04
 Operator : UA\AJ
 Sample : J3048-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2-D

Manual Integrations
 APPROVED

UGO
 6/28/2018 11:30:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:32:22 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.935	122.9E6	36760168	15.535	13.286m
28)	SA Decachlor...	8.015	8.949	46432511	14940954	7.695	7.531

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062718\
Data File : PL037460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2018 16:04
Operator : UA\AJ
Sample : J3048-15
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-2-D


Manual Integrations
APPROVED

UGO
6/28/2018 11:30:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:32:22 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

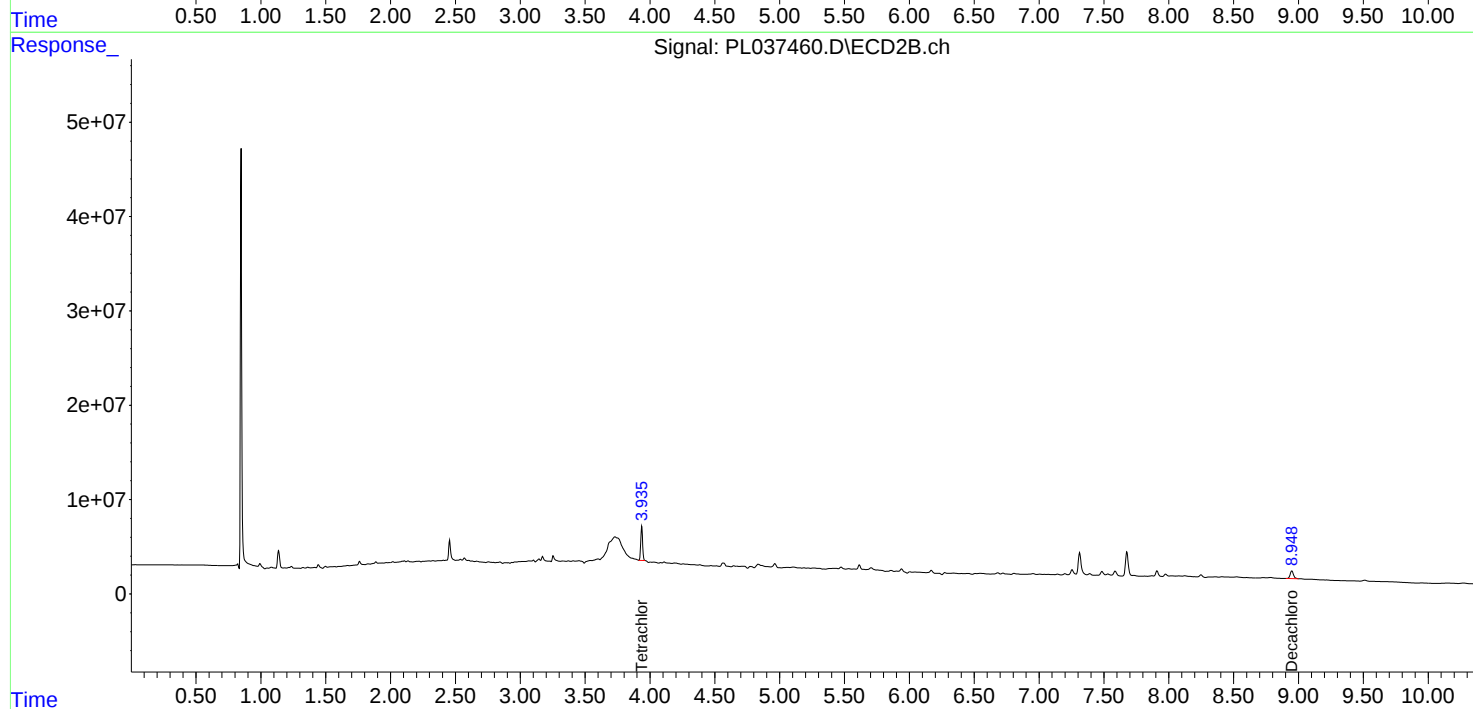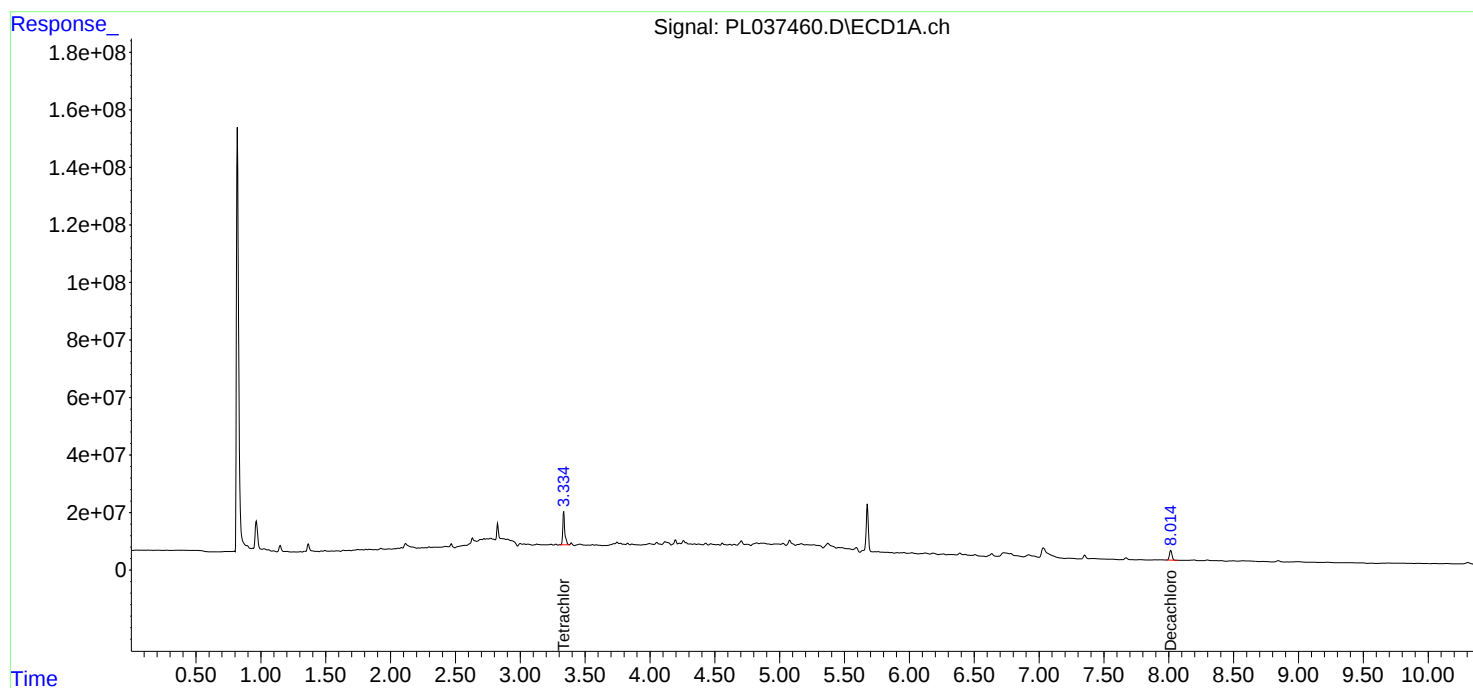

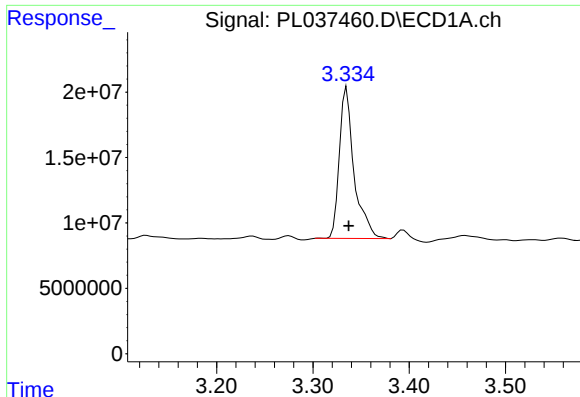


#1 Tetrachloro-m-xylene

R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 122886422
Conc: 15.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-D


Manual Integrations
APPROVED

UGO
6/28/2018 11:30:28 AM

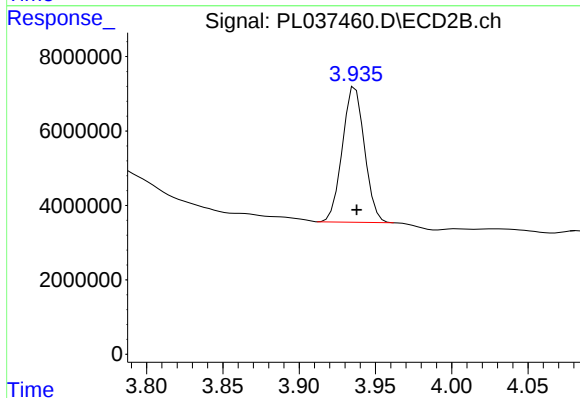


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.002 min
Response: 36760168
Conc: 13.29 ng/ml m

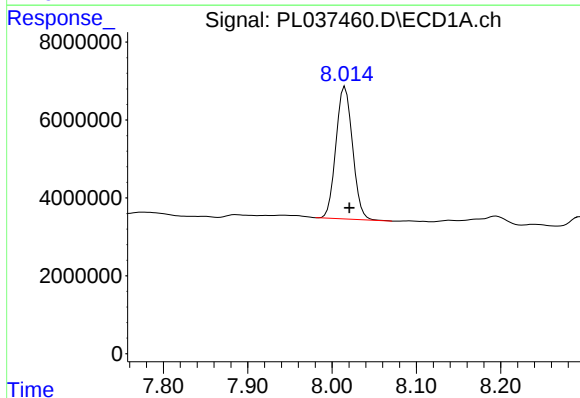

#28 Decachlorobiphenyl

R.T.: 8.015 min
Delta R.T.: -0.005 min
Response: 46432511
Conc: 7.70 ng/ml

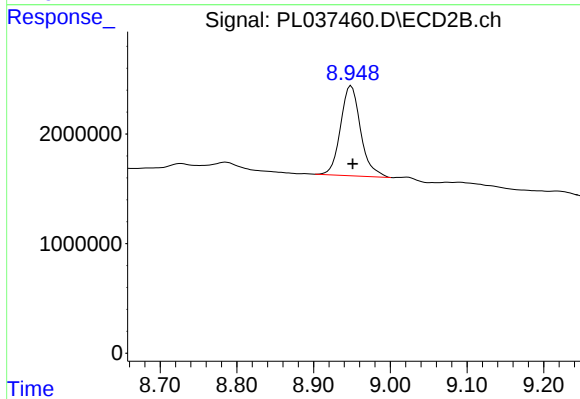

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.002 min
Response: 14940954
Conc: 7.53 ng/ml