

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062719\
 Data File : PL049932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2019 14:03
 Operator : SM\AJ
 Sample : K3504-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-013-B038-062019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:27:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	3.933	194.3E6	47877634	17.227	15.637
28)	SA Decachlor...	7.984	8.965	158.7E6	46458531	12.493	13.839
Target Compounds							
7)	B delta-BHC	0.000	4.988	0	10112852	N.D.	2.567 #
15)	B Endosulfa...	6.098	6.855	61987998	17473572	4.254	5.425 #
27)	Chlordane-5	6.098	0.000	61987998	0	110.455	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062719\
Data File : PL049932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2019 14:03
Operator : SM\AJ
Sample : K3504-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-013-B038-062019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:27:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

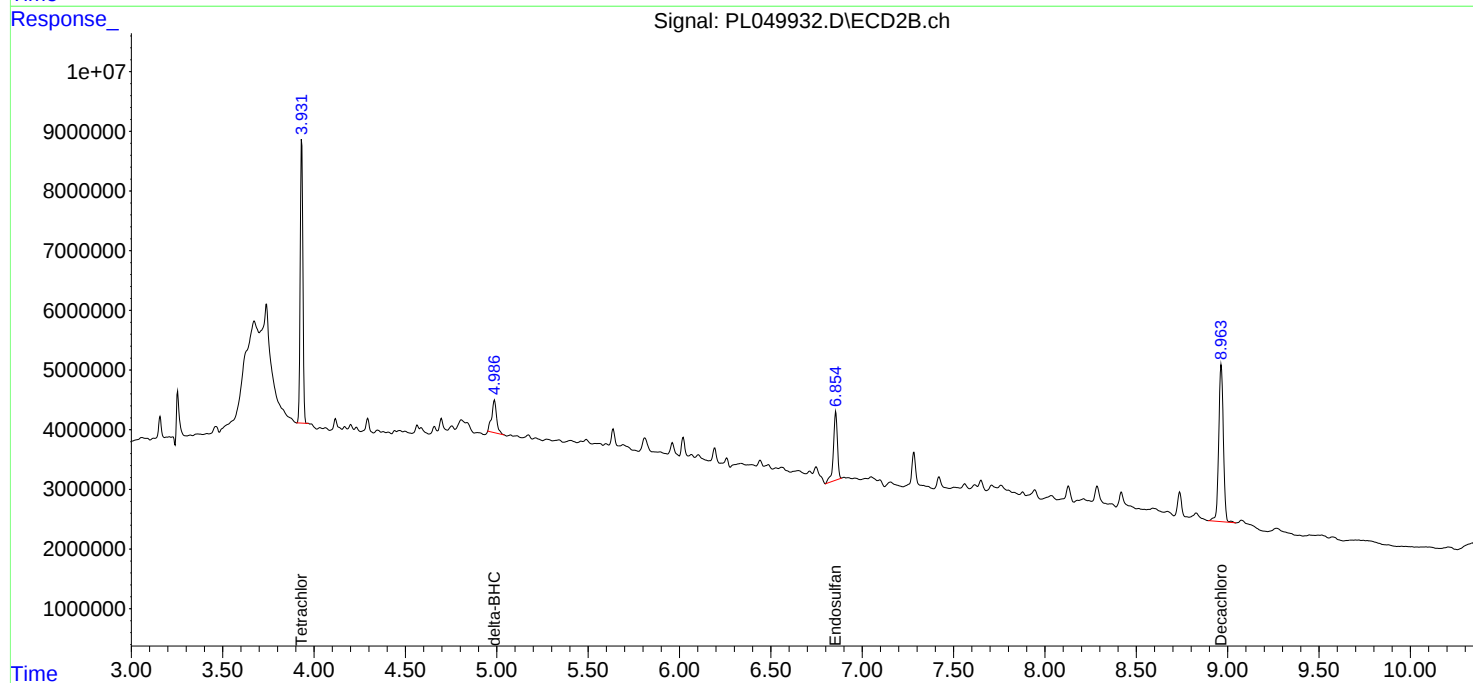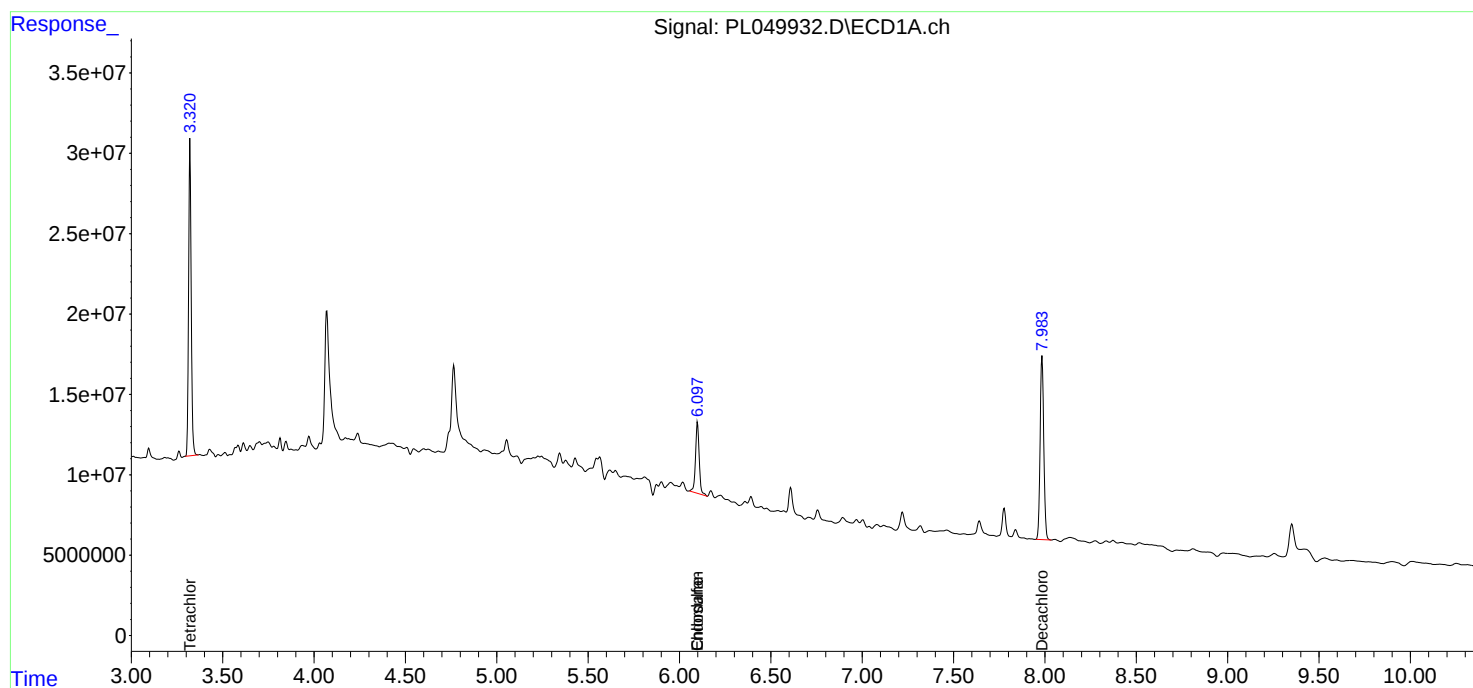


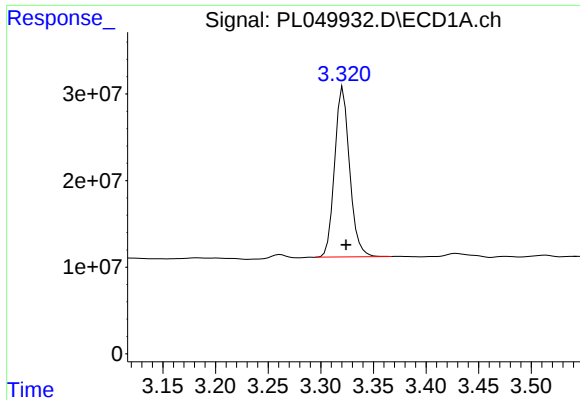

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: -0.003 min
Response: 194286026
Conc: 17.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-B038-062019

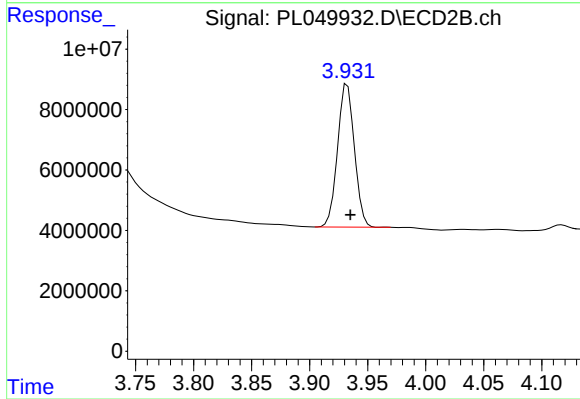


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.003 min
Response: 47877634
Conc: 15.64 ng/ml

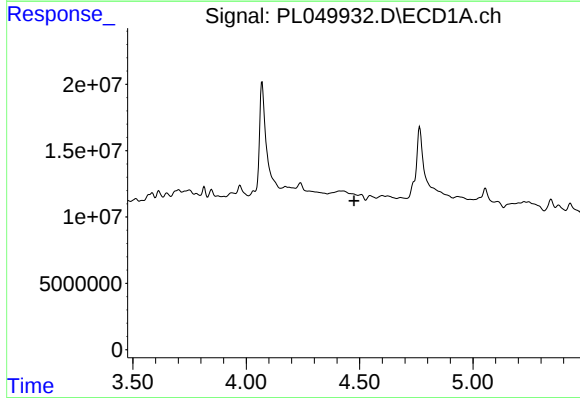


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.476 min
Response: 0
Conc: N.D.

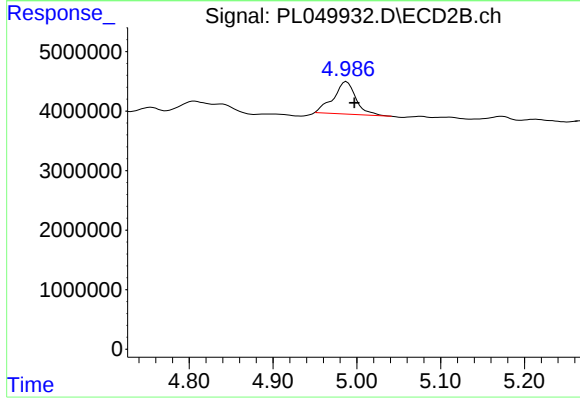

#7 delta-BHC


R.T.: 4.988 min
Delta R.T.: -0.009 min
Response: 10112852
Conc: 2.57 ng/ml

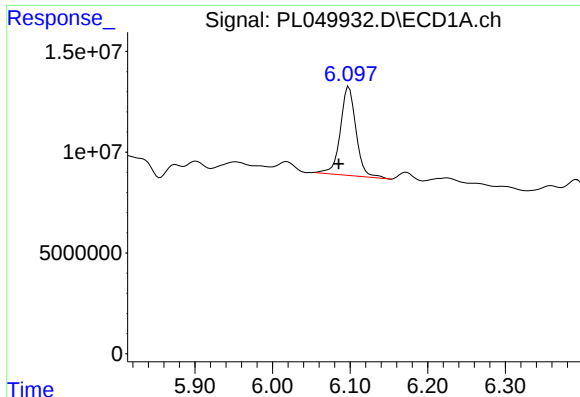

#15 Endosulfan II


R.T.: 6.098 min
Delta R.T.: 0.013 min
Response: 61987998
Conc: 4.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-B038-062019

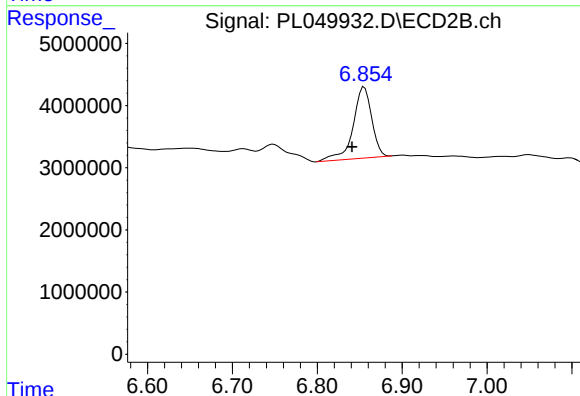


#15 Endosulfan II

R.T.: 6.855 min
Delta R.T.: 0.014 min
Response: 17473572
Conc: 5.43 ng/ml

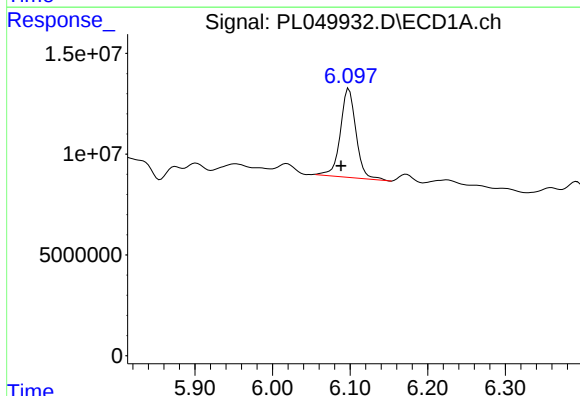


#27 Chlordane-5

R.T.: 6.098 min
Delta R.T.: 0.010 min
Response: 61987998
Conc: 110.45 ng/ml

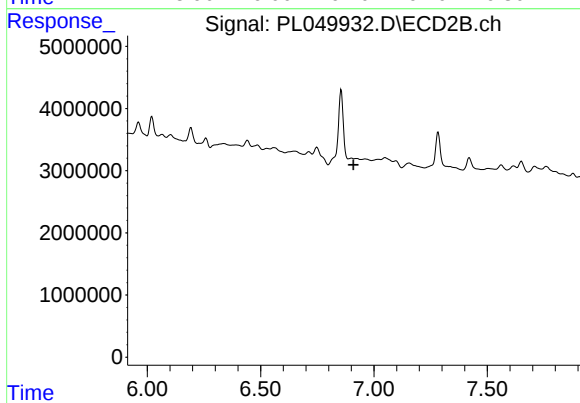

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.910 min
Response: 0
Conc: N.D.

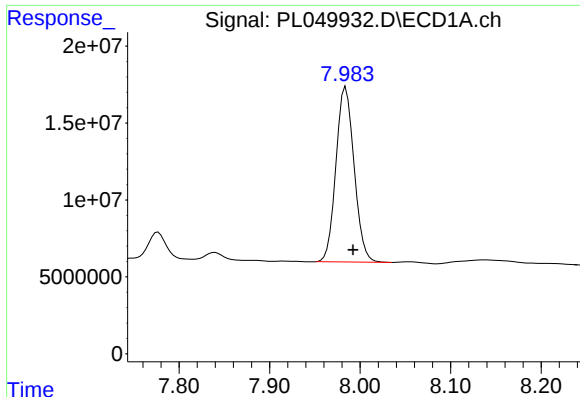

#28 Decachlorobiphenyl


R.T.: 7.984 min

Delta R.T.: -0.008 min

Response: 158739067

Conc: 12.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-B038-062019

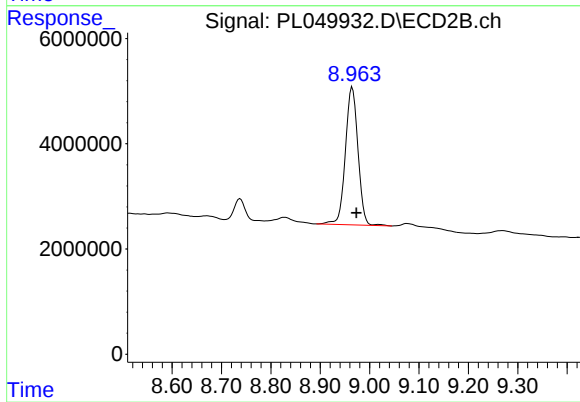

#28 Decachlorobiphenyl

R.T.: 8.965 min

Delta R.T.: -0.008 min

Response: 46458531

Conc: 13.84 ng/ml