

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062719\
 Data File : PL049937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2019 15:18
 Operator : SM\AJ
 Sample : K3504-17
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-013-SW105-062019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:27:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.933	183.1E6	36854569	16.239	12.037 #
28)	SA Decachlor...	7.985	8.965	156.8E6	49582926	12.341	14.770
Target Compounds							
4)	MA Heptachlor	4.284f	0.000	48297496	0	2.657	N.D. #
6)	B beta-BHC	4.284	4.795	48297496	11643786	6.603	6.011
9)	A Endosulfan I	0.000	6.142	0	19947189	N.D.	5.871 #
11)	B alpha-Chl...	0.000	6.077f	0	41725990	N.D.	11.282 #
13)	MA Dieldrin	0.000	6.433f	0	18346424	N.D.	5.172 #
16)	A 4,4'-DDD	5.931	0.000	27210487	0	2.155	N.D. #
24)	Chlordane-2	4.683f	0.000	93337353	0	159.815	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062719\
Data File : PL049937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2019 15:18
Operator : SM\AJ
Sample : K3504-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-013-SW105-062019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:27:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

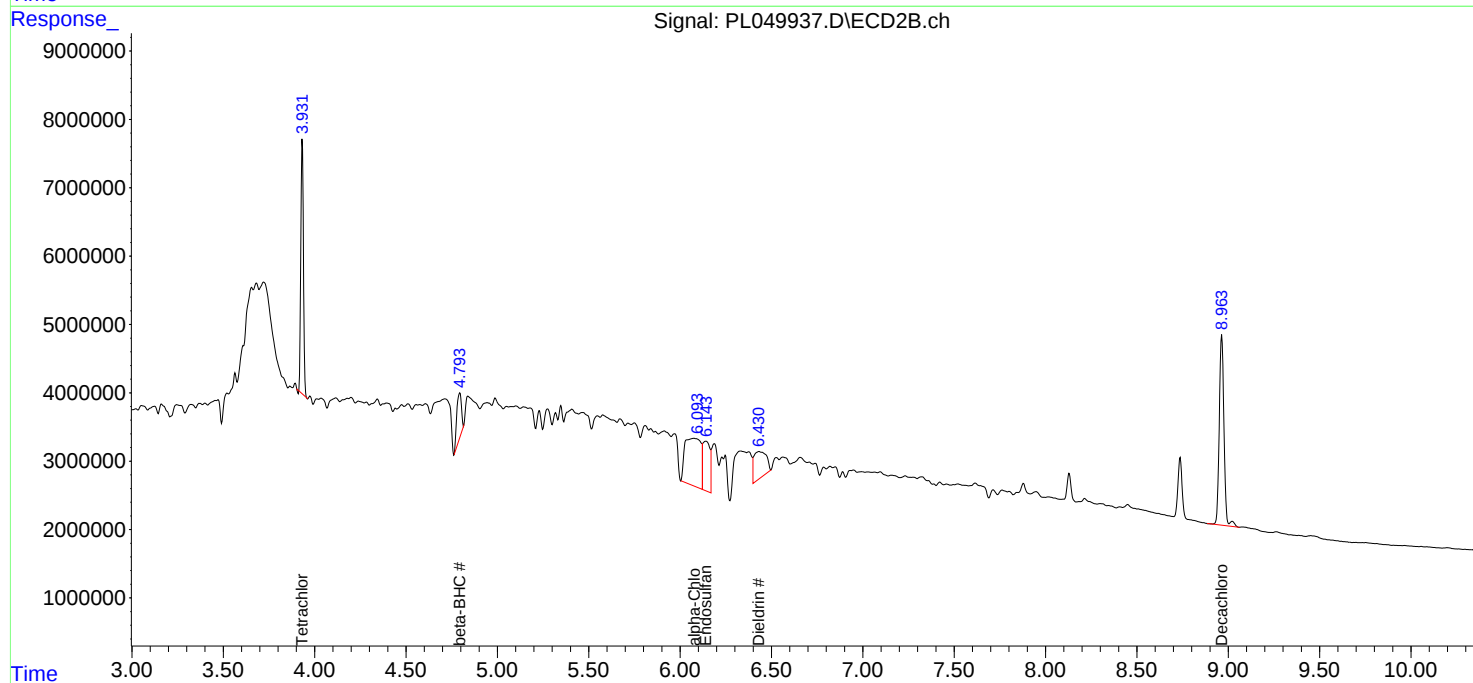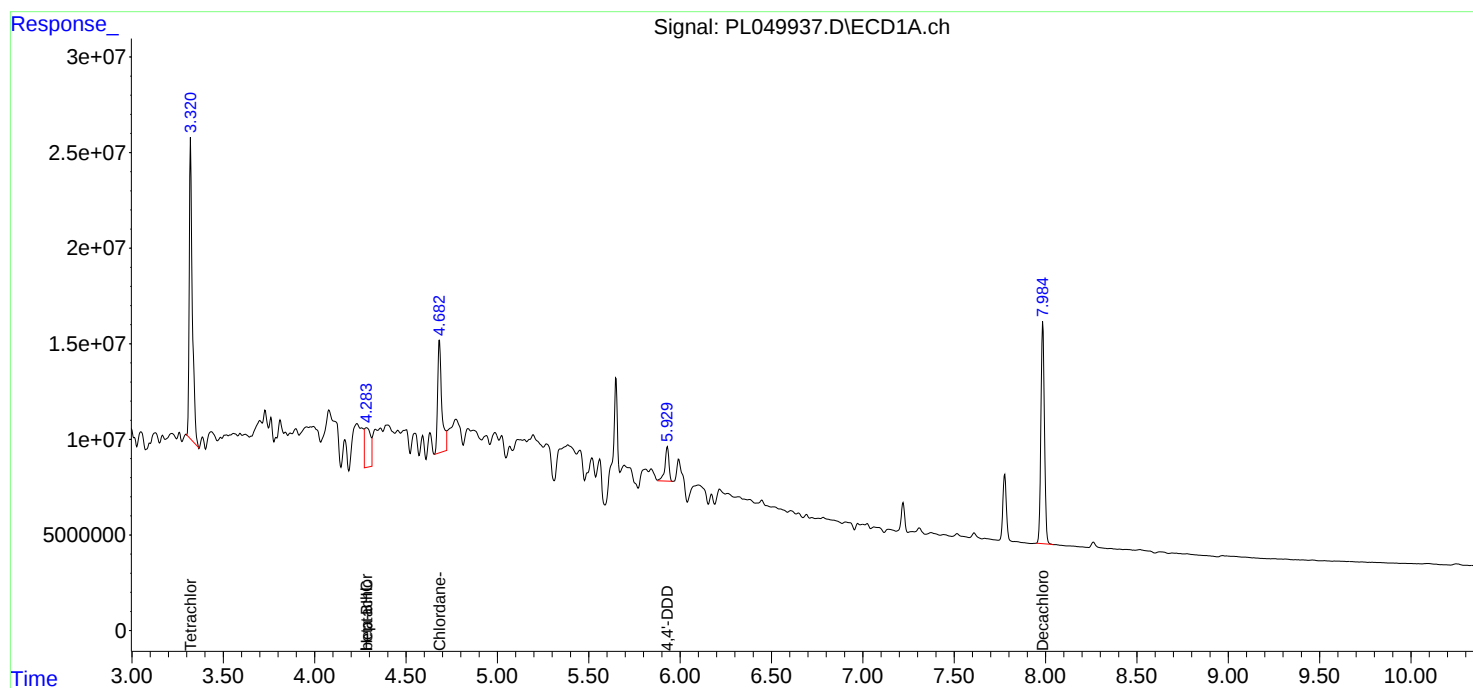


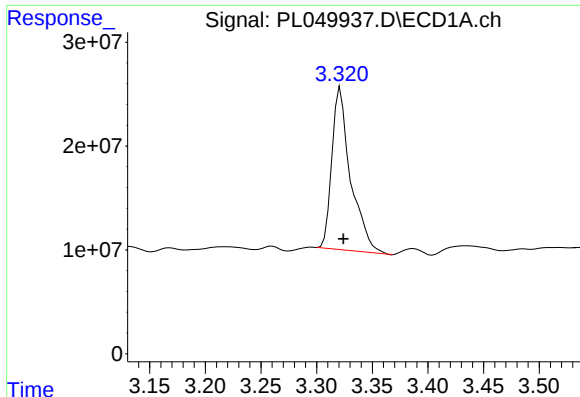

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 183137129
Conc: 16.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-SW105-062019

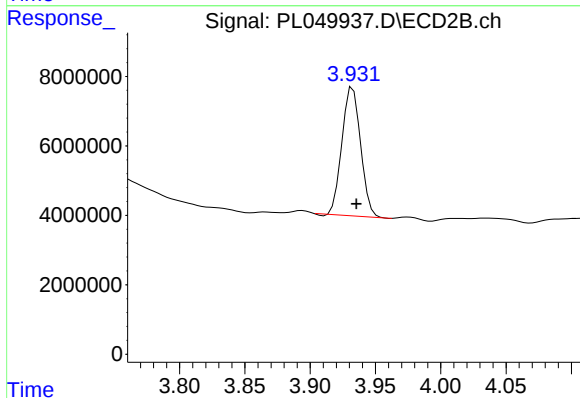


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.003 min
Response: 36854569
Conc: 12.04 ng/ml

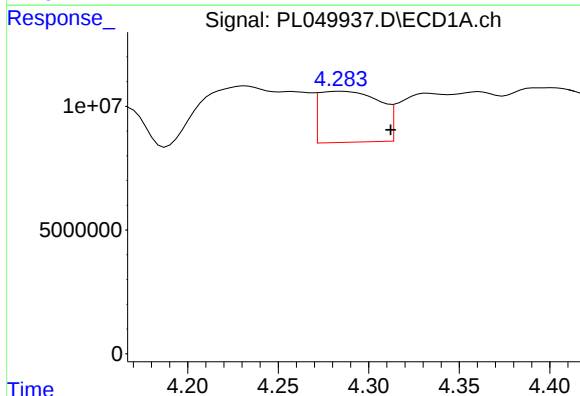


#4 Heptachlor

R.T.: 4.284 min
Delta R.T.: -0.028 min
Response: 48297496
Conc: 2.66 ng/ml

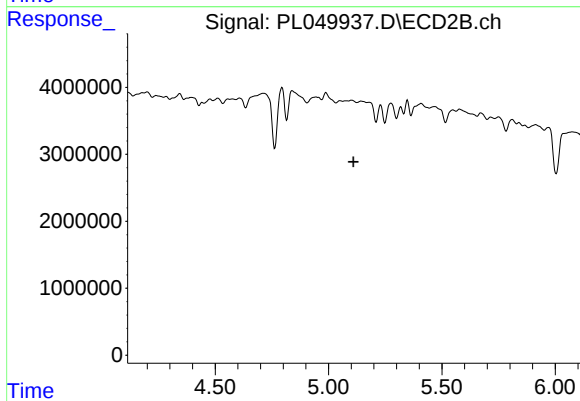

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.110 min
Response: 0
Conc: N.D.

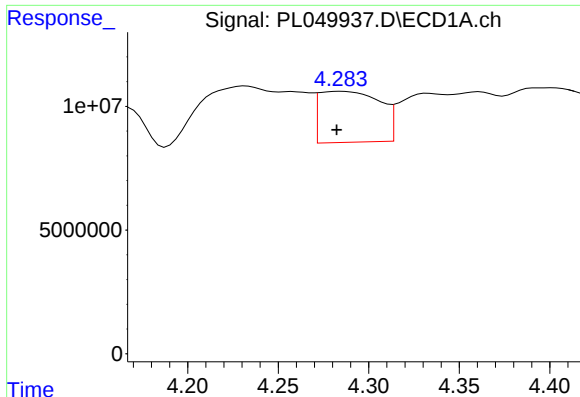

#6 beta-BHC


R.T.: 4.284 min
Delta R.T.: 0.002 min
Response: 48297496
Conc: 6.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-SW105-062019

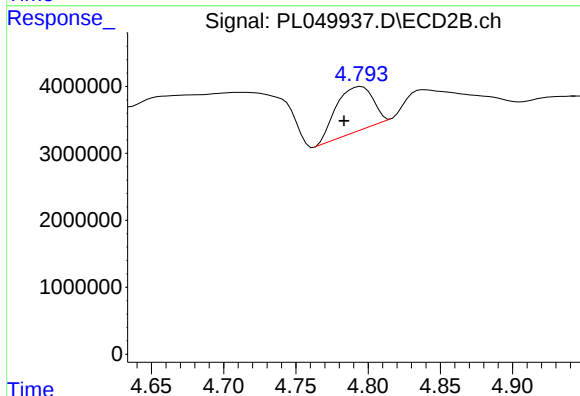


#6 beta-BHC

R.T.: 4.795 min
Delta R.T.: 0.012 min
Response: 11643786
Conc: 6.01 ng/ml

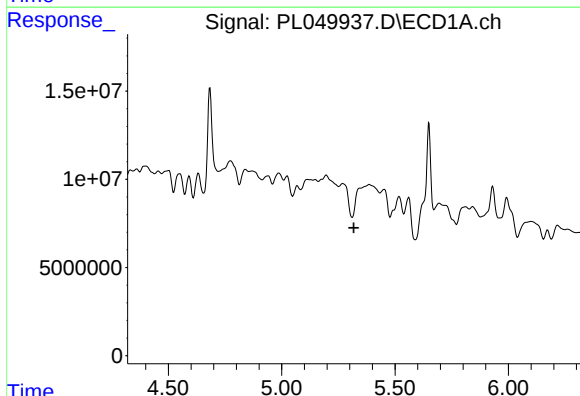


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.319 min
Response: 0
Conc: N.D.

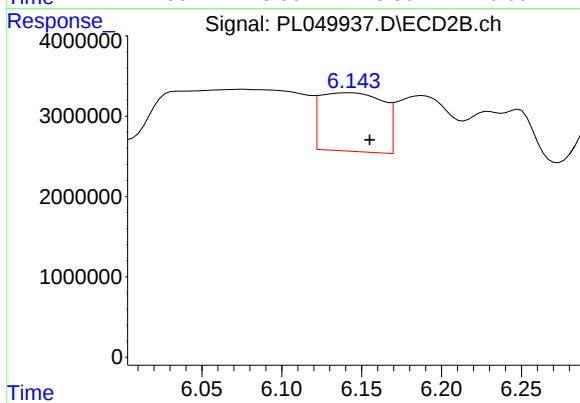

#9 Endosulfan I


R.T.: 6.142 min
Delta R.T.: -0.013 min
Response: 19947189
Conc: 5.87 ng/ml

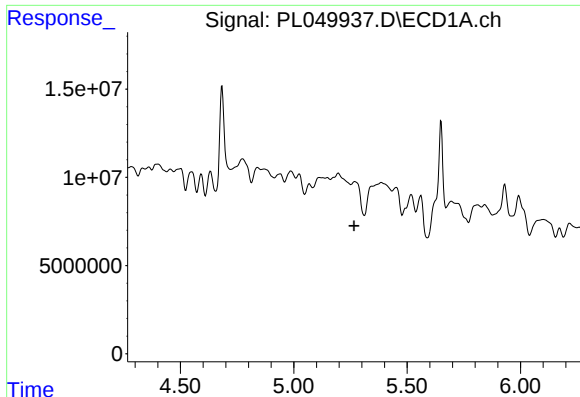

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-013-SW105-062019

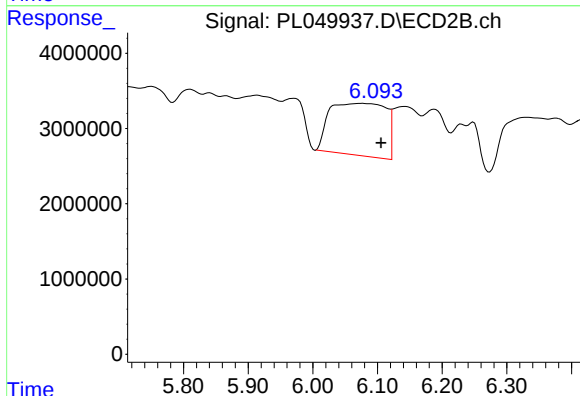


#11 alpha-Chlordane

R.T.: 6.077 min
Delta R.T.: -0.028 min
Response: 41725990
Conc: 11.28 ng/ml

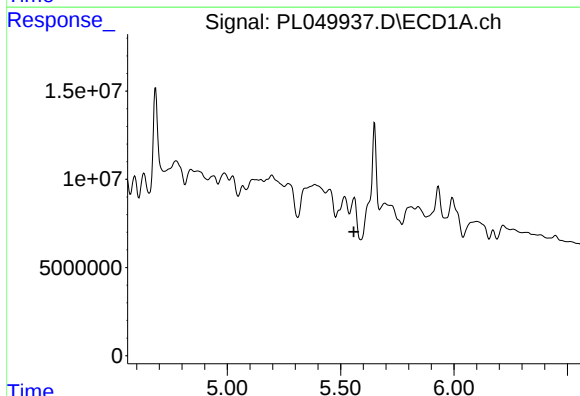


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.558 min
Response: 0
Conc: N.D.

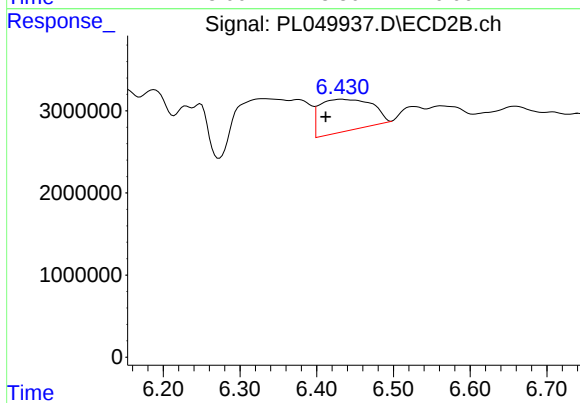

#13 Dieldrin


R.T.: 6.433 min
Delta R.T.: 0.020 min
Response: 18346424
Conc: 5.17 ng/ml

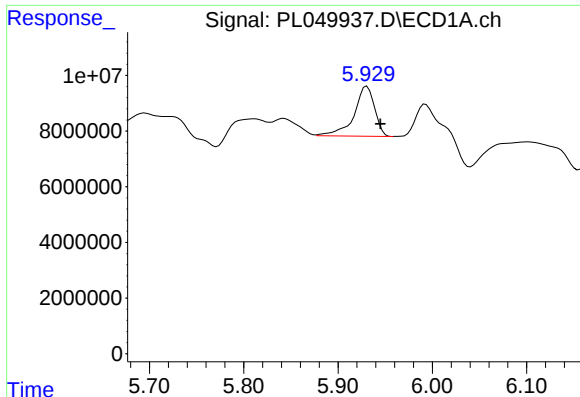

#16 4,4'-DDD


R.T.: 5.931 min
Delta R.T.: -0.014 min
Response: 27210487
Conc: 2.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-SW105-062019

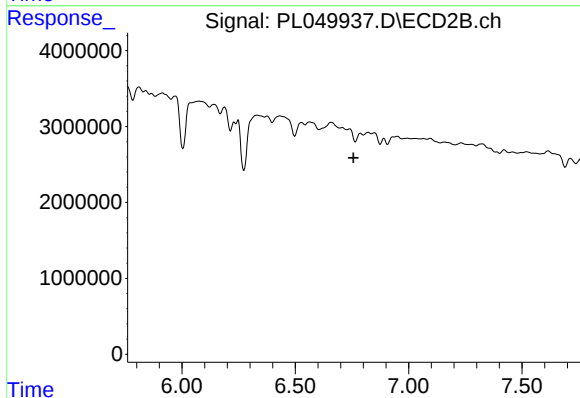


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.757 min
Response: 0
Conc: N.D.

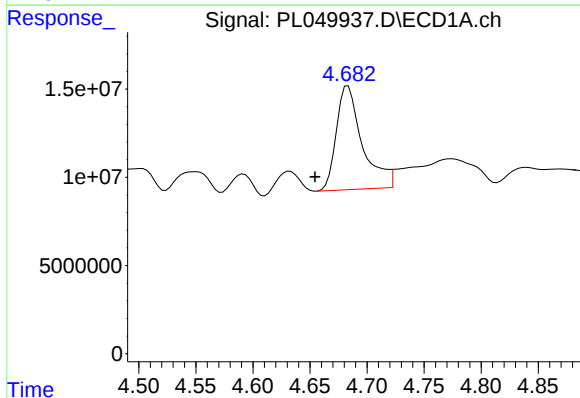


#24 Chlordane-2

R.T.: 4.683 min
Delta R.T.: 0.029 min
Response: 93337353
Conc: 159.81 ng/ml

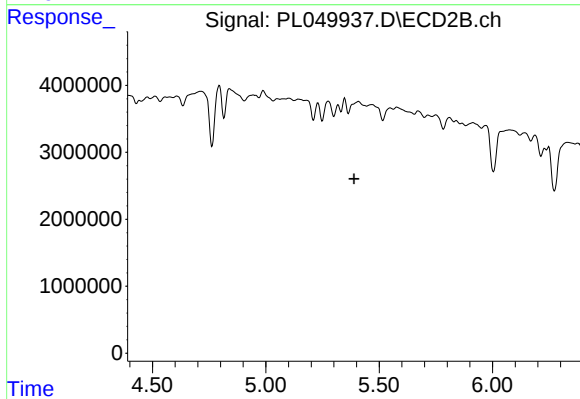

#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.390 min
Response: 0
Conc: N.D.

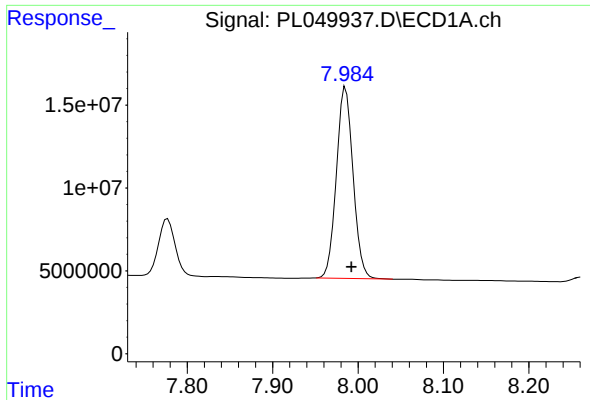

#28 Decachlorobiphenyl


R.T.: 7.985 min

Delta R.T.: -0.007 min

Response: 156812241

Conc: 12.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-SW105-062019

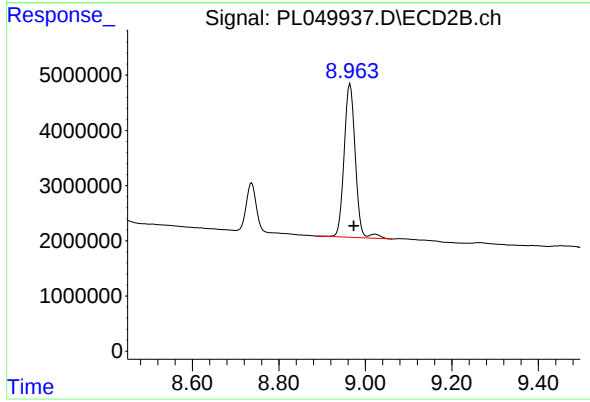

#28 Decachlorobiphenyl

R.T.: 8.965 min

Delta R.T.: -0.008 min

Response: 49582926

Conc: 14.77 ng/ml