

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062719\
 Data File : PL049950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2019 19:05
 Operator : SM\AJ
 Sample : K3157-13
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-062619-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:29:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.932	148.8E6	32449129	13.193	10.598
28)	SA Decachlor...	7.986	8.966	106.7E6	37279972	8.396	11.105 #
Target Compounds							
6)	B beta-BHC	0.000	4.798f	0	5084675	N.D.	2.625 #
10)	B gamma-Chl...	0.000	6.029	0	7955500	N.D.	2.135 #
11)	B alpha-Chl...	0.000	6.102	0	15656663	N.D.	4.233 #
23)	Chlordane-1	4.162	4.918	28911634	5481615	50.760	37.299 #
25)	Chlordane-3	0.000	6.029	0	7955500	N.D.	15.987 #
26)	Chlordane-4	0.000	6.102	0	15656663	N.D.	26.343 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062719\
Data File : PL049950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2019 19:05
Operator : SM\AJ
Sample : K3157-13
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
CL-02-062619-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:29:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

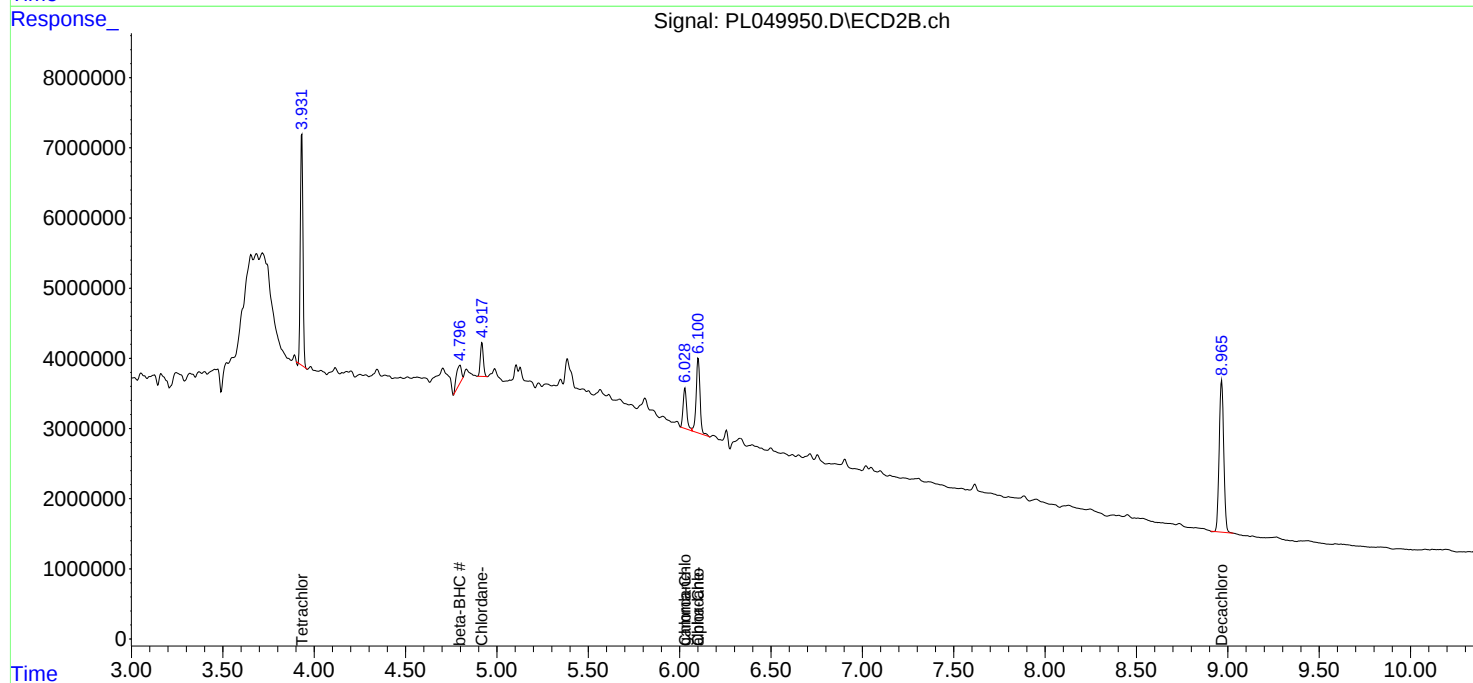


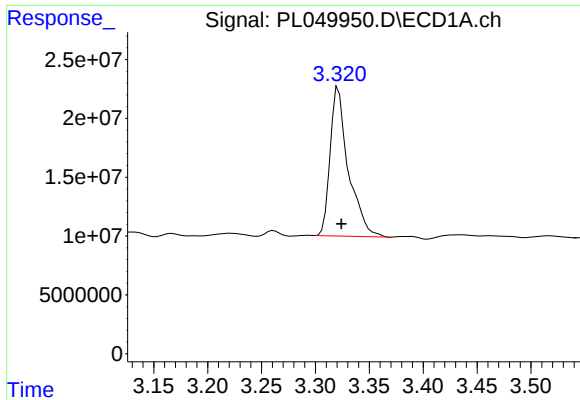

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 148782722
Conc: 13.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-062619-B

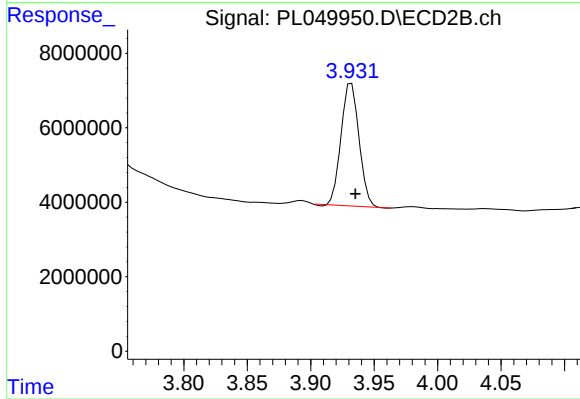


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.003 min
Response: 32449129
Conc: 10.60 ng/ml

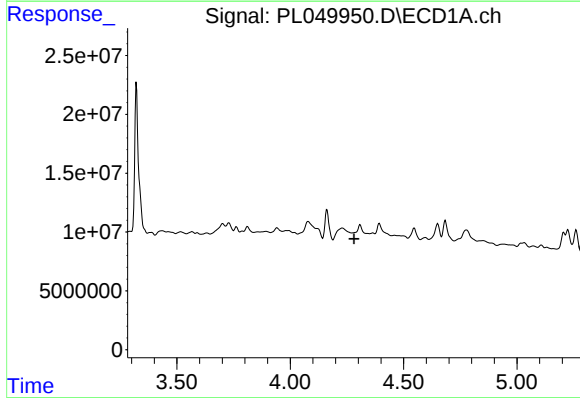


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

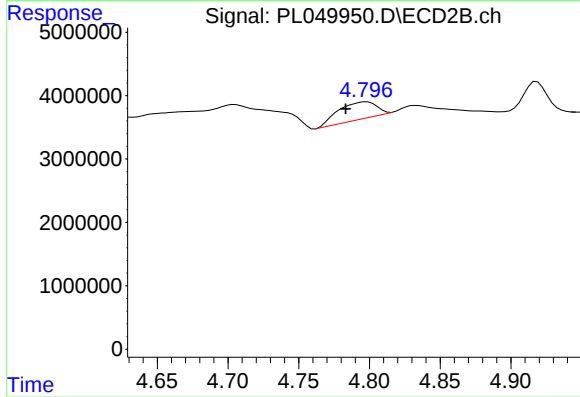

#6 beta-BHC


R.T.: 4.798 min
Delta R.T.: 0.015 min
Response: 5084675
Conc: 2.62 ng/ml

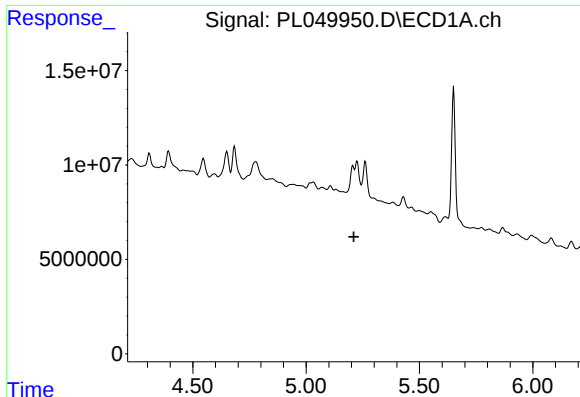

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CL-02-062619-B

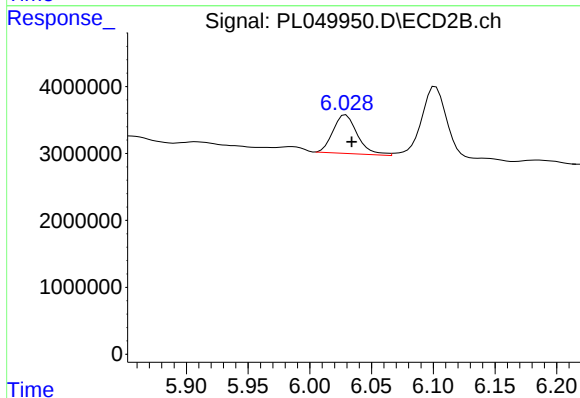


#10 gamma-Chlordane

R.T.: 6.029 min
Delta R.T.: -0.005 min
Response: 7955500
Conc: 2.13 ng/ml

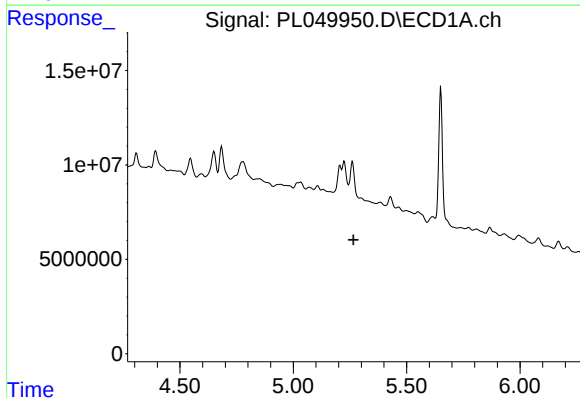


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

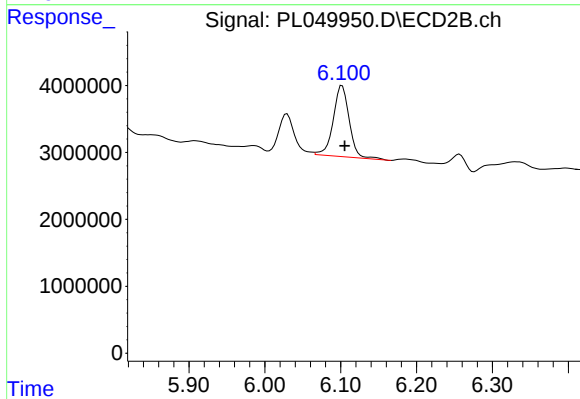

#11 alpha-Chlordane


R.T.: 6.102 min
Delta R.T.: -0.004 min
Response: 15656663
Conc: 4.23 ng/ml

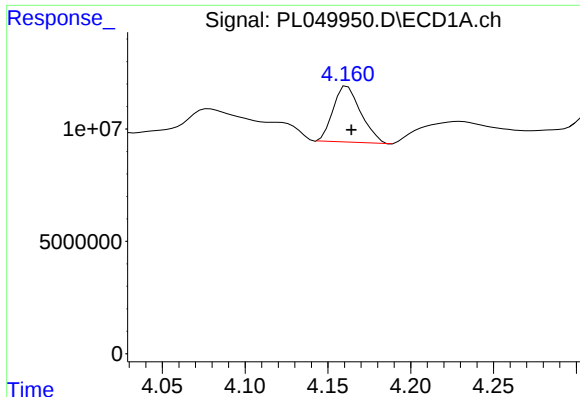

#23 Chlordane-1


R.T.: 4.162 min
Delta R.T.: -0.002 min
Response: 28911634
Conc: 50.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-062619-B

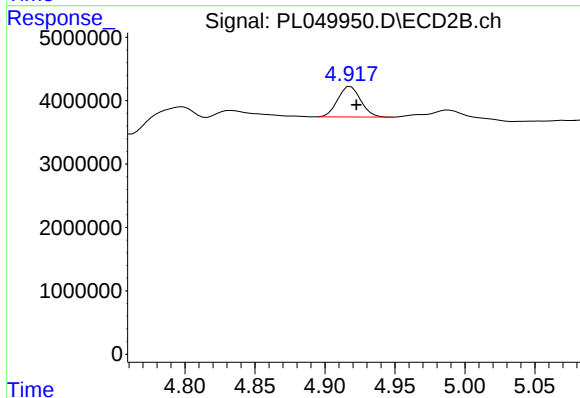


#23 Chlordane-1

R.T.: 4.918 min
Delta R.T.: -0.004 min
Response: 5481615
Conc: 37.30 ng/ml

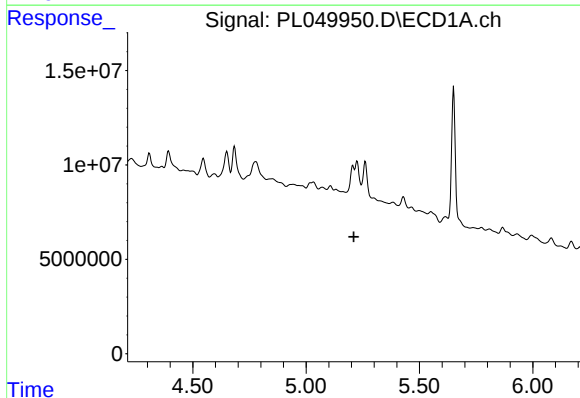


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.211 min
Response: 0
Conc: N.D.

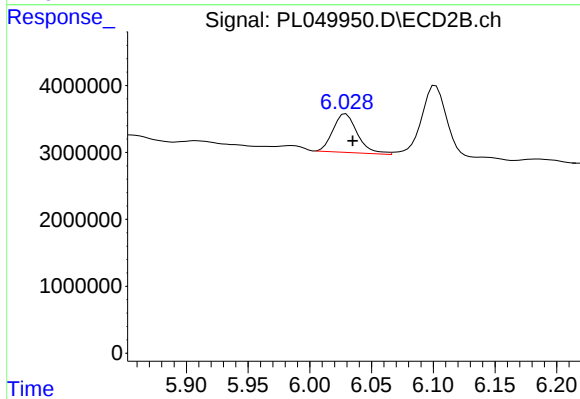

#25 Chlordane-3


R.T.: 6.029 min
Delta R.T.: -0.005 min
Response: 7955500
Conc: 15.99 ng/ml

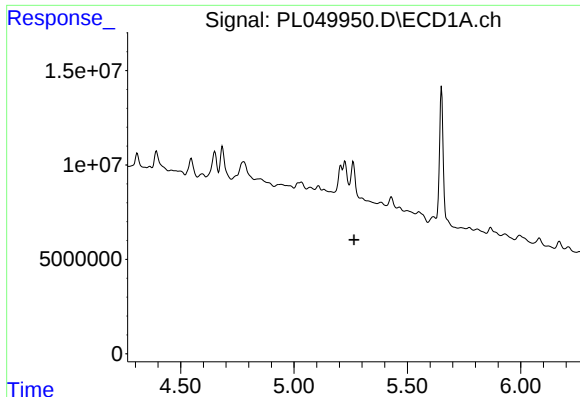

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CL-02-062619-B

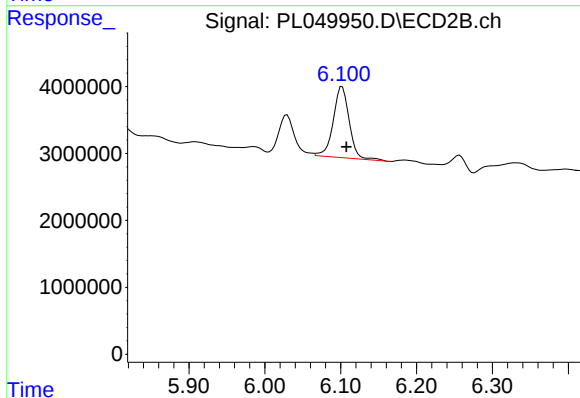


#26 Chlordane-4

R.T.: 6.102 min
Delta R.T.: -0.006 min
Response: 15656663
Conc: 26.34 ng/ml

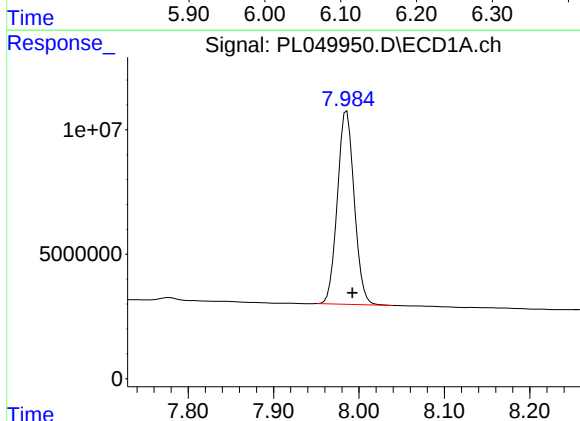

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.006 min
Response: 106683677
Conc: 8.40 ng/ml

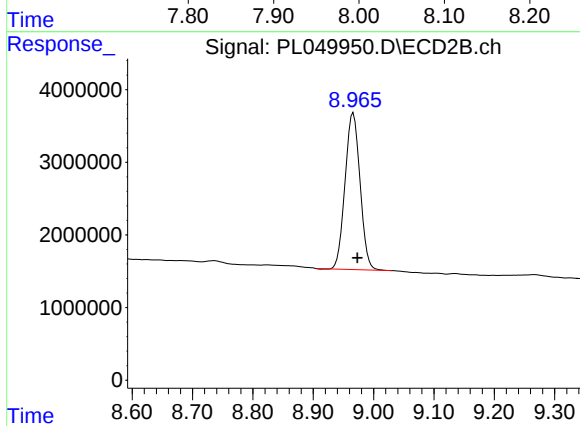

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: -0.007 min
Response: 37279972
Conc: 11.11 ng/ml