

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062719\
 Data File : PL049922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2019 11:33
 Operator : SM\AJ
 Sample : K3504-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-001-B200-062019

Manual Integrations
 APPROVED

Ankita
 6/28/2019 10:15:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:25:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.933	141.9E6	38229697	12.583	12.486
28)	SA Decachlor...	7.985	8.965	98315772	29027045	7.737	8.647
Target Compounds							
10)	B gamma-Chl...	5.205	6.027	5305872	2614674	0.310m	0.702m#
11)	B alpha-Chl...	5.259	6.101	8159558	4027731	0.492m	1.089m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062719\
Data File : PL049922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2019 11:33
Operator : SM\AJ
Sample : K3504-06
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
PST-001-B200-062019


Manual Integrations
APPROVED

Ankita
6/28/2019 10:15:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:25:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

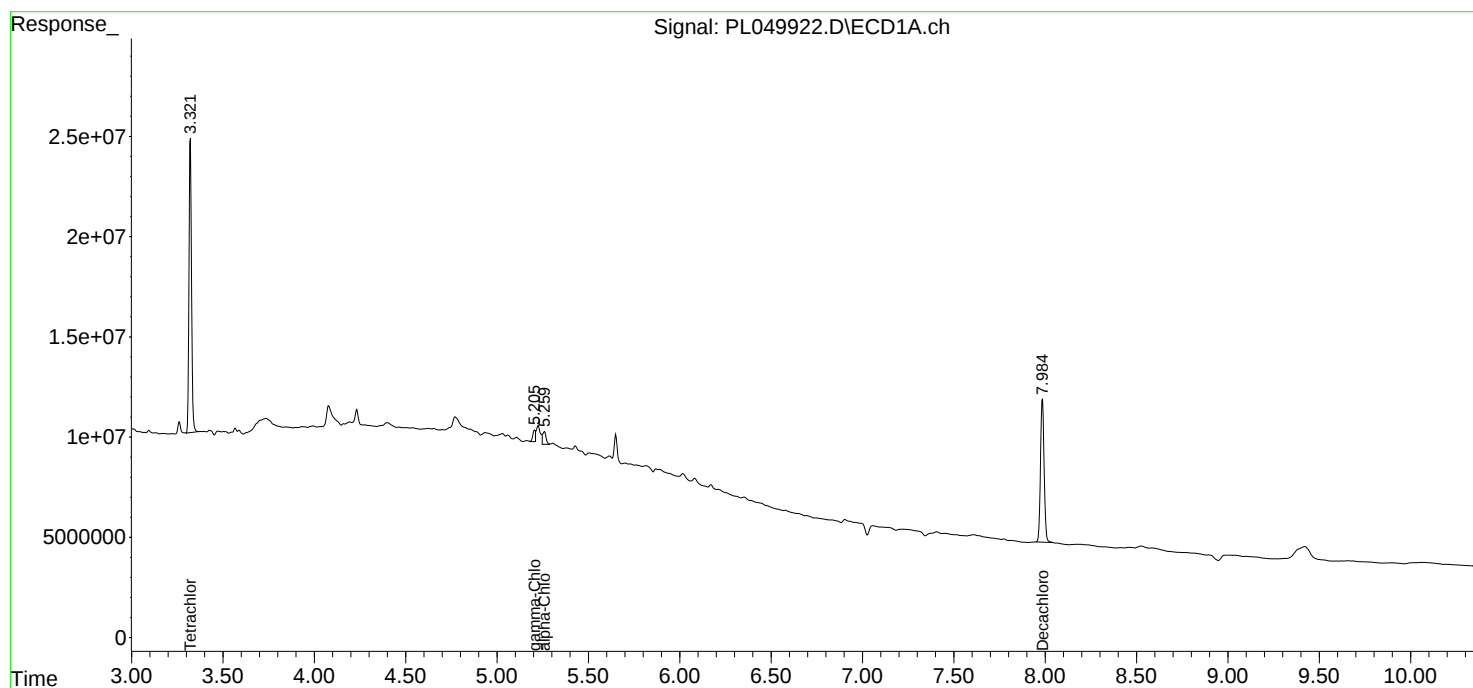

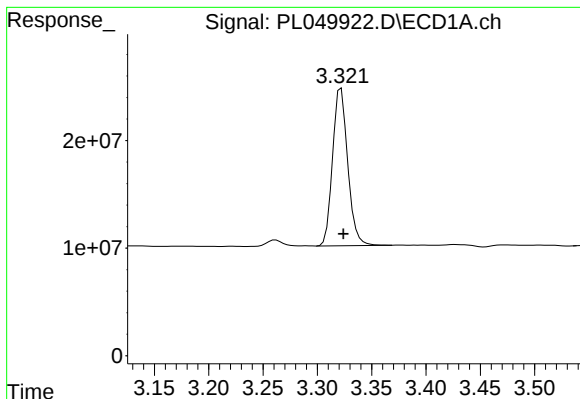


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 141910786
Conc: 12.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-001-B200-062019


Manual Integrations
APPROVED

Ankita
6/28/2019 10:15:28 AM

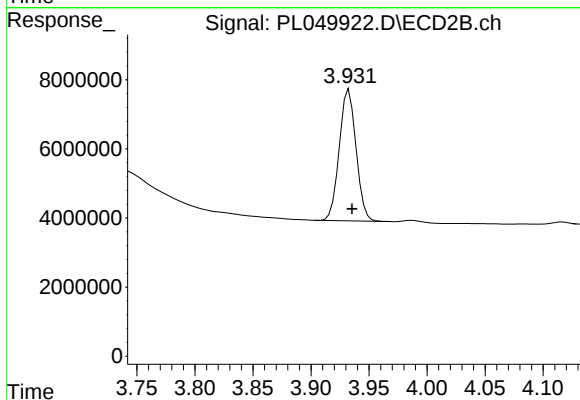


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.002 min
Response: 38229697
Conc: 12.49 ng/ml

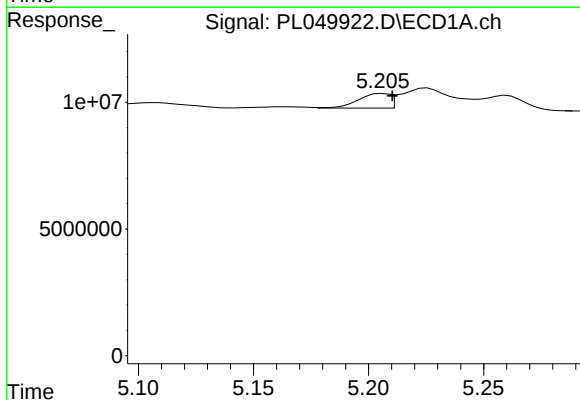


#10 gamma-Chlordane

R.T.: 5.205 min
Delta R.T.: -0.005 min
Response: 5305872
Conc: 0.31 ng/ml m

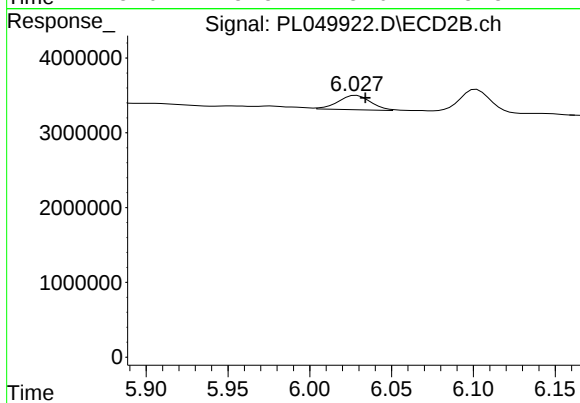

#10 gamma-Chlordane

R.T.: 6.027 min
Delta R.T.: -0.007 min
Response: 2614674
Conc: 0.70 ng/ml m

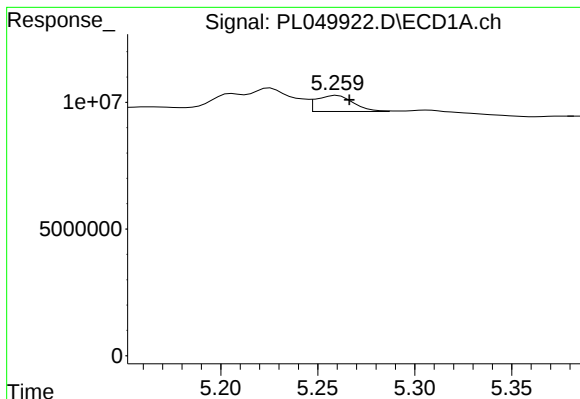


#11 alpha-Chlordane

R.T.: 5.259 min
Delta R.T.: -0.008 min
Response: 8159558
Conc: 0.49 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PST-001-B200-062019


Manual Integrations
APPROVED

Ankita
6/28/2019 10:15:28 AM

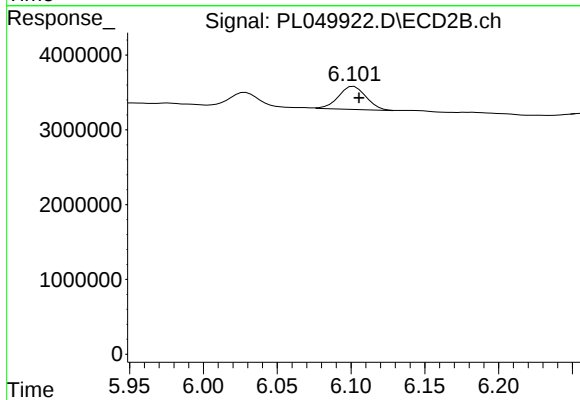


#11 alpha-Chlordane

R.T.: 6.101 min
Delta R.T.: -0.005 min
Response: 4027731
Conc: 1.09 ng/ml m

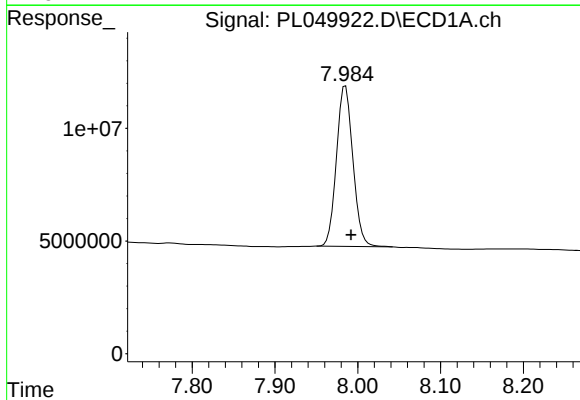

#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.007 min
Response: 98315772
Conc: 7.74 ng/ml

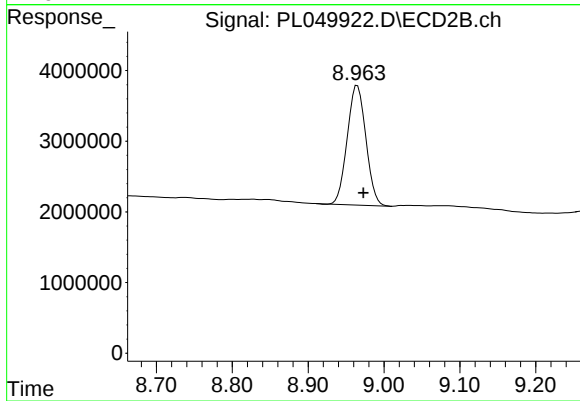

#28 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: -0.008 min
Response: 29027045
Conc: 8.65 ng/ml