

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062719\
 Data File : PL049950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2019 19:05
 Operator : SM\AJ
 Sample : K3157-13
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-062619-B

Manual Integrations
 APPROVED

Ankita
 6/28/2019 10:16:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:29:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	3.931	148.8E6	33258544	13.193	10.863m
2) SA Decachlor...	7.986	8.966	106.7E6	37279972	8.396	11.105 #
Target Compounds						
10) B gamma-Chl...	5.205	6.029	17461732	7955500	1.022m	2.135 #
11) B alpha-Chl...	5.260	6.100	24905255	15500789	1.500m	4.191m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062719\
Data File : PL049950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2019 19:05
Operator : SM\AJ
Sample : K3157-13
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
CL-02-062619-B


Manual Integrations
APPROVED

Ankita
6/28/2019 10:16:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:29:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

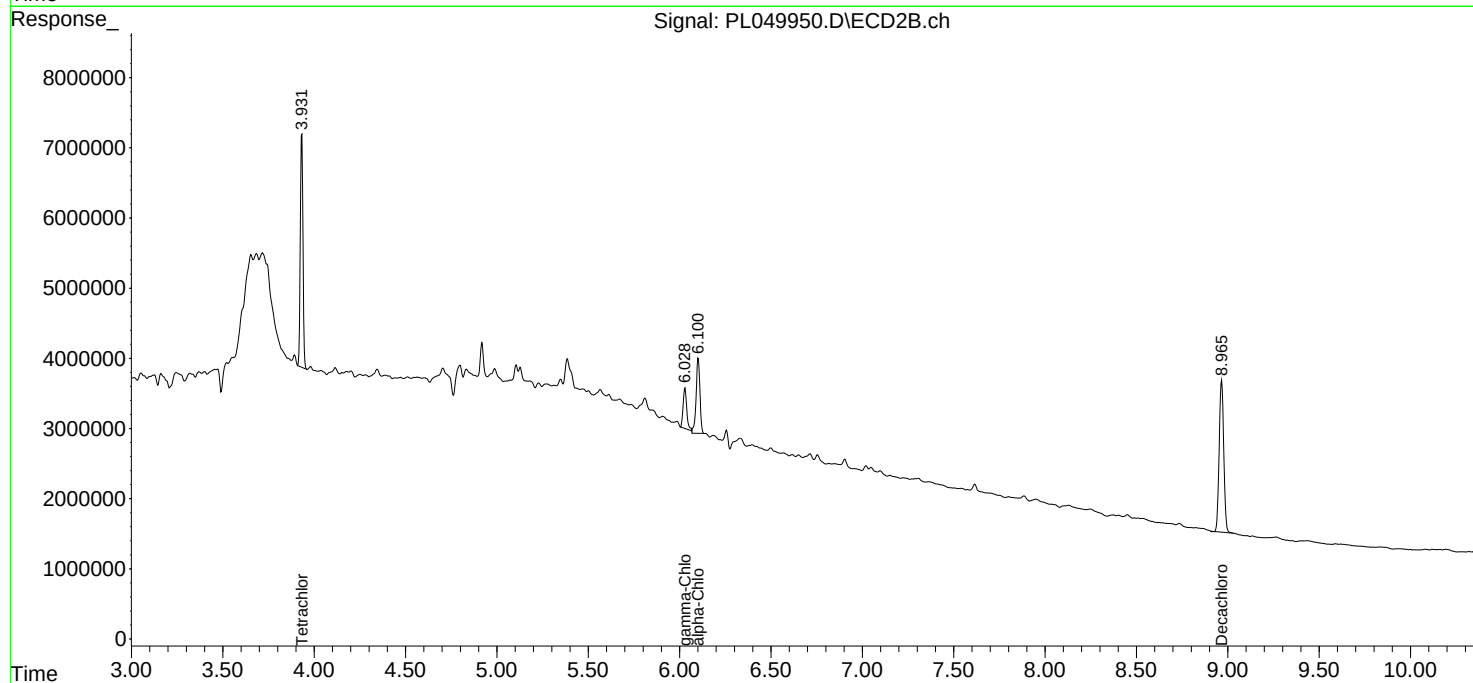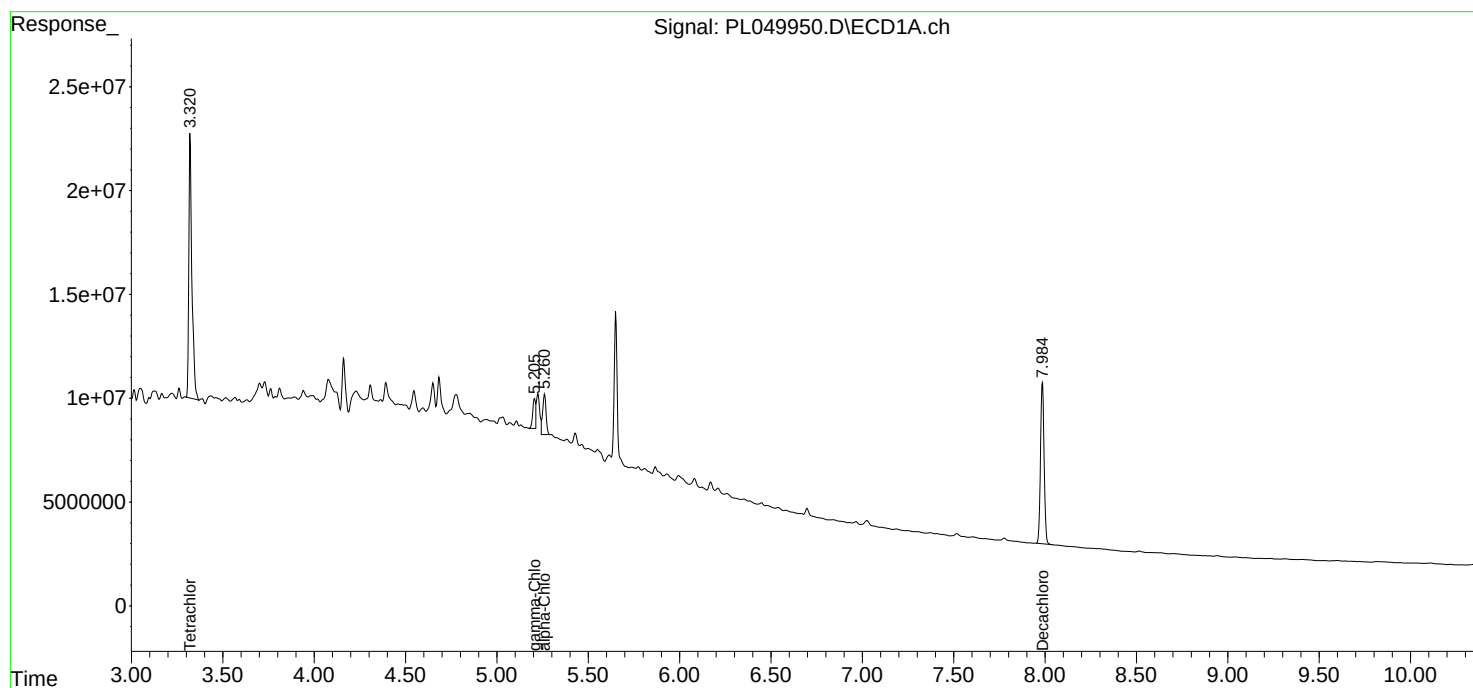

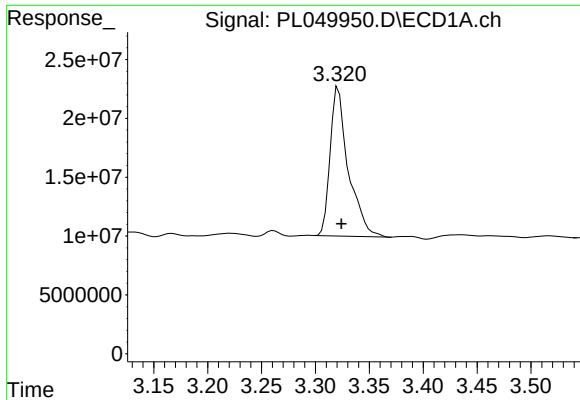


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 148782722
Conc: 13.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-062619-B


Manual Integrations
APPROVED

Ankita
6/28/2019 10:16:08 AM

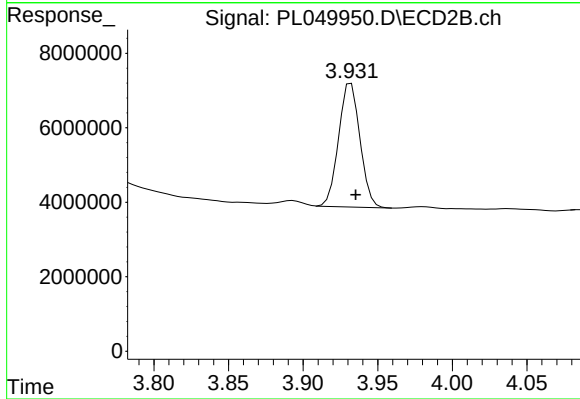


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.004 min
Response: 33258544
Conc: 10.86 ng/ml m

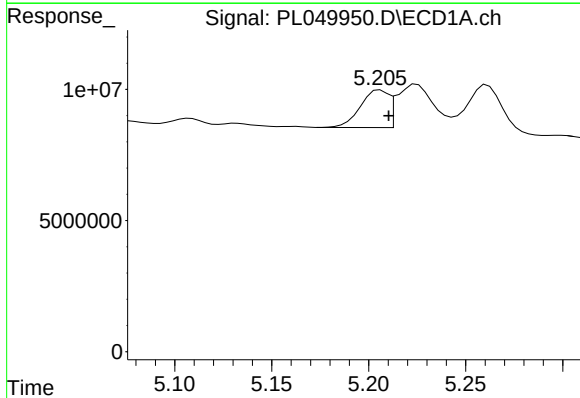


#10 gamma-Chlordane

R.T.: 5.205 min
Delta R.T.: -0.006 min
Response: 17461732
Conc: 1.02 ng/ml m

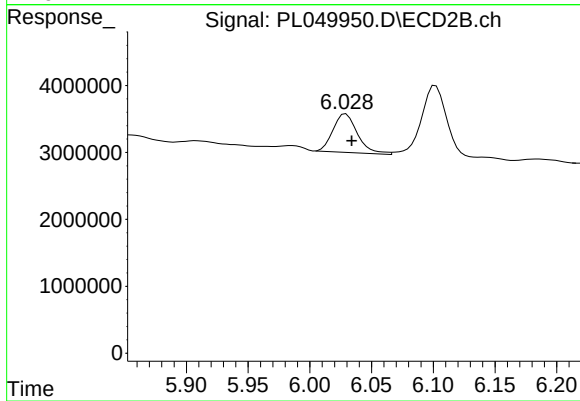

#10 gamma-Chlordane

R.T.: 6.029 min
Delta R.T.: -0.005 min
Response: 7955500
Conc: 2.13 ng/ml

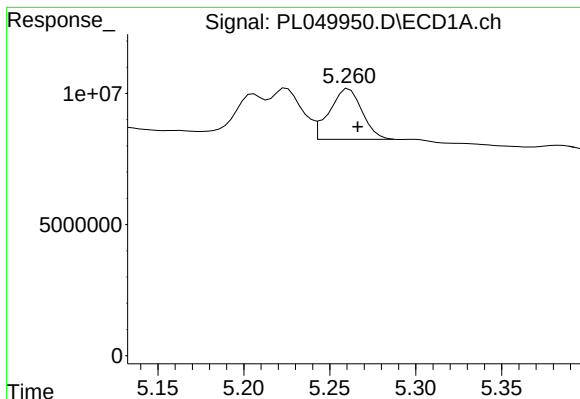


#11 alpha-Chlordane

R.T.: 5.260 min
Delta R.T.: -0.006 min
Response: 24905255
Conc: 1.50 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-02-062619-B


Manual Integrations
APPROVED

Ankita
6/28/2019 10:16:08 AM

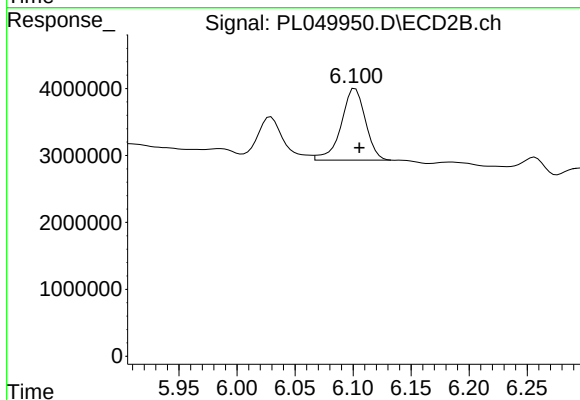


#11 alpha-Chlordane

R.T.: 6.100 min
Delta R.T.: -0.005 min
Response: 15500789
Conc: 4.19 ng/ml m

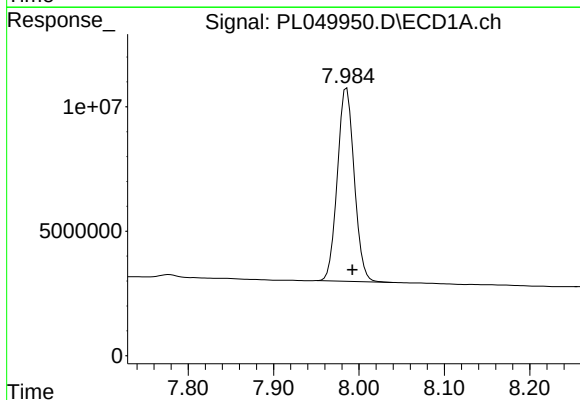

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.006 min
Response: 106683677
Conc: 8.40 ng/ml

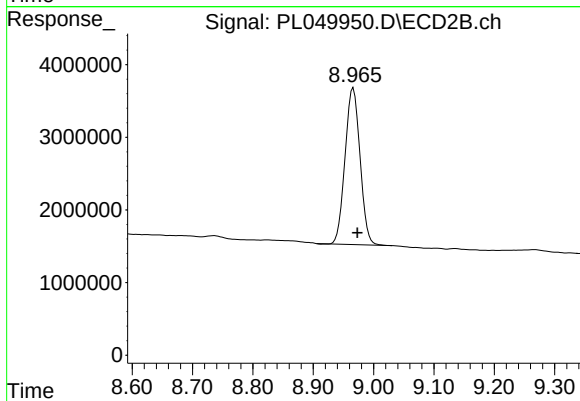

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: -0.007 min
Response: 37279972
Conc: 11.11 ng/ml