

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062722\
 Data File : PL076035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2022 08:58
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 15:13:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.634	15120197	37888057	19.992	19.977
28)	SA Decachlor...	11.635	10.375	12707690	28511580	20.194	18.564
Target Compounds							
7)	B delta-BHC	0.000	6.396	0	366620	N.D.	0.162 #
11)	B alpha-Chl...	0.000	7.385f	0	37518	N.D.	0.020 #
14)	MA Endrin	0.000	8.060f	0	633834	N.D.	0.417 #
15)	B Endosulfa...	9.303	0.000	378768	0	0.597	N.D. #
17)	MA 4,4'-DDT	0.000	8.460	0	41593	N.D.	0.028 #
18)	B Endrin al...	0.000	8.537	0	83584	N.D.	0.070 #
19)	B Endosulfa...	0.000	8.764	0	280880	N.D.	0.183 #
21)	B Endrin ke...	10.183f	0.000	705609	0	0.979	N.D. #
26)	Chlordane-4	0.000	7.385f	0	37518	N.D.	0.199 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062722\
Data File : PL076035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2022 08:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 15:13:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

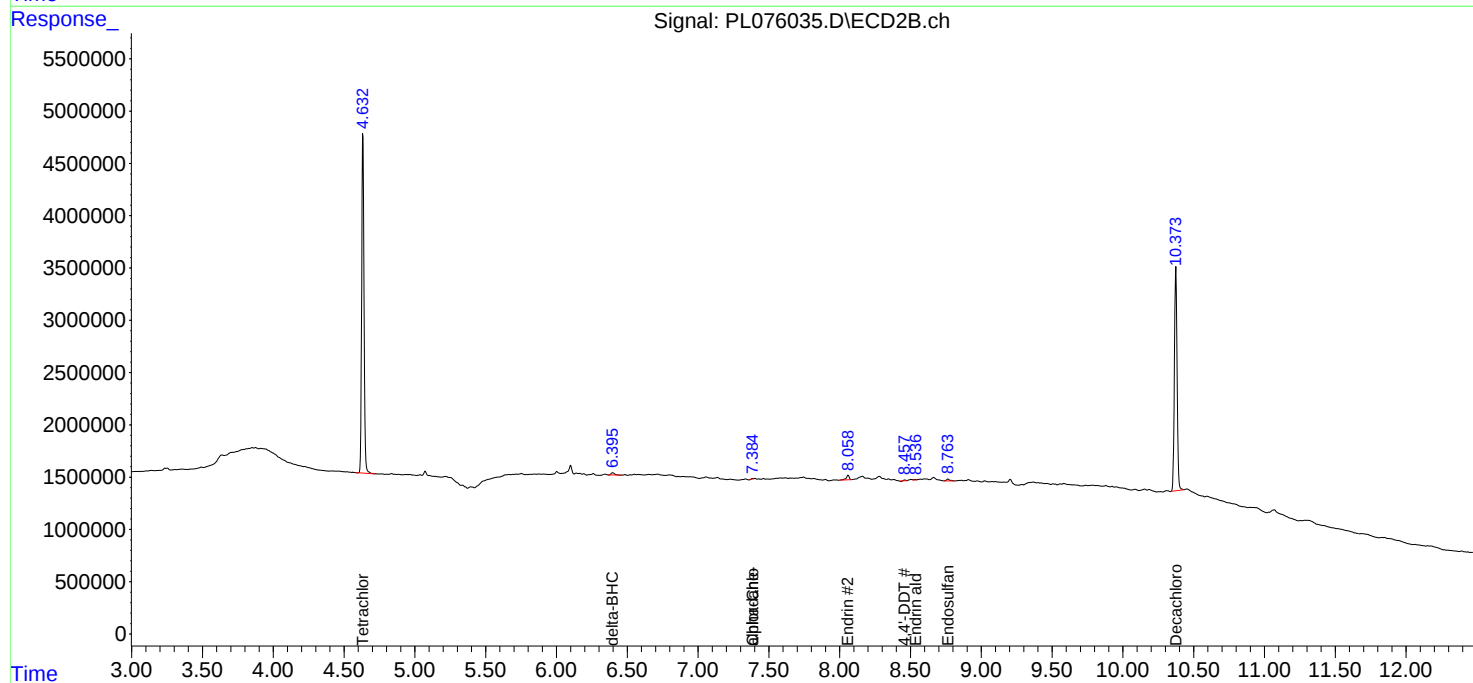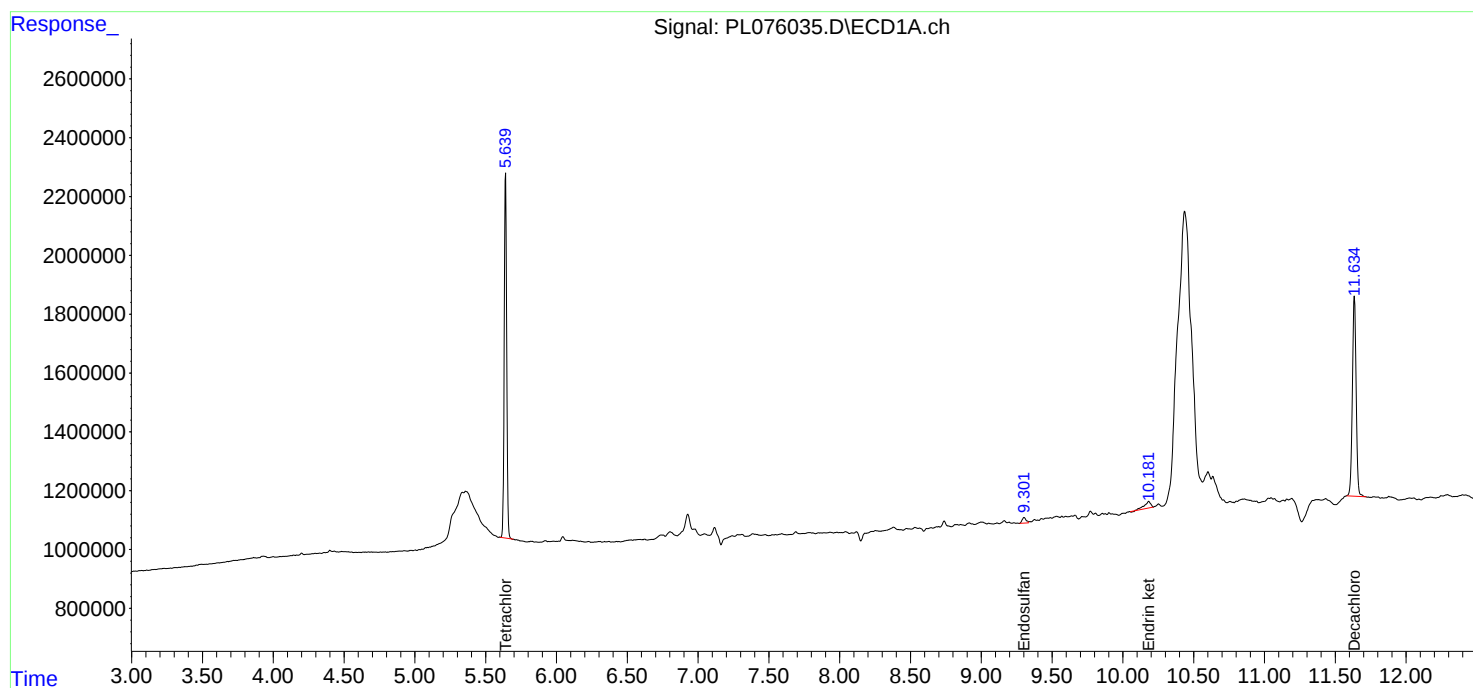


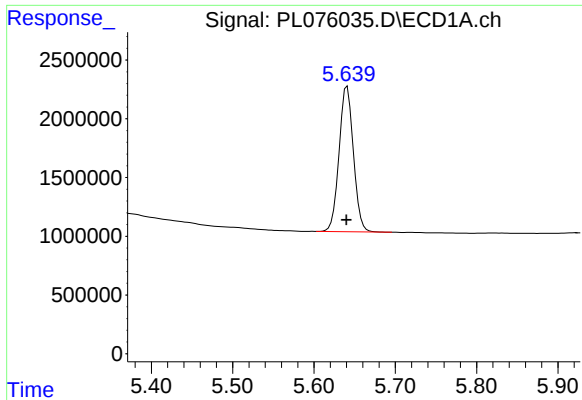

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 15120197
Conc: 19.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

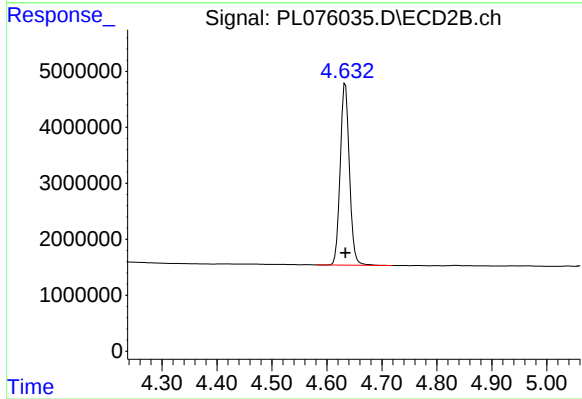


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 37888057
Conc: 19.98 ng/ml

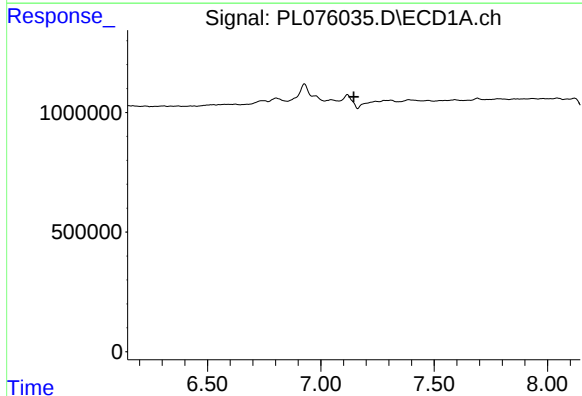


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

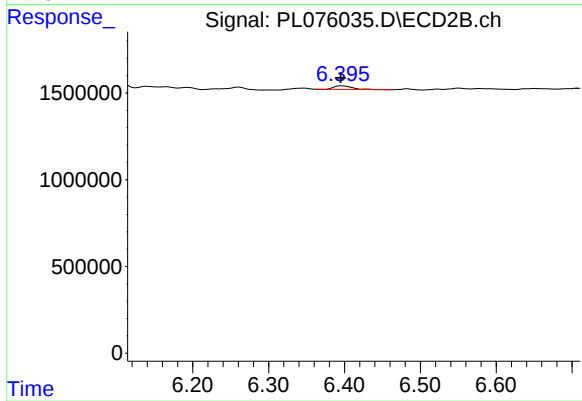

#7 delta-BHC

R.T.: 6.396 min
Delta R.T.: 0.001 min
Response: 366620
Conc: 0.16 ng/ml

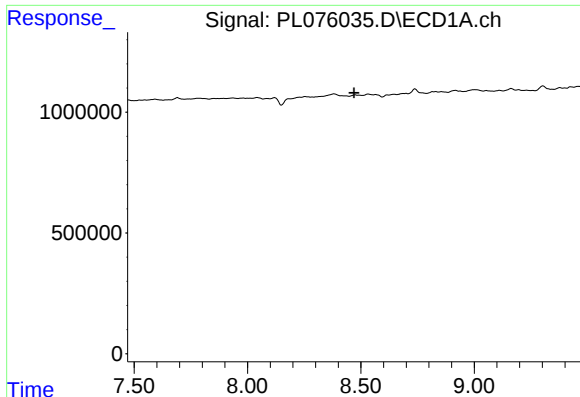

#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#11 alpha-Chlordane


R.T.: 7.385 min
Delta R.T.: -0.021 min
Response: 37518
Conc: 0.02 ng/ml

#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

#14 Endrin


R.T.: 8.060 min
Delta R.T.: 0.022 min
Response: 633834
Conc: 0.42 ng/ml

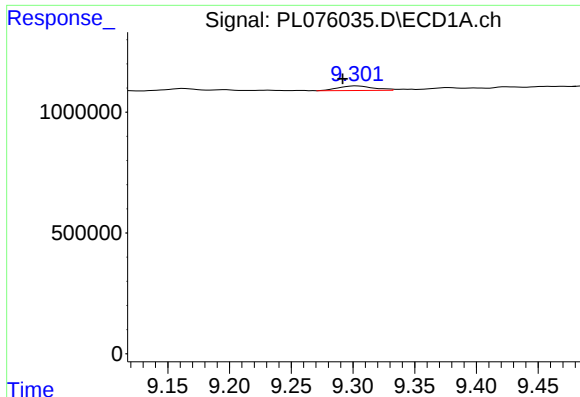

#15 Endosulfan II


R.T.: 9.303 min
Delta R.T.: 0.011 min
Response: 378768
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

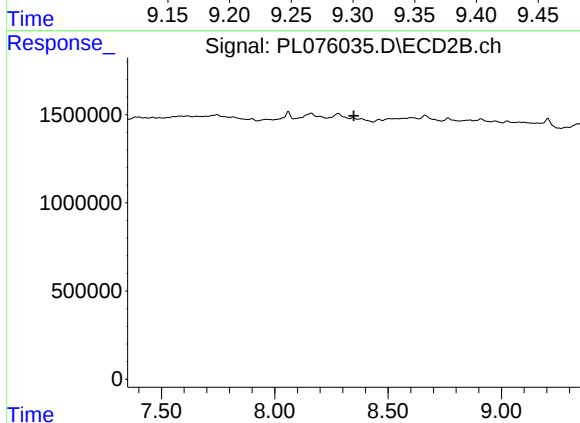


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

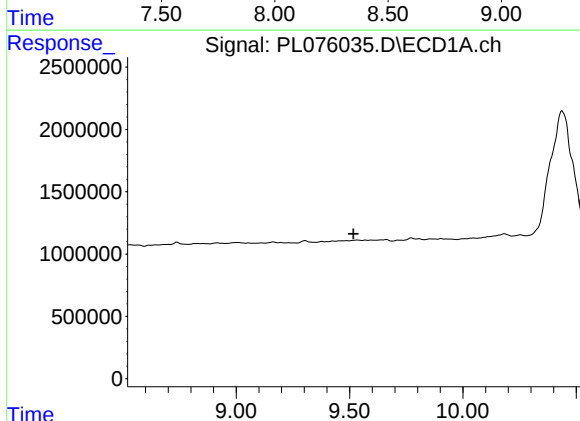


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.518 min
Response: 0
Conc: N.D.

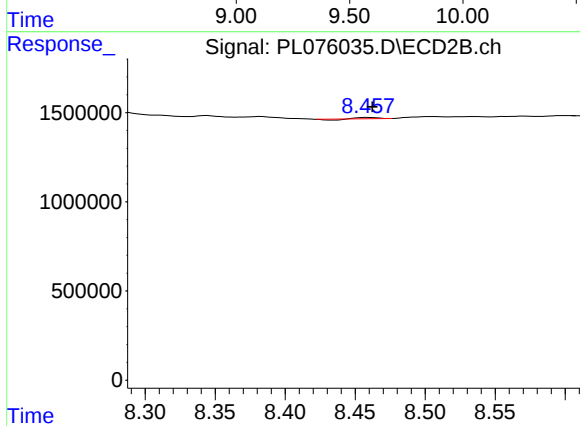

#17 4,4'-DDT


R.T.: 8.460 min
Delta R.T.: -0.002 min
Response: 41593
Conc: 0.03 ng/ml

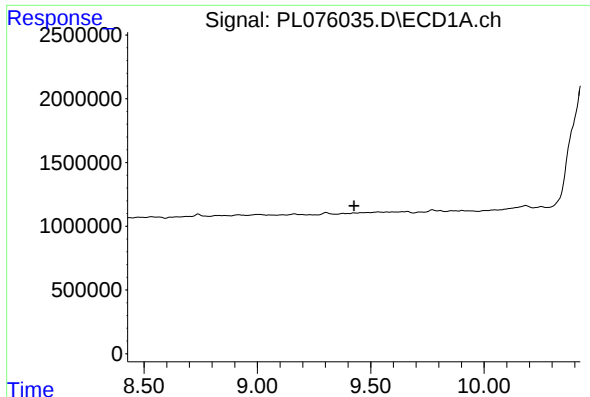

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 9.426 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

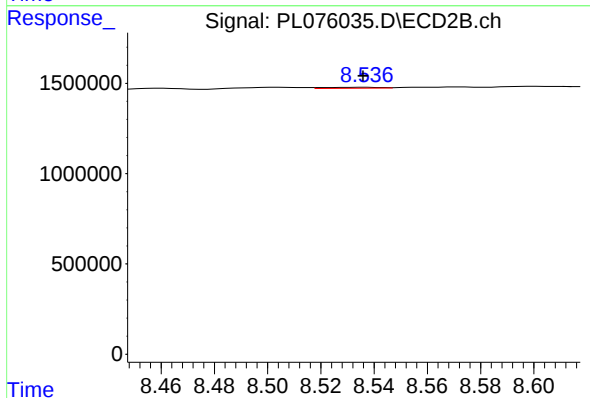


#18 Endrin aldehyde

R.T.: 8.537 min
Delta R.T.: 0.002 min
Response: 83584
Conc: 0.07 ng/ml

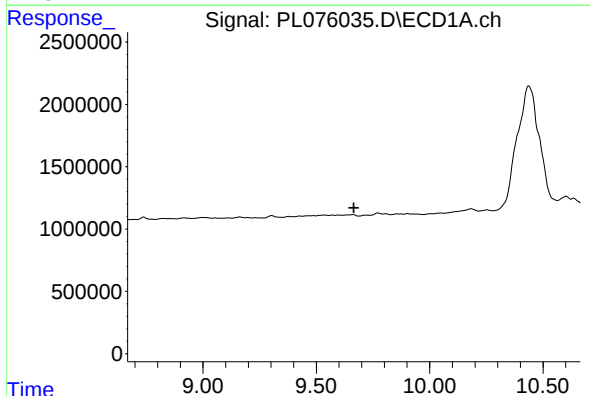


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.665 min
Response: 0
Conc: N.D.

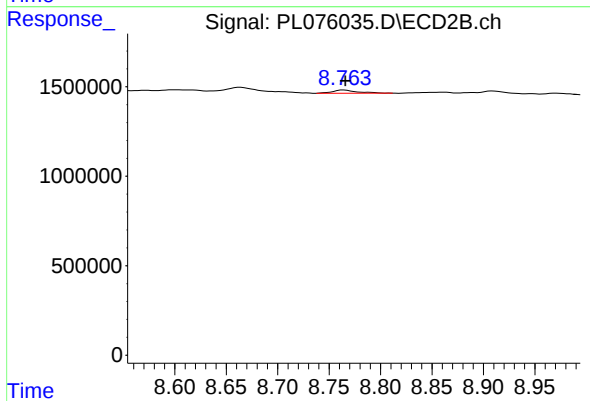

#19 Endosulfan Sulfate

R.T.: 8.764 min
Delta R.T.: -0.001 min
Response: 280880
Conc: 0.18 ng/ml

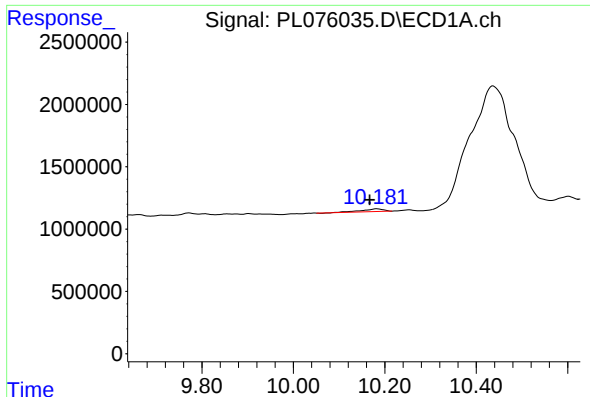

#21 Endrin ketone

R.T.: 10.183 min
Delta R.T.: 0.016 min
Response: 705609
Conc: 0.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.472 min
Response: 0
Conc: N.D.

#26 Chlordane-4


R.T.: 7.385 min
Delta R.T.: -0.019 min
Response: 37518
Conc: 0.20 ng/ml

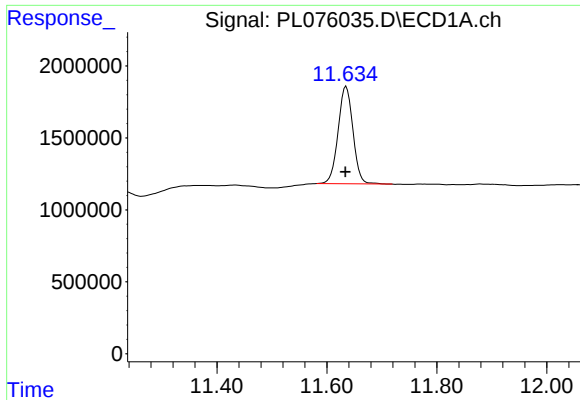

#28 Decachlorobiphenyl

R.T.: 11.635 min
Delta R.T.: 0.001 min
Response: 12707690
Conc: 20.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

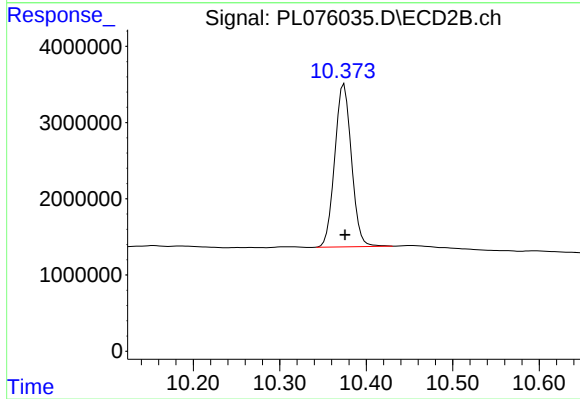

#28 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.000 min
Response: 28511580
Conc: 18.56 ng/ml