

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062722\
 Data File : PL076046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2022 13:58
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 15:16:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.633	15025331	38501381	19.866	20.300
28)	SA Decachlor...	11.634	10.373	13257687	29829060	21.068	19.421
Target Compounds							
4)	MA Heptachlor	0.000	6.140f	0	107604	N.D.	0.047 #
6)	B beta-BHC	0.000	6.140	0	107604	N.D.	0.103 #
7)	B delta-BHC	0.000	6.398	0	352732	N.D.	0.156 #
10)	B gamma-Chl...	0.000	7.332	0	227432	N.D.	0.118 #
11)	B alpha-Chl...	0.000	7.385f	0	36734	N.D.	0.019 #
13)	MA Dieldrin	0.000	7.743	0	301388	N.D.	0.167 #
14)	MA Endrin	0.000	8.058f	0	506174	N.D.	0.333 #
15)	B Endosulfa...	9.300	0.000	268528	0	0.423	N.D. #
21)	B Endrin ke...	10.182	0.000	402069	0	0.558	N.D. #
25)	Chlordane-3	0.000	7.332	0	227432	N.D.	1.290 #
26)	Chlordane-4	0.000	7.385f	0	36734	N.D.	0.195 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062722\
Data File : PL076046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2022 13:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 15:16:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

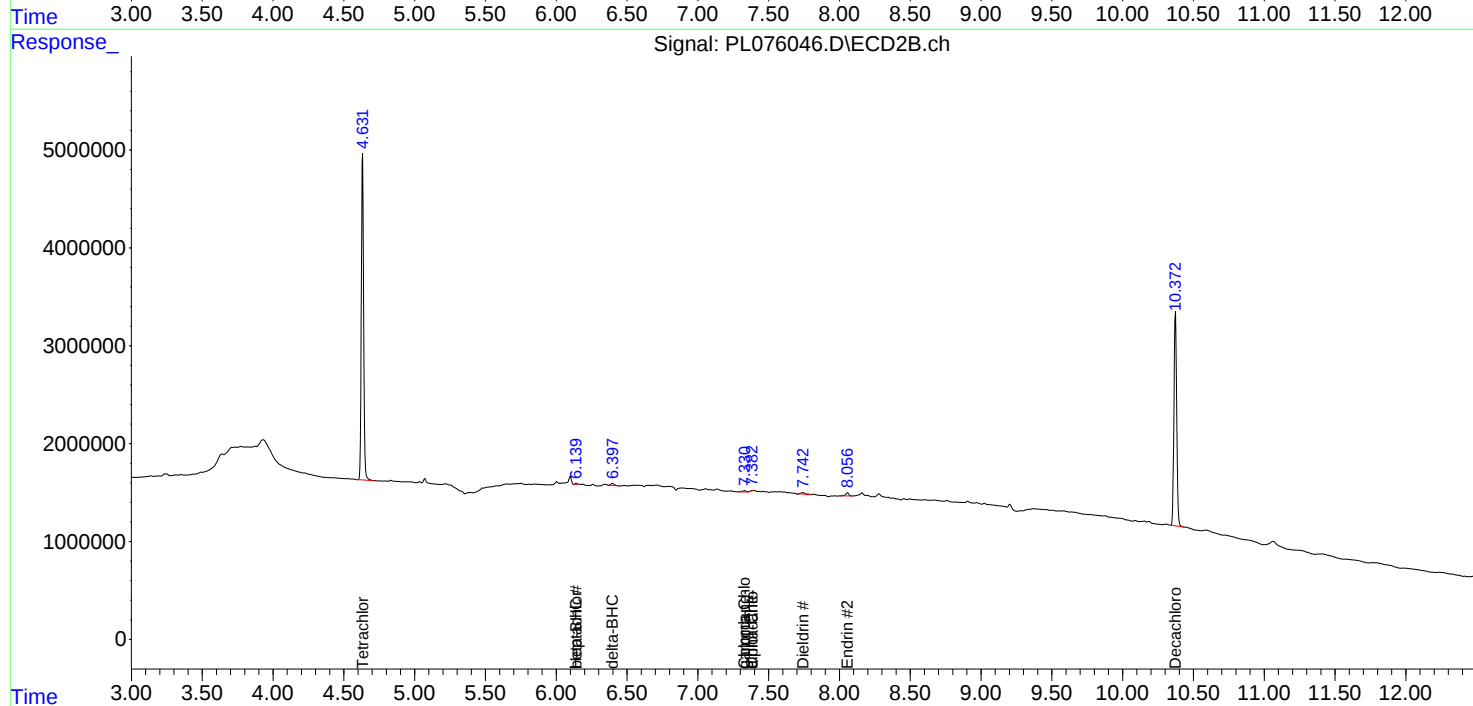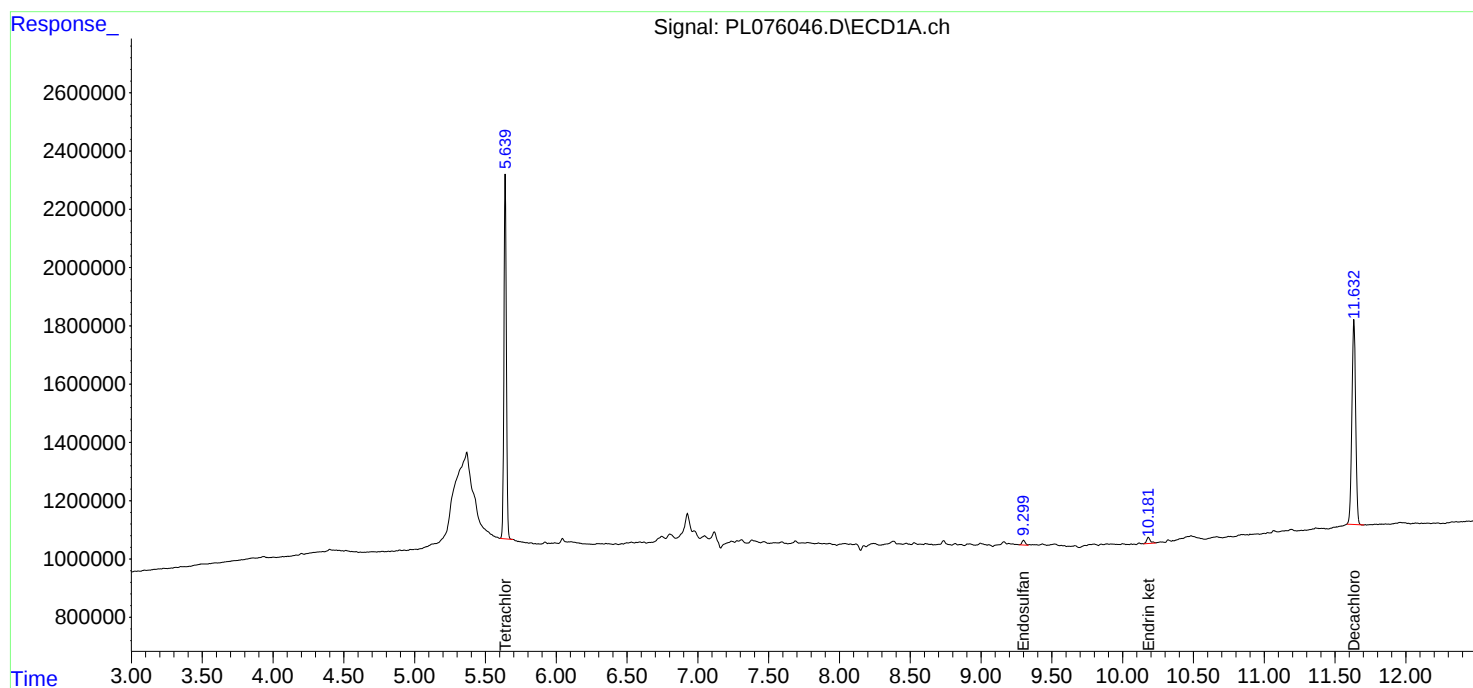


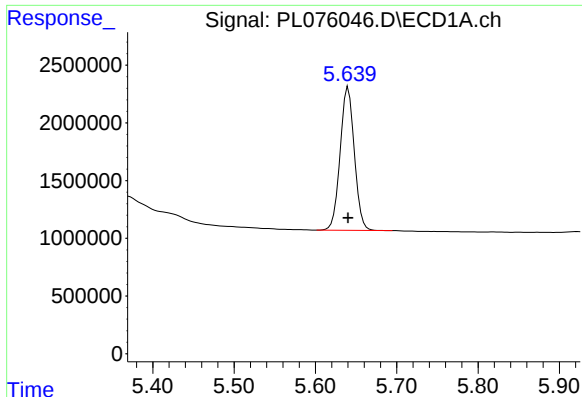

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 15025331
Conc: 19.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

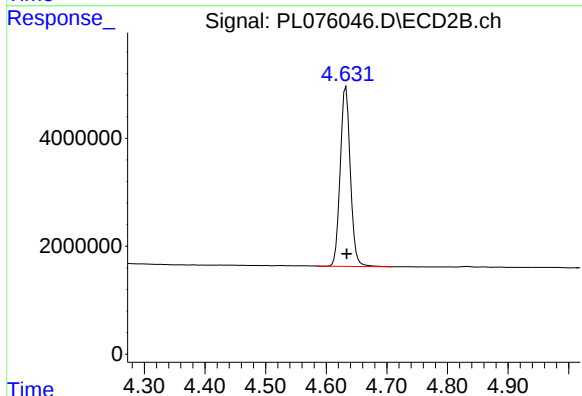


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: -0.001 min
Response: 38501381
Conc: 20.30 ng/ml

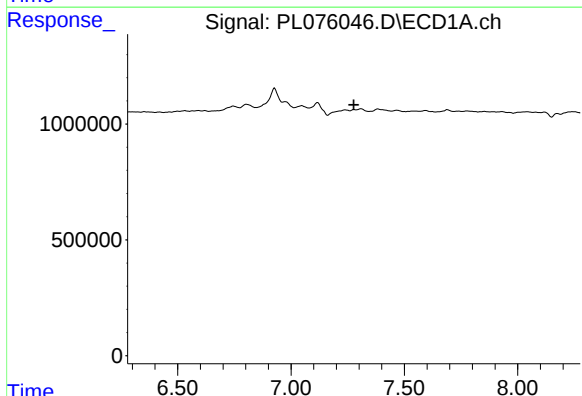


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.277 min
Response: 0
Conc: N.D.

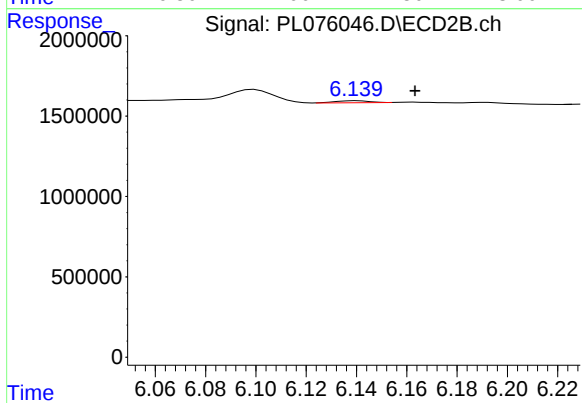

#4 Heptachlor


R.T.: 6.140 min
Delta R.T.: -0.023 min
Response: 107604
Conc: 0.05 ng/ml

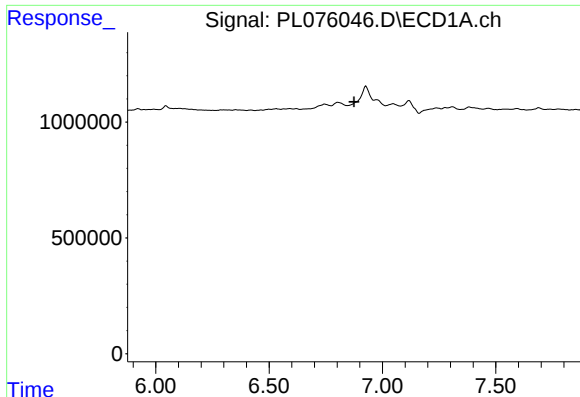

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.875 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

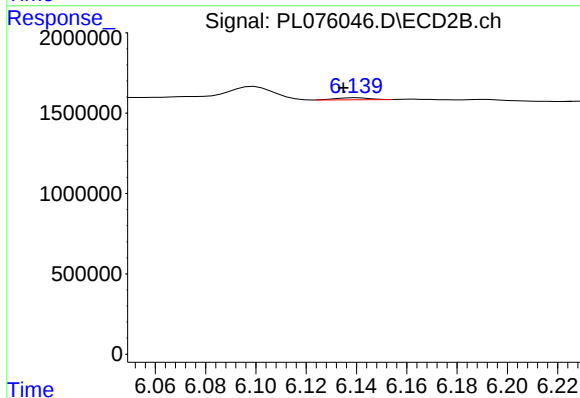


#6 beta-BHC

R.T.: 6.140 min
Delta R.T.: 0.005 min
Response: 107604
Conc: 0.10 ng/ml

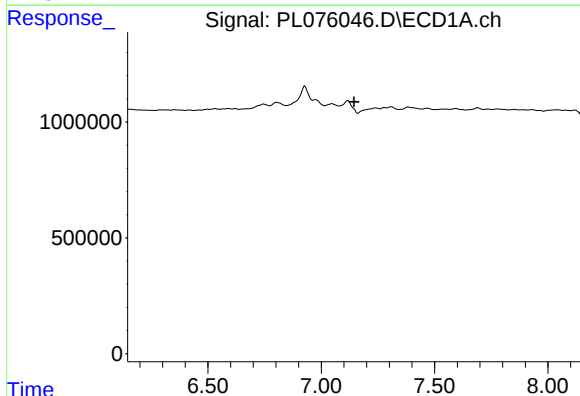


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

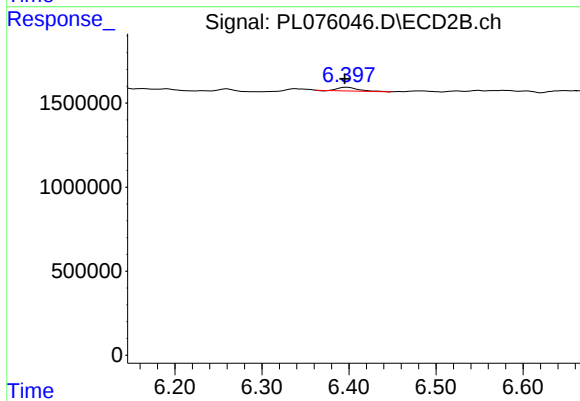

#7 delta-BHC


R.T.: 6.398 min
Delta R.T.: 0.003 min
Response: 352732
Conc: 0.16 ng/ml

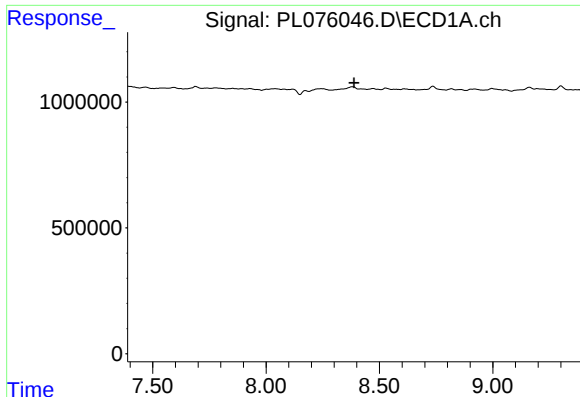

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

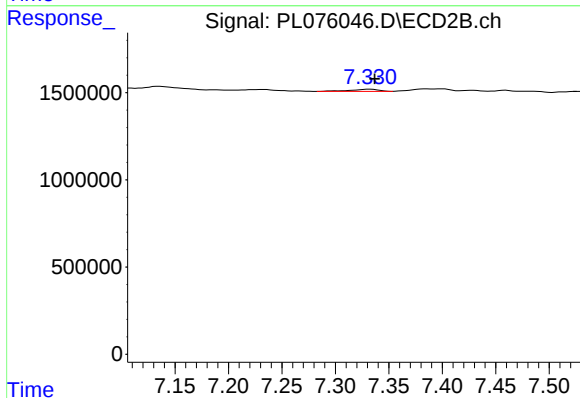


#10 gamma-Chlordane

R.T.: 7.332 min
Delta R.T.: -0.005 min
Response: 227432
Conc: 0.12 ng/ml

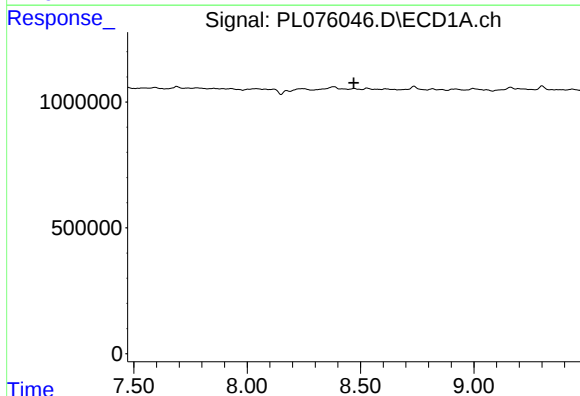


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.470 min
Response: 0
Conc: N.D.

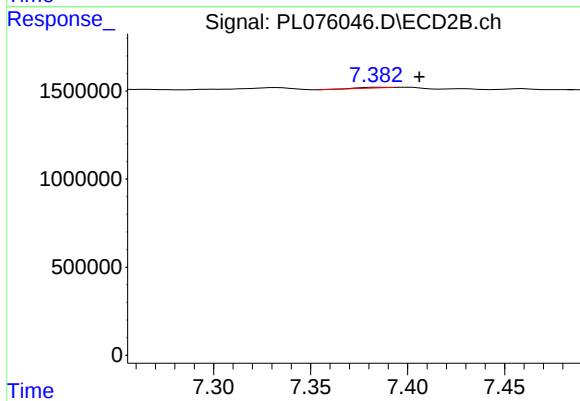

#11 alpha-Chlordane


R.T.: 7.385 min
Delta R.T.: -0.021 min
Response: 36734
Conc: 0.02 ng/ml

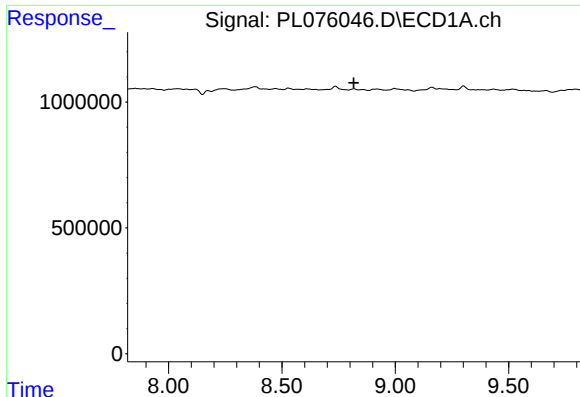

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

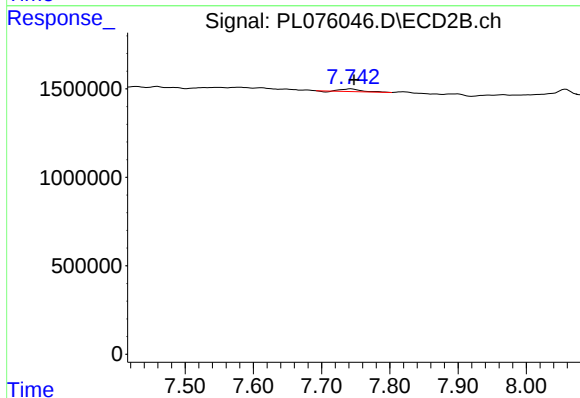


#13 Dieldrin

R.T.: 7.743 min
Delta R.T.: -0.005 min
Response: 301388
Conc: 0.17 ng/ml

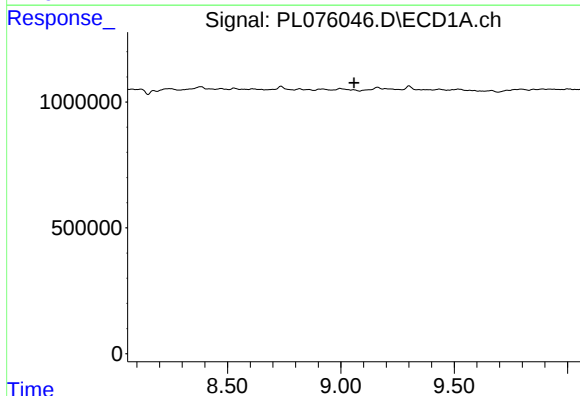


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.058 min
Response: 0
Conc: N.D.

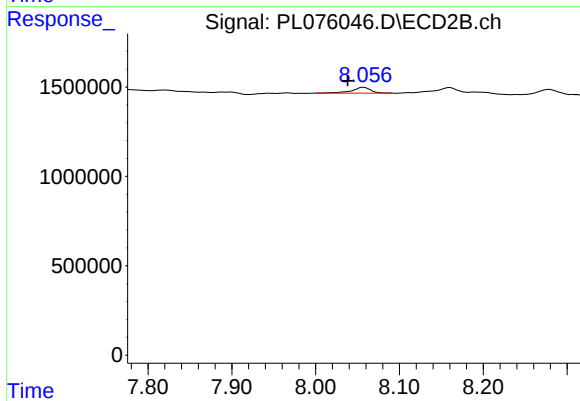

#14 Endrin


R.T.: 8.058 min
Delta R.T.: 0.019 min
Response: 506174
Conc: 0.33 ng/ml

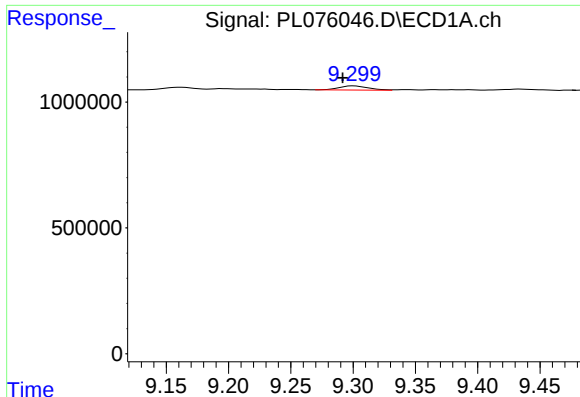

#15 Endosulfan II


R.T.: 9.300 min
Delta R.T.: 0.009 min
Response: 268528
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

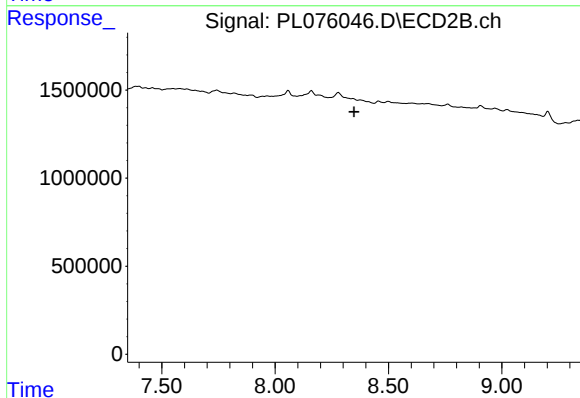


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

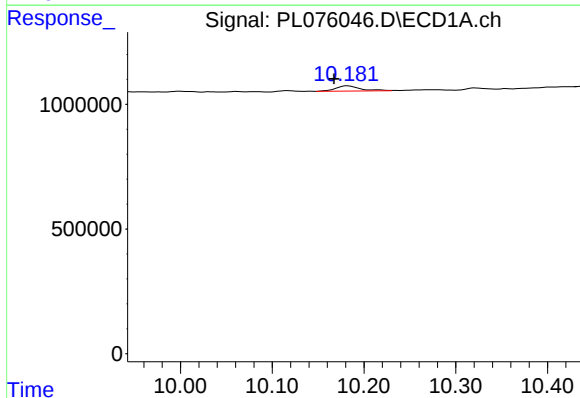


#21 Endrin ketone

R.T.: 10.182 min
Delta R.T.: 0.015 min
Response: 402069
Conc: 0.56 ng/ml

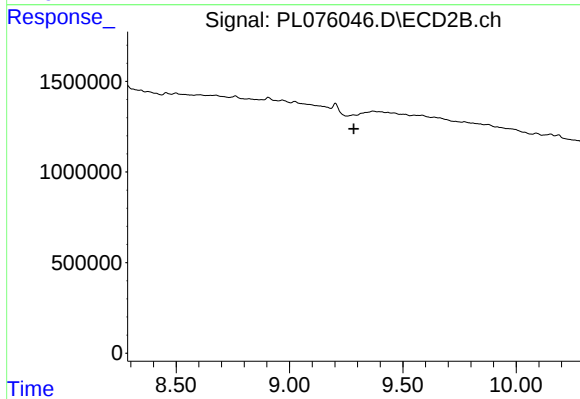

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

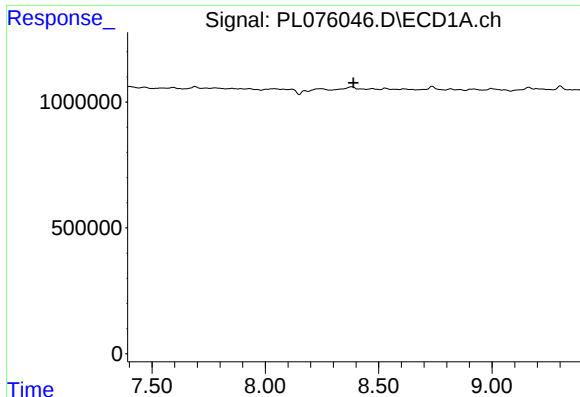

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

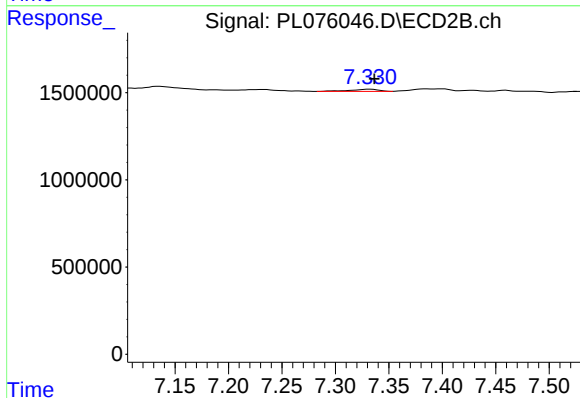


#25 Chlordane-3

R.T.: 7.332 min
Delta R.T.: -0.005 min
Response: 227432
Conc: 1.29 ng/ml

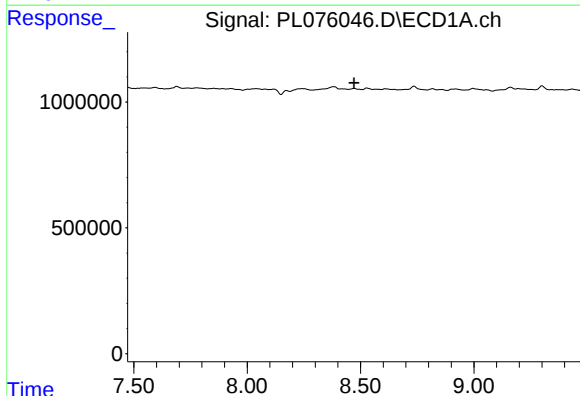


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

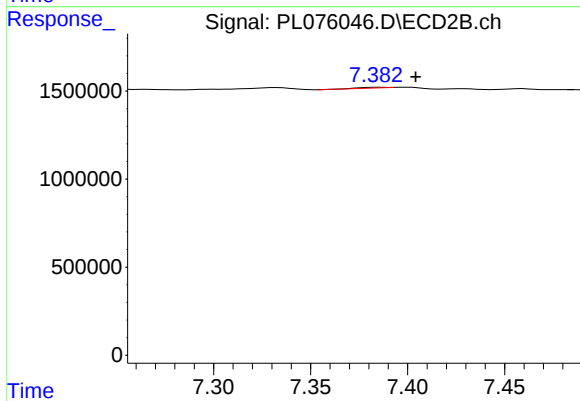

#26 Chlordane-4


R.T.: 7.385 min
Delta R.T.: -0.019 min
Response: 36734
Conc: 0.19 ng/ml

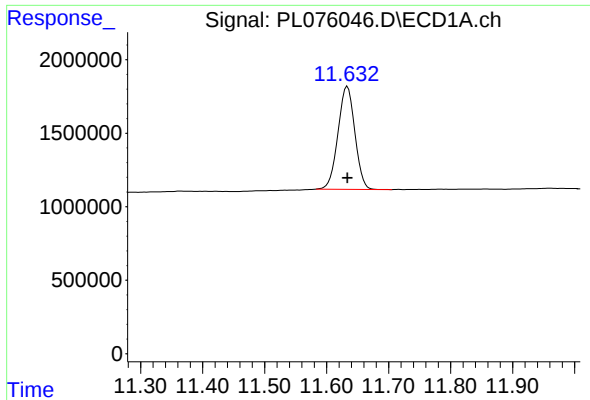

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: 0.000 min
Response: 13257687
Conc: 21.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

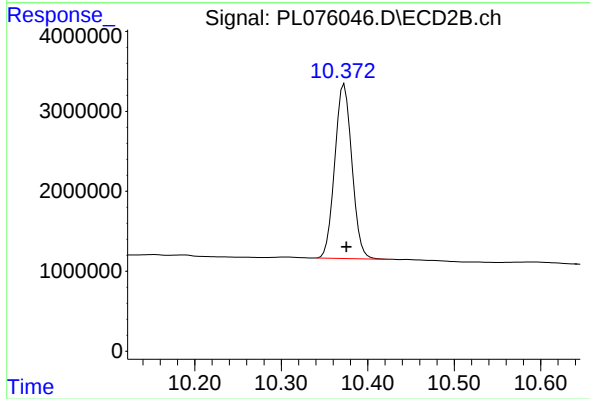

#28 Decachlorobiphenyl

R.T.: 10.373 min
Delta R.T.: -0.002 min
Response: 29829060
Conc: 19.42 ng/ml