

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062722\
 Data File : PL076069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2022 21:56
 Operator : AR\AJ
 Sample : N3494-17
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 00:25:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.632	13539726	32449087	17.902	17.109
28)	SA Decachlor...	11.632	10.372	11993029	27016159	19.059	17.590
Target Compounds							
2)	A alpha-BHC	0.000	5.351f	0	2353030	N.D.	0.963 #
4)	MA Heptachlor	0.000	6.139f	0	662330	N.D.	0.292 #
5)	MB Aldrin	0.000	6.482	0	159225	N.D.	0.077 #
6)	B beta-BHC	0.000	6.139	0	662330	N.D.	0.635 #
7)	B delta-BHC	7.121f	6.397	1400569	354858	1.794	0.157 #
11)	B alpha-Chl...	0.000	7.378f	0	232766	N.D.	0.122 #
14)	MA Endrin	0.000	8.059f	0	275462	N.D.	0.181 #
15)	B Endosulfa...	9.304	0.000	263604	0	0.415	N.D. #
19)	B Endosulfa...	0.000	8.759	0	3386066	N.D.	2.207 #
21)	B Endrin ke...	10.183f	0.000	235575	0	0.327	N.D. #
26)	Chlordane-4	0.000	7.378f	0	232766	N.D.	1.235 #
27)	Chlordane-5	0.000	8.135f	0	76858	N.D.	1.680 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062722\
Data File : PL076069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2022 21:56
Operator : AR\AJ
Sample : N3494-17
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 00:25:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

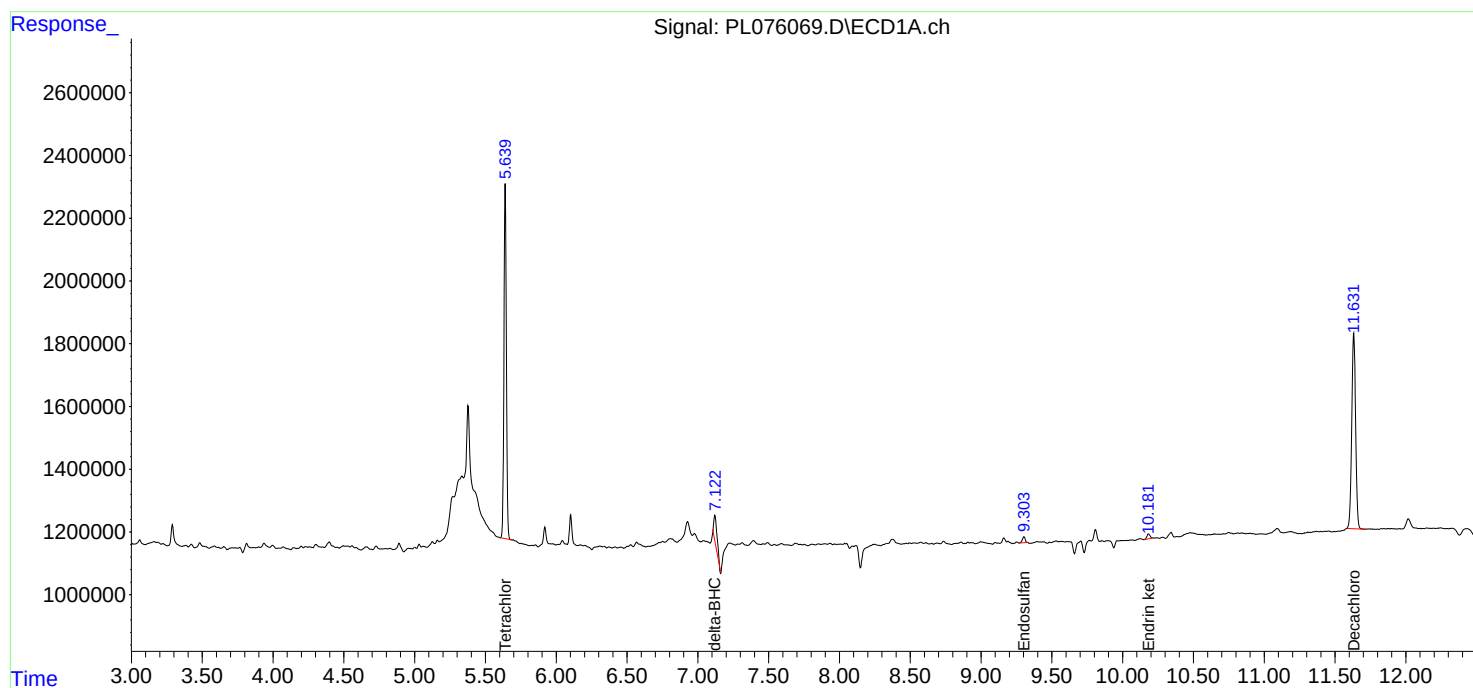


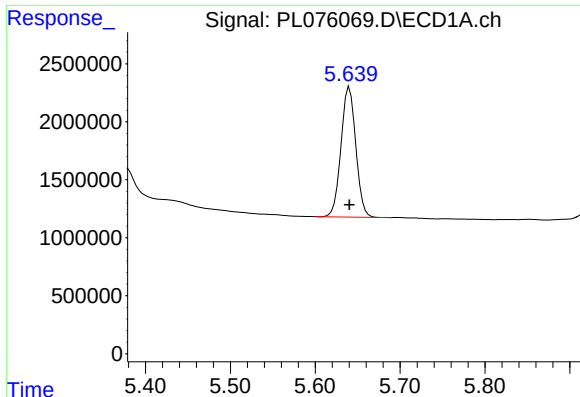

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 13539726
Conc: 17.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

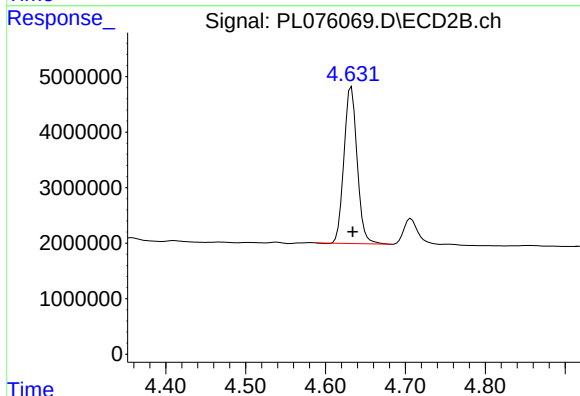


#1 Tetrachloro-m-xylene

R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 32449087
Conc: 17.11 ng/ml

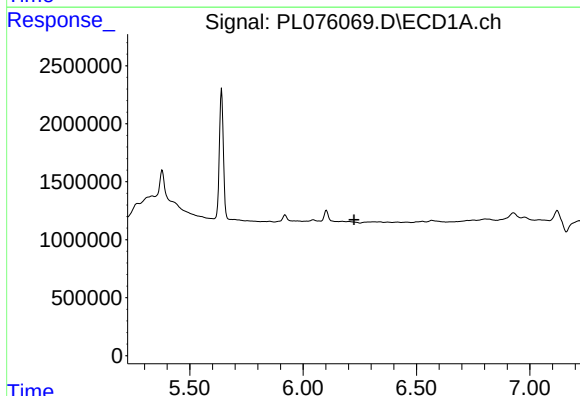


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 6.225 min
Response: 0
Conc: N.D.

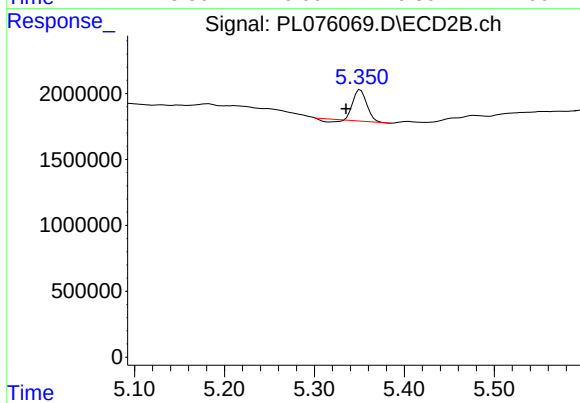

#2 alpha-BHC


R.T.: 5.351 min
Delta R.T.: 0.016 min
Response: 2353030
Conc: 0.96 ng/ml

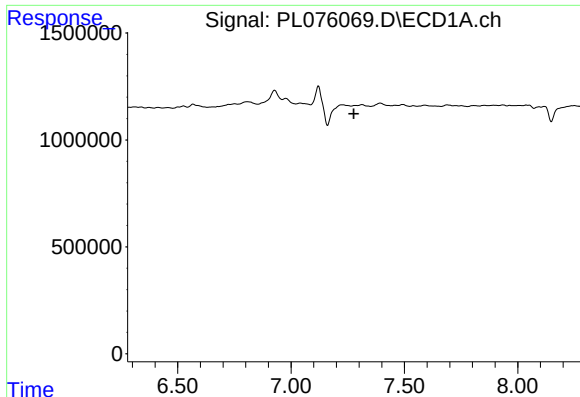

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

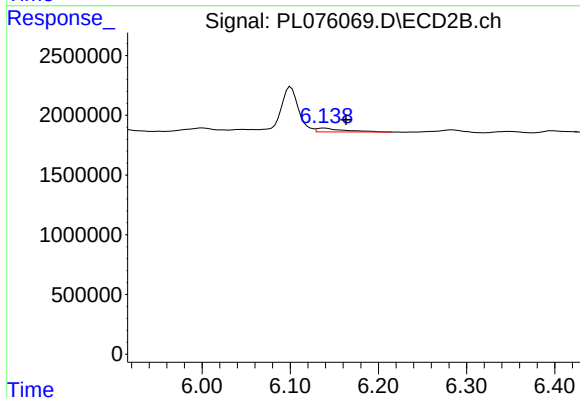


#4 Heptachlor

R.T.: 6.139 min
Delta R.T.: -0.024 min
Response: 662330
Conc: 0.29 ng/ml

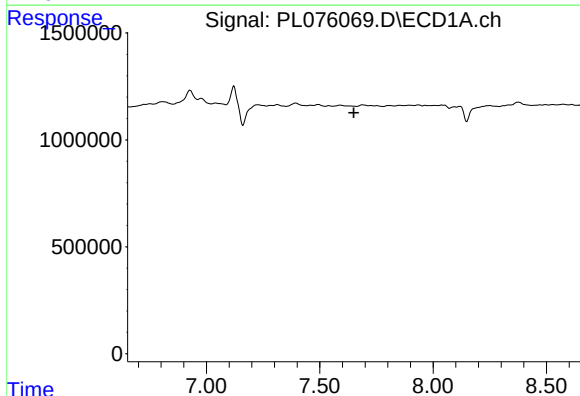


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 7.651 min
Response: 0
Conc: N.D.

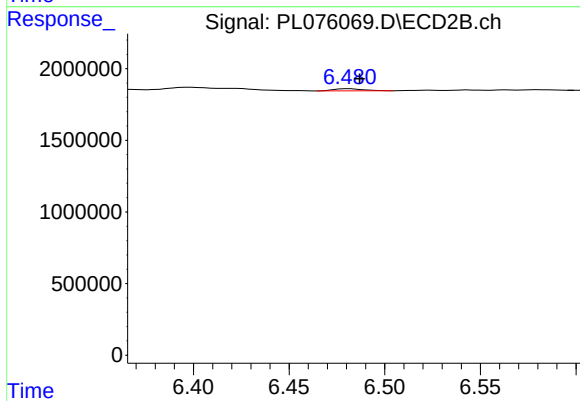

#5 Aldrin


R.T.: 6.482 min
Delta R.T.: -0.005 min
Response: 159225
Conc: 0.08 ng/ml

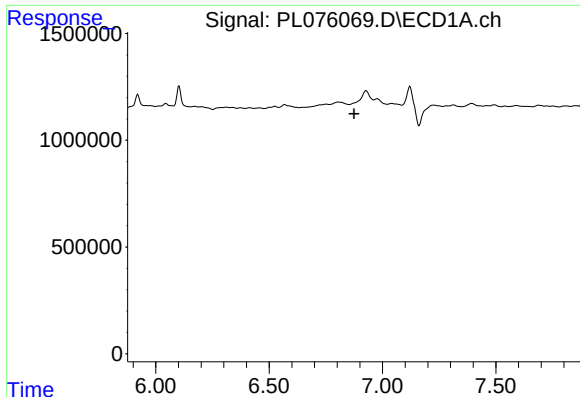

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.875 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

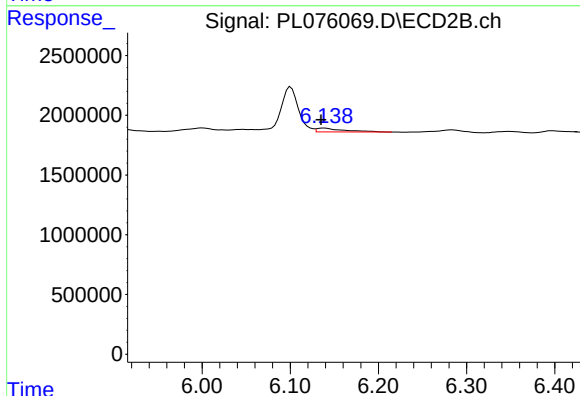


#6 beta-BHC

R.T.: 6.139 min
Delta R.T.: 0.004 min
Response: 662330
Conc: 0.63 ng/ml

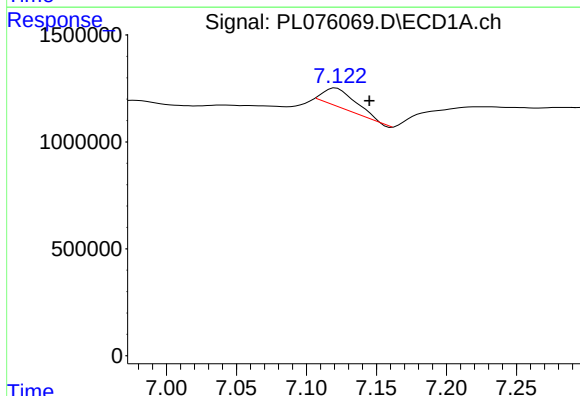


#7 delta-BHC

R.T.: 7.121 min
Delta R.T.: -0.024 min
Response: 1400569
Conc: 1.79 ng/ml

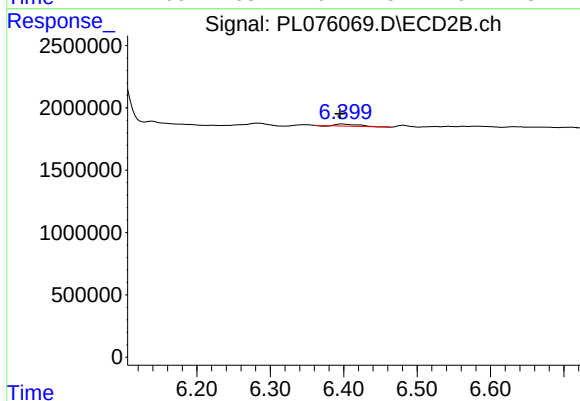

#7 delta-BHC


R.T.: 6.397 min
Delta R.T.: 0.002 min
Response: 354858
Conc: 0.16 ng/ml

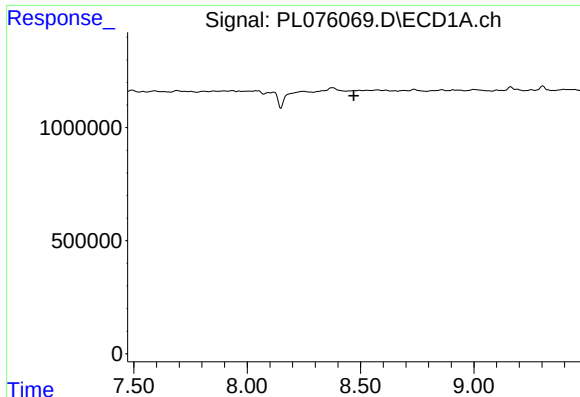

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

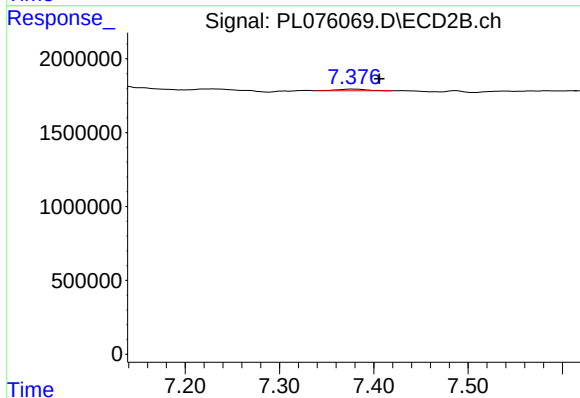


#11 alpha-Chlordane

R.T.: 7.378 min
Delta R.T.: -0.028 min
Response: 232766
Conc: 0.12 ng/ml

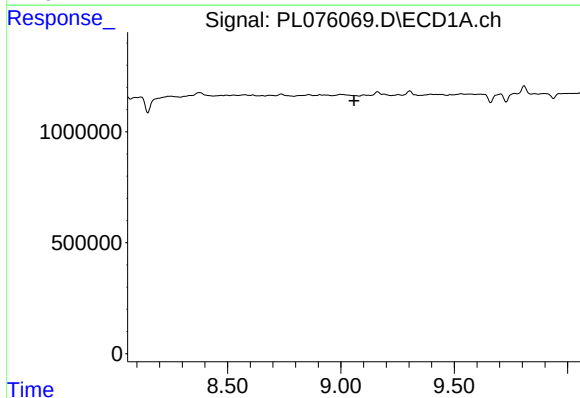


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

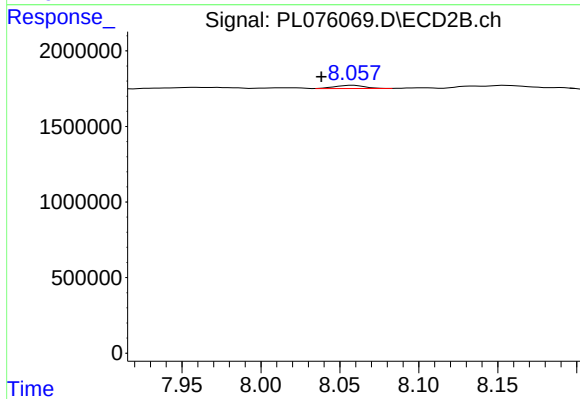

#14 Endrin


R.T.: 8.059 min
Delta R.T.: 0.020 min
Response: 275462
Conc: 0.18 ng/ml

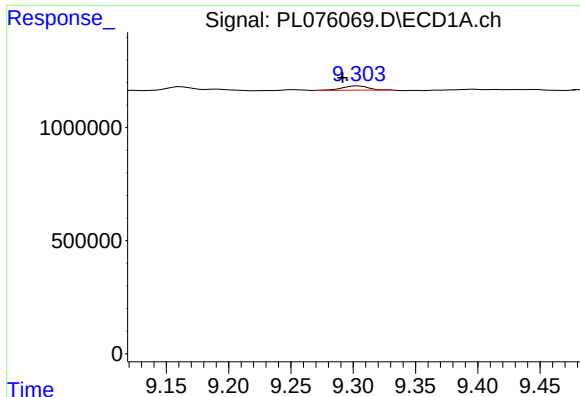

#15 Endosulfan II


R.T.: 9.304 min
Delta R.T.: 0.012 min
Response: 263604
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

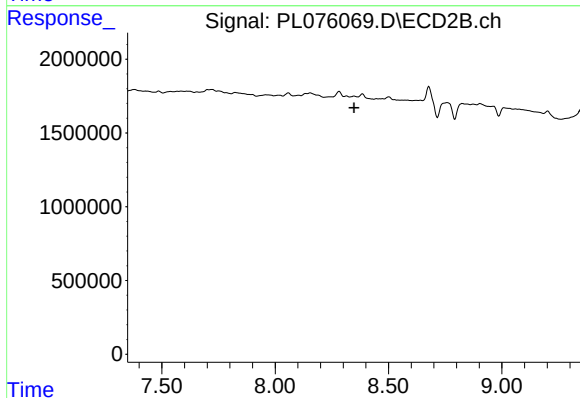


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

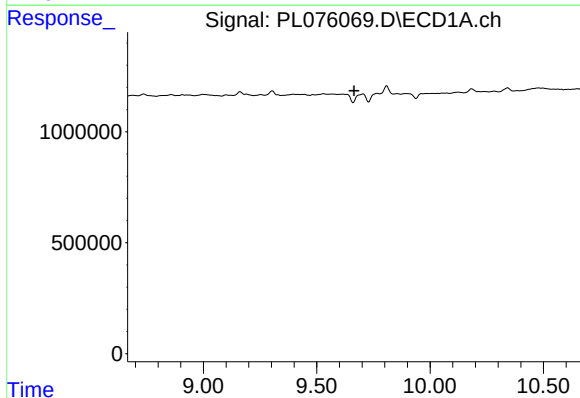


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.665 min
Response: 0
Conc: N.D.

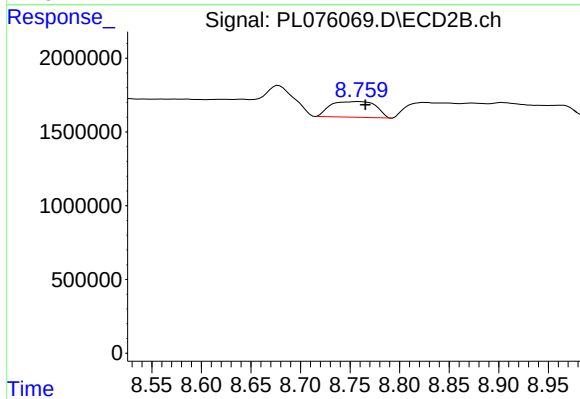

#19 Endosulfan Sulfate


R.T.: 8.759 min
Delta R.T.: -0.007 min
Response: 3386066
Conc: 2.21 ng/ml

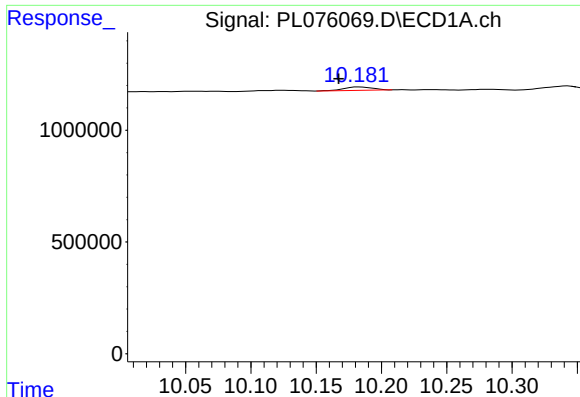

#21 Endrin ketone


R.T.: 10.183 min
Delta R.T.: 0.015 min
Response: 235575
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

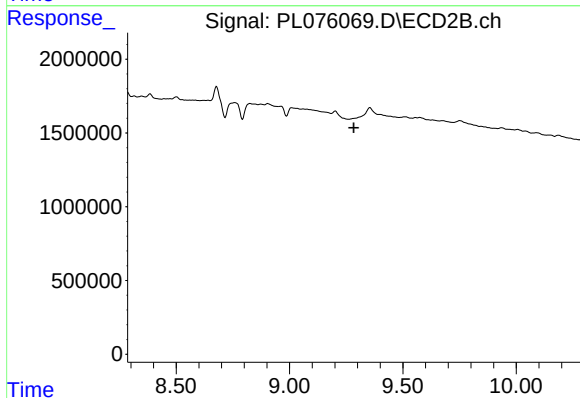


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

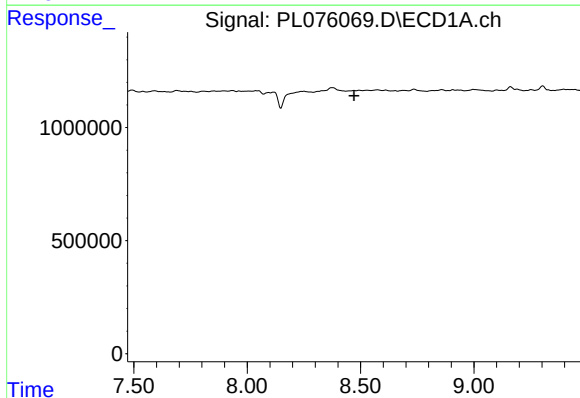


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.472 min
Response: 0
Conc: N.D.

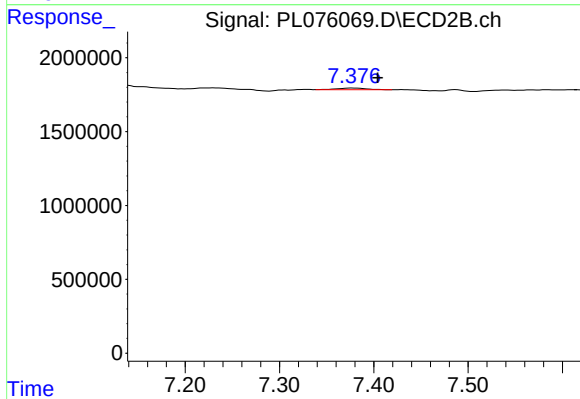

#26 Chlordane-4


R.T.: 7.378 min
Delta R.T.: -0.026 min
Response: 232766
Conc: 1.23 ng/ml

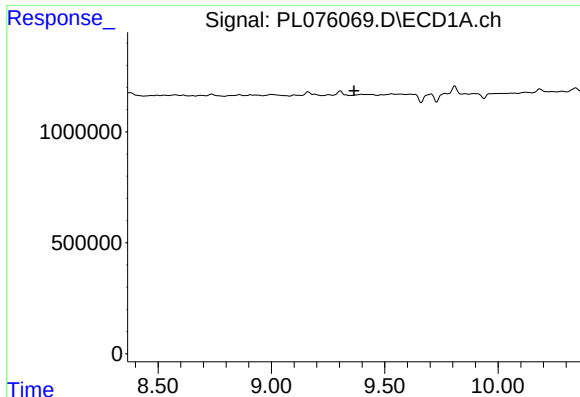

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.365 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

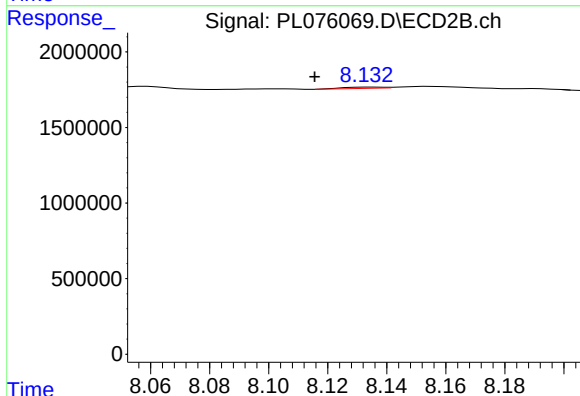


#27 Chlordane-5

R.T.: 8.135 min
Delta R.T.: 0.019 min
Response: 76858
Conc: 1.68 ng/ml

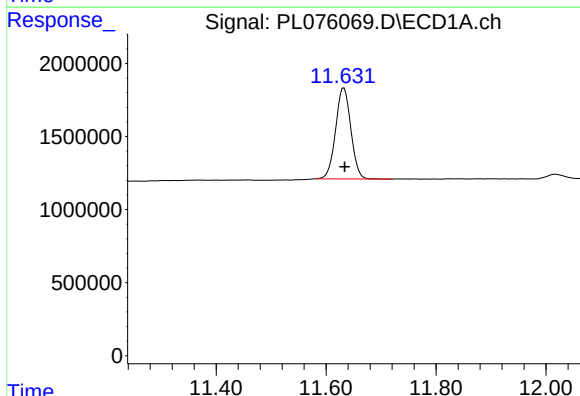

#28 Decachlorobiphenyl

R.T.: 11.632 min
Delta R.T.: -0.001 min
Response: 11993029
Conc: 19.06 ng/ml

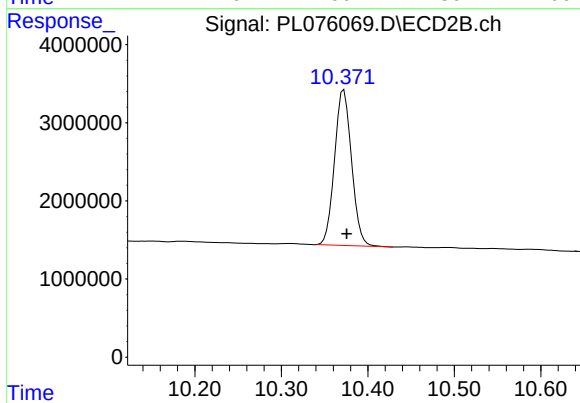

#28 Decachlorobiphenyl

R.T.: 10.372 min
Delta R.T.: -0.003 min
Response: 27016159
Conc: 17.59 ng/ml