

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062722\
 Data File : PL076071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2022 22:29
 Operator : AR\AJ
 Sample : N3494-27
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 00:26:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.633	12994583	31307298	17.181	16.507
28)	SA Decachlor...	11.633	10.372	10411409	23468699	16.545	15.280
Target Compounds							
3)	MA gamma-BHC...	0.000	5.748	0	459605	N.D.	0.199 #
5)	MB Aldrin	0.000	6.481	0	176332	N.D.	0.085 #
7)	B delta-BHC	7.121f	6.401	2215248	346517	2.837	0.153 #
10)	B gamma-Chl...	8.381	0.000	263291	0	0.339	N.D. #
13)	MA Dieldrin	0.000	7.722f	0	159440	N.D.	0.089 #
14)	MA Endrin	0.000	8.057f	0	255705	N.D.	0.168 #
15)	B Endosulfa...	9.304	0.000	295989	0	0.467	N.D. #
19)	B Endosulfa...	0.000	8.758	0	992873	N.D.	0.647 #
21)	B Endrin ke...	10.182	0.000	233342	0	0.324	N.D. #
23)	Chlordane-1	0.000	5.979f	0	346362	N.D.	6.186 #
25)	Chlordane-3	8.381	0.000	263291	0	2.589	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062722\
Data File : PL076071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2022 22:29
Operator : AR\AJ
Sample : N3494-27
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 00:26:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

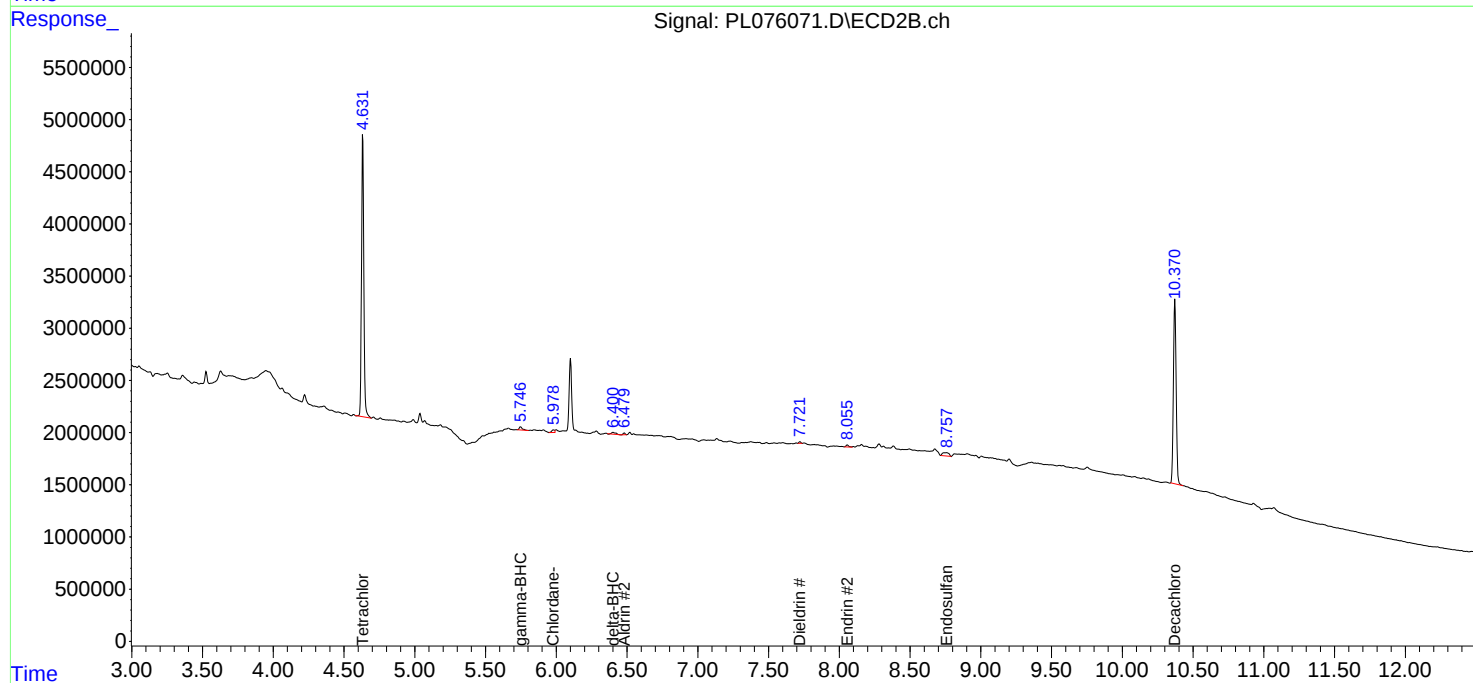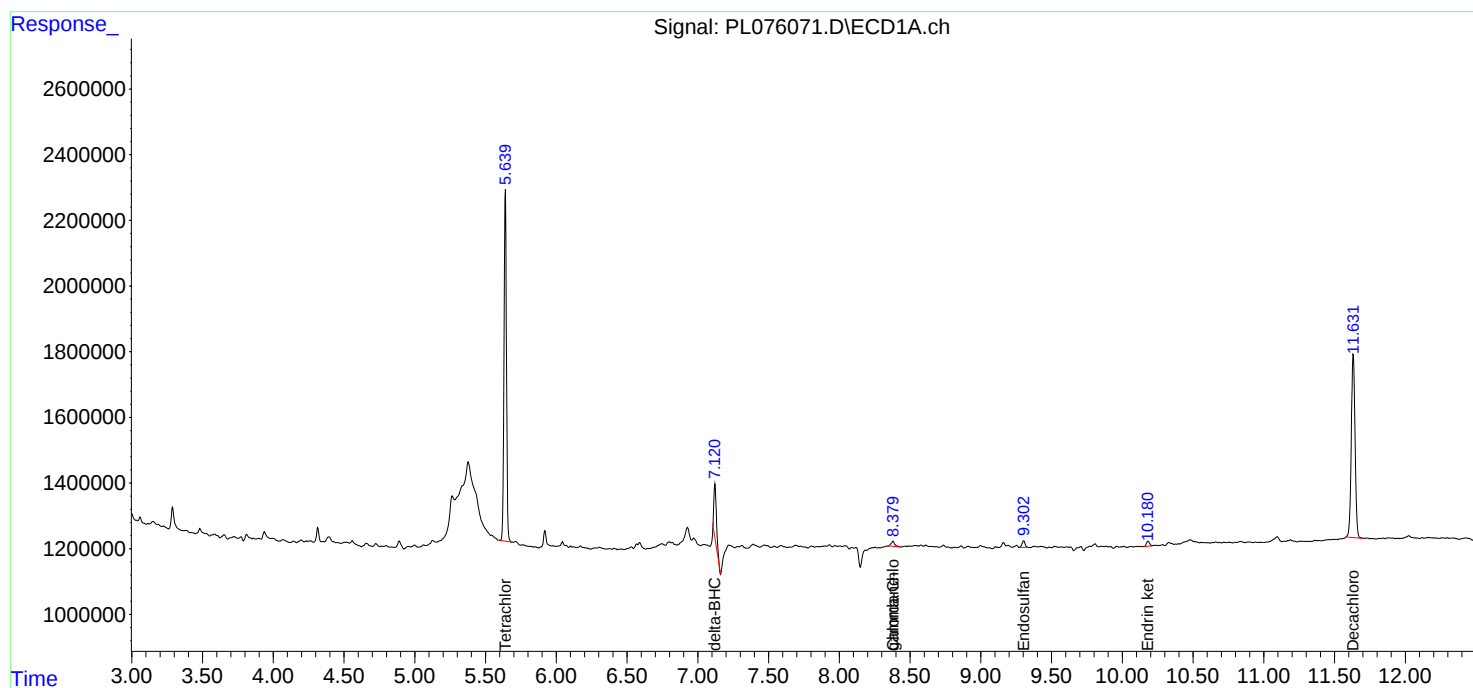


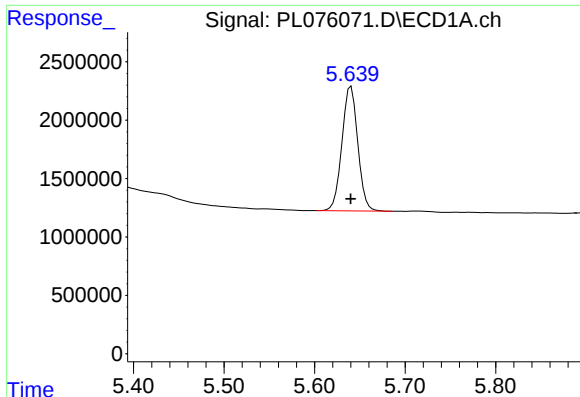

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 12994583
Conc: 17.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

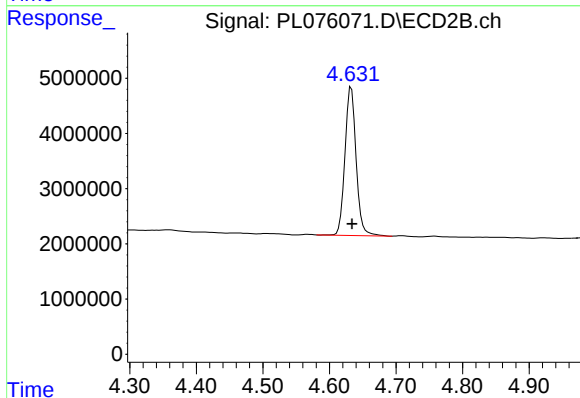


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: -0.001 min
Response: 31307298
Conc: 16.51 ng/ml

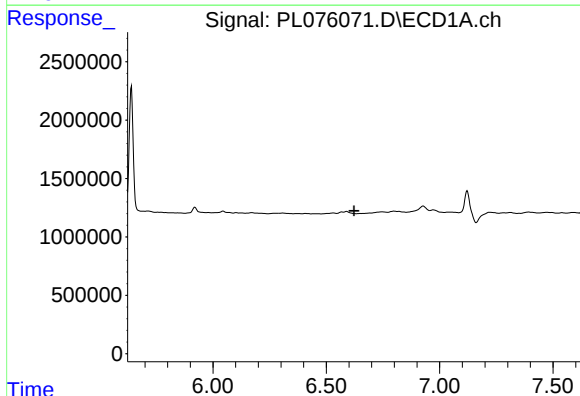


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.623 min
Response: 0
Conc: N.D.

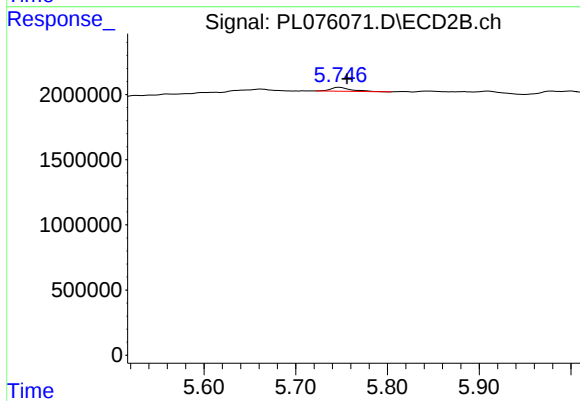

#3 gamma-BHC (Lindane)


R.T.: 5.748 min
Delta R.T.: -0.008 min
Response: 459605
Conc: 0.20 ng/ml

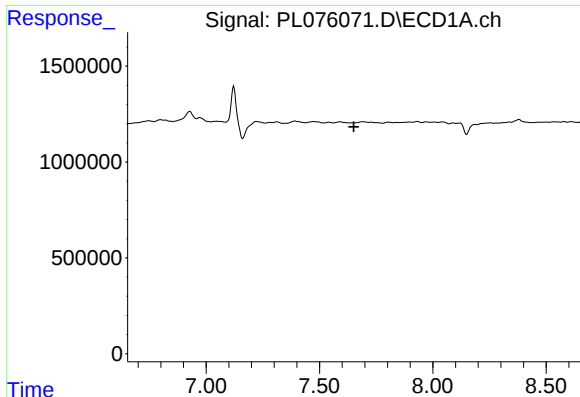

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 7.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

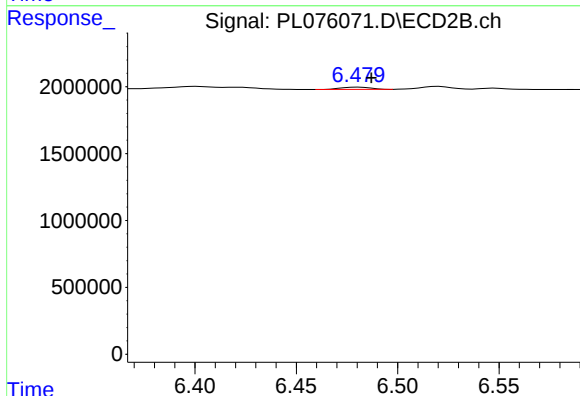


#5 Aldrin

R.T.: 6.481 min
Delta R.T.: -0.006 min
Response: 176332
Conc: 0.09 ng/ml

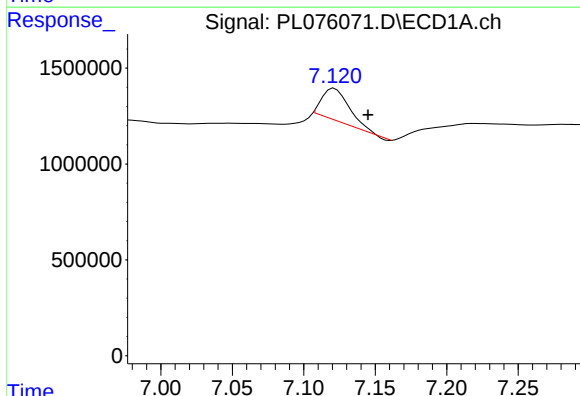


#7 delta-BHC

R.T.: 7.121 min
Delta R.T.: -0.024 min
Response: 2215248
Conc: 2.84 ng/ml

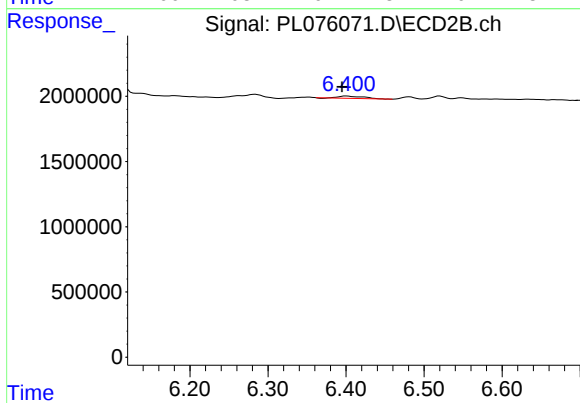

#7 delta-BHC


R.T.: 6.401 min
Delta R.T.: 0.005 min
Response: 346517
Conc: 0.15 ng/ml

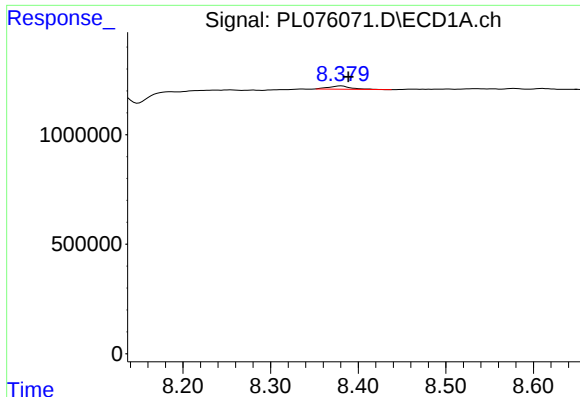

#10 gamma-Chlordane


R.T.: 8.381 min
Delta R.T.: -0.008 min
Response: 263291
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

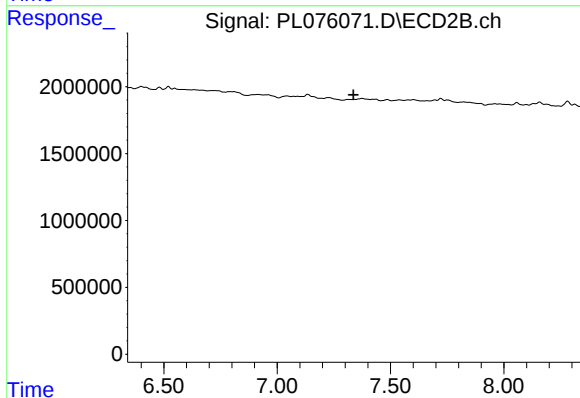


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.337 min
Response: 0
Conc: N.D.

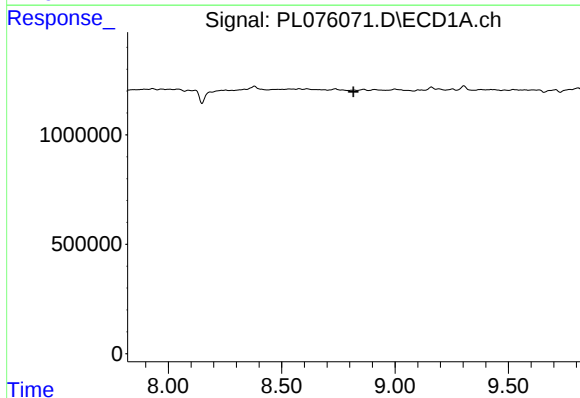


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.817 min
Response: 0
Conc: N.D.

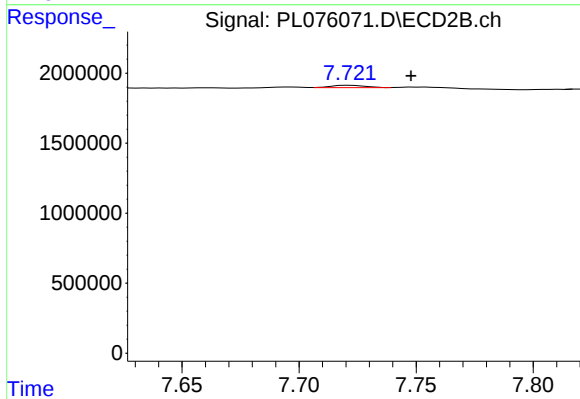

#13 Dieldrin


R.T.: 7.722 min
Delta R.T.: -0.026 min
Response: 159440
Conc: 0.09 ng/ml

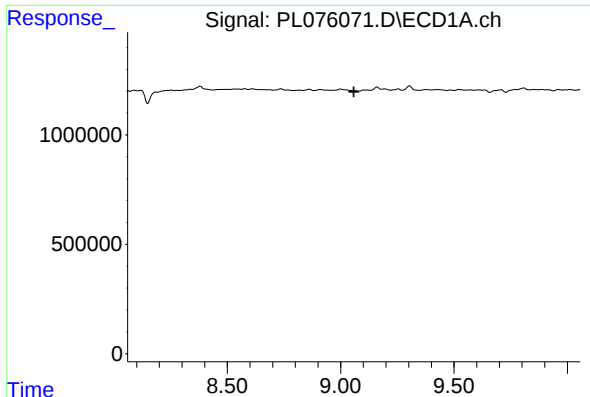

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

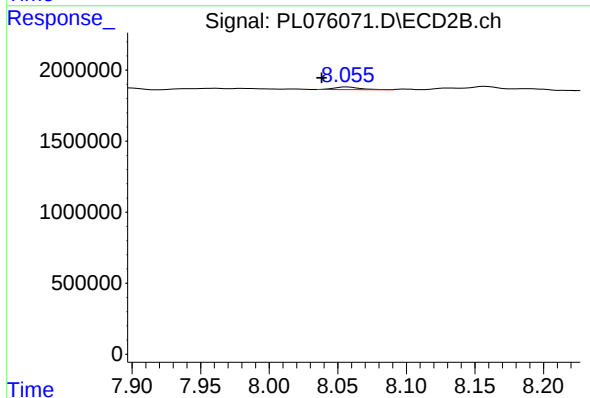


#14 Endrin

R.T.: 8.057 min
Delta R.T.: 0.018 min
Response: 255705
Conc: 0.17 ng/ml

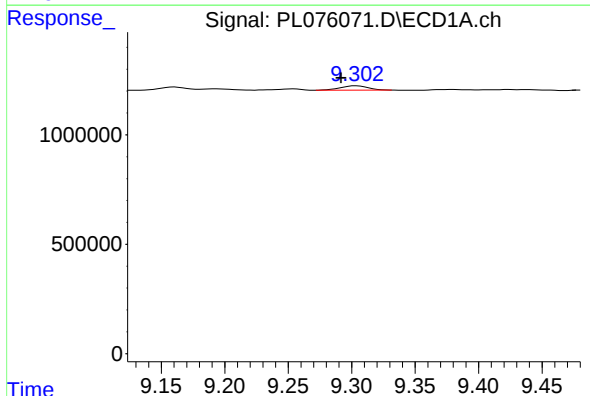


#15 Endosulfan II

R.T.: 9.304 min
Delta R.T.: 0.012 min
Response: 295989
Conc: 0.47 ng/ml

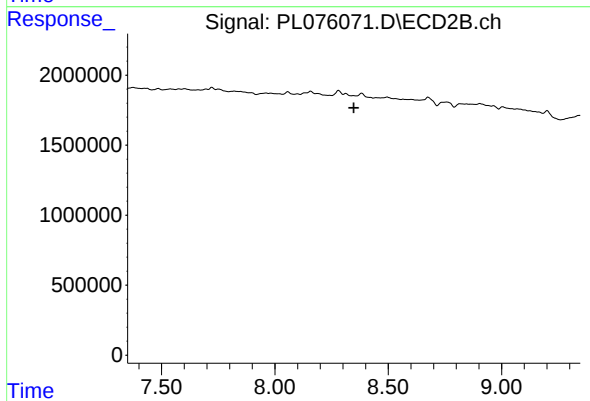

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.349 min
Response: 0
Conc: N.D.

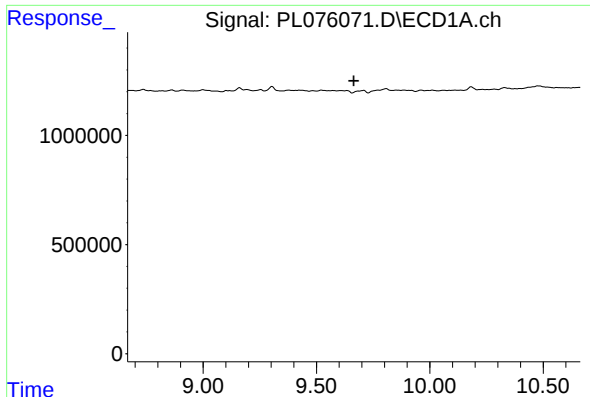

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.665 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

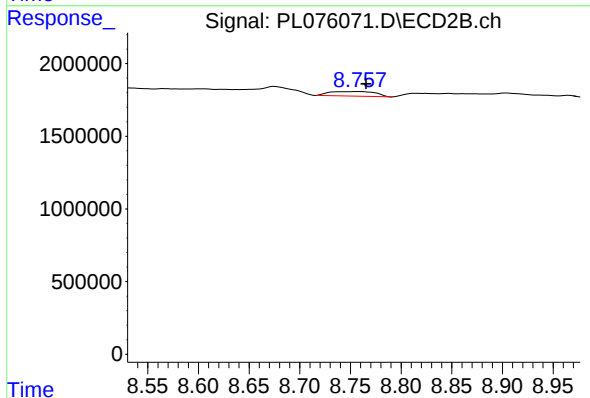


#19 Endosulfan Sulfate

R.T.: 8.758 min
Delta R.T.: -0.008 min
Response: 992873
Conc: 0.65 ng/ml

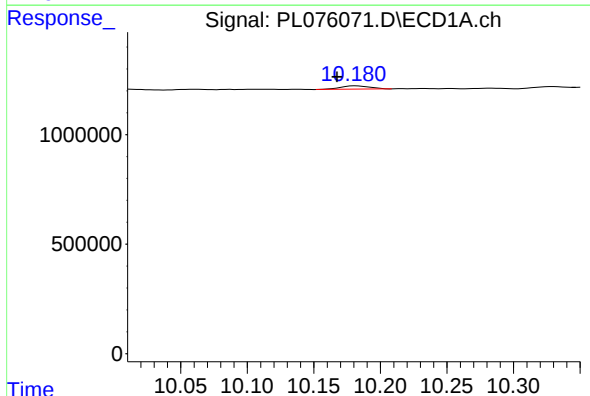


#21 Endrin ketone

R.T.: 10.182 min
Delta R.T.: 0.015 min
Response: 233342
Conc: 0.32 ng/ml

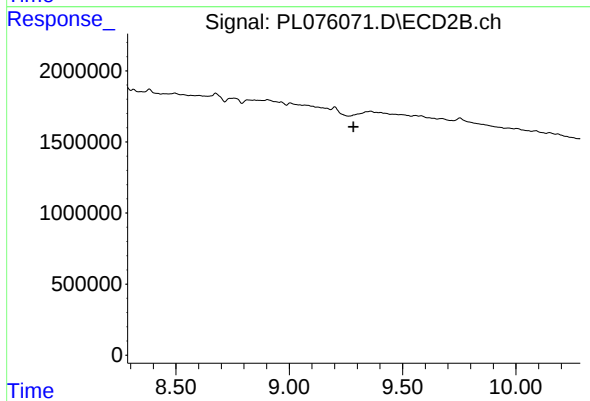

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.284 min
Response: 0
Conc: N.D.

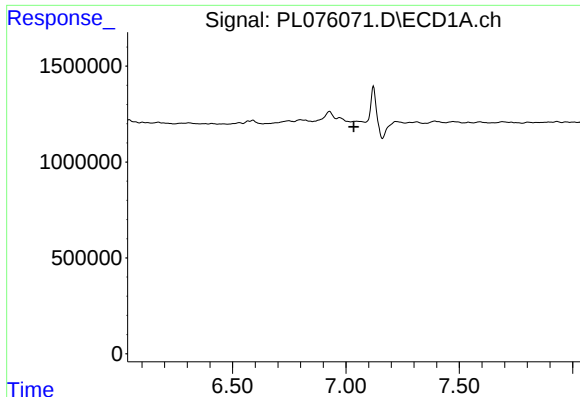

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 7.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

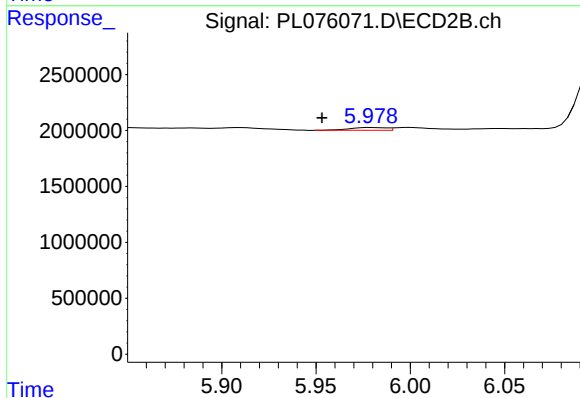


#23 Chlordane-1

R.T.: 5.979 min
Delta R.T.: 0.026 min
Response: 346362
Conc: 6.19 ng/ml

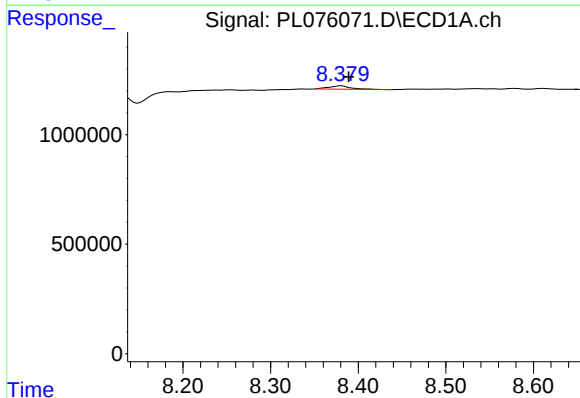


#25 Chlordane-3

R.T.: 8.381 min
Delta R.T.: -0.008 min
Response: 263291
Conc: 2.59 ng/ml

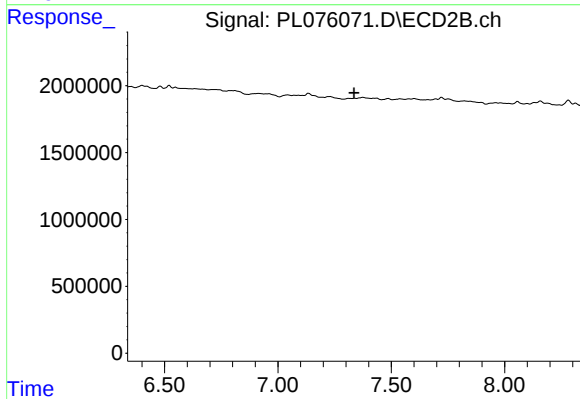

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.337 min
Response: 0
Conc: N.D.

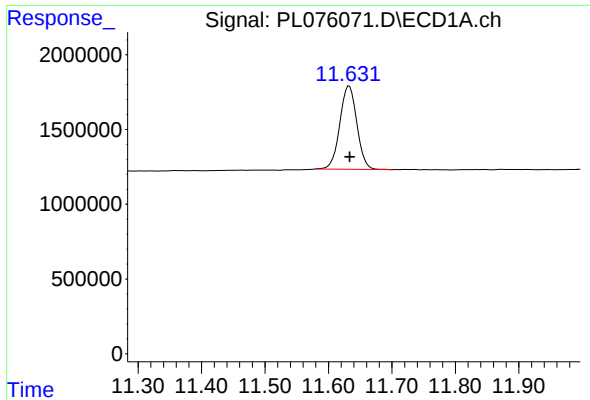

#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: 0.000 min
Response: 10411409
Conc: 16.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

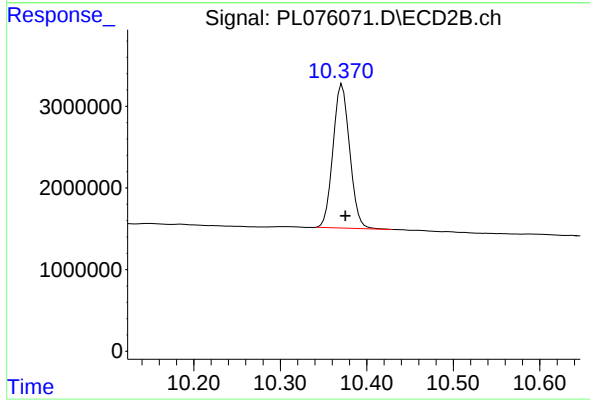

#28 Decachlorobiphenyl

R.T.: 10.372 min
Delta R.T.: -0.004 min
Response: 23468699
Conc: 15.28 ng/ml