

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062722\
 Data File : PL076073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2022 23:02
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 00:26:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.632	15301065	38233385	20.231	20.159
28)	SA Decachlor...	11.632	10.372	13930575	31790344	22.138	20.698
Target Compounds							
4)	MA Heptachlor	0.000	6.140f	0	105561	N.D.	0.047 #
6)	B beta-BHC	0.000	6.140	0	105561	N.D.	0.101 #
7)	B delta-BHC	0.000	6.397	0	417396	N.D.	0.185 #
13)	MA Dieldrin	0.000	7.744	0	252382	N.D.	0.140 #
14)	MA Endrin	0.000	8.058f	0	479136	N.D.	0.315 #
15)	B Endosulfa...	9.302	0.000	237262	0	0.374	N.D. #
17)	MA 4,4'-DDT	0.000	8.455	0	32446	N.D.	0.022 #
21)	B Endrin ke...	10.182	0.000	236016	0	0.327	N.D. #
24)	Chlordane-2	0.000	6.664f	0	1016253	N.D.	14.615 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062722\
Data File : PL076073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2022 23:02
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 00:26:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

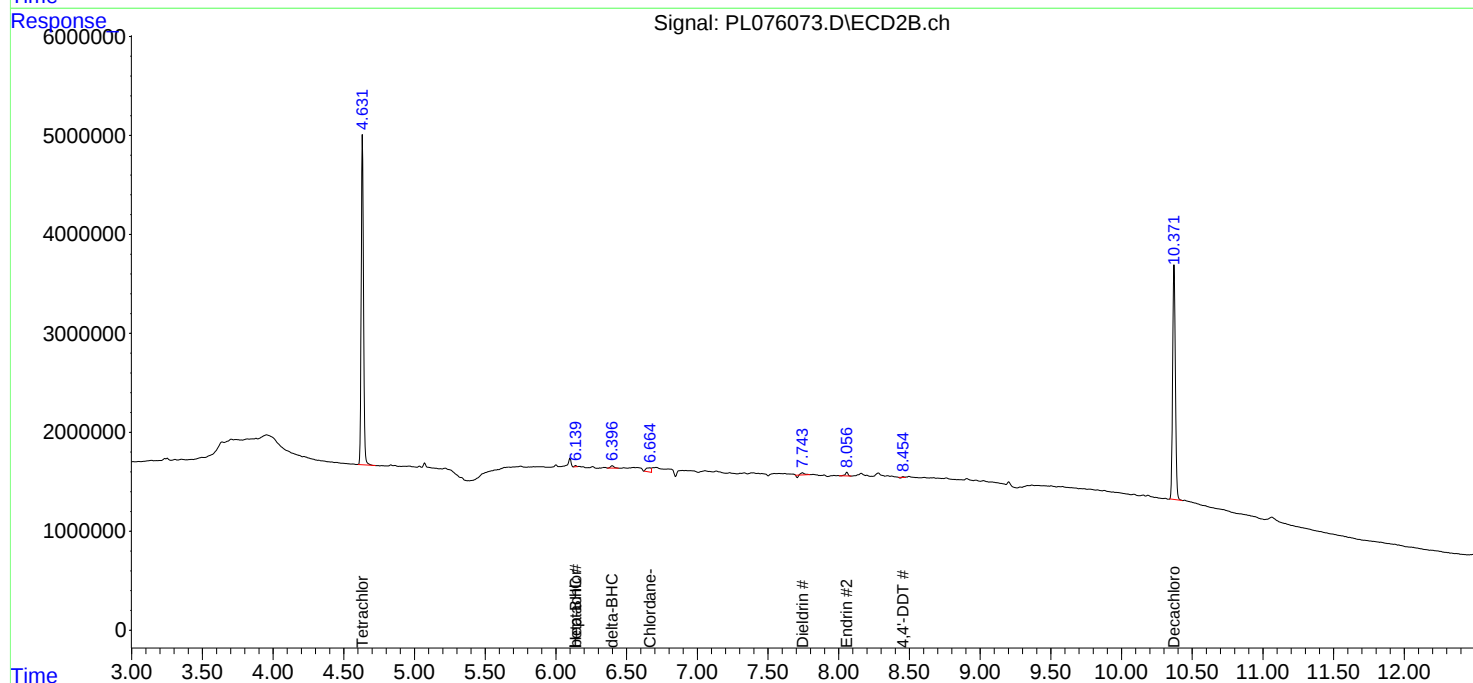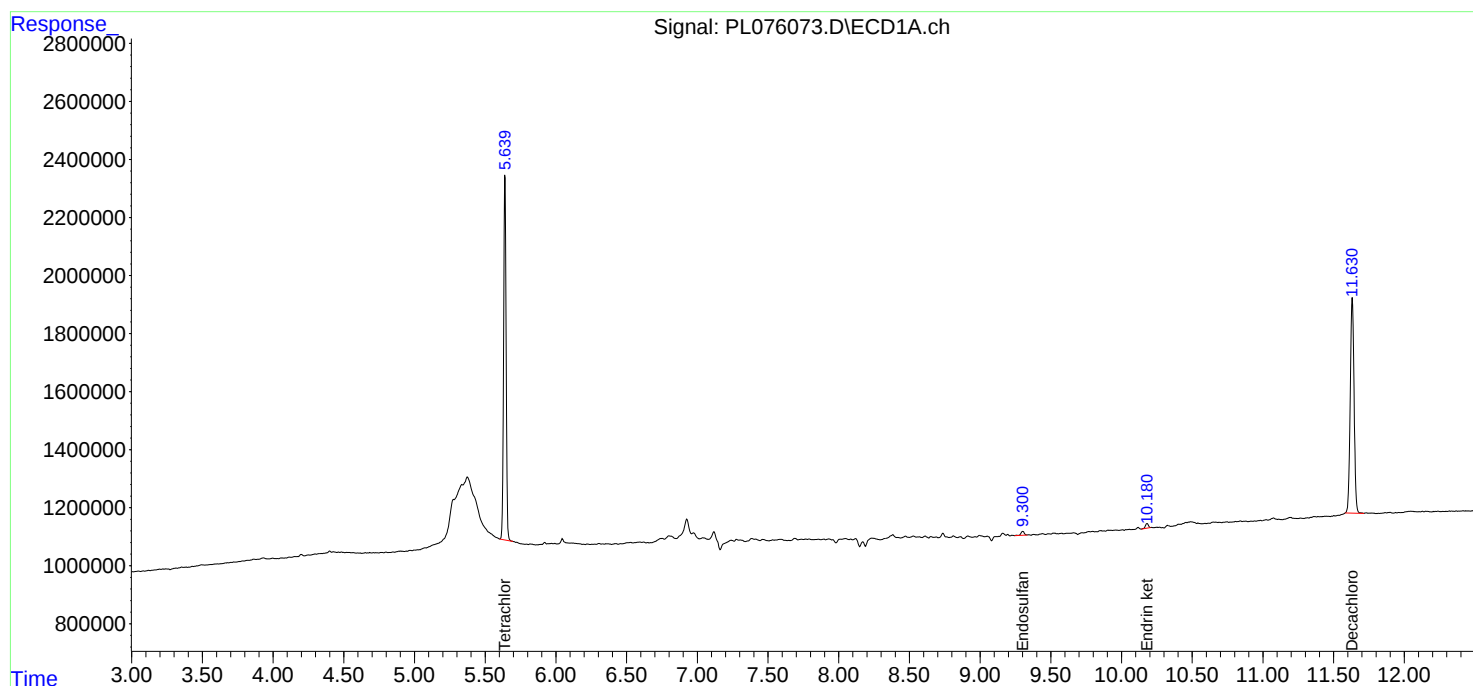


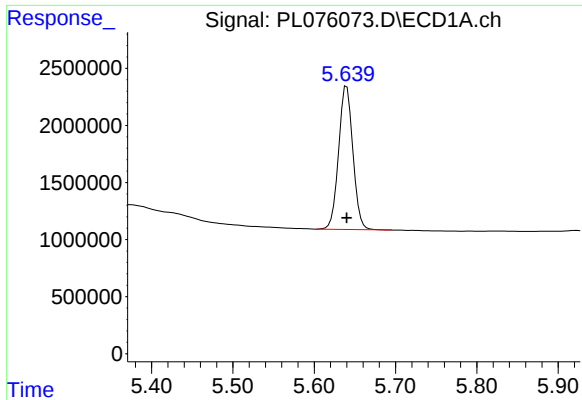

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 15301065
Conc: 20.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

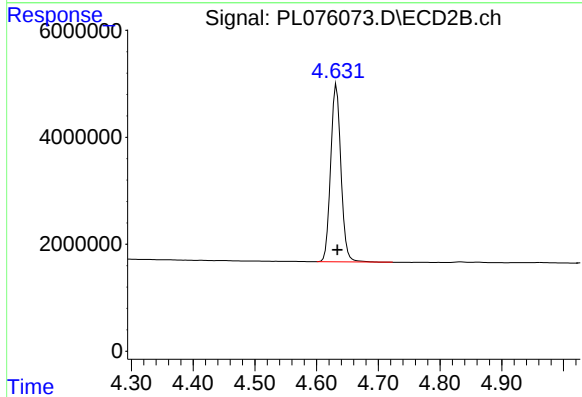


#1 Tetrachloro-m-xylene

R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 38233385
Conc: 20.16 ng/ml

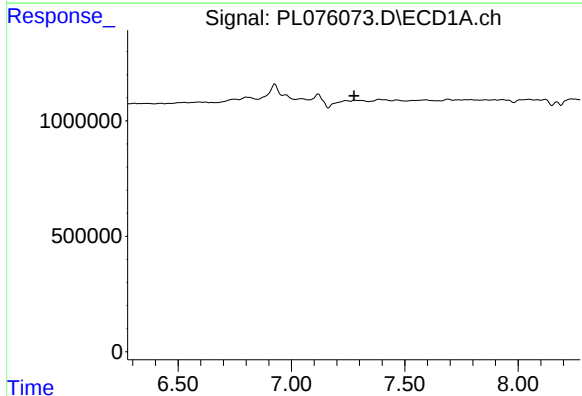


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.277 min
Response: 0
Conc: N.D.

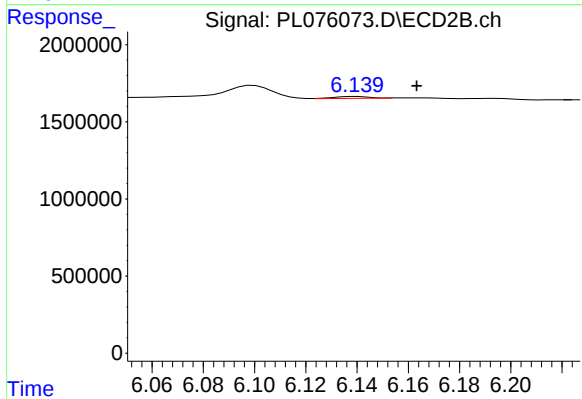

#4 Heptachlor


R.T.: 6.140 min
Delta R.T.: -0.023 min
Response: 105561
Conc: 0.05 ng/ml

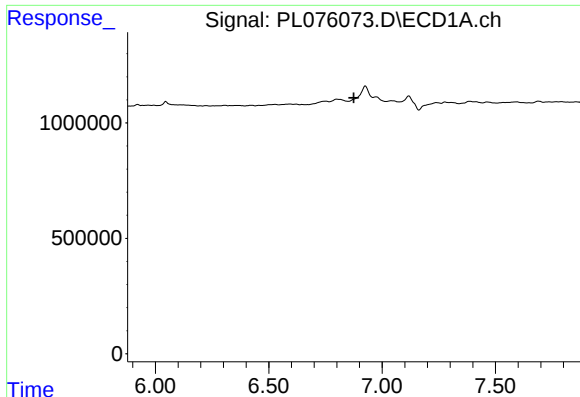

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.875 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

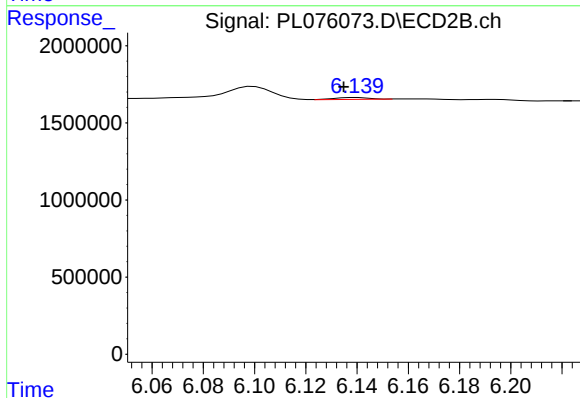


#6 beta-BHC

R.T.: 6.140 min
Delta R.T.: 0.005 min
Response: 105561
Conc: 0.10 ng/ml

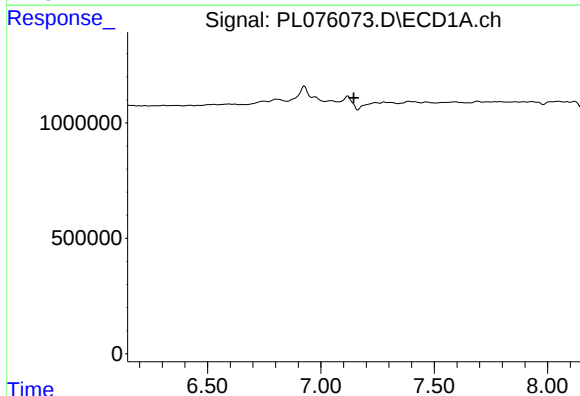


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

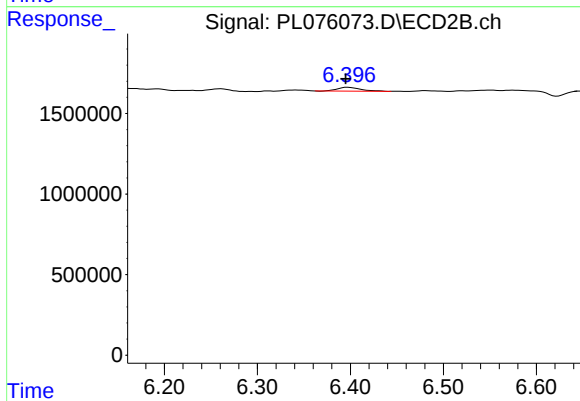

#7 delta-BHC


R.T.: 6.397 min
Delta R.T.: 0.002 min
Response: 417396
Conc: 0.18 ng/ml

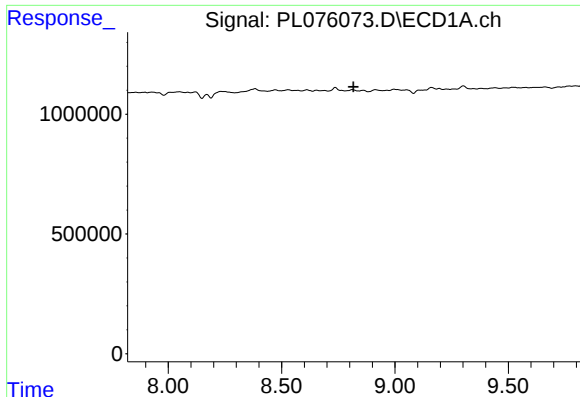

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

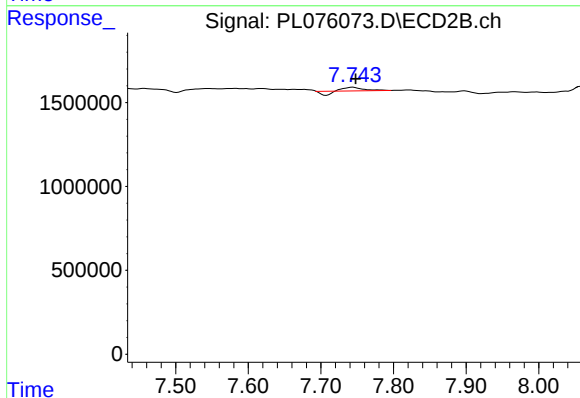


#13 Dieldrin

R.T.: 7.744 min
Delta R.T.: -0.003 min
Response: 252382
Conc: 0.14 ng/ml

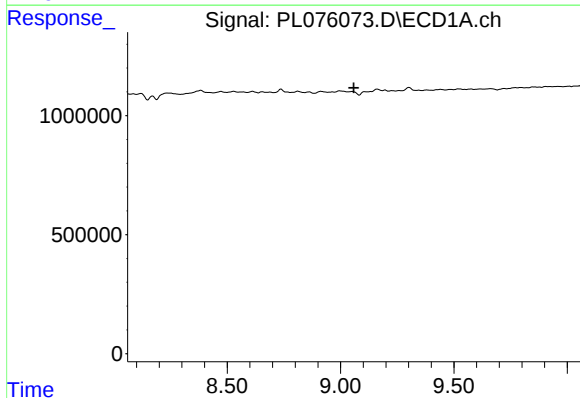


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.058 min
Response: 0
Conc: N.D.

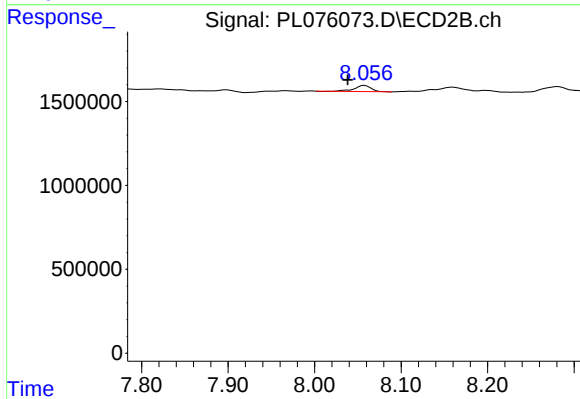

#14 Endrin


R.T.: 8.058 min
Delta R.T.: 0.019 min
Response: 479136
Conc: 0.32 ng/ml

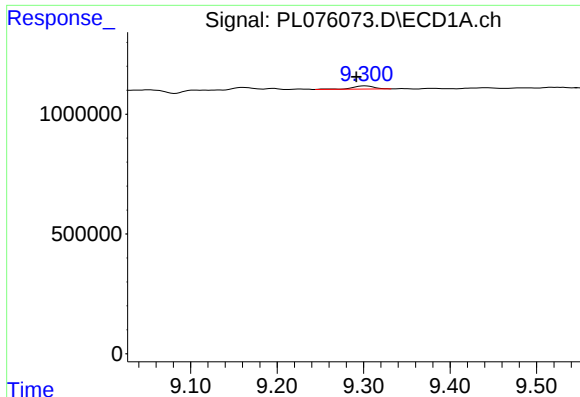

#15 Endosulfan II


R.T.: 9.302 min
Delta R.T.: 0.010 min
Response: 237262
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

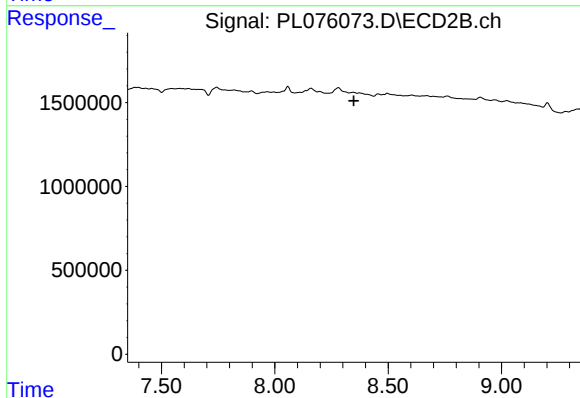


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

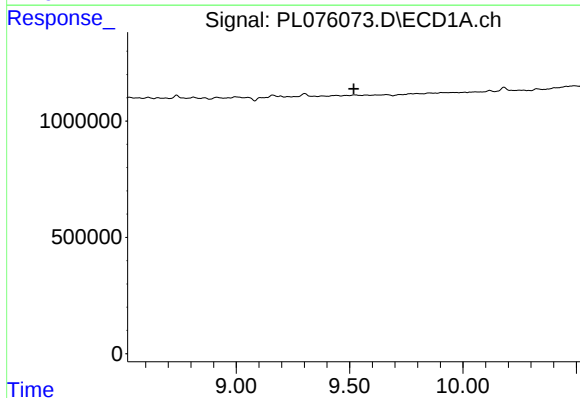


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.518 min
Response: 0
Conc: N.D.

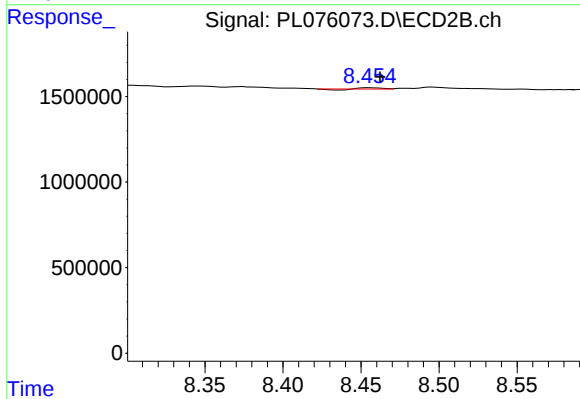

#17 4,4'-DDT


R.T.: 8.455 min
Delta R.T.: -0.007 min
Response: 32446
Conc: 0.02 ng/ml

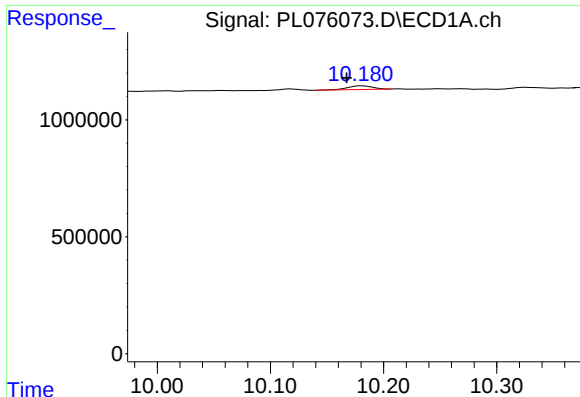

#21 Endrin ketone


R.T.: 10.182 min
Delta R.T.: 0.014 min
Response: 236016
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

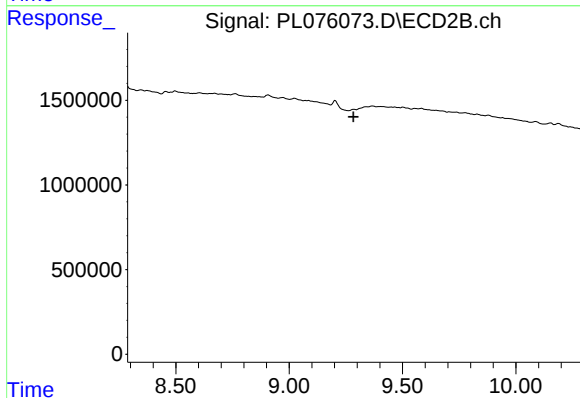


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

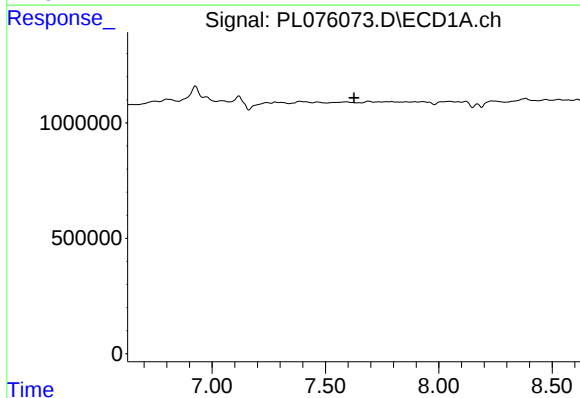


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.627 min
Response: 0
Conc: N.D.

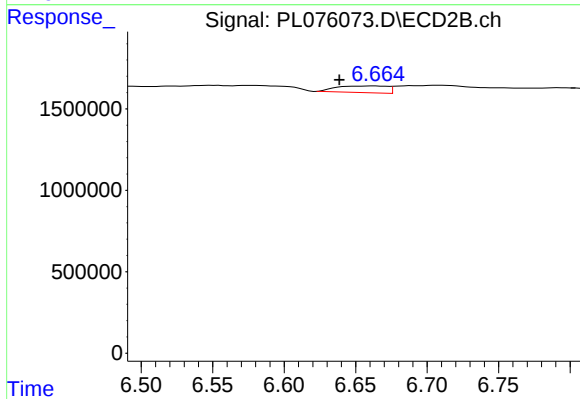

#24 Chlordane-2


R.T.: 6.664 min
Delta R.T.: 0.026 min
Response: 1016253
Conc: 14.61 ng/ml

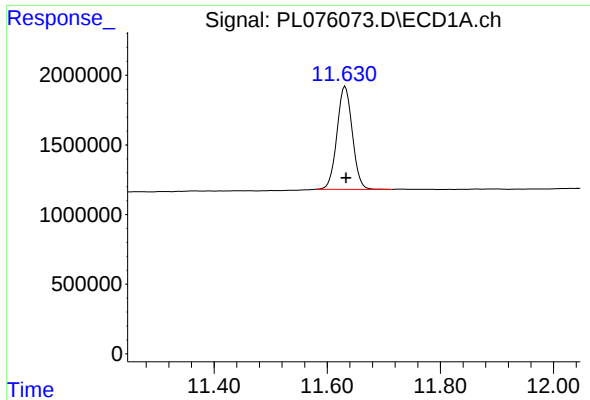

#28 Decachlorobiphenyl

R.T.: 11.632 min
Delta R.T.: -0.002 min
Response: 13930575
Conc: 22.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

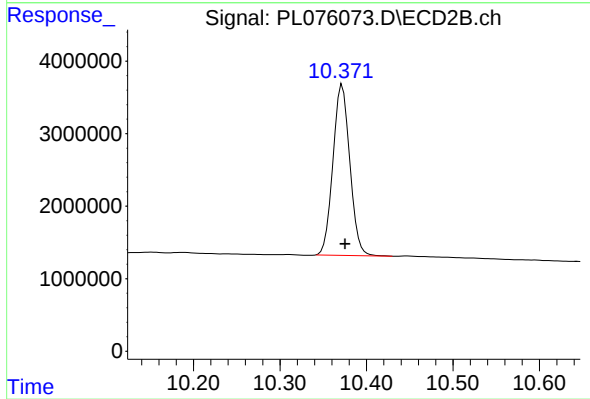

#28 Decachlorobiphenyl

R.T.: 10.372 min
Delta R.T.: -0.003 min
Response: 31790344
Conc: 20.70 ng/ml