

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062725\
 Data File : PL096192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2025 12:17
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 23:14:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062625.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 26 18:02:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	5.718	0.000	33350191	0	8.576 N.D. #
9) A	Endosulfan I	6.098	0.000	13439920	0	3.714 N.D. #
10) B	gamma-Chl...	5.973	0.000	11213704	0	2.902 N.D. #
13) MA	Dieldrin	0.000	5.494	0 35885947	N.D.	6.160 #
14) MA	Endrin	0.000	5.785	0 24544553	N.D.	4.603 #
15) B	Endosulfa...	6.796	0.000	6268996	0	1.767 N.D. #
18) B	Endrin al...	6.920f	0.000	3820626	0	1.575 N.D. #
24)	Chlordane-2	0.000	4.469	0 10318618	N.D.	46.219 #
25)	Chlordane-3	5.973	0.000	11213704	0	16.793 N.D. #
27)	Chlordane-5	6.920f	0.000	3820626	0	26.000 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062725\
Data File : PL096192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2025 12:17
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 23:14:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062625.M
Quant Title : GC Extractables
QLast Update : Thu Jun 26 18:02:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

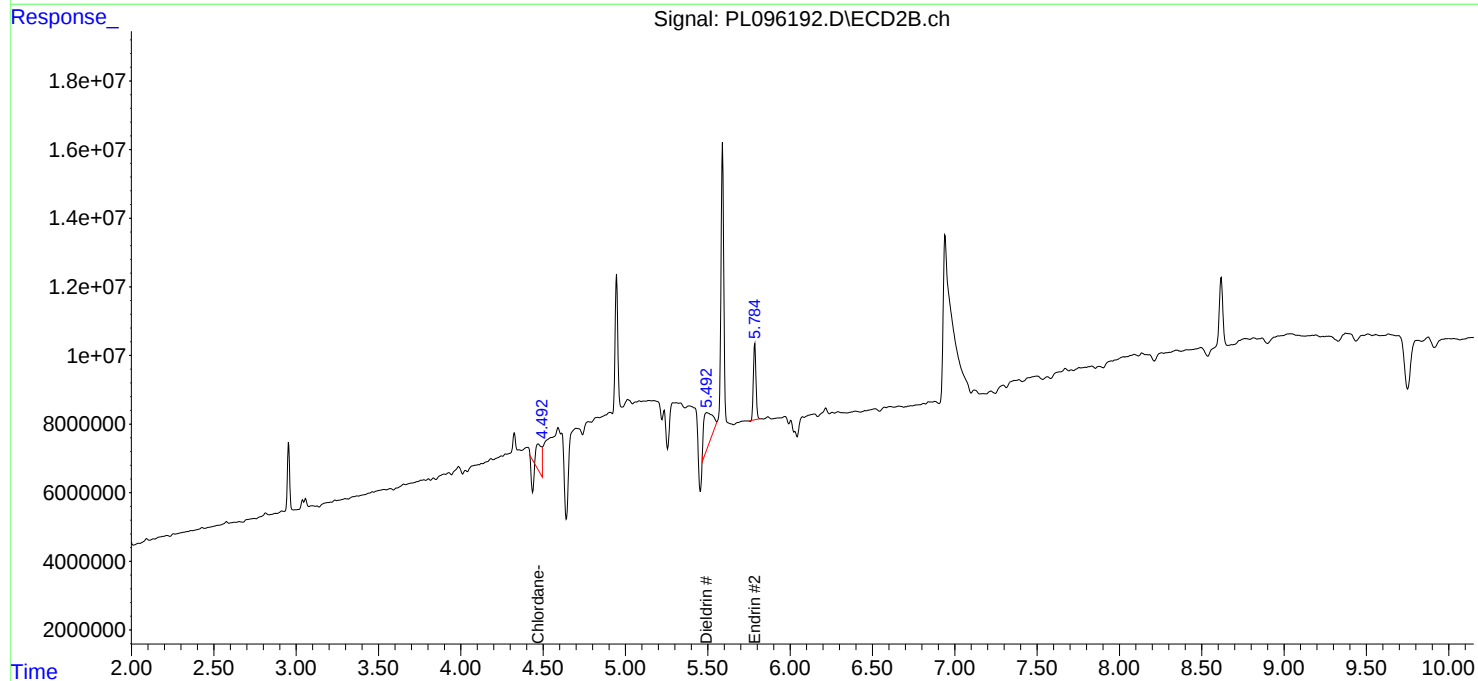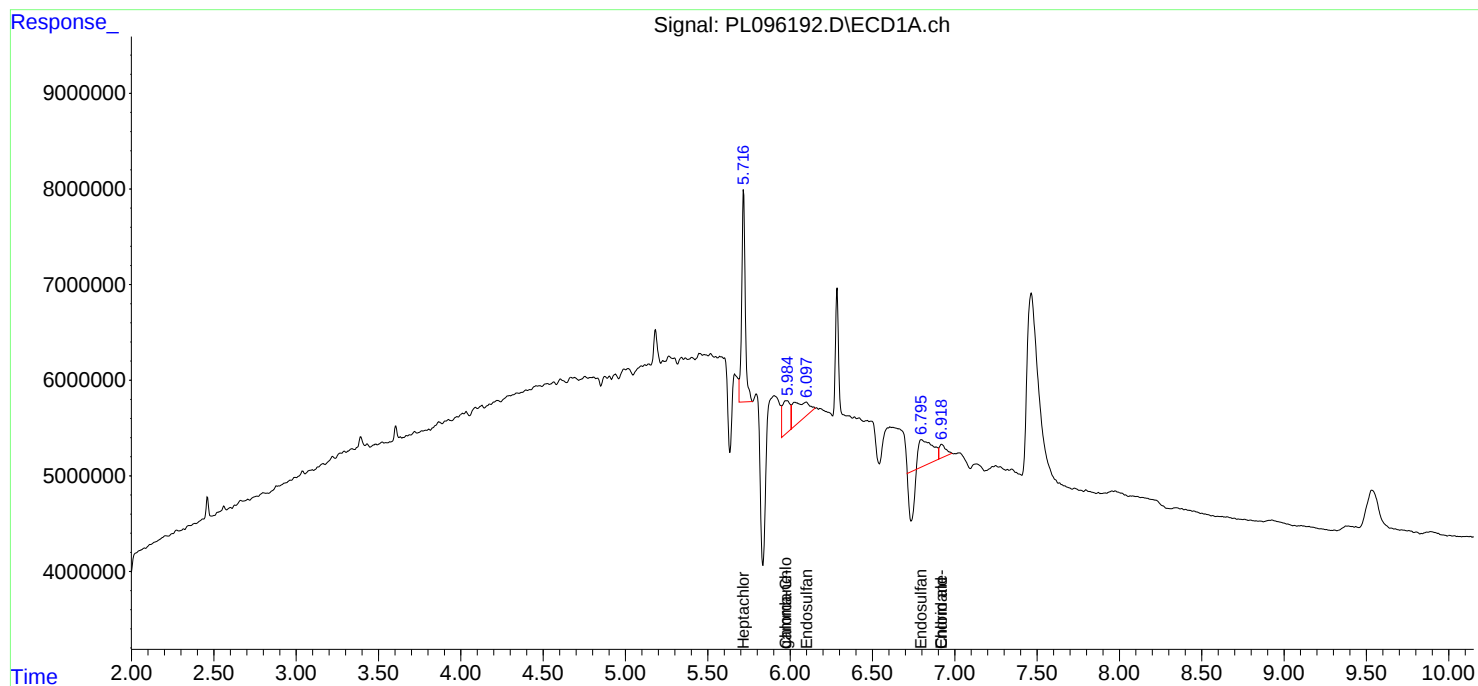


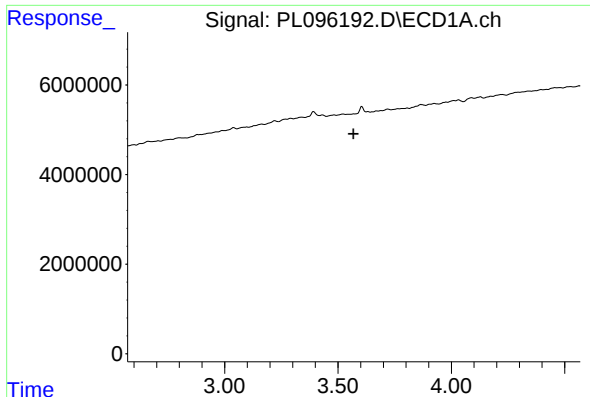

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

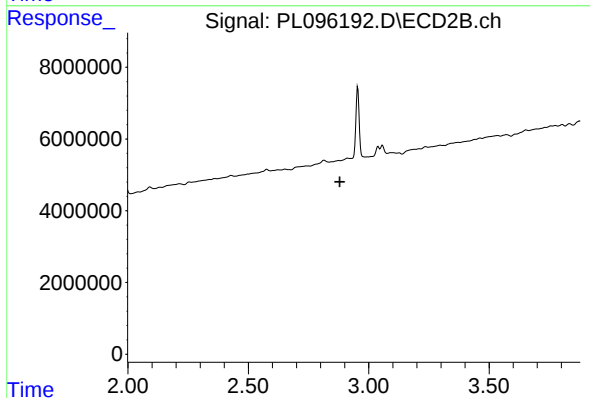


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

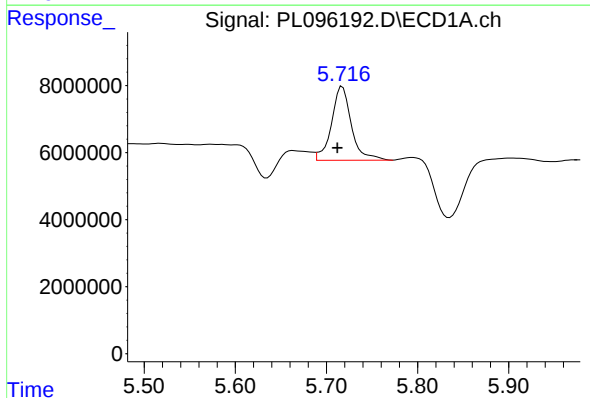


#8 Heptachlor epoxide

R.T.: 5.718 min
Delta R.T.: 0.005 min
Response: 33350191
Conc: 8.58 ng/ml

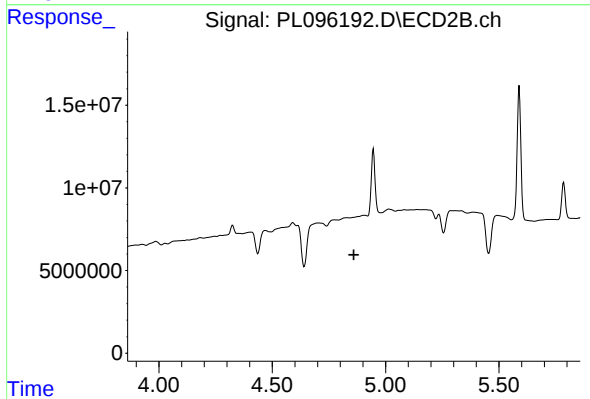

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.860 min
Response: 0
Conc: N.D.

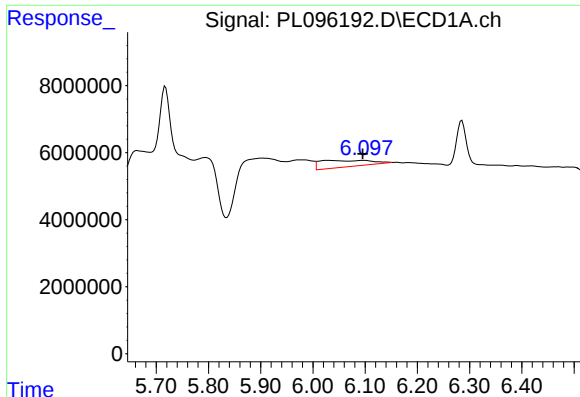

#9 Endosulfan I


R.T.: 6.098 min
Delta R.T.: 0.003 min
Response: 13439920
Conc: 3.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

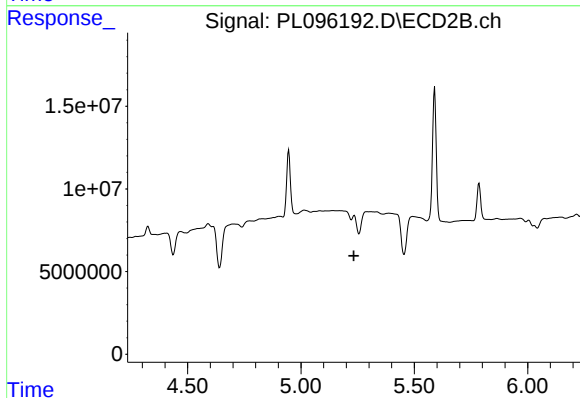


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.233 min
Response: 0
Conc: N.D.

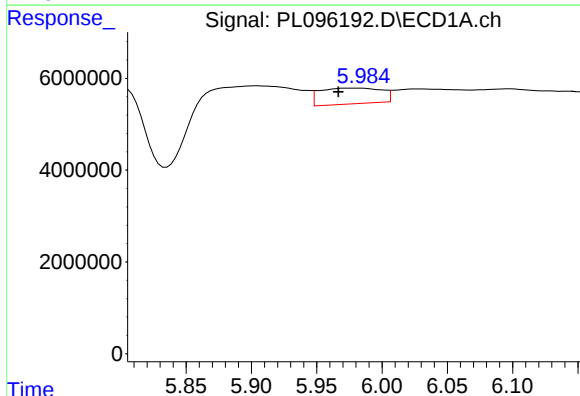


#10 gamma-Chlordane

R.T.: 5.973 min
Delta R.T.: 0.006 min
Response: 11213704
Conc: 2.90 ng/ml

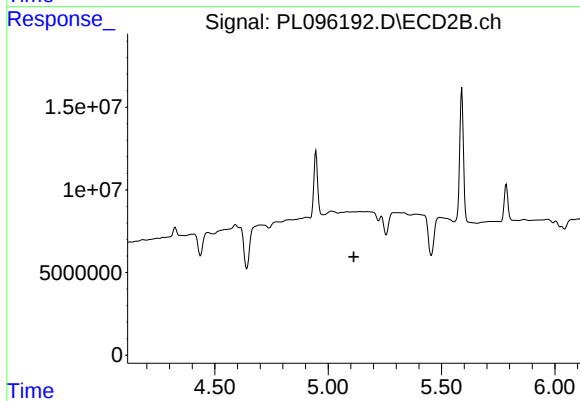

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.113 min
Response: 0
Conc: N.D.

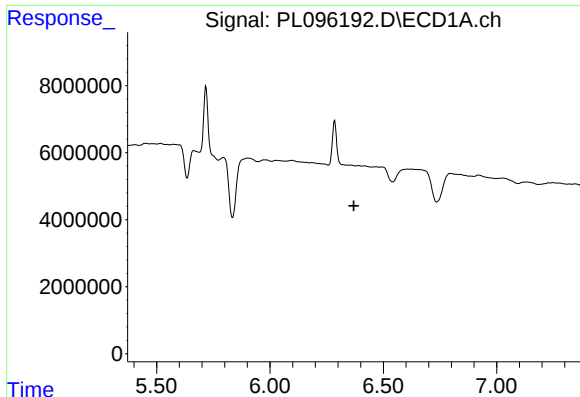

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

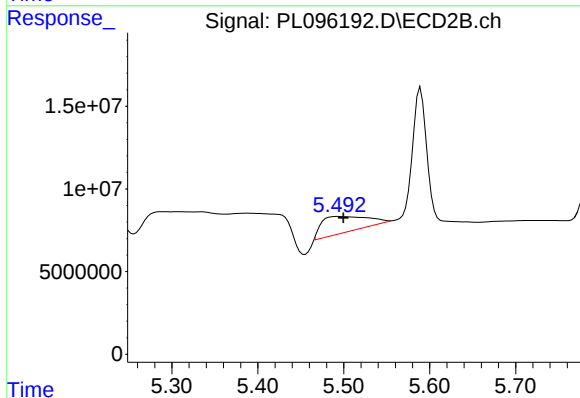


#13 Dieldrin

R.T.: 5.494 min
Delta R.T.: -0.005 min
Response: 35885947
Conc: 6.16 ng/ml

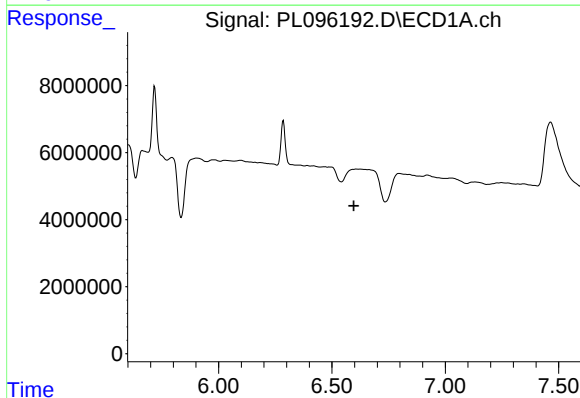


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.596 min
Response: 0
Conc: N.D.

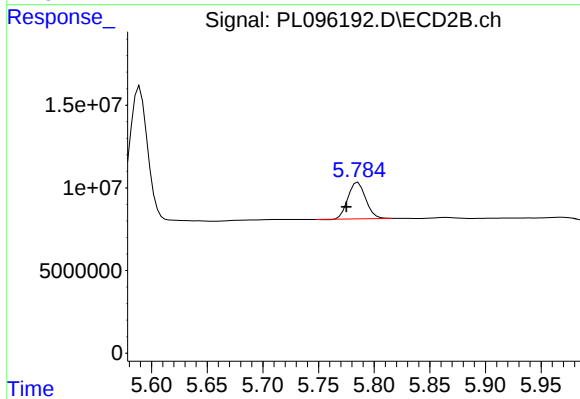

#14 Endrin


R.T.: 5.785 min
Delta R.T.: 0.010 min
Response: 24544553
Conc: 4.60 ng/ml

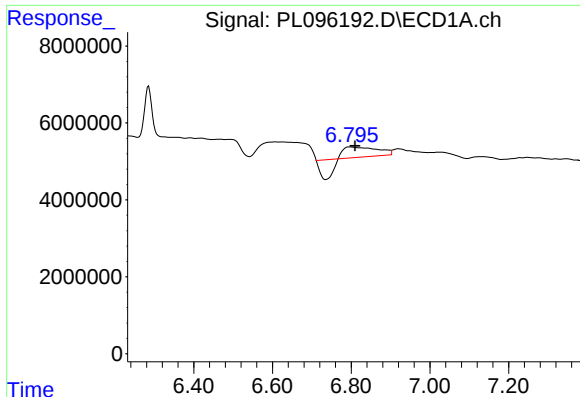

#15 Endosulfan II


R.T.: 6.796 min
Delta R.T.: -0.014 min
Response: 6268996
Conc: 1.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

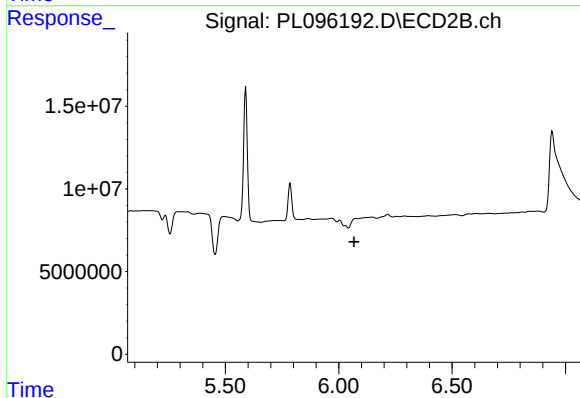


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.068 min
Response: 0
Conc: N.D.

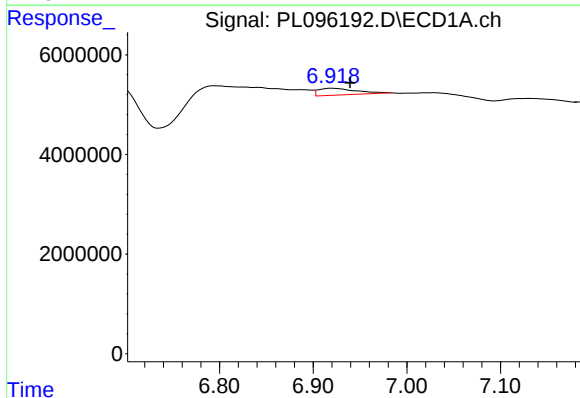


#18 Endrin aldehyde

R.T.: 6.920 min
Delta R.T.: -0.019 min
Response: 3820626
Conc: 1.57 ng/ml

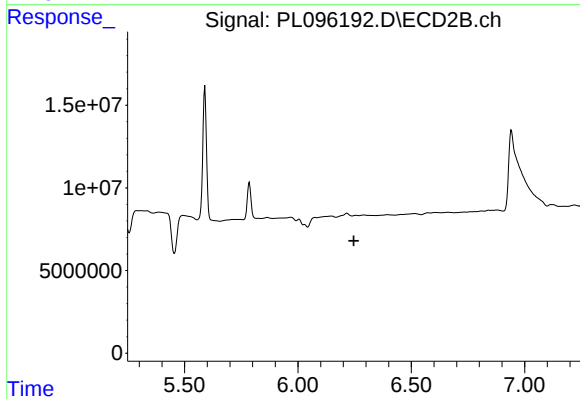

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.247 min
Response: 0
Conc: N.D.

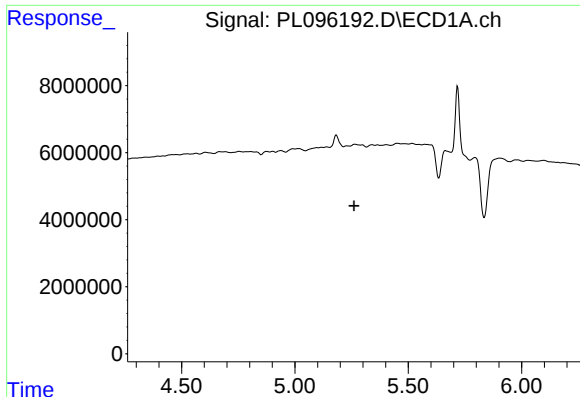

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

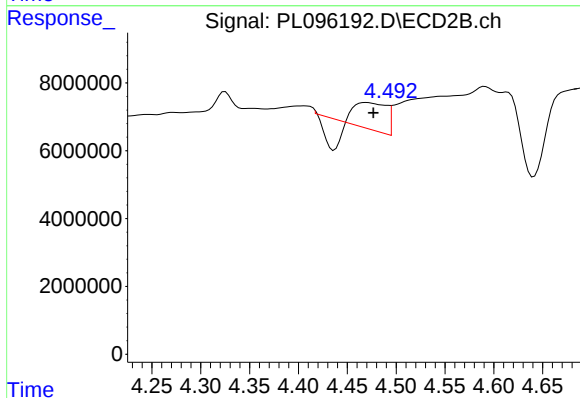


#24 Chlordane-2

R.T.: 4.469 min
Delta R.T.: -0.008 min
Response: 10318618
Conc: 46.22 ng/ml

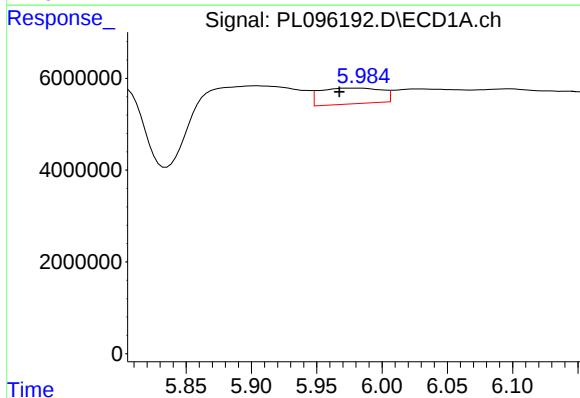


#25 Chlordane-3

R.T.: 5.973 min
Delta R.T.: 0.006 min
Response: 11213704
Conc: 16.79 ng/ml

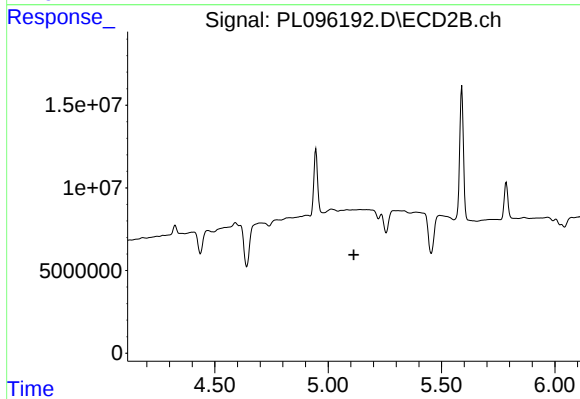

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.113 min
Response: 0
Conc: N.D.

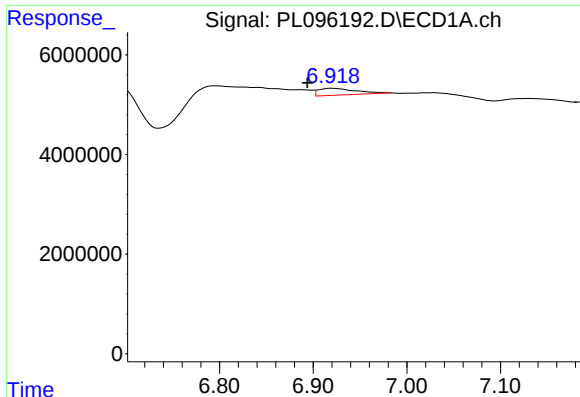

#27 Chlordane-5


R.T.: 6.920 min
Delta R.T.: 0.027 min
Response: 3820626
Conc: 26.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

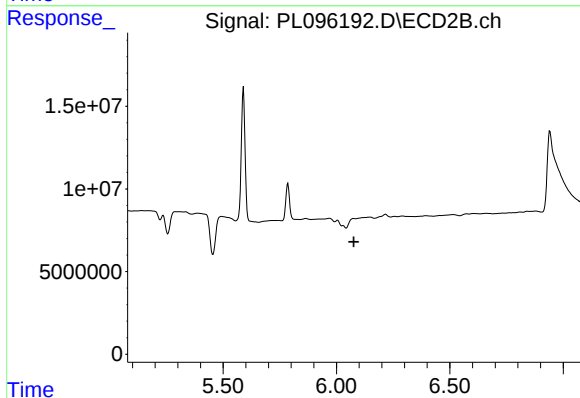


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

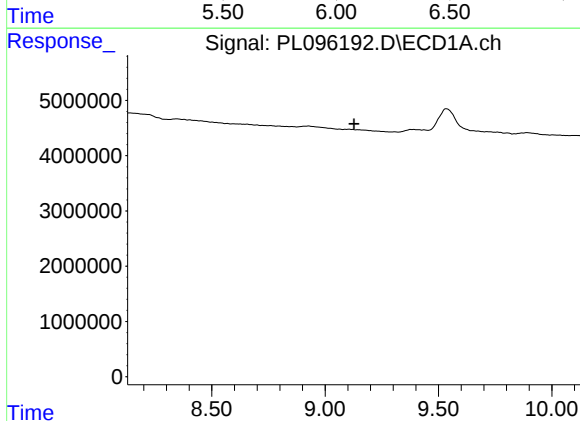

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.127 min
Response: 0
Conc: N.D.

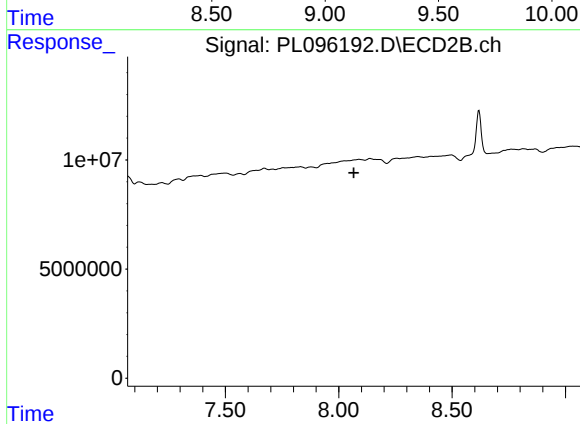

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.066 min
Response: 0
Conc: N.D.