

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062819\
 Data File : PL050024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2019 14:47
 Operator : SM\AJ
 Sample : K3558-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-016-B236-062619

Manual Integrations
 APPROVED

Ankita
 7/1/2019 10:19:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 23:08:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	3.933	218.8E6	55850134	19.400	18.241
28)	SA Decachlor...	7.985	8.965	164.7E6	48647373	12.960	14.491
Target Compounds							
17)	MA 4,4'-DDT	6.171	7.046	11087856	1760802	0.835m	0.601m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062819\
Data File : PL050024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2019 14:47
Operator : SM\AJ
Sample : K3558-14
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PST-016-B236-062619


Manual Integrations
APPROVED

Ankita
7/1/2019 10:19:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 23:08:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

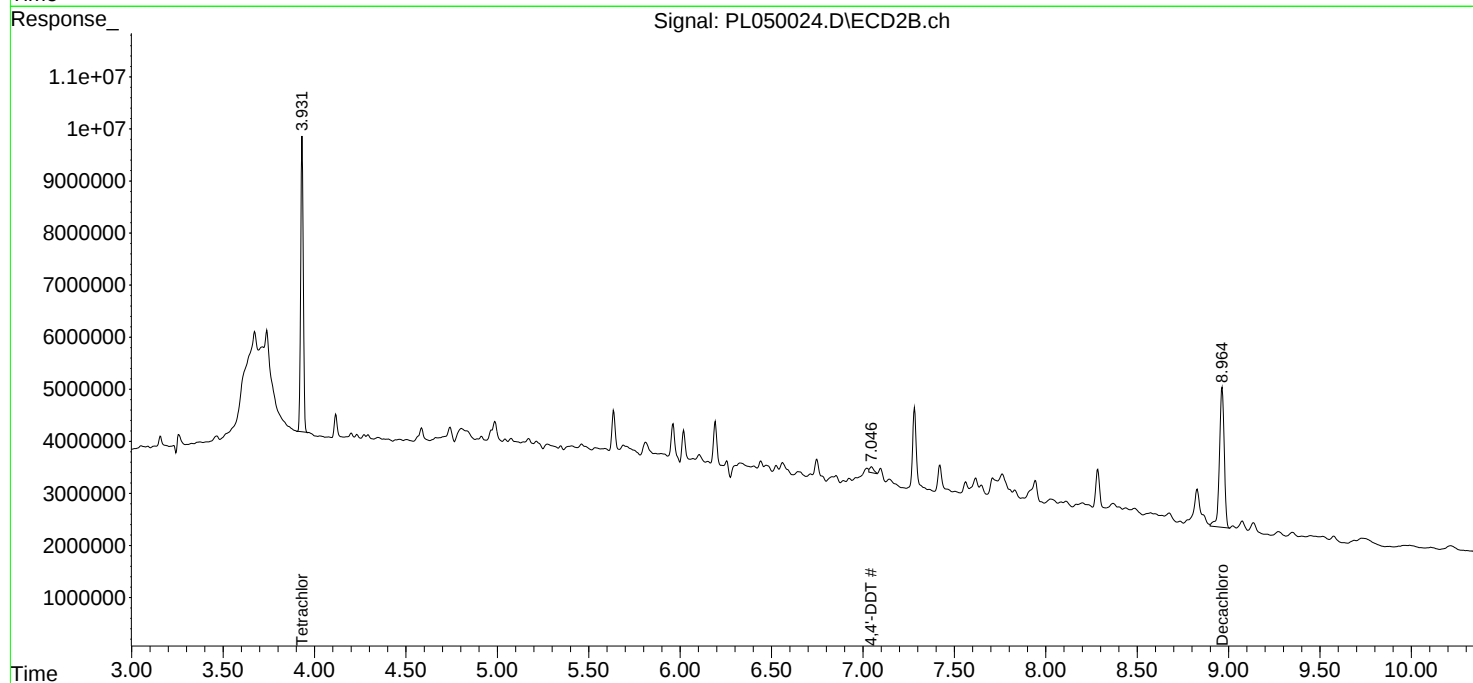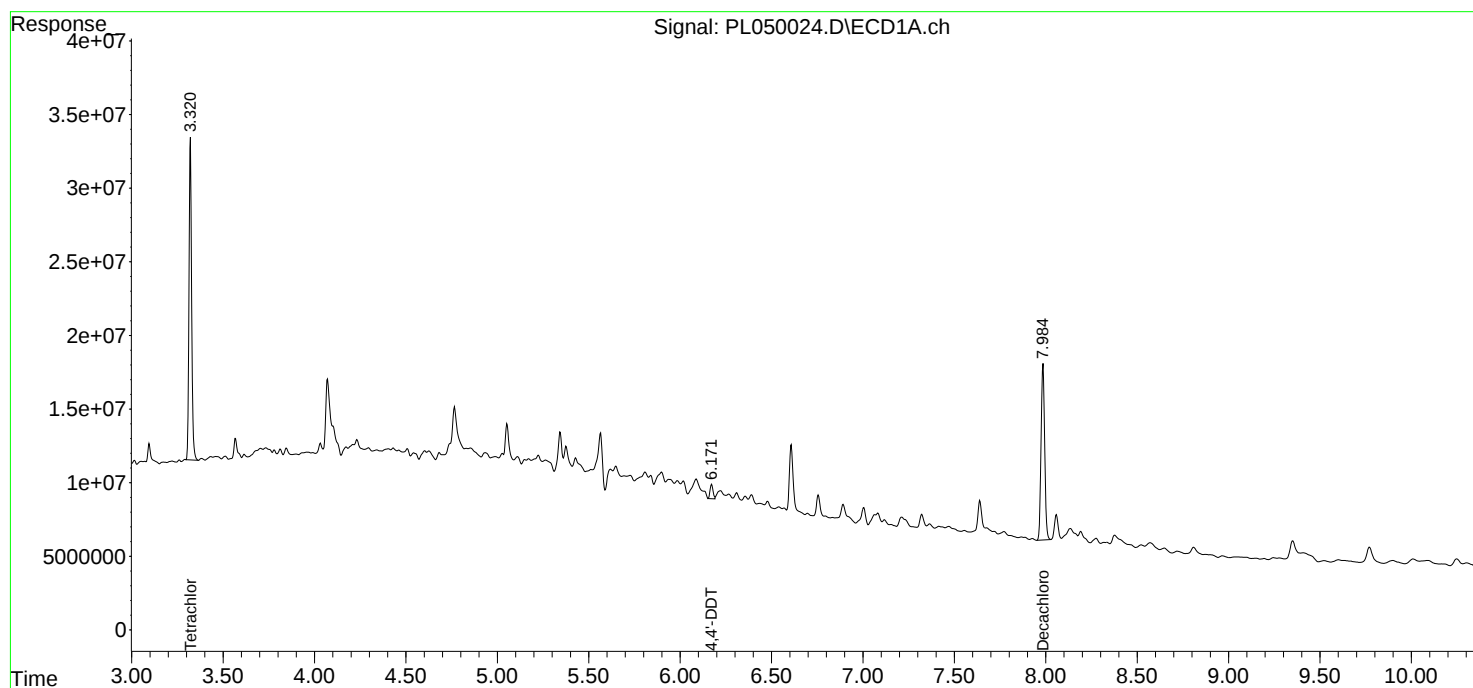

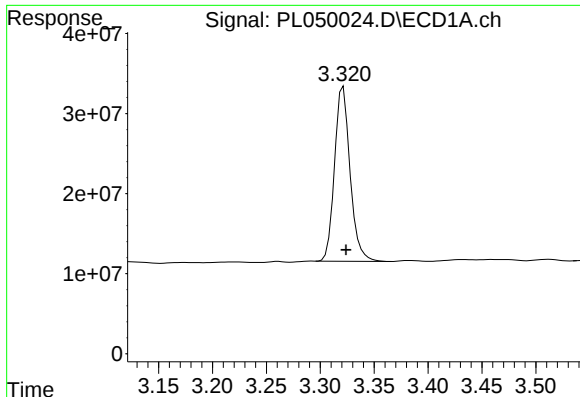


#1 Tetrachloro-m-xylene

R.T.: 3.321 min
Delta R.T.: -0.003 min
Response: 218789443
Conc: 19.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-016-B236-062619


Manual Integrations
APPROVED

Ankita
7/1/2019 10:19:01 AM

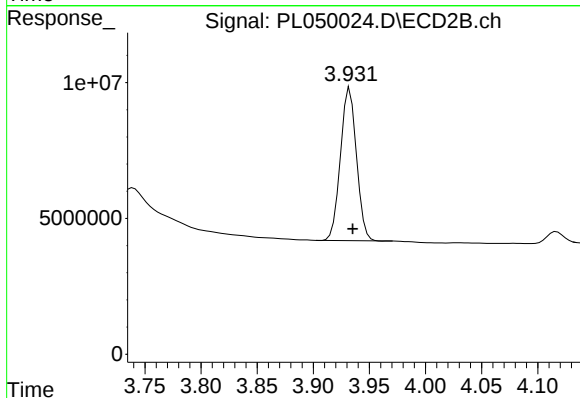


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.003 min
Response: 55850134
Conc: 18.24 ng/ml

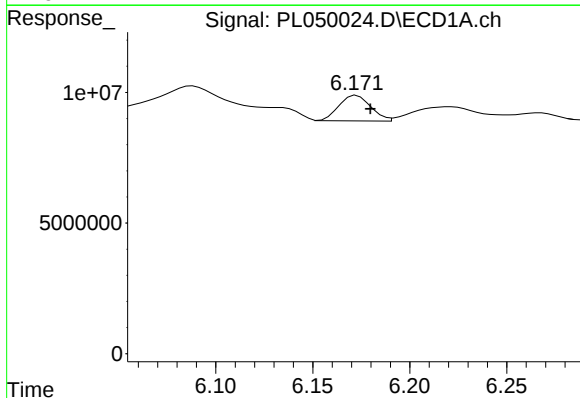


#17 4,4'-DDT

R.T.: 6.171 min
Delta R.T.: -0.008 min
Response: 11087856
Conc: 0.84 ng/ml m

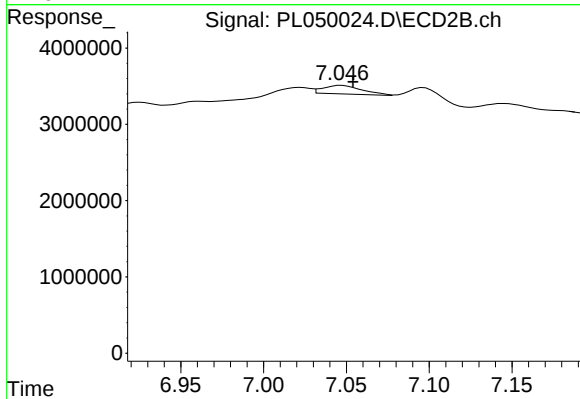

#17 4,4'-DDT

R.T.: 7.046 min
Delta R.T.: -0.008 min
Response: 1760802
Conc: 0.60 ng/ml m

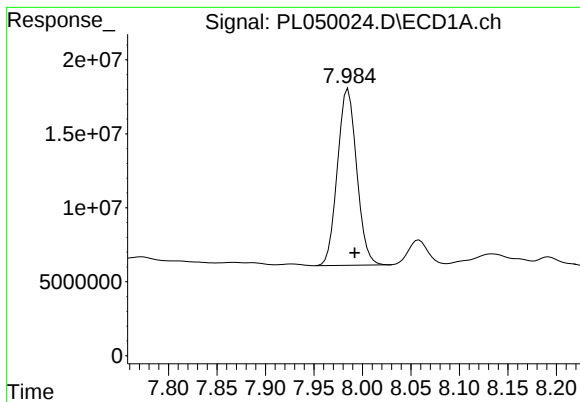


#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.007 min
Response: 164681135
Conc: 12.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-016-B236-062619

Manual Integrations
APPROVED

Ankita
7/1/2019 10:19:01 AM

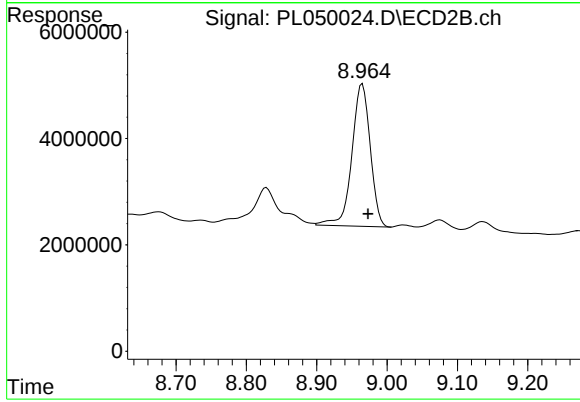

#28 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: -0.008 min
Response: 48647373
Conc: 14.49 ng/ml