

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062819\
 Data File : PL050031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2019 16:32
 Operator : SM\AJ
 Sample : K3558-19
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-016-SW095-062619

Manual Integrations
 APPROVED

Ankita
 7/1/2019 10:19:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 23:09:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.933	170.6E6	44496710	15.128	14.533
28)	SA Decachlor...	7.985	8.965	114.2E6	32505295	8.989	9.683
Target Compounds							
13)	MA Dieldrin	5.554	6.406	150.3E6	15759154	9.025	4.442 #
17)	MA 4,4'-DDT	6.173	7.047	21091093	5514597	1.589	1.883m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062819\
Data File : PL050031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2019 16:32
Operator : SM\AJ
Sample : K3558-19
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EXT-016-SW095-062619


Manual Integrations
APPROVED

Ankita
7/1/2019 10:19:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 23:09:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

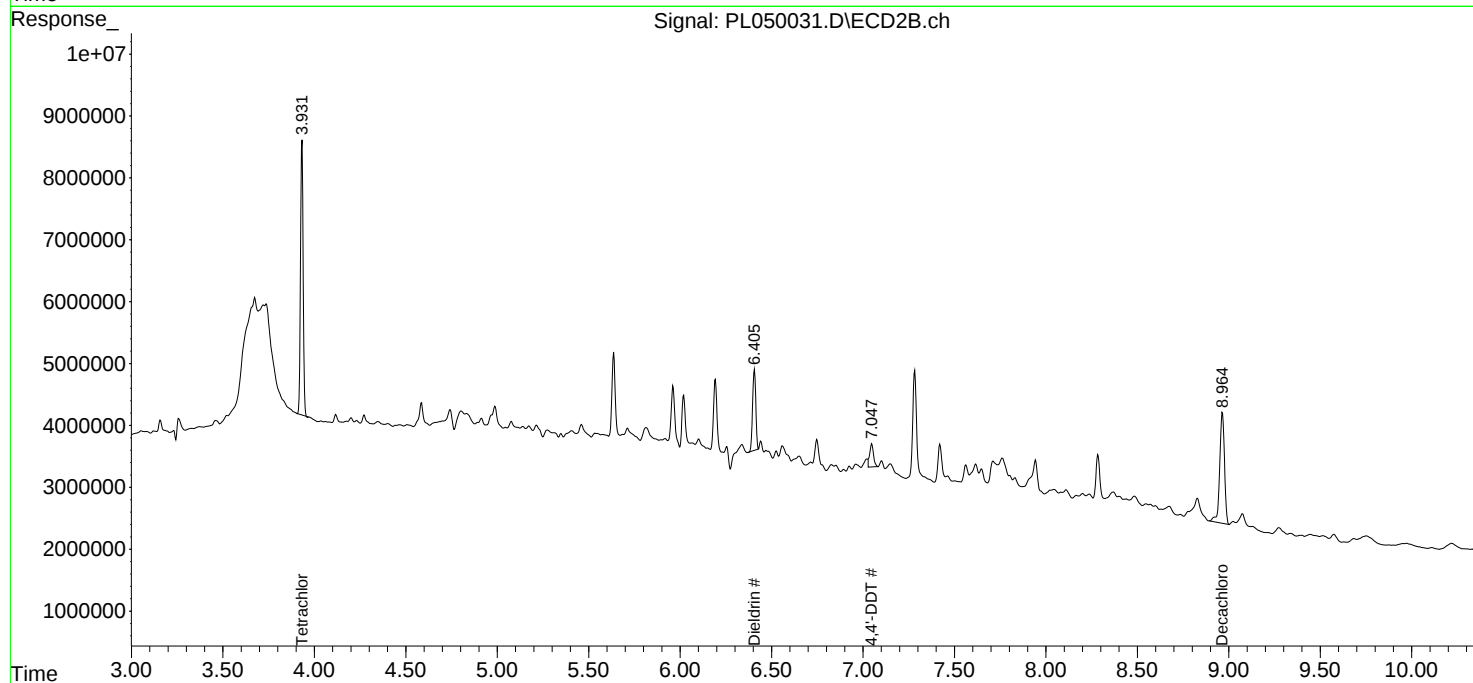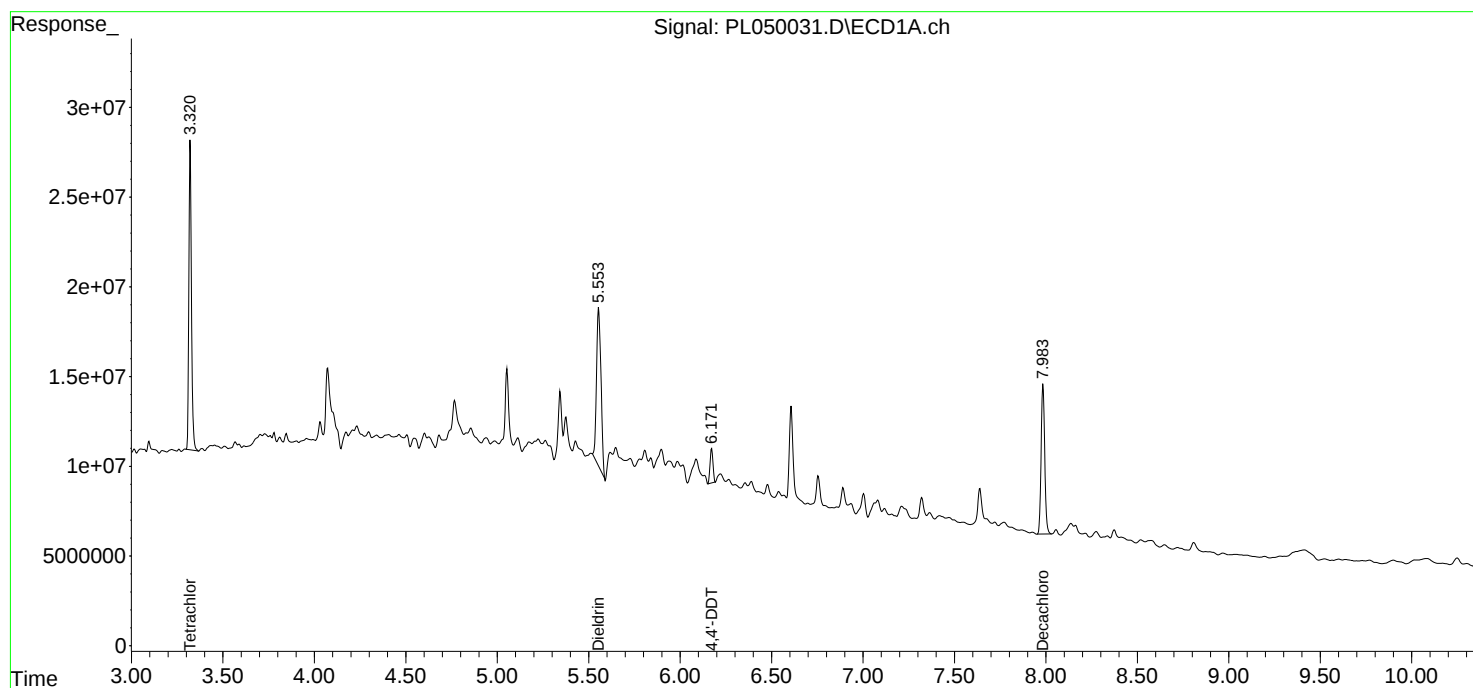

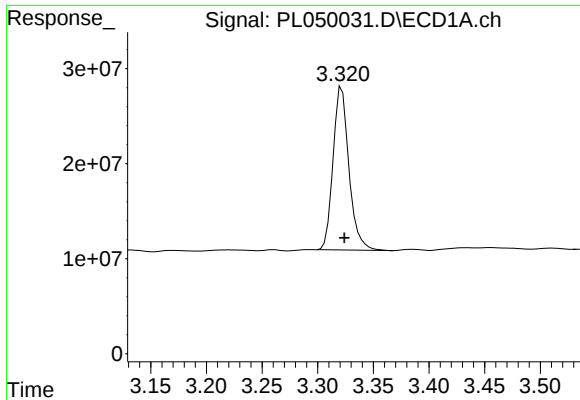


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 170610510
Conc: 15.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-016-SW095-062619


Manual Integrations
APPROVED

Ankita
7/1/2019 10:19:09 AM

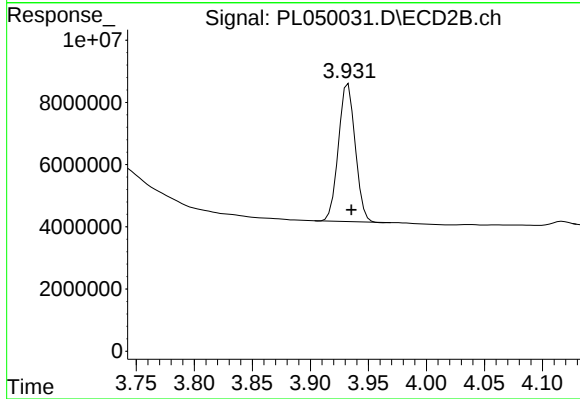


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.003 min
Response: 44496710
Conc: 14.53 ng/ml

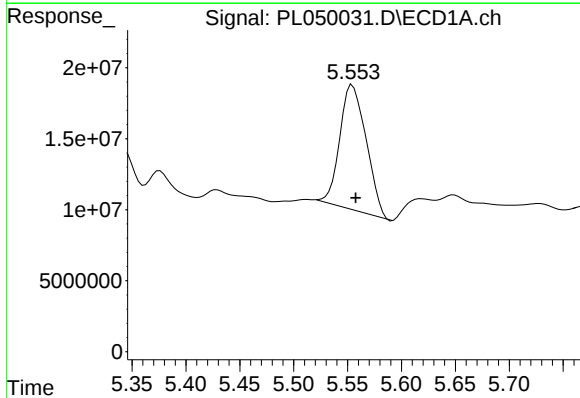


#13 Dieldrin

R.T.: 5.554 min
Delta R.T.: -0.003 min
Response: 150331489
Conc: 9.02 ng/ml

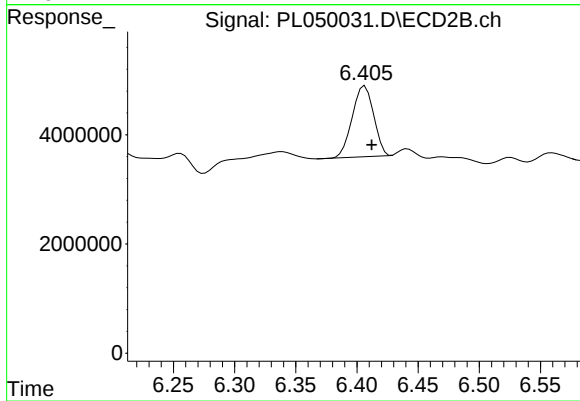

#13 Dieldrin

R.T.: 6.406 min
Delta R.T.: -0.006 min
Response: 15759154
Conc: 4.44 ng/ml

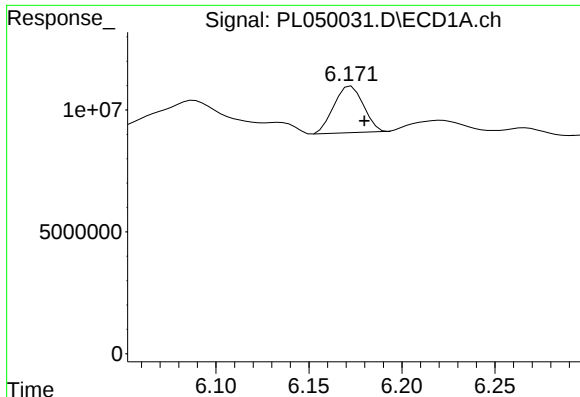


#17 4,4'-DDT

R.T.: 6.173 min
Delta R.T.: -0.007 min
Response: 21091093
Conc: 1.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-016-SW095-062619


Manual Integrations
APPROVED

Ankita
7/1/2019 10:19:09 AM

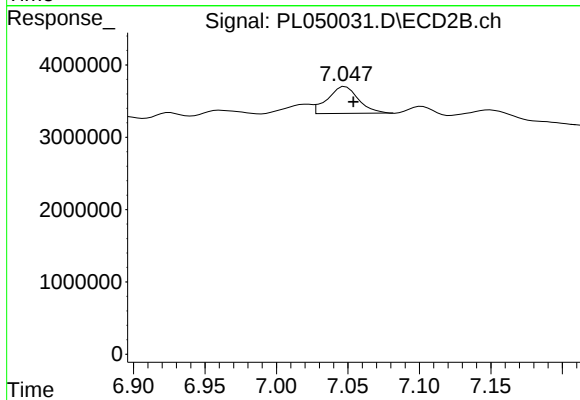


#17 4,4'-DDT

R.T.: 7.047 min
Delta R.T.: -0.007 min
Response: 5514597
Conc: 1.88 ng/ml m

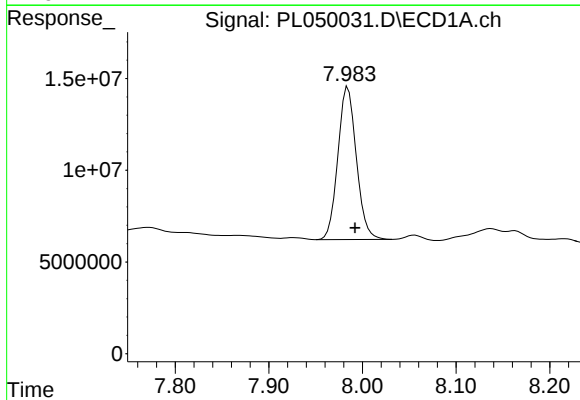

#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.008 min
Response: 114215649
Conc: 8.99 ng/ml

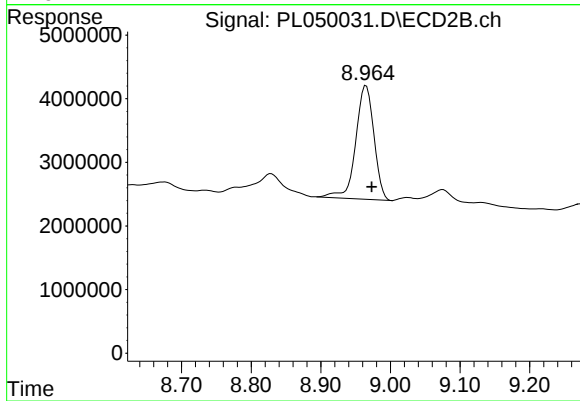

#28 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: -0.008 min
Response: 32505295
Conc: 9.68 ng/ml