

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
 Data File : PL067845.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2021 14:49
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 06:39:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.525	10827886	19623033	19.695	20.815
28)	SA Decachlor...	10.217	11.420	14400433	20372141	20.320	20.453
Target Compounds							
2)	A alpha-BHC	5.188	0.000	2709892	0	3.684	N.D. #
4)	MA Heptachlor	5.988f	0.000	542289	0	0.719	N.D. #
6)	B beta-BHC	5.988	0.000	542289	0	1.516	N.D. #
15)	B Endosulfa...	0.000	9.173f	0	657381	N.D.	0.825 #
16)	A 4,4'-DDD	8.028f	0.000	207066	0	0.356	N.D. #
21)	B Endrin ke...	0.000	10.045f	0	377163	N.D.	0.416 #
23)	Chlordane-1	0.000	6.934f	0	357886	N.D.	12.674 #
24)	Chlordane-2	6.486	0.000	253198	0	9.455	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
Data File : PL067845.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2021 14:49
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 06:39:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

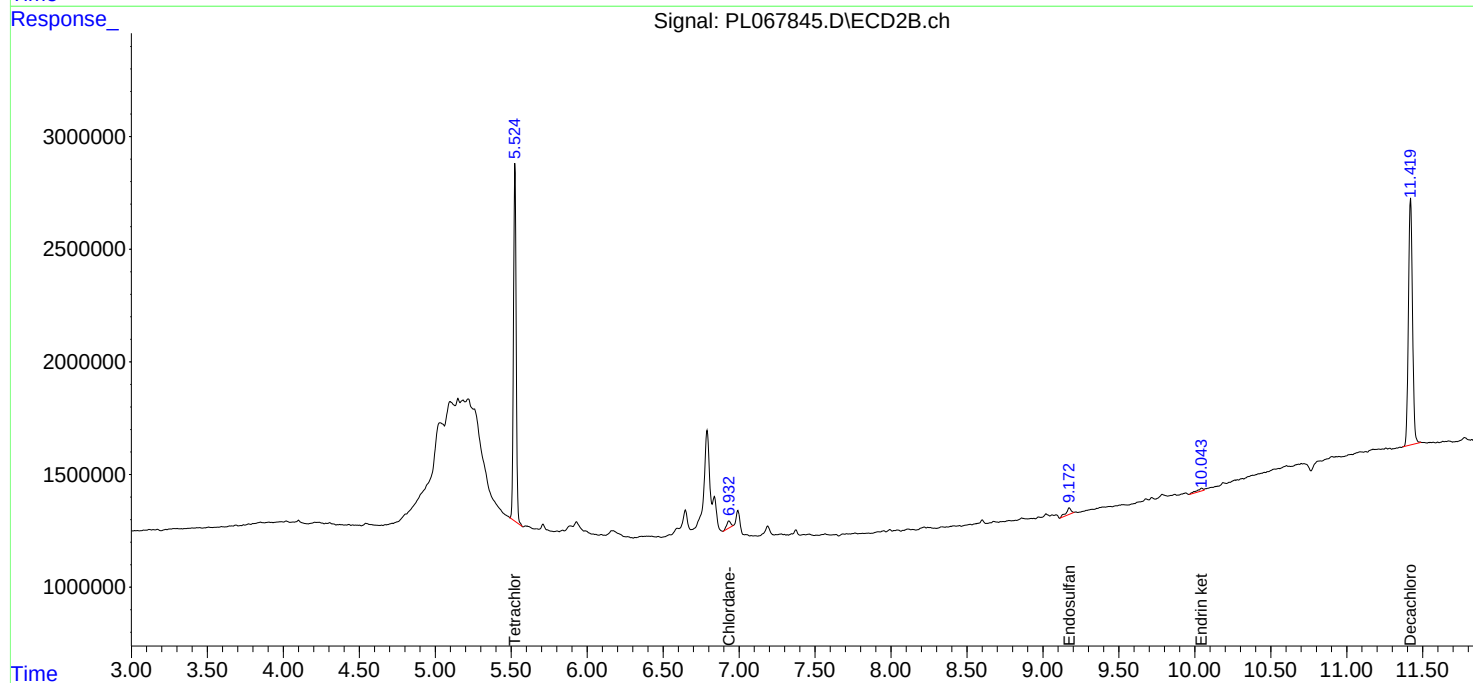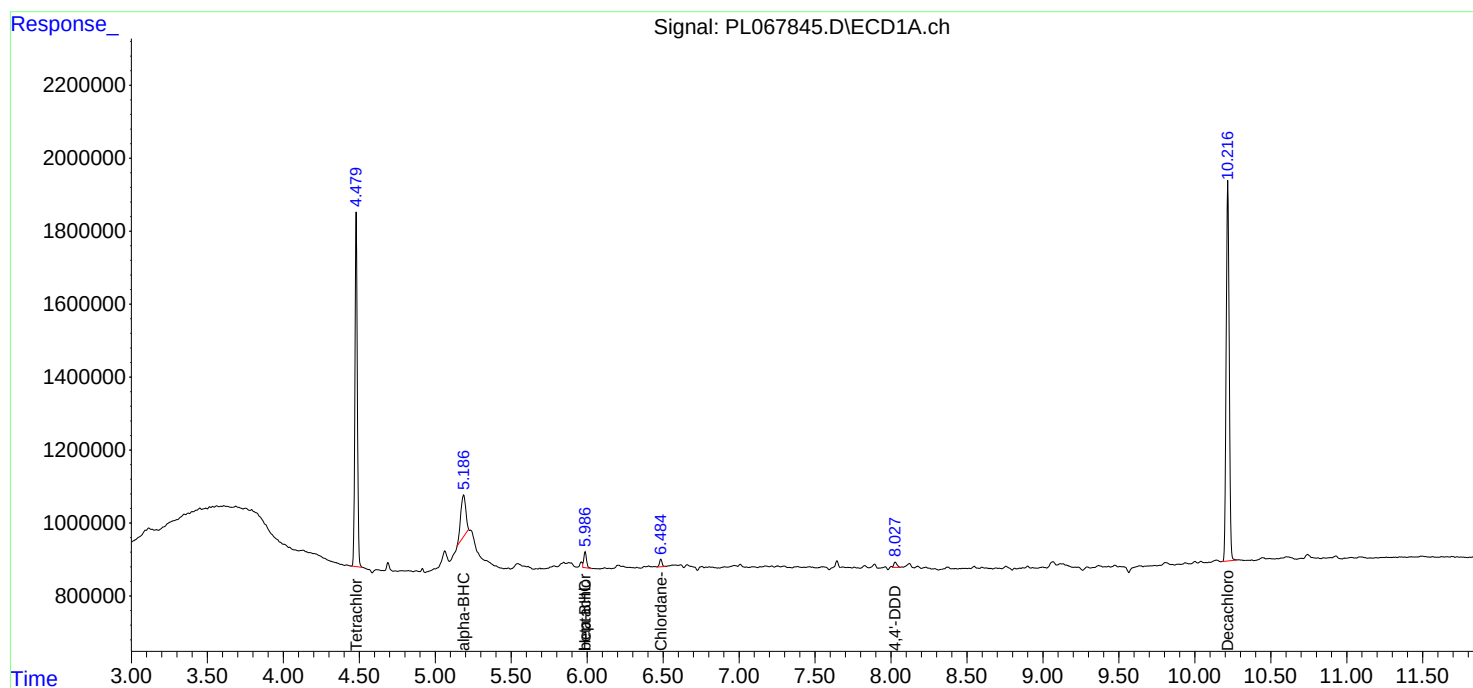


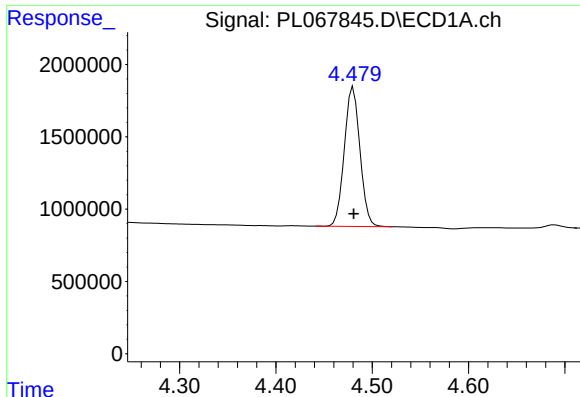

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 10827886
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

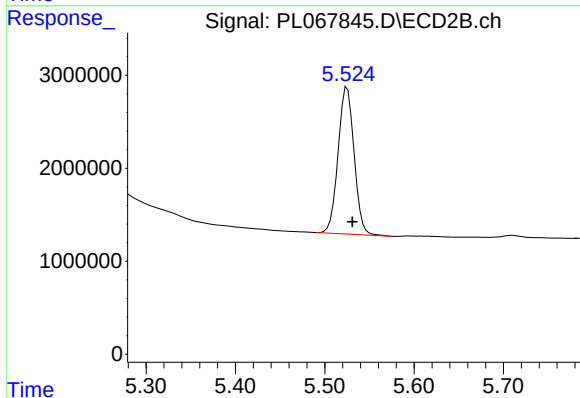


#1 Tetrachloro-m-xylene

R.T.: 5.525 min
Delta R.T.: -0.006 min
Response: 19623033
Conc: 20.82 ng/ml

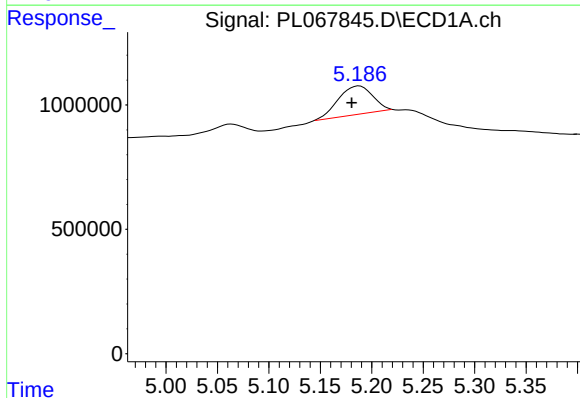


#2 alpha-BHC

R.T.: 5.188 min
Delta R.T.: 0.007 min
Response: 2709892
Conc: 3.68 ng/ml

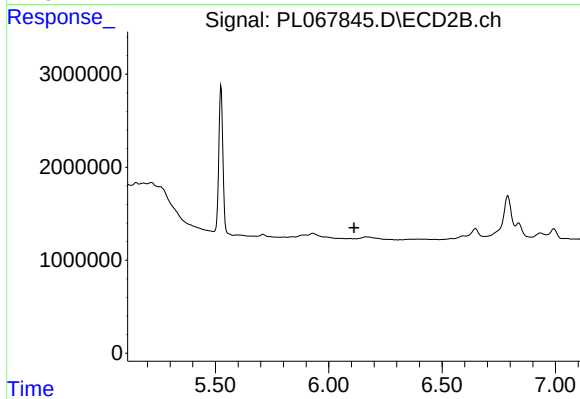

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

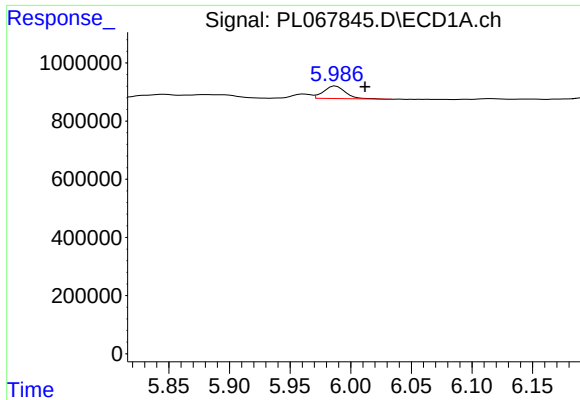

#4 Heptachlor


R.T.: 5.988 min
Delta R.T.: -0.024 min
Response: 542289
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

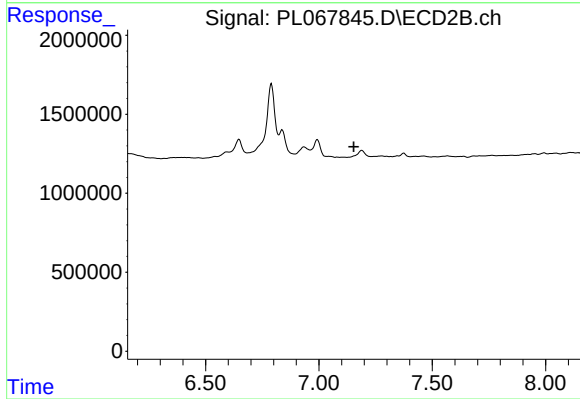


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

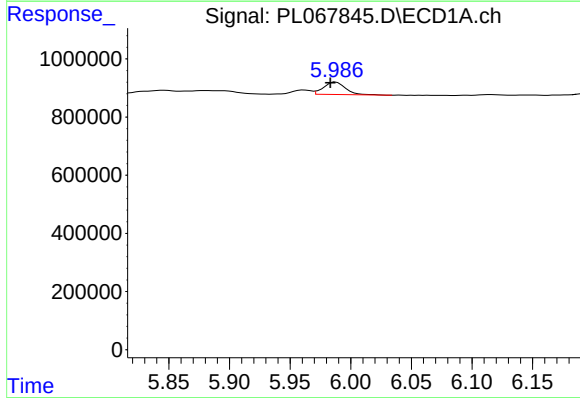


#6 beta-BHC

R.T.: 5.988 min
Delta R.T.: 0.004 min
Response: 542289
Conc: 1.52 ng/ml

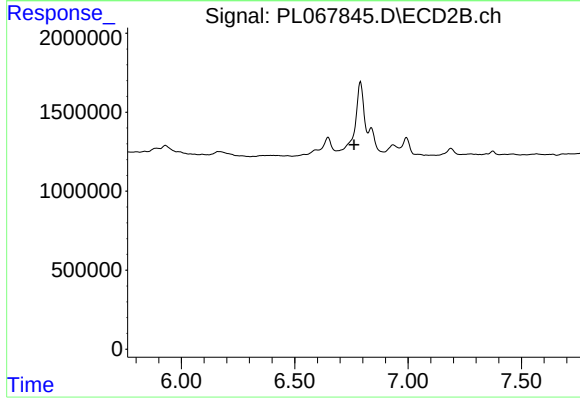

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

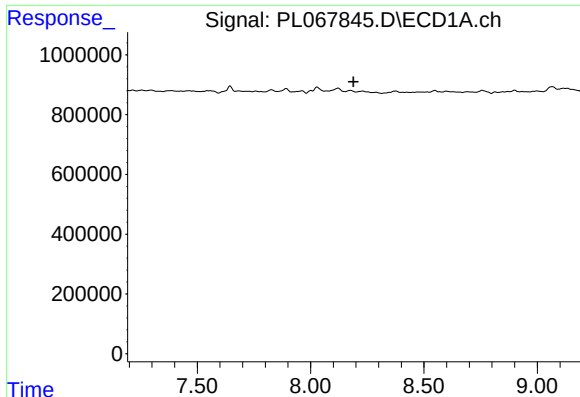

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

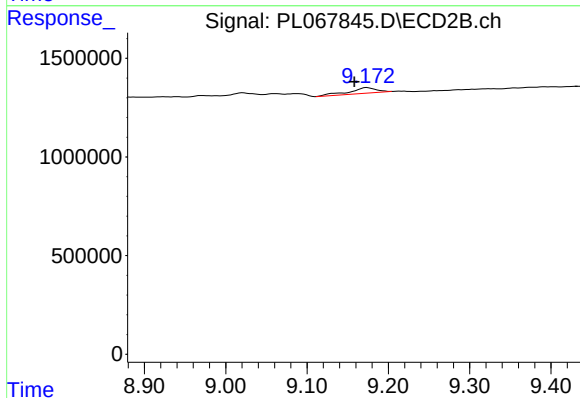


#15 Endosulfan II

R.T.: 9.173 min
Delta R.T.: 0.015 min
Response: 657381
Conc: 0.82 ng/ml

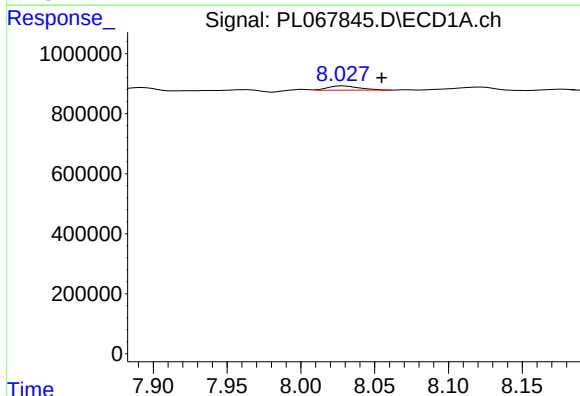


#16 4,4'-DDD

R.T.: 8.028 min
Delta R.T.: -0.026 min
Response: 207066
Conc: 0.36 ng/ml

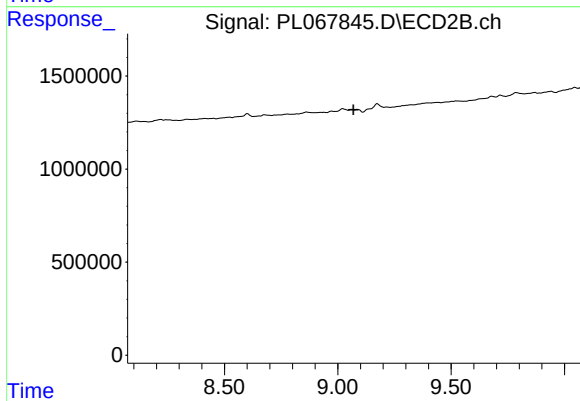

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 9.069 min
Response: 0
Conc: N.D.

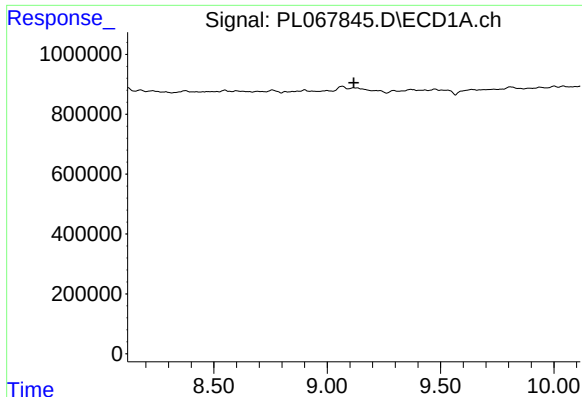

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

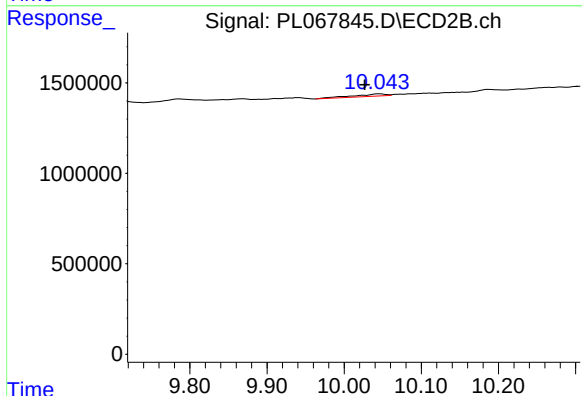


#21 Endrin ketone

R.T.: 10.045 min
Delta R.T.: 0.018 min
Response: 377163
Conc: 0.42 ng/ml

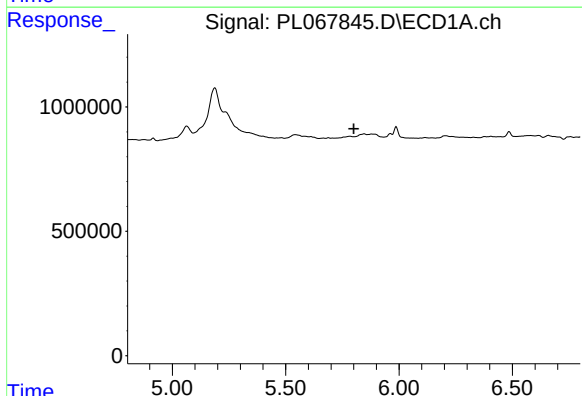


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

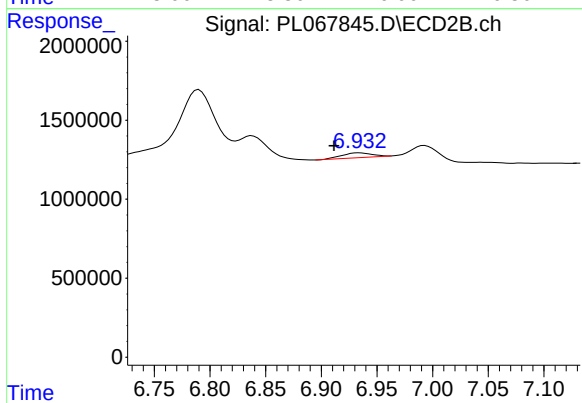

#23 Chlordane-1


R.T.: 6.934 min
Delta R.T.: 0.022 min
Response: 357886
Conc: 12.67 ng/ml

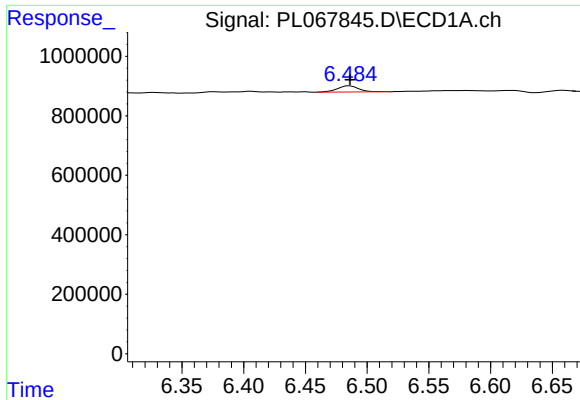

#24 Chlordane-2


R.T.: 6.486 min
Delta R.T.: 0.000 min
Response: 253198
Conc: 9.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

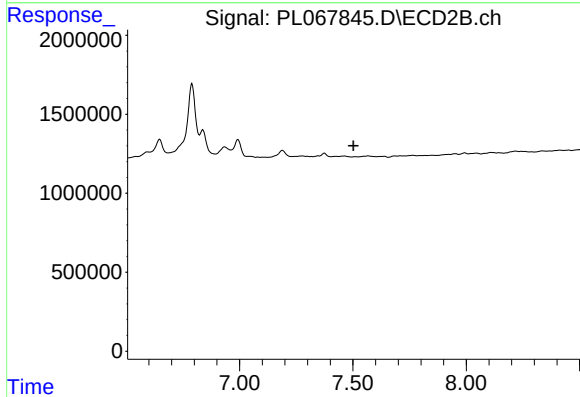


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

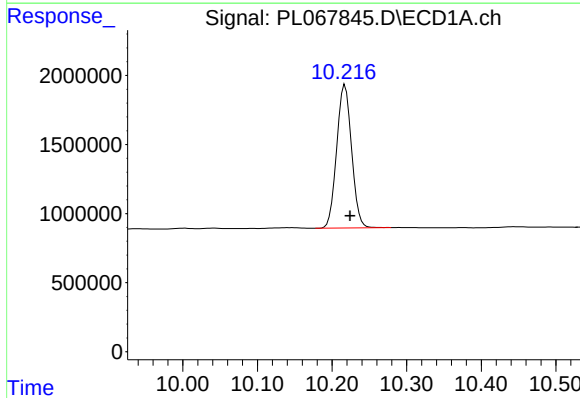

#28 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: -0.007 min
Response: 14400433
Conc: 20.32 ng/ml

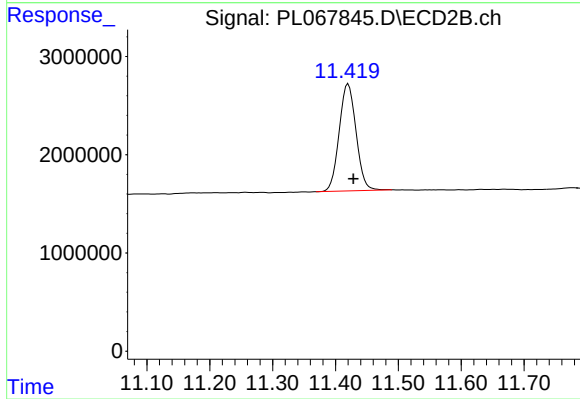

#28 Decachlorobiphenyl

R.T.: 11.420 min
Delta R.T.: -0.008 min
Response: 20372141
Conc: 20.45 ng/ml