

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
 Data File : PL067854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2021 19:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 06:41:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	10734519	19293071	19.525	20.465
28)	SA Decachlor...	10.218	11.425	13932845	19850165	19.660	19.929
Target Compounds							
2)	A alpha-BHC	5.177	0.000	253669	0	0.345	N.D. #
4)	MA Heptachlor	5.987f	0.000	527897	0	0.700	N.D. #
6)	B beta-BHC	5.987	0.000	527897	0	1.475	N.D. #
14)	MA Endrin	7.894f	0.000	360703	0	0.550	N.D. #
15)	B Endosulfa...	0.000	9.179f	0	477942	N.D.	0.599 #
16)	A 4,4'-DDD	8.027f	0.000	286000	0	0.492	N.D. #
21)	B Endrin ke...	0.000	10.049f	0	2543845	N.D.	2.807 #
24)	Chlordane-2	6.485	0.000	399363	0	14.914	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
Data File : PL067854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2021 19:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 06:41:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

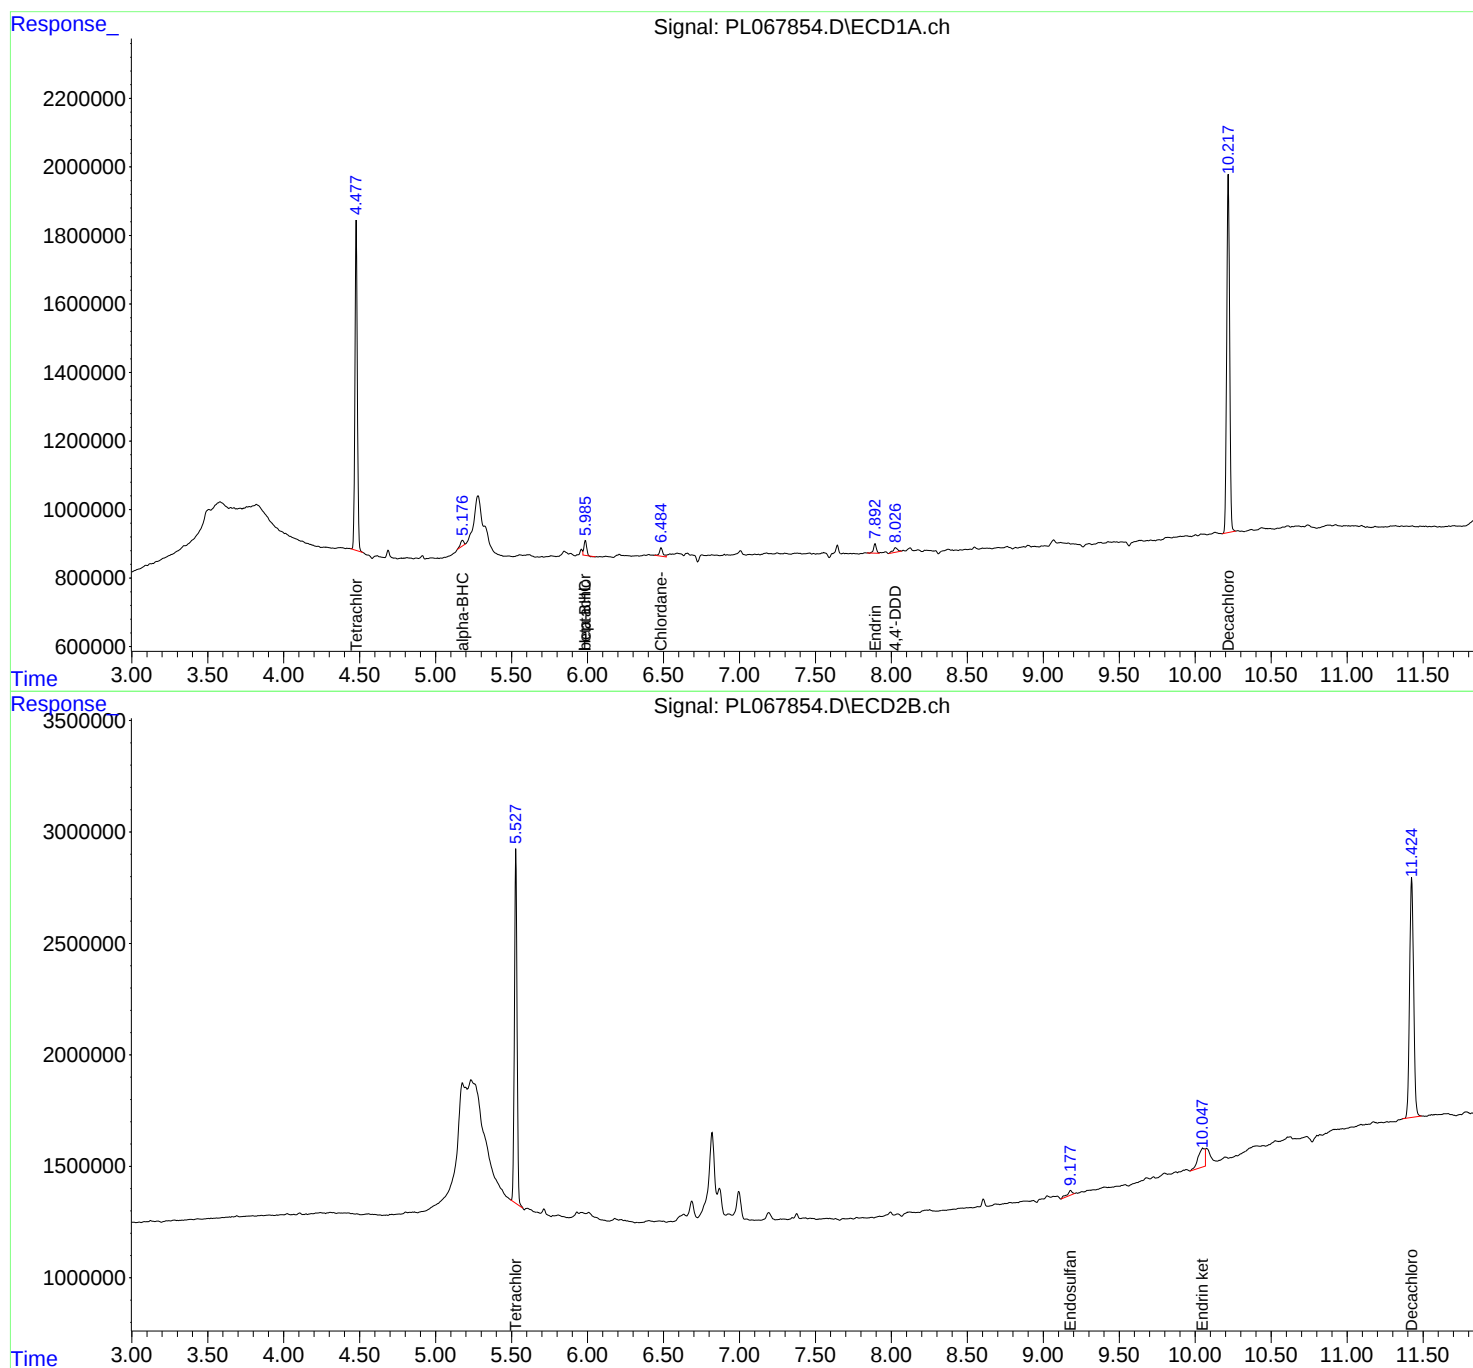


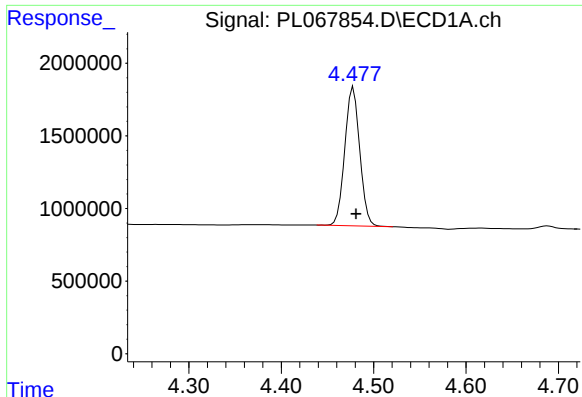

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 10734519
Conc: 19.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

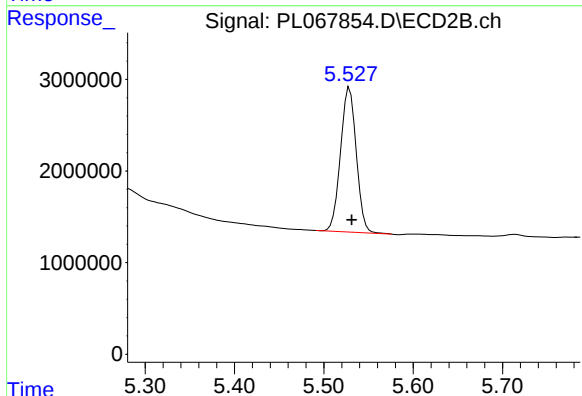


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 19293071
Conc: 20.47 ng/ml

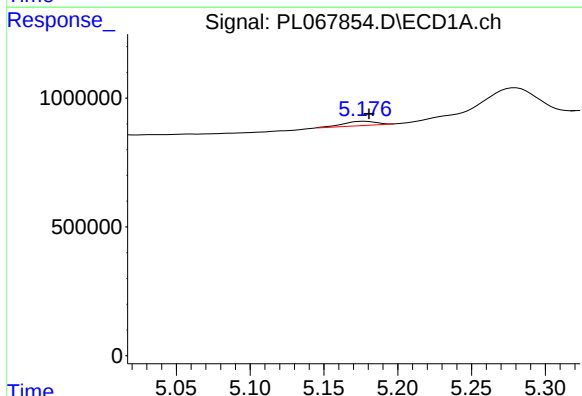


#2 alpha-BHC

R.T.: 5.177 min
Delta R.T.: -0.003 min
Response: 253669
Conc: 0.34 ng/ml

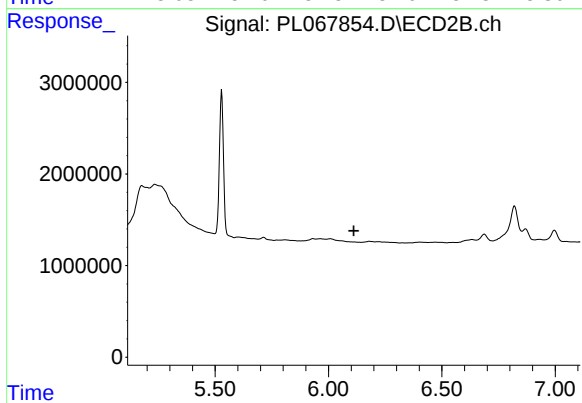

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

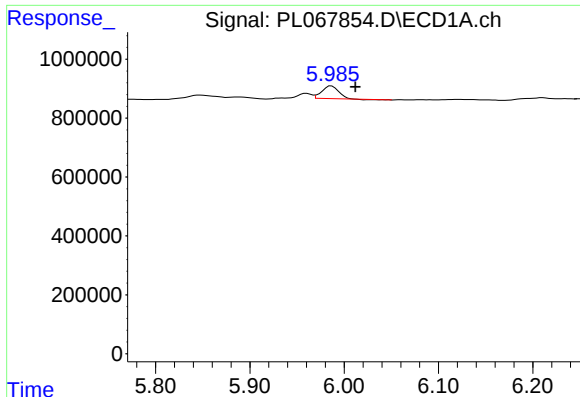

#4 Heptachlor


R.T.: 5.987 min
Delta R.T.: -0.025 min
Response: 527897
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

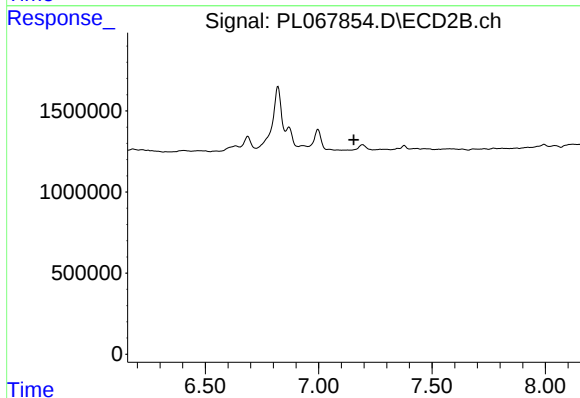


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

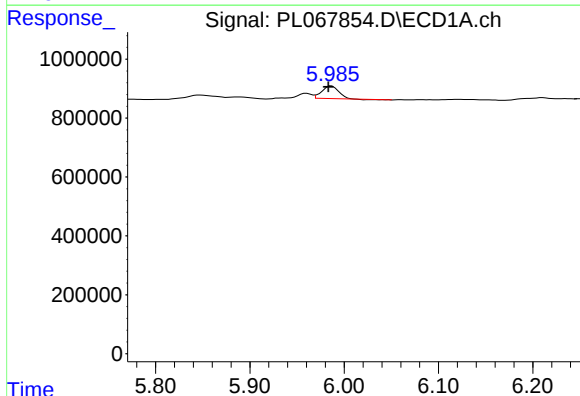


#6 beta-BHC

R.T.: 5.987 min
Delta R.T.: 0.003 min
Response: 527897
Conc: 1.48 ng/ml

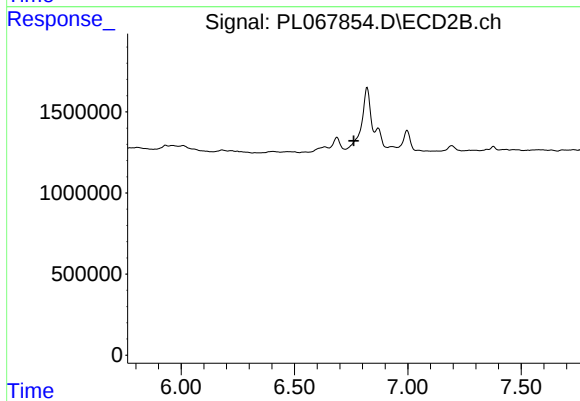

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

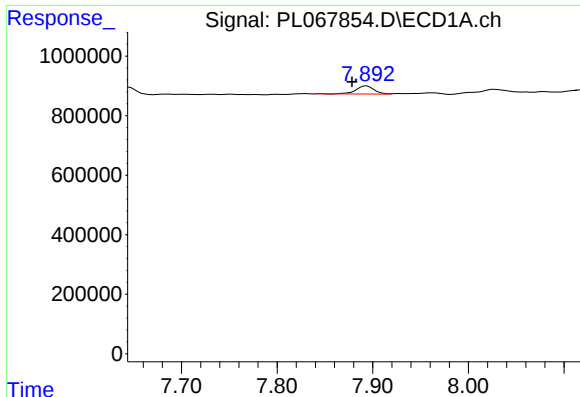

#14 Endrin


R.T.: 7.894 min
Delta R.T.: 0.015 min
Response: 360703
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

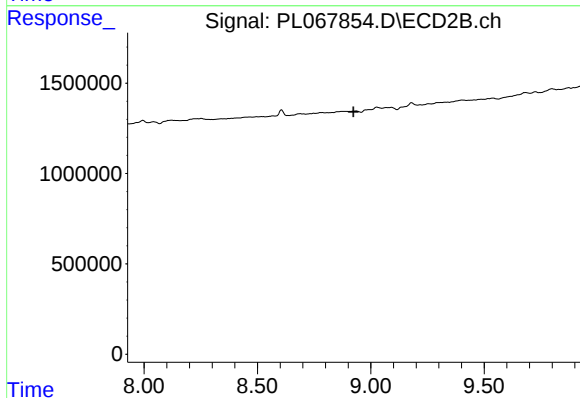


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

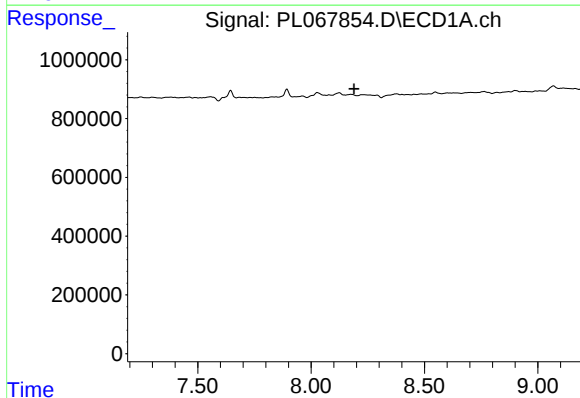


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

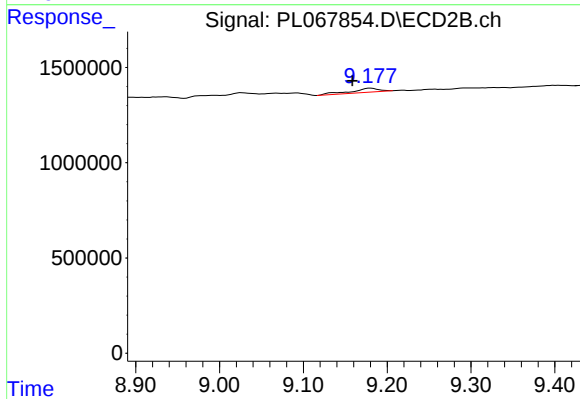

#15 Endosulfan II


R.T.: 9.179 min
Delta R.T.: 0.021 min
Response: 477942
Conc: 0.60 ng/ml

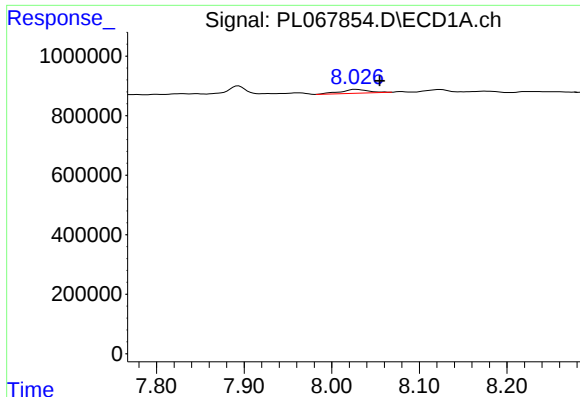

#16 4,4'-DDD


R.T.: 8.027 min
Delta R.T.: -0.027 min
Response: 286000
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

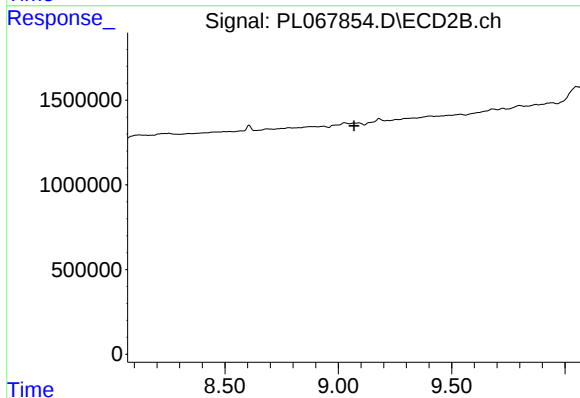


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

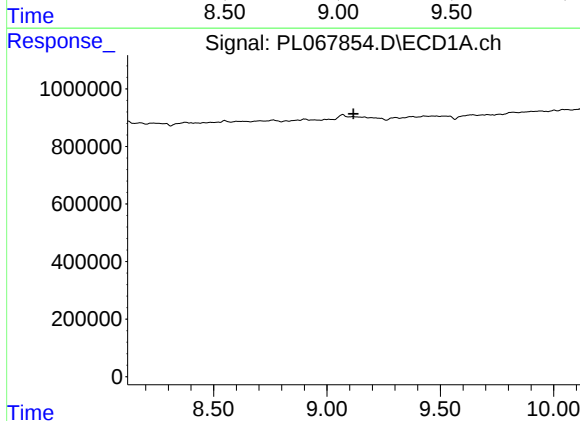


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

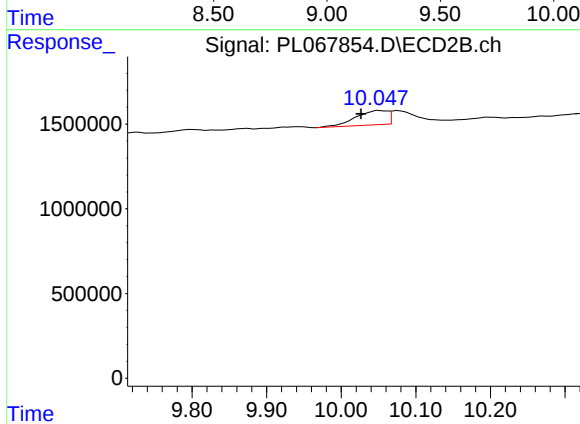

#21 Endrin ketone


R.T.: 10.049 min
Delta R.T.: 0.023 min
Response: 2543845
Conc: 2.81 ng/ml

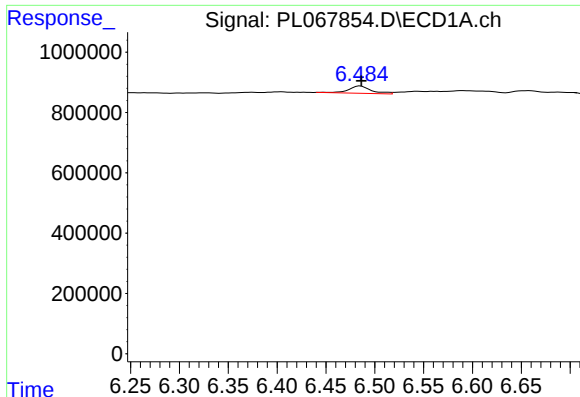

#24 Chlordane-2


R.T.: 6.485 min
Delta R.T.: -0.001 min
Response: 399363
Conc: 14.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

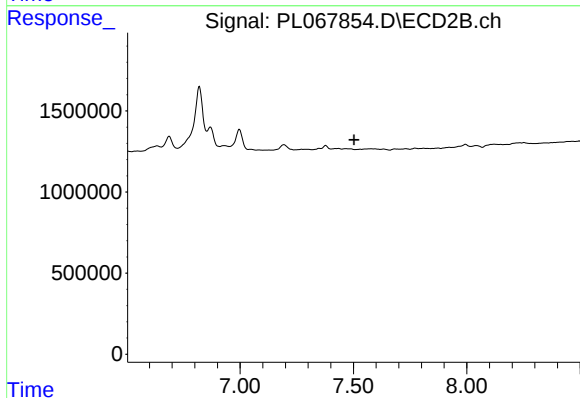


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

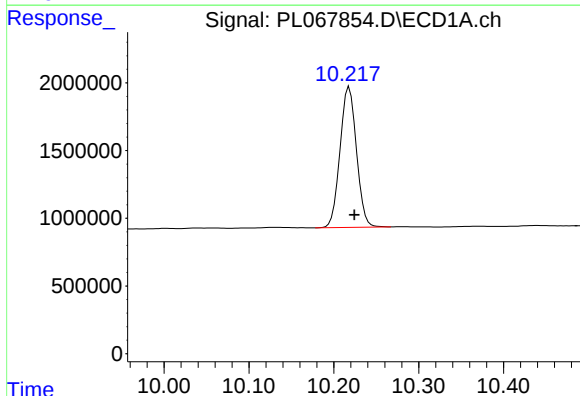

#28 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: -0.006 min
Response: 13932845
Conc: 19.66 ng/ml

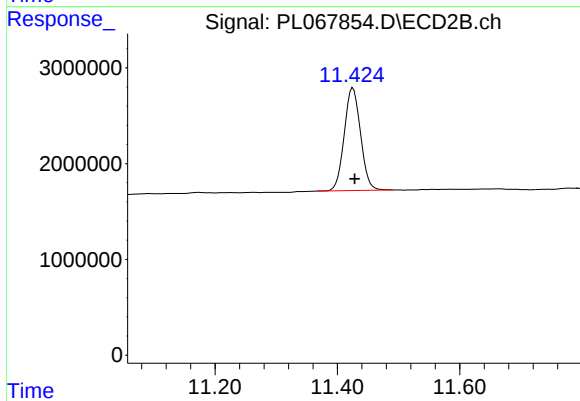

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 19850165
Conc: 19.93 ng/ml