

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
 Data File : PL067835.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2021 10:12
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 06:14:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.528	28644576	48895013	52.101	51.865
28)	SA Decachlor...	10.220	11.426	34320053	46388040	48.428	46.572
Target Compounds							
23)	Chlordane-1	5.799	6.910	9612051	15096212	519.517	534.606
24)	Chlordane-2	6.485	7.501	13535234	18757302	505.456	514.658
25)	Chlordane-3	7.183	8.258	34364327	67784497	511.445	506.467
26)	Chlordane-4	7.249	8.340	37480570	81342670	512.880	501.804
27)	Chlordane-5	8.190	9.226	11405032	14431504	521.276	496.309



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
Data File : PL067835.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2021 10:12
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 06:14:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

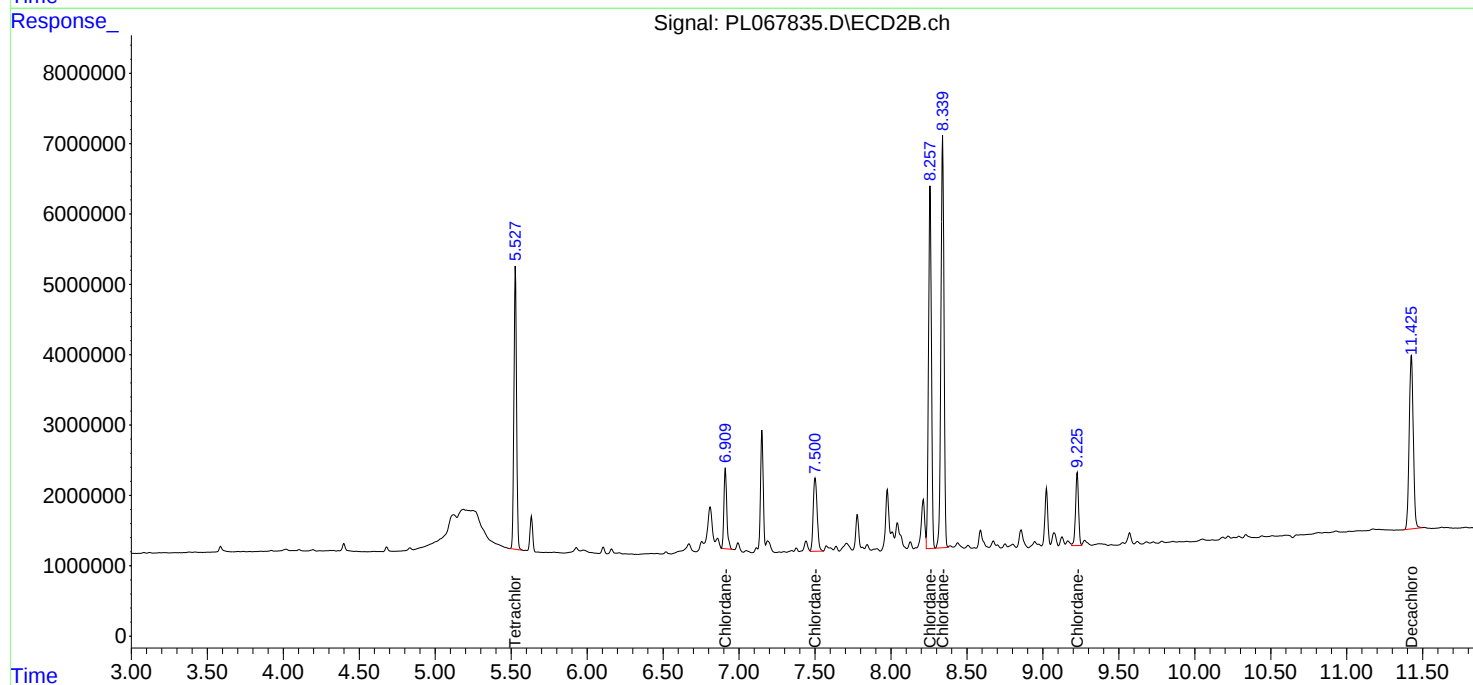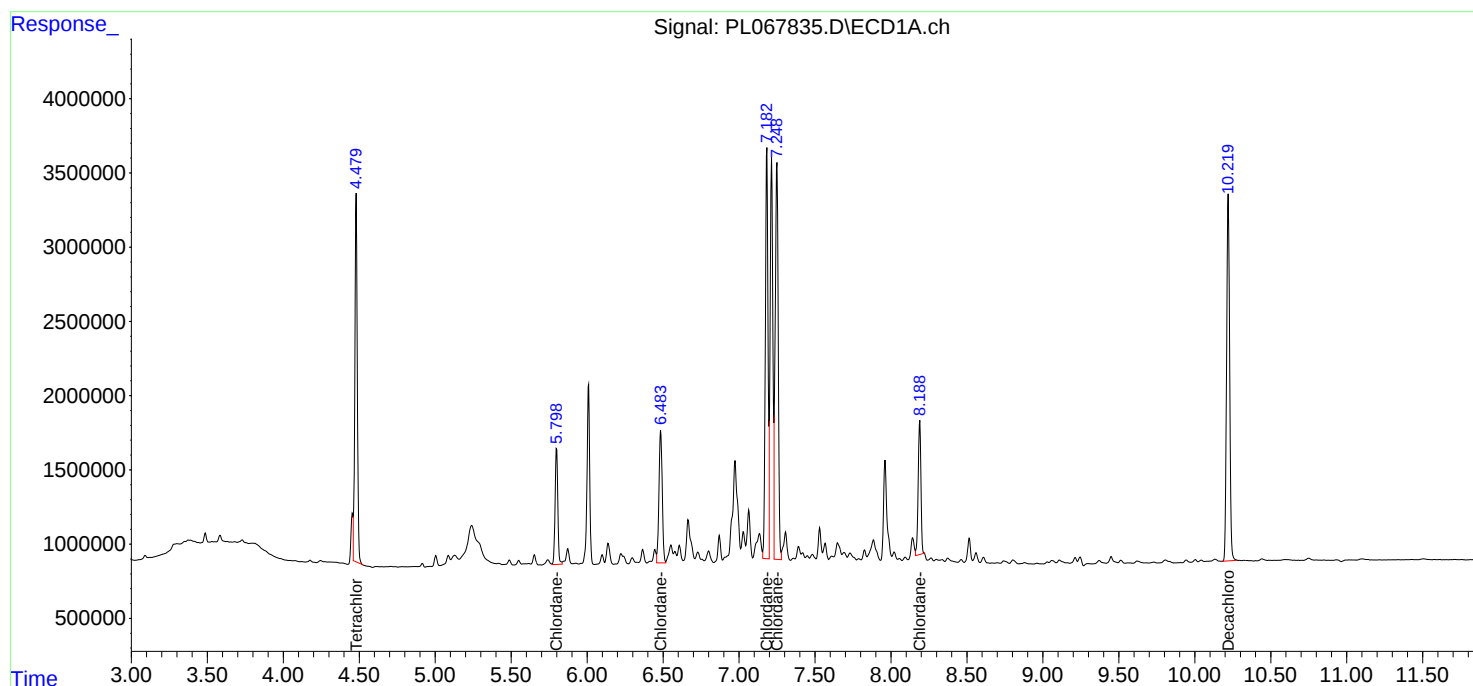


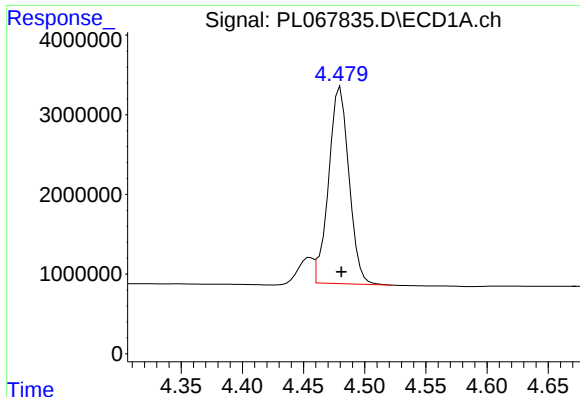

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 28644576
Conc: 52.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

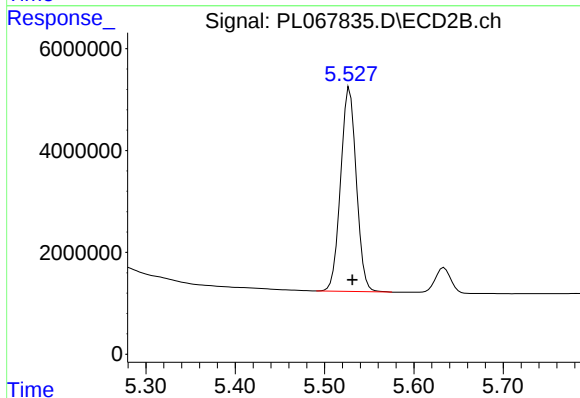


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 48895013
Conc: 51.87 ng/ml

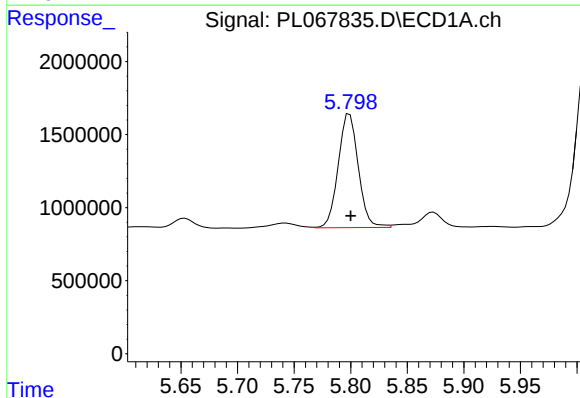


#23 Chlordane-1

R.T.: 5.799 min
Delta R.T.: 0.000 min
Response: 9612051
Conc: 519.52 ng/ml

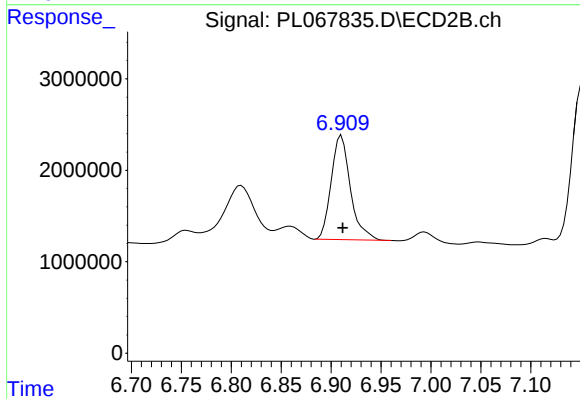

#23 Chlordane-1


R.T.: 6.910 min
Delta R.T.: -0.001 min
Response: 15096212
Conc: 534.61 ng/ml

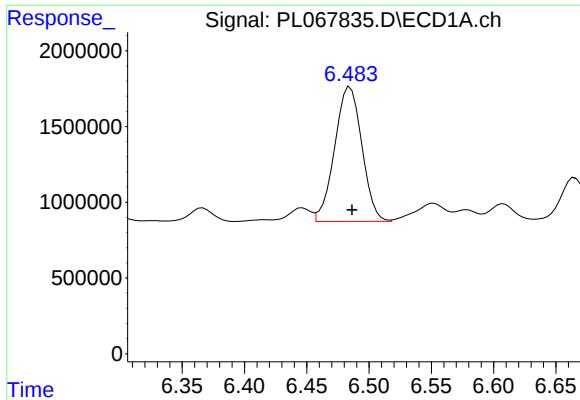

#24 Chlordane-2


R.T.: 6.485 min
Delta R.T.: -0.002 min
Response: 13535234
Conc: 505.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

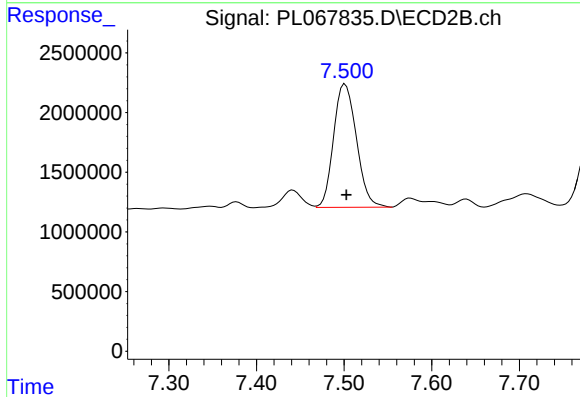


#24 Chlordane-2

R.T.: 7.501 min
Delta R.T.: -0.002 min
Response: 18757302
Conc: 514.66 ng/ml

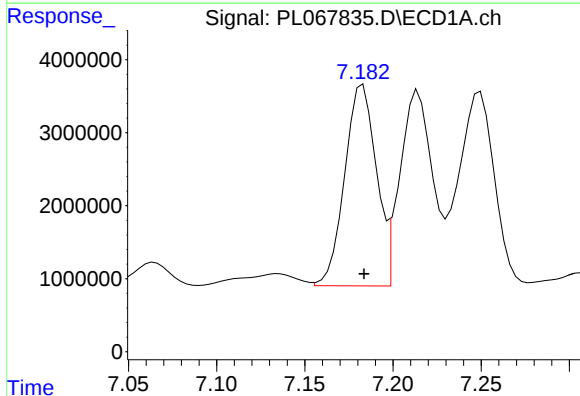


#25 Chlordane-3

R.T.: 7.183 min
Delta R.T.: 0.000 min
Response: 34364327
Conc: 511.45 ng/ml

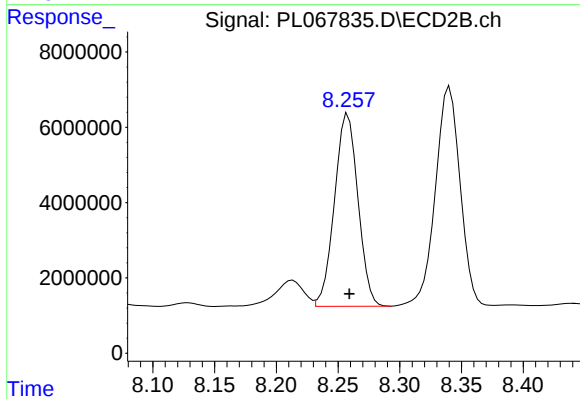

#25 Chlordane-3


R.T.: 8.258 min
Delta R.T.: -0.001 min
Response: 67784497
Conc: 506.47 ng/ml

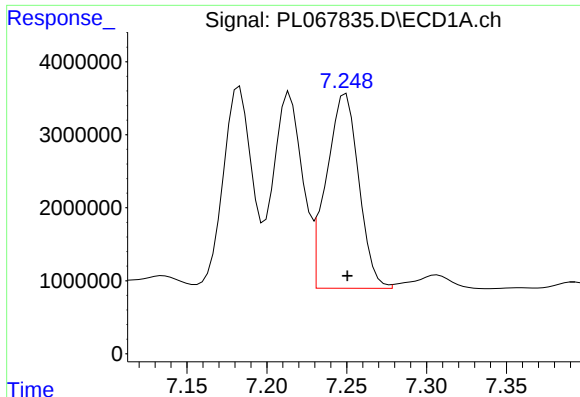

#26 Chlordane-4


R.T.: 7.249 min
Delta R.T.: -0.001 min
Response: 37480570
Conc: 512.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

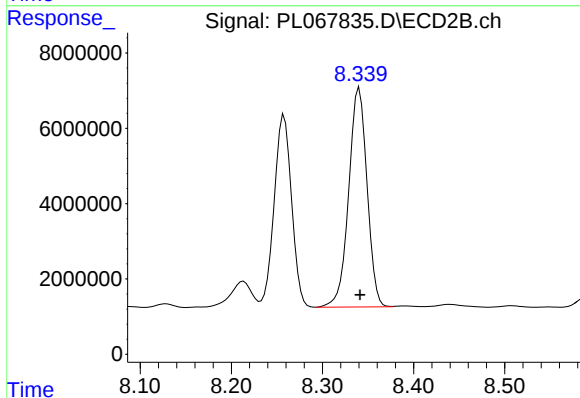


#26 Chlordane-4

R.T.: 8.340 min
Delta R.T.: 0.000 min
Response: 81342670
Conc: 501.80 ng/ml

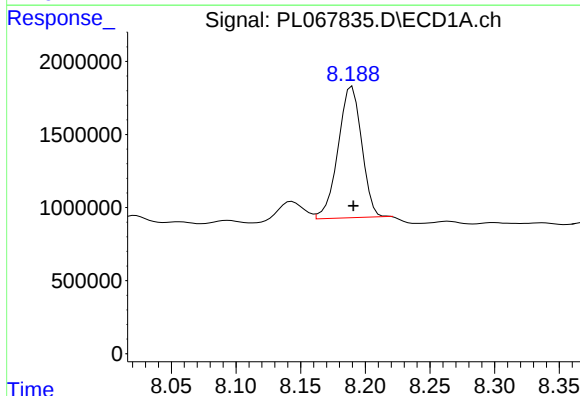


#27 Chlordane-5

R.T.: 8.190 min
Delta R.T.: -0.001 min
Response: 11405032
Conc: 521.28 ng/ml

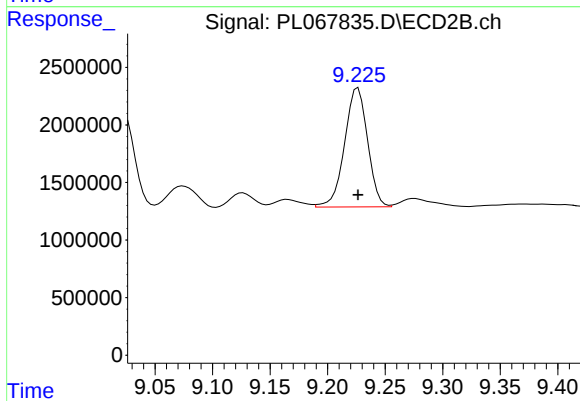

#27 Chlordane-5


R.T.: 9.226 min
Delta R.T.: 0.000 min
Response: 14431504
Conc: 496.31 ng/ml

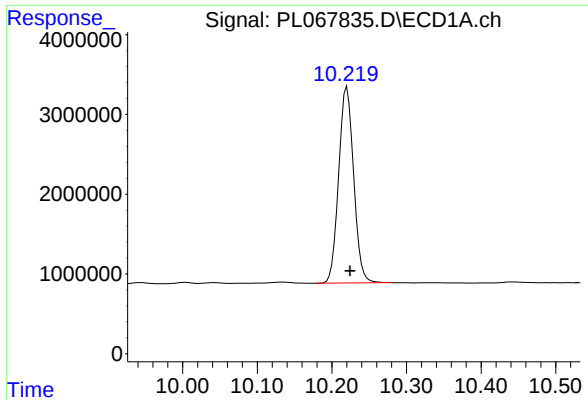

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 34320053
Conc: 48.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

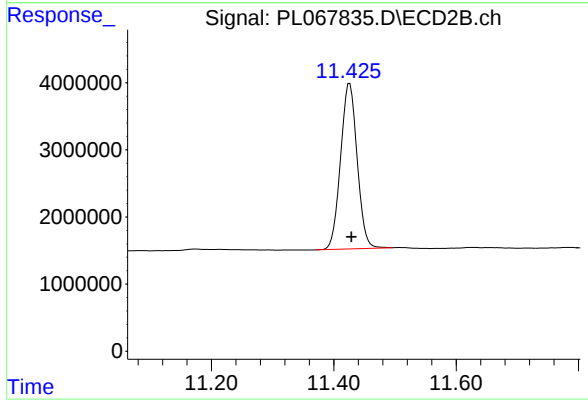

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 46388040
Conc: 46.57 ng/ml