

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
 Data File : PL067837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2021 11:15
 Operator : AR\AJ
 Sample : PB137329BS
 Misc : CHLOR BS
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB137329BS

Manual Integrations
 APPROVED

Ankita
 6/29/2021 12:26:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 06:15:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.525	11791436	20038897	21.447	21.256
28)	SA Decachlor...	10.219	11.422	15098148	20516996	21.304	20.598
Target Compounds							
23)	Chlordane-1	5.800	6.906	4385300	7987254	237.019	282.855m
24)	Chlordane-2	6.485	7.498	6346114	7648443	236.988	209.856
25)	Chlordane-3	7.182	8.255	13805590	26895773	205.469	200.958
26)	Chlordane-4	7.249	8.337	15105936	32886836	206.708	202.879
27)	Chlordane-5	8.189	9.222	4759372	5812665	217.531	199.901

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
Data File : PL067837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2021 11:15
Operator : AR\AJ
Sample : PB137329BS
Misc : CHLOR BS
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB137329BS


Manual Integrations
APPROVED

Ankita
6/29/2021 12:26:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 06:15:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

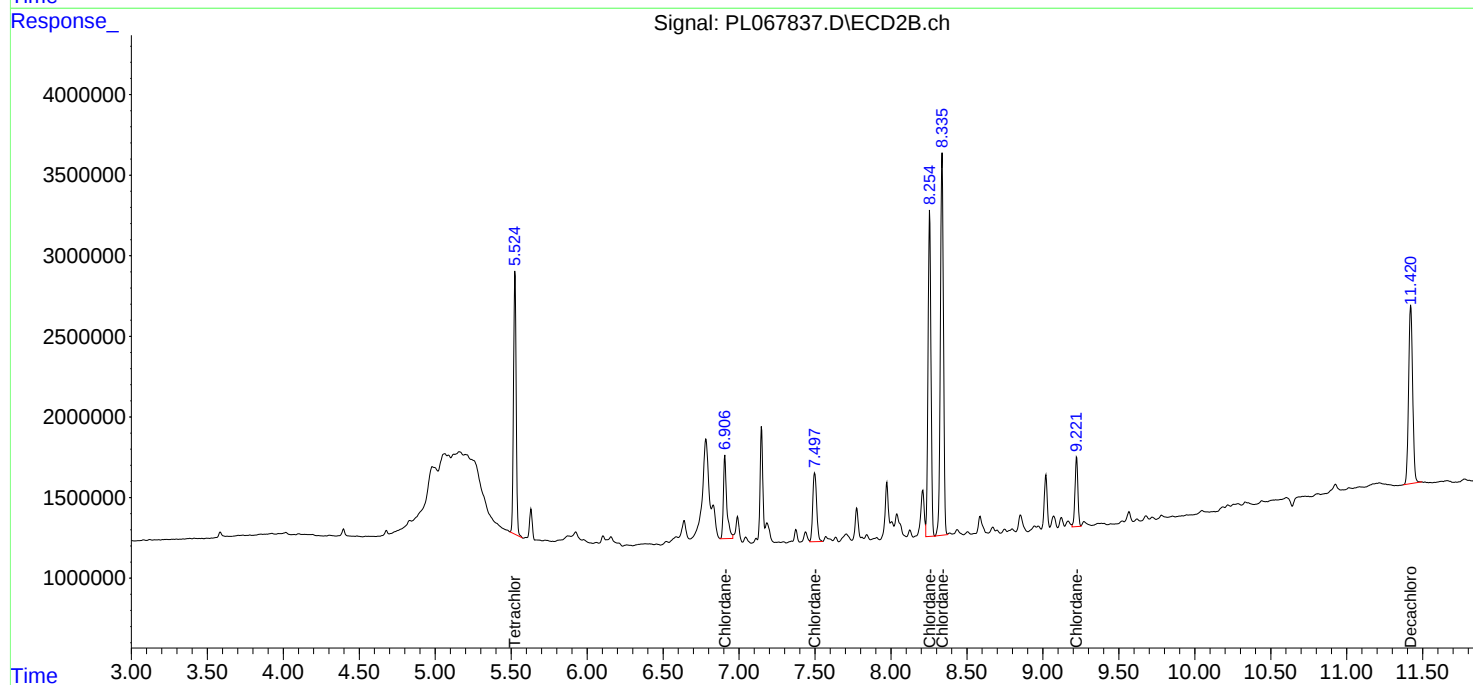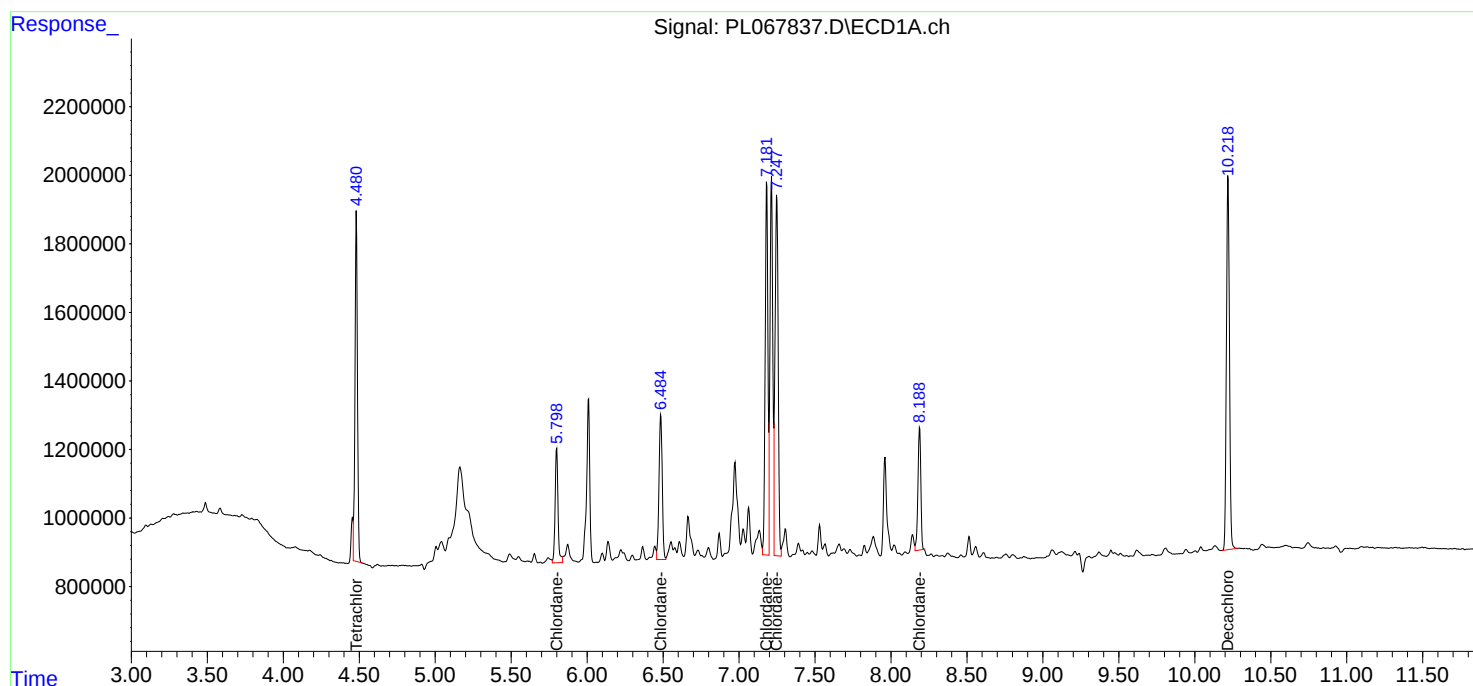

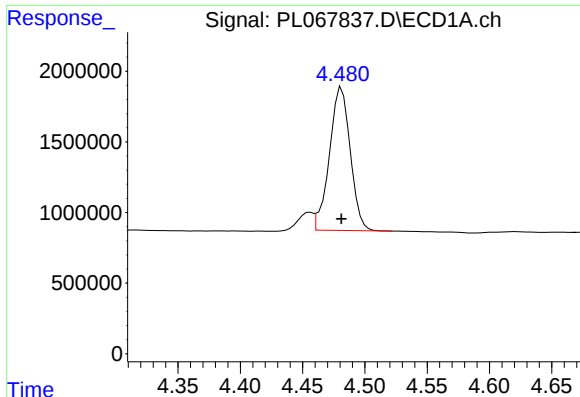


#1 Tetrachloro-m-xylene

R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 11791436
Conc: 21.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137329BS


Manual Integrations
APPROVED

Ankita
6/29/2021 12:26:33 PM

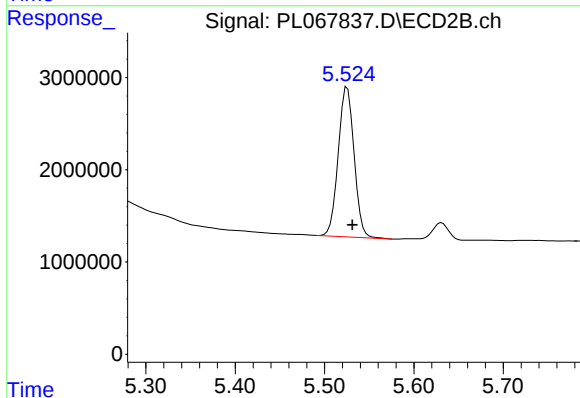


#1 Tetrachloro-m-xylene

R.T.: 5.525 min
Delta R.T.: -0.006 min
Response: 20038897
Conc: 21.26 ng/ml

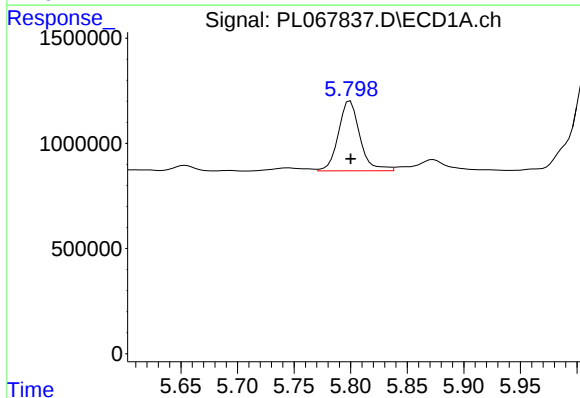


#23 Chlordane-1

R.T.: 5.800 min
Delta R.T.: 0.000 min
Response: 4385300
Conc: 237.02 ng/ml

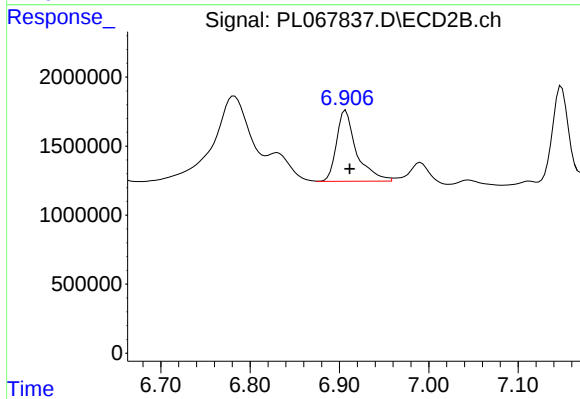

#23 Chlordane-1

R.T.: 6.906 min
Delta R.T.: -0.006 min
Response: 7987254
Conc: 282.85 ng/ml m

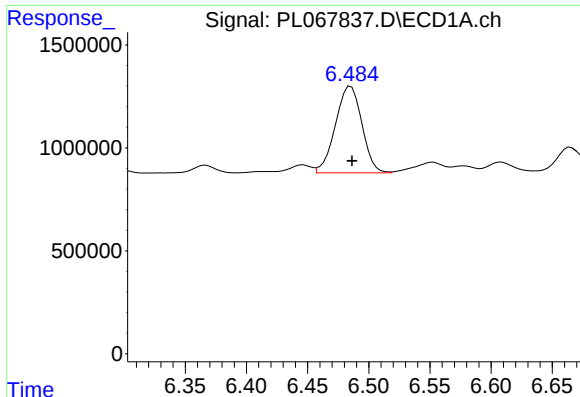


#24 Chlordane-2

R.T.: 6.485 min
Delta R.T.: 0.000 min
Response: 6346114
Conc: 236.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137329BS


Manual Integrations
APPROVED

Ankita
6/29/2021 12:26:33 PM

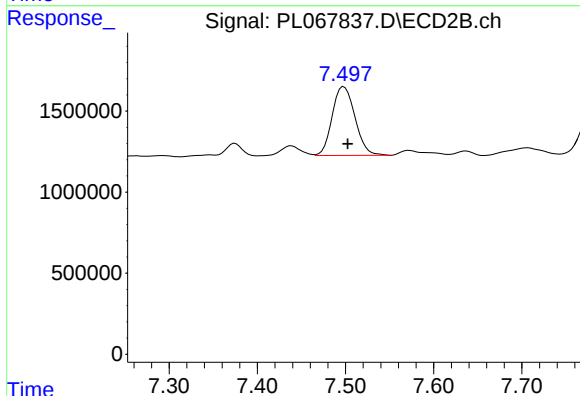


#24 Chlordane-2

R.T.: 7.498 min
Delta R.T.: -0.004 min
Response: 7648443
Conc: 209.86 ng/ml

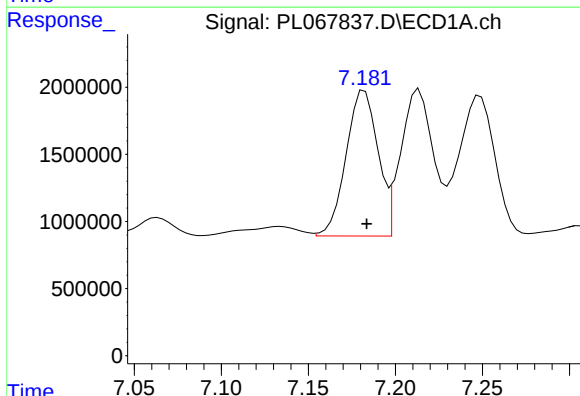


#25 Chlordane-3

R.T.: 7.182 min
Delta R.T.: -0.001 min
Response: 13805590
Conc: 205.47 ng/ml

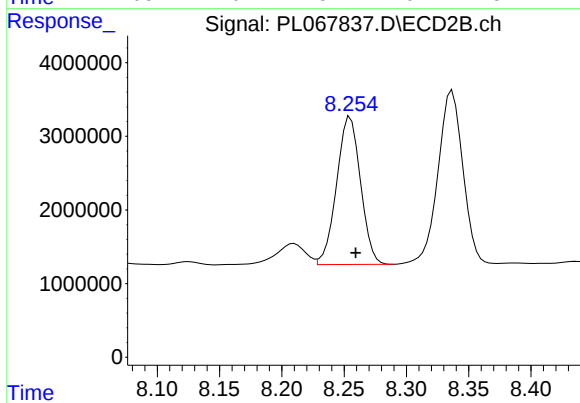

#25 Chlordane-3

R.T.: 8.255 min
Delta R.T.: -0.004 min
Response: 26895773
Conc: 200.96 ng/ml

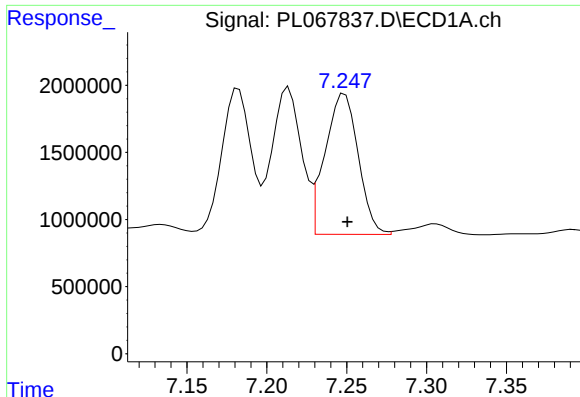


#26 Chlordane-4

R.T.: 7.249 min
Delta R.T.: -0.002 min
Response: 15105936
Conc: 206.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137329BS


Manual Integrations
APPROVED

Ankita
6/29/2021 12:26:33 PM

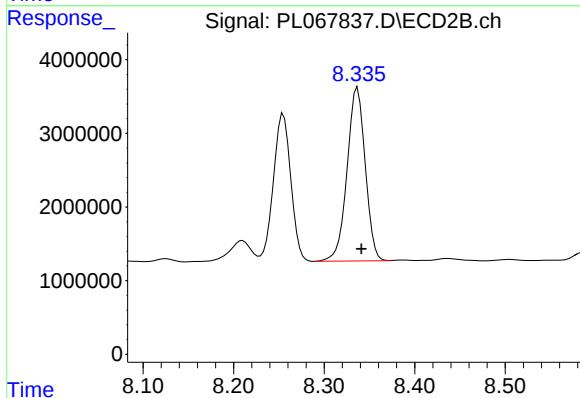


#26 Chlordane-4

R.T.: 8.337 min
Delta R.T.: -0.004 min
Response: 32886836
Conc: 202.88 ng/ml

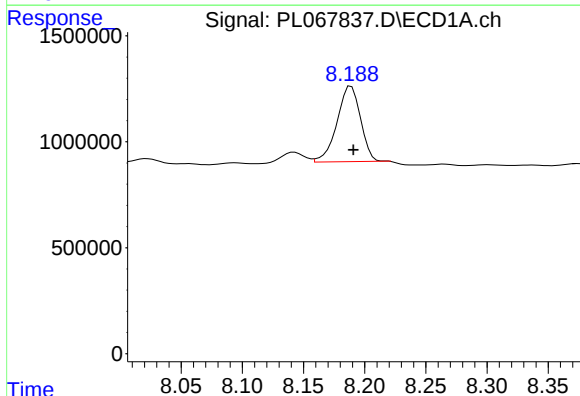


#27 Chlordane-5

R.T.: 8.189 min
Delta R.T.: -0.002 min
Response: 4759372
Conc: 217.53 ng/ml

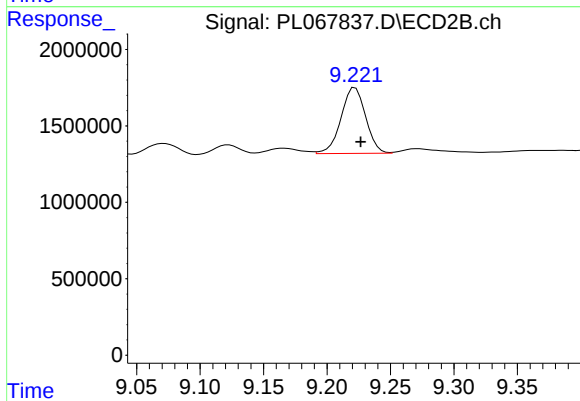

#27 Chlordane-5

R.T.: 9.222 min
Delta R.T.: -0.004 min
Response: 5812665
Conc: 199.90 ng/ml

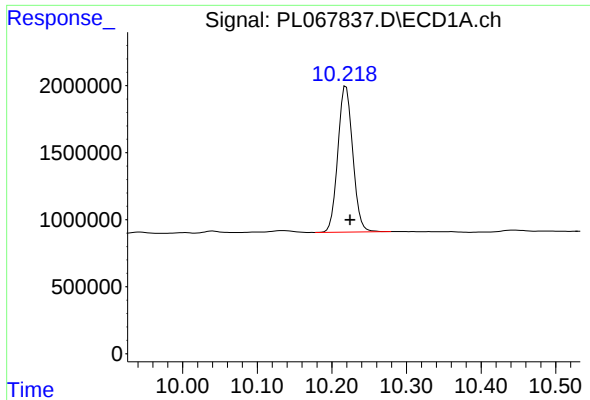


#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 15098148
Conc: 21.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137329BS

Manual Integrations
APPROVED

Ankita
6/29/2021 12:26:33 PM

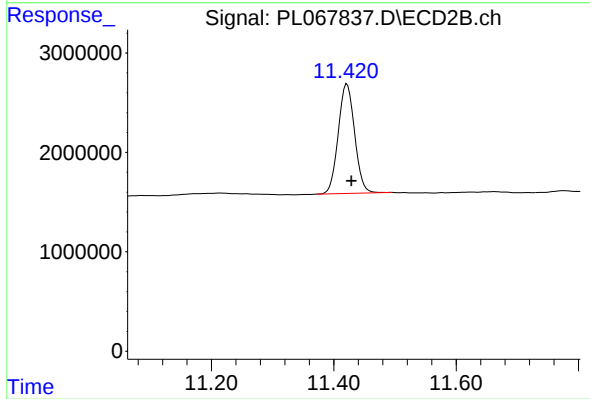

#28 Decachlorobiphenyl

R.T.: 11.422 min
Delta R.T.: -0.007 min
Response: 20516996
Conc: 20.60 ng/ml