

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
 Data File : PL067847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2021 16:37
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 06:15:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.483	5.526	28697888	50086356	52.198	53.129
28)	SA Decachlor...	10.222	11.426	33843788	48020460	47.756	48.211
Target Compounds							
23)	Chlordane-1	5.802	6.908	9606214	18740159	519.202	663.650 #
24)	Chlordane-2	6.487	7.499	13338993	19404352	498.128	532.411
25)	Chlordane-3	7.185	8.257	34239958	70237023	509.594	524.792
26)	Chlordane-4	7.251	8.339	37263491	84819216	509.909	523.251
27)	Chlordane-5	8.191	9.225	11087346	14990970	506.756	515.549



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
Data File : PL067847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2021 16:37
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 06:15:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

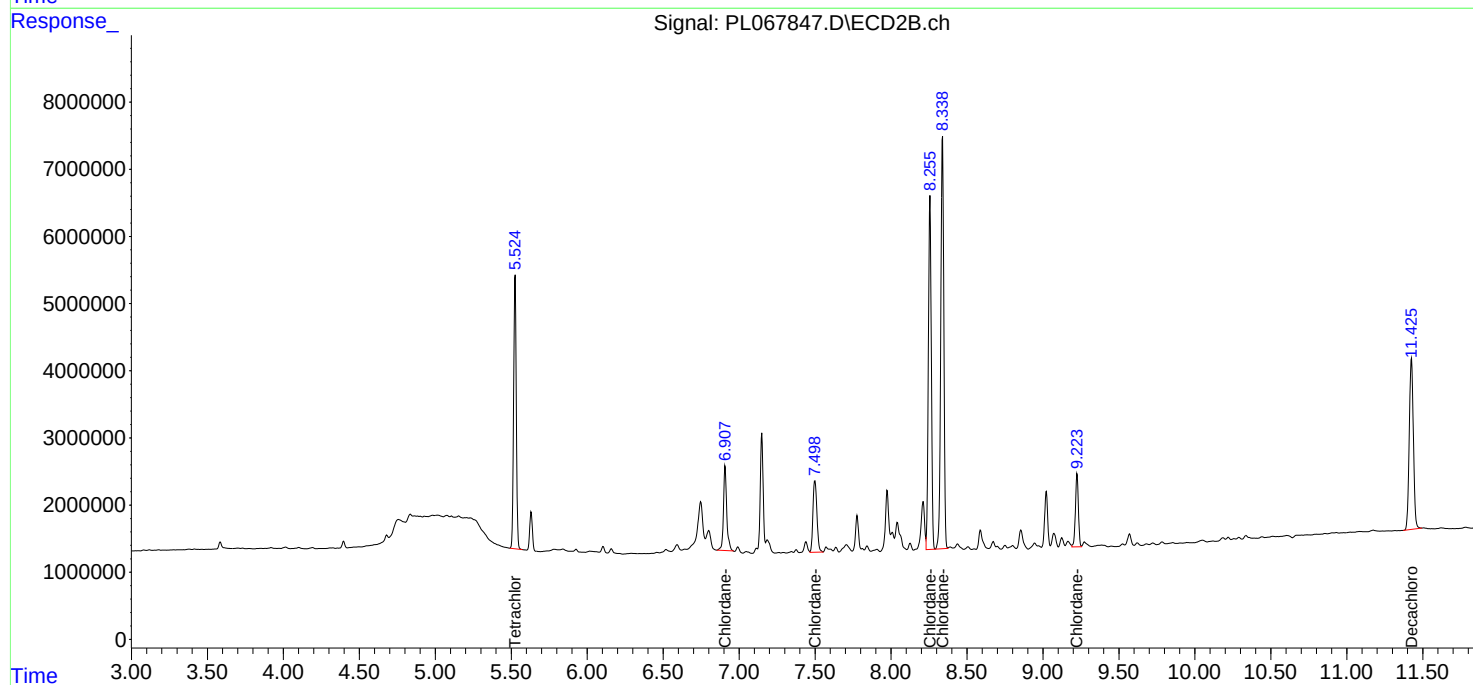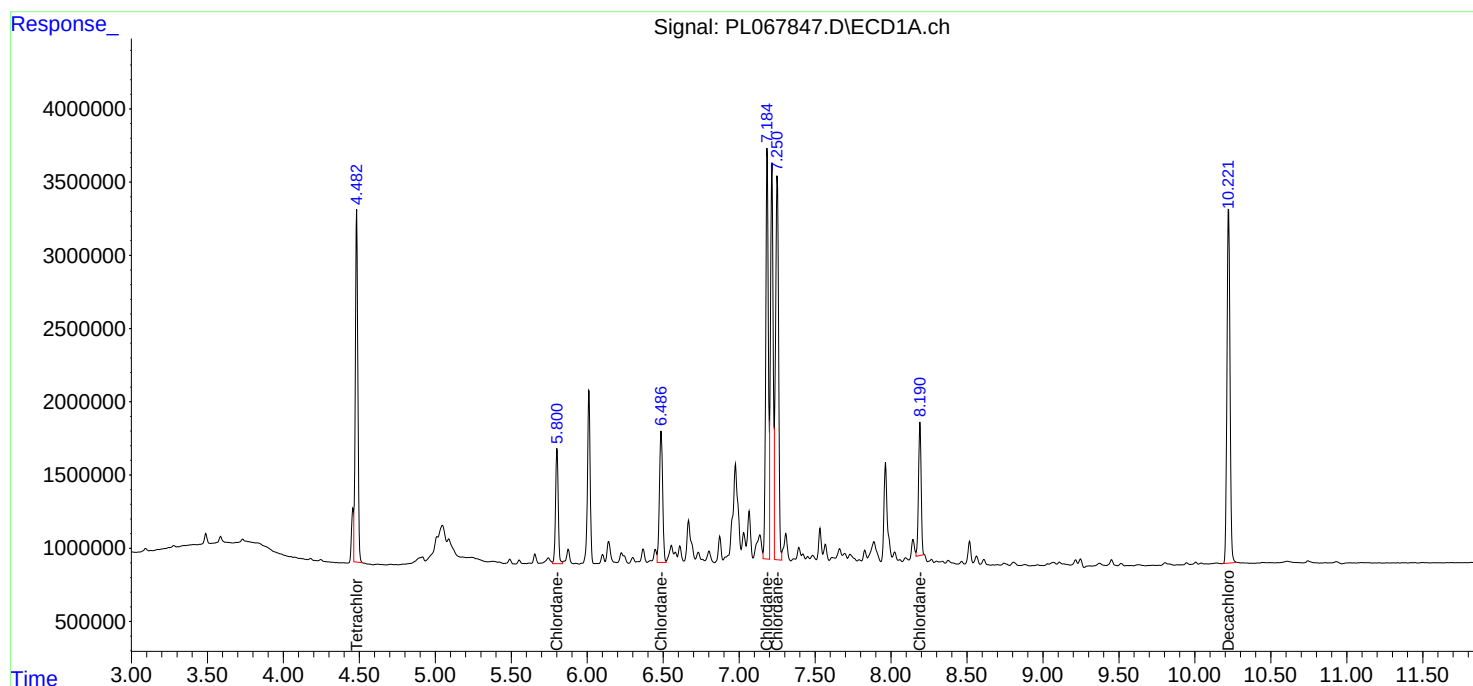


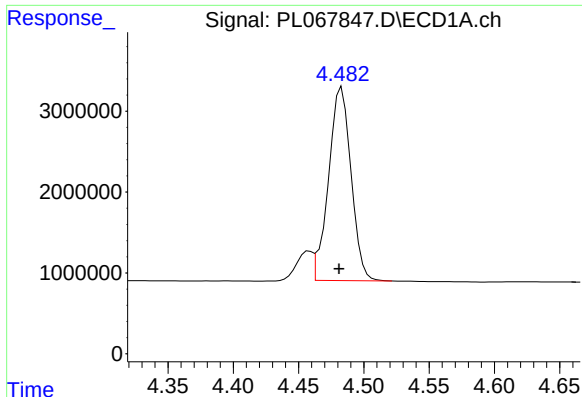

#1 Tetrachloro-m-xylene


R.T.: 4.483 min
Delta R.T.: 0.002 min
Response: 28697888
Conc: 52.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

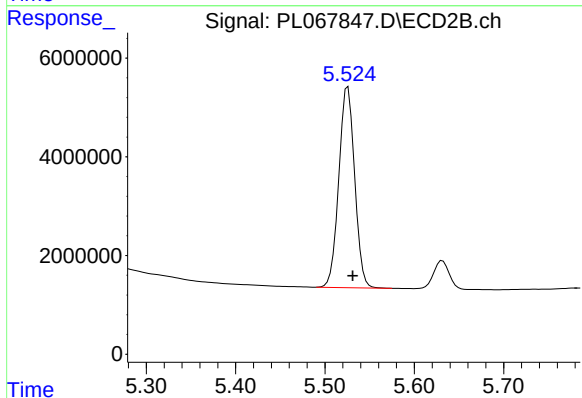


#1 Tetrachloro-m-xylene

R.T.: 5.526 min
Delta R.T.: -0.005 min
Response: 50086356
Conc: 53.13 ng/ml

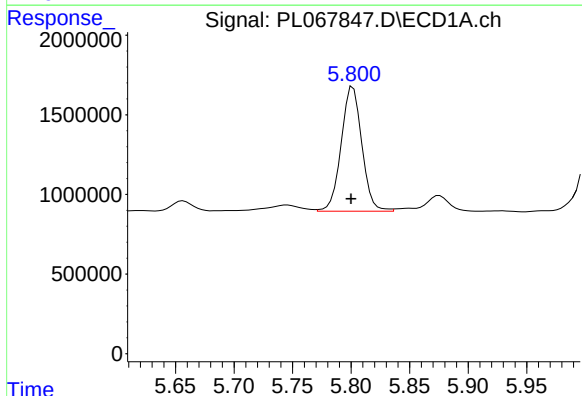


#23 Chlordane-1

R.T.: 5.802 min
Delta R.T.: 0.002 min
Response: 9606214
Conc: 519.20 ng/ml

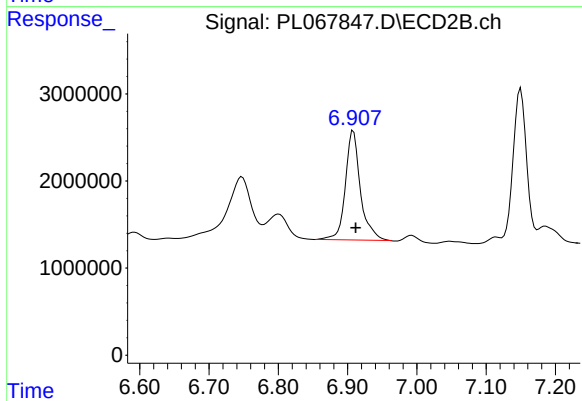

#23 Chlordane-1


R.T.: 6.908 min
Delta R.T.: -0.003 min
Response: 18740159
Conc: 663.65 ng/ml

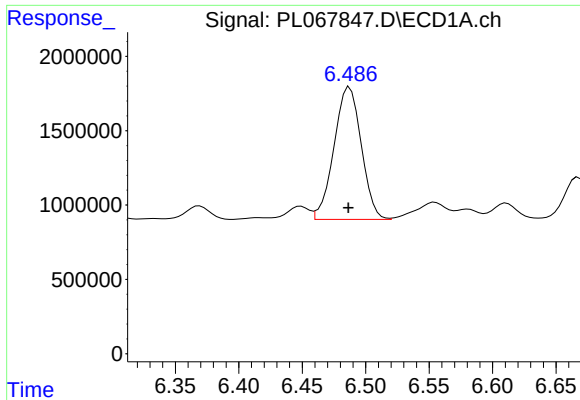

#24 Chlordane-2


R.T.: 6.487 min
Delta R.T.: 0.001 min
Response: 13338993
Conc: 498.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

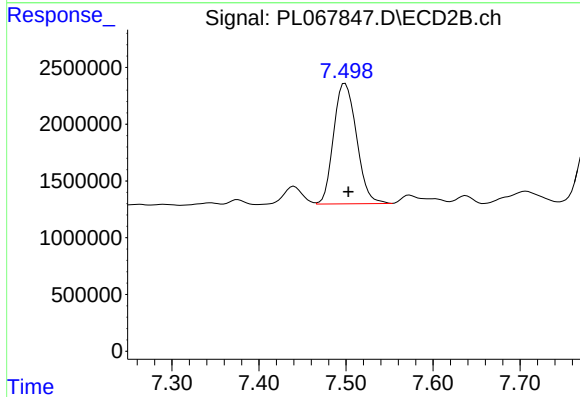


#24 Chlordane-2

R.T.: 7.499 min
Delta R.T.: -0.004 min
Response: 19404352
Conc: 532.41 ng/ml

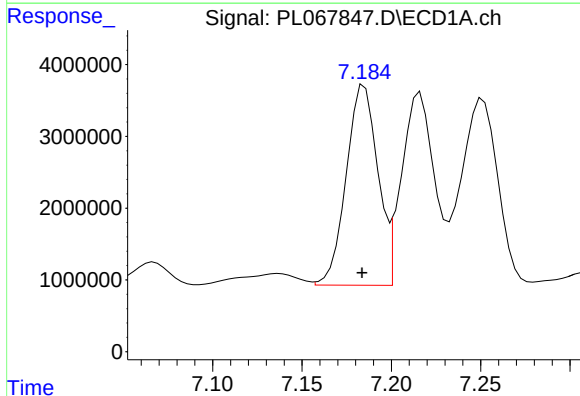


#25 Chlordane-3

R.T.: 7.185 min
Delta R.T.: 0.001 min
Response: 34239958
Conc: 509.59 ng/ml

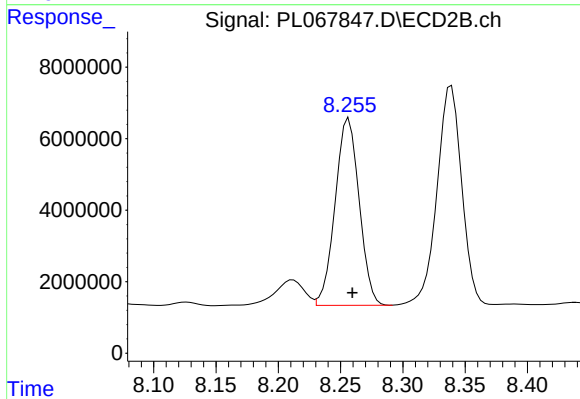

#25 Chlordane-3


R.T.: 8.257 min
Delta R.T.: -0.003 min
Response: 70237023
Conc: 524.79 ng/ml

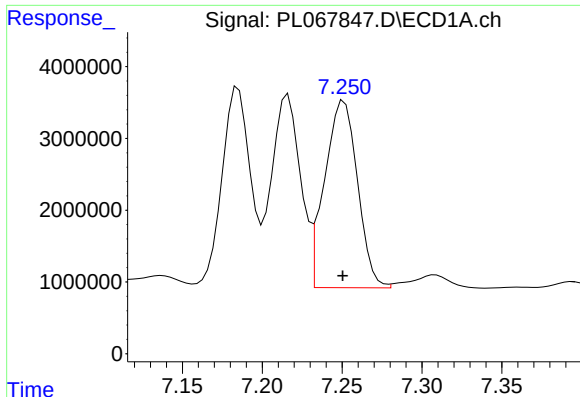

#26 Chlordane-4


R.T.: 7.251 min
Delta R.T.: 0.000 min
Response: 37263491
Conc: 509.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

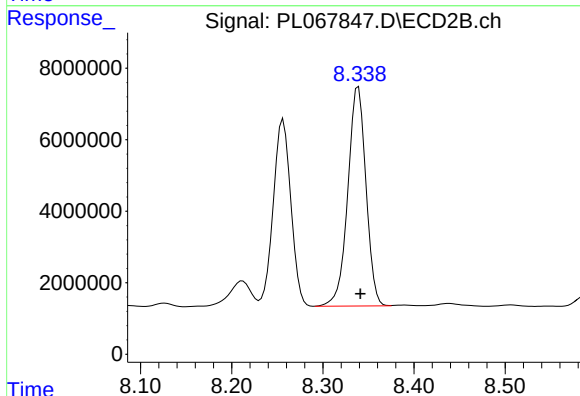


#26 Chlordane-4

R.T.: 8.339 min
Delta R.T.: -0.002 min
Response: 84819216
Conc: 523.25 ng/ml

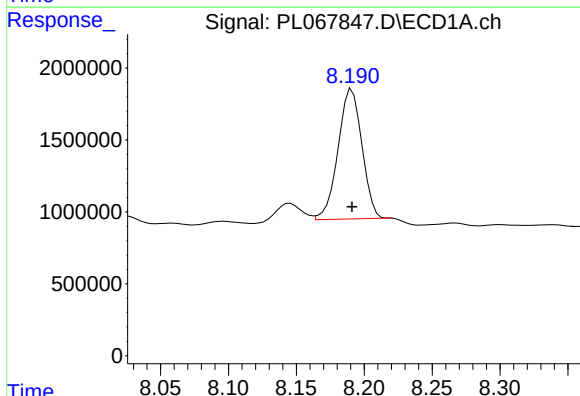


#27 Chlordane-5

R.T.: 8.191 min
Delta R.T.: 0.000 min
Response: 11087346
Conc: 506.76 ng/ml

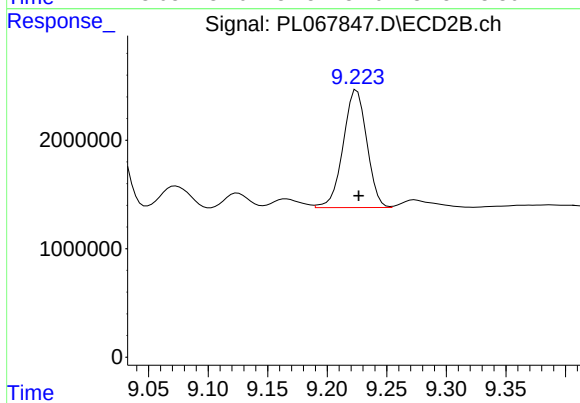

#27 Chlordane-5


R.T.: 9.225 min
Delta R.T.: -0.002 min
Response: 14990970
Conc: 515.55 ng/ml

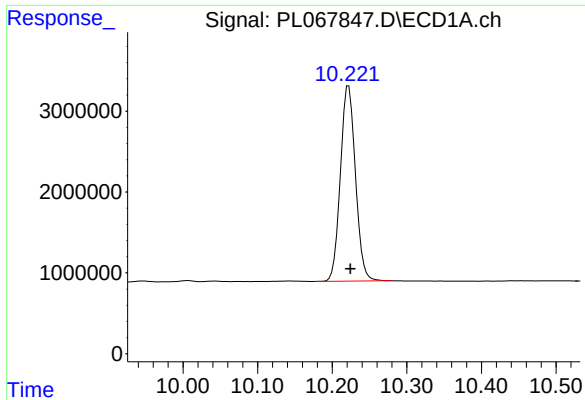

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.002 min
Response: 33843788
Conc: 47.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

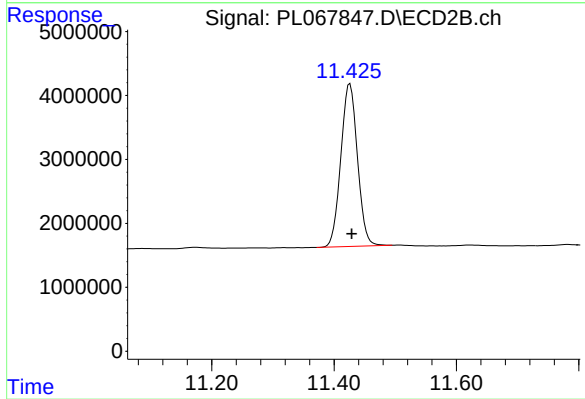

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 48020460
Conc: 48.21 ng/ml