

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
 Data File : PL067859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2021 20:36
 Operator : AR\AJ
 Sample : M2866-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 124030

Manual Integrations
 APPROVED

Ankita
 6/29/2021 12:26:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 06:42:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	7927220	14088710	14.419	14.945
28)	SA Decachlor...	10.218	11.425	11067683	16365798	15.617	16.431
Target Compounds							
12)	B 4,4'-DDE	7.467	8.520	1010808	572748	1.519	0.632 #
17)	MA 4,4'-DDT	8.304	9.381	502784	339419	0.864	0.463m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062821\
Data File : PL067859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2021 20:36
Operator : AR\AJ
Sample : M2866-03
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
124030


Manual Integrations
APPROVED

Ankita
6/29/2021 12:26:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 06:42:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

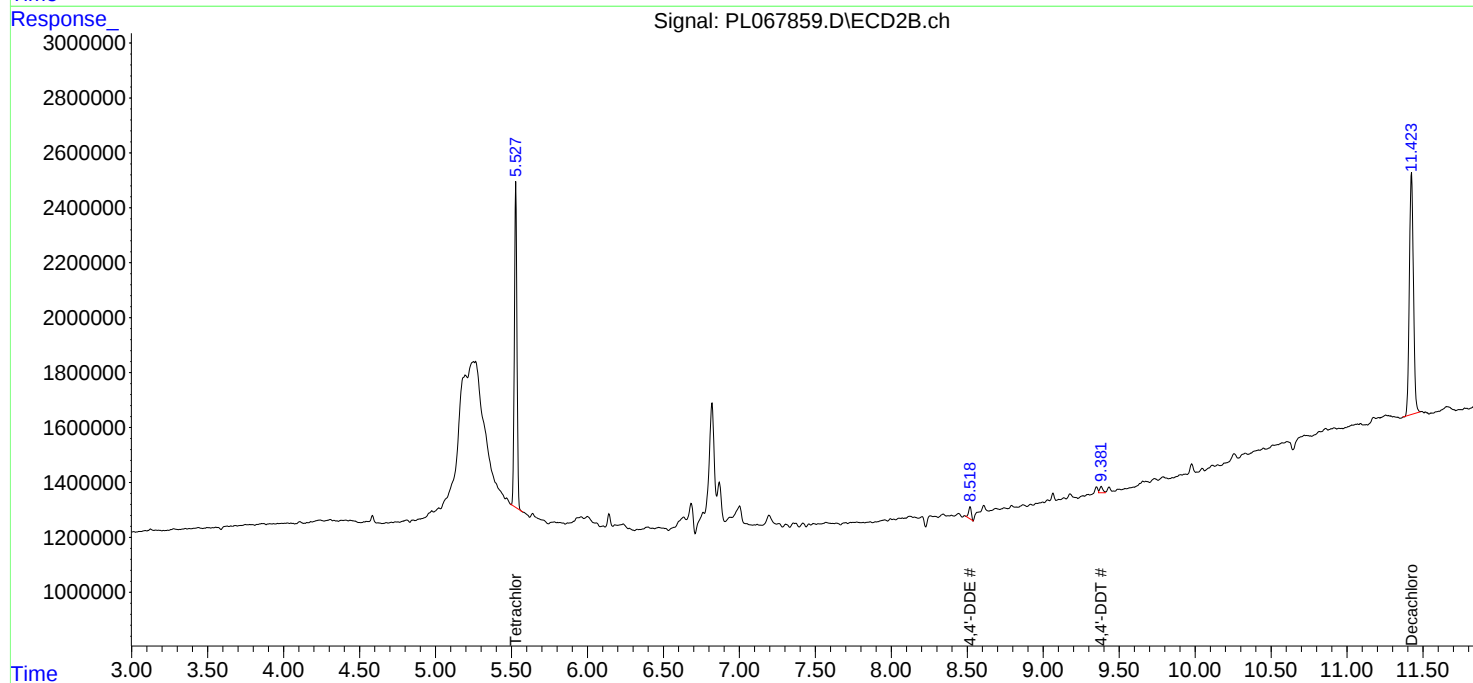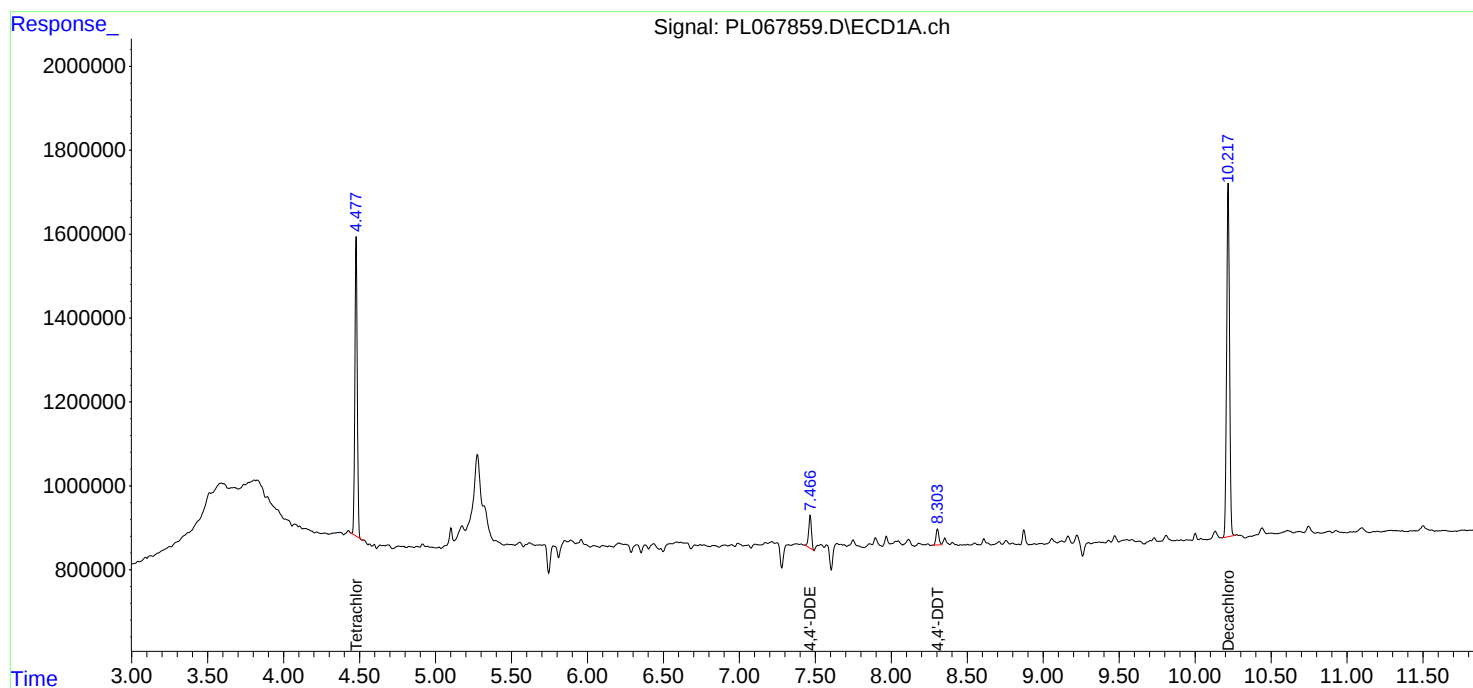

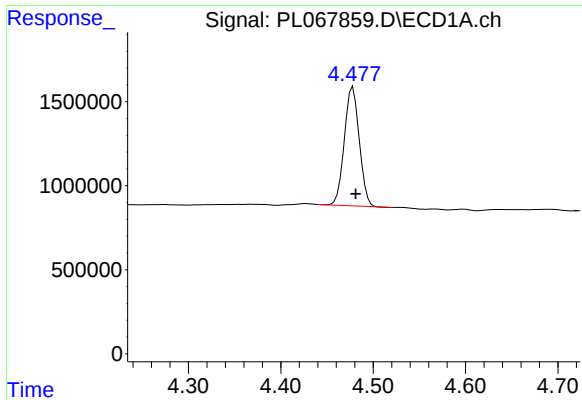


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 7927220
Conc: 14.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
124030


Manual Integrations
APPROVED

Ankita
6/29/2021 12:26:47 PM

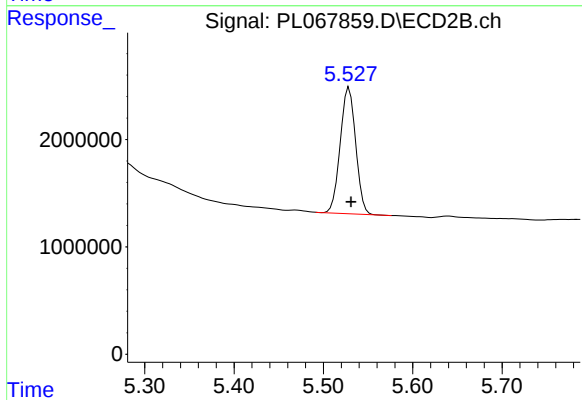


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 14088710
Conc: 14.94 ng/ml

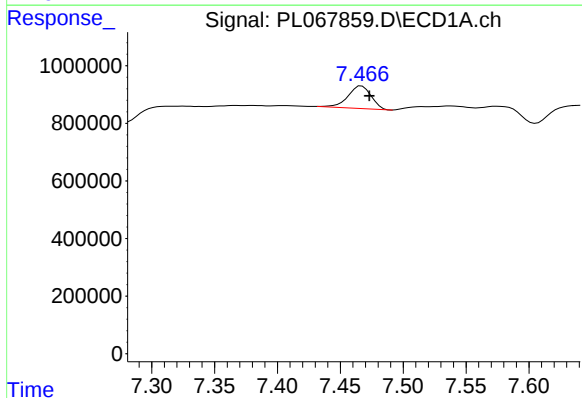


#12 4,4'-DDE

R.T.: 7.467 min
Delta R.T.: -0.006 min
Response: 1010808
Conc: 1.52 ng/ml

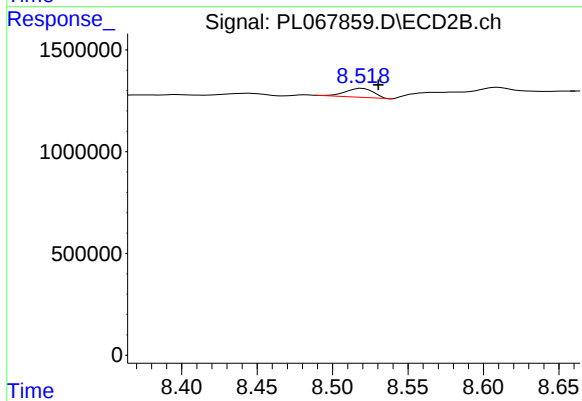

#12 4,4'-DDE

R.T.: 8.520 min
Delta R.T.: -0.010 min
Response: 572748
Conc: 0.63 ng/ml

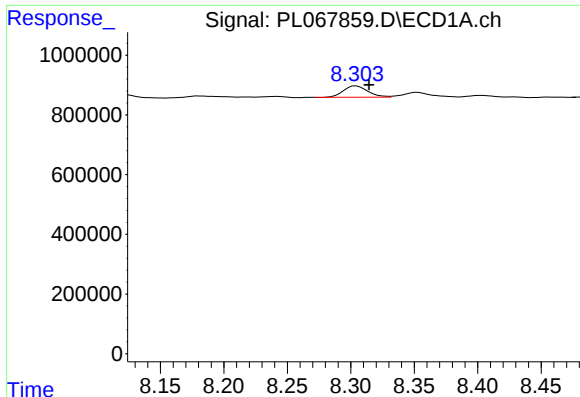


#17 4,4'-DDT

R.T.: 8.304 min
Delta R.T.: -0.010 min
Response: 502784
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
124030


Manual Integrations
APPROVED

Ankita
6/29/2021 12:26:47 PM

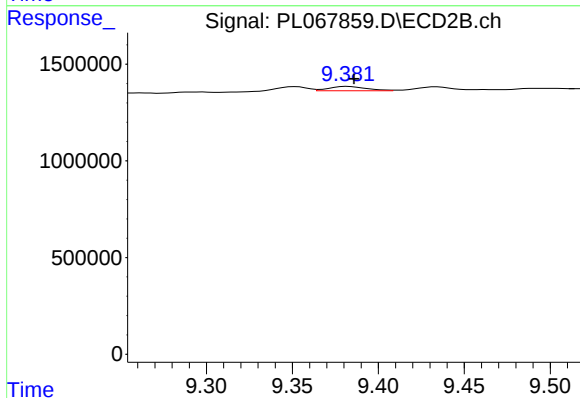


#17 4,4'-DDT

R.T.: 9.381 min
Delta R.T.: -0.005 min
Response: 339419
Conc: 0.46 ng/ml m

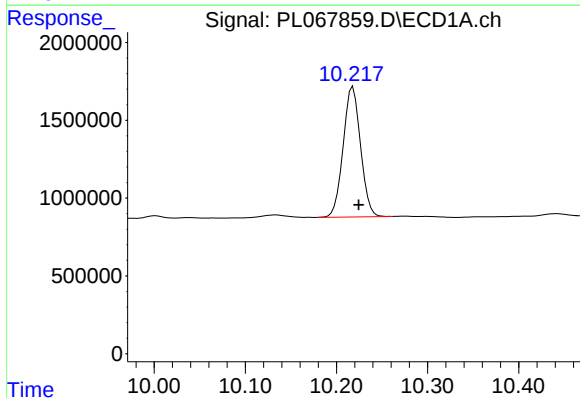

#28 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: -0.006 min
Response: 11067683
Conc: 15.62 ng/ml

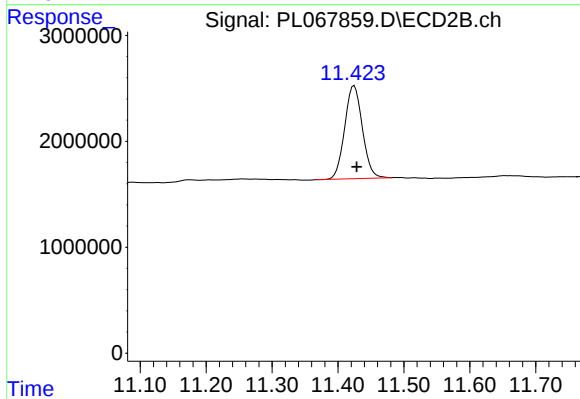

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.004 min
Response: 16365798
Conc: 16.43 ng/ml